
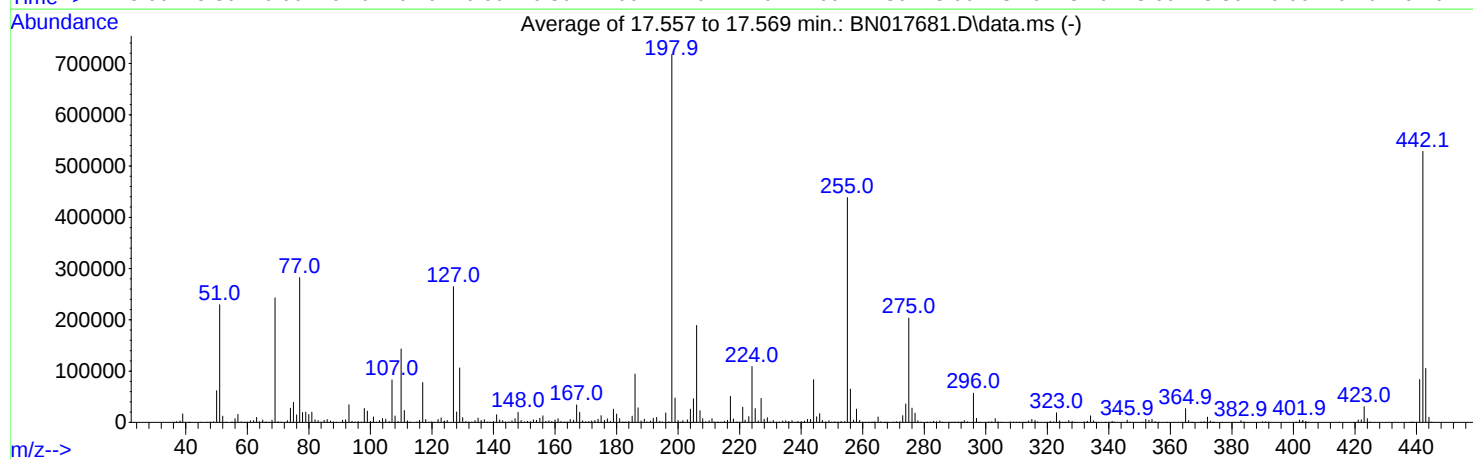


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120221\
 Data File : BN017681.D
 Acq On : 02 Dec 2021 13:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN113021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 02 01:51:49 2021

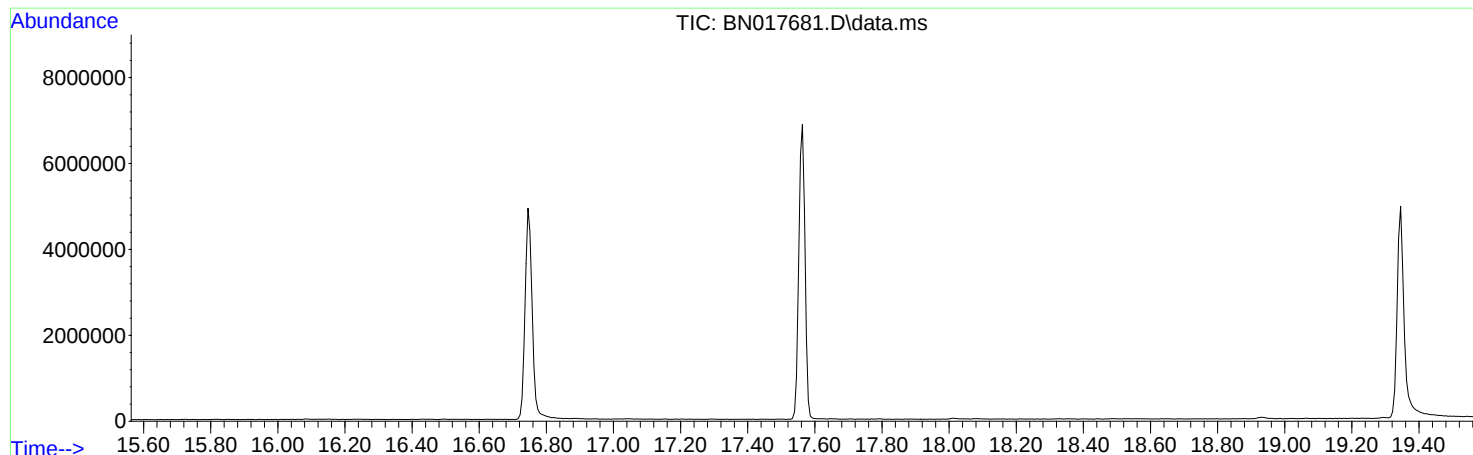

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	229450	PASS
68	69	0.00	2	1.7	4224	PASS
69	198	0.00	100	33.8	242762	PASS
70	69	0.00	2	0.7	1724	PASS
127	198	10	80	36.9	264811	PASS
197	198	0.00	2	0.2	1379	PASS
198	198	100	100	100.0	717632	PASS
199	198	5	9	6.6	47437	PASS
275	198	10	60	28.4	203605	PASS
365	198	1	100	3.7	26792	PASS
441	198	0.01	100	11.7	83685	PASS
442	442	50	100	100.0	528747	PASS
443	442	15	24	19.9	105101	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/2/2021	BNA_N	<u>BN017681.D</u>
Compound Name	Response	Retention Time
DDT	2022749	20.59
DDD	25604	20.15
DDE	894	19.63
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26498	2049247	1.29

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120221\
Data File : BN017681.D
Acq On : 02 Dec 2021 13:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 03 03:30:42 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 03 03:30:36 2021
Response via : Initial Calibration

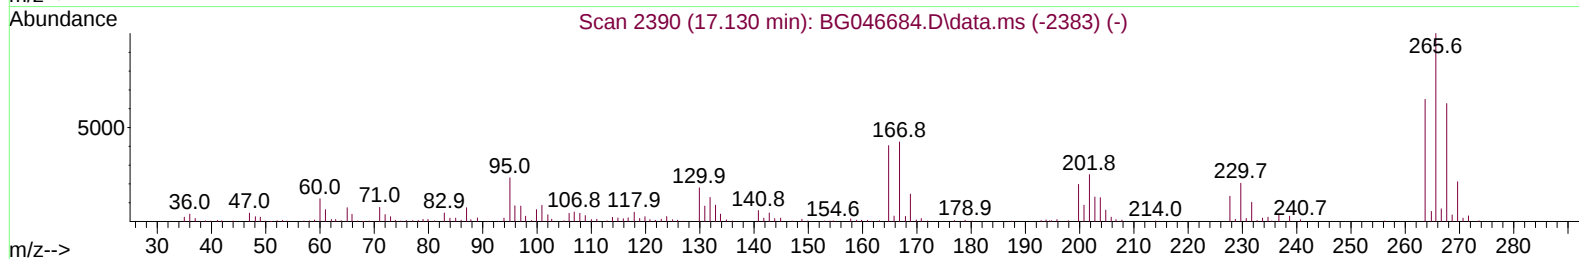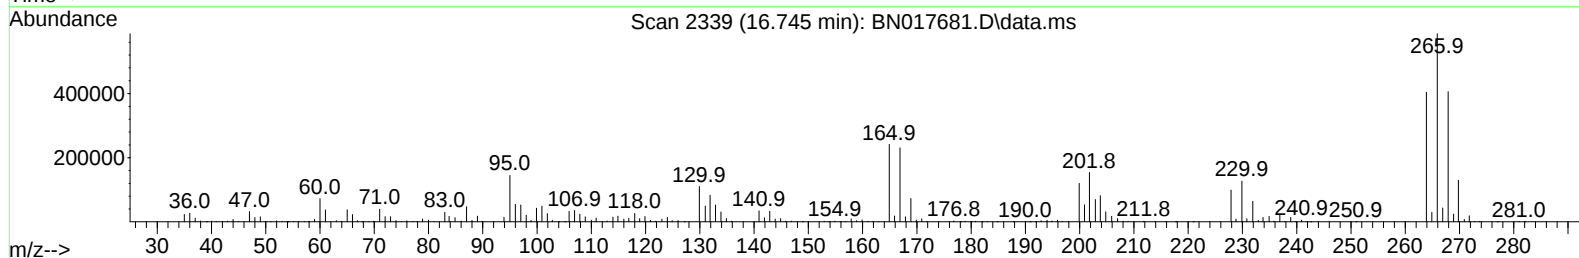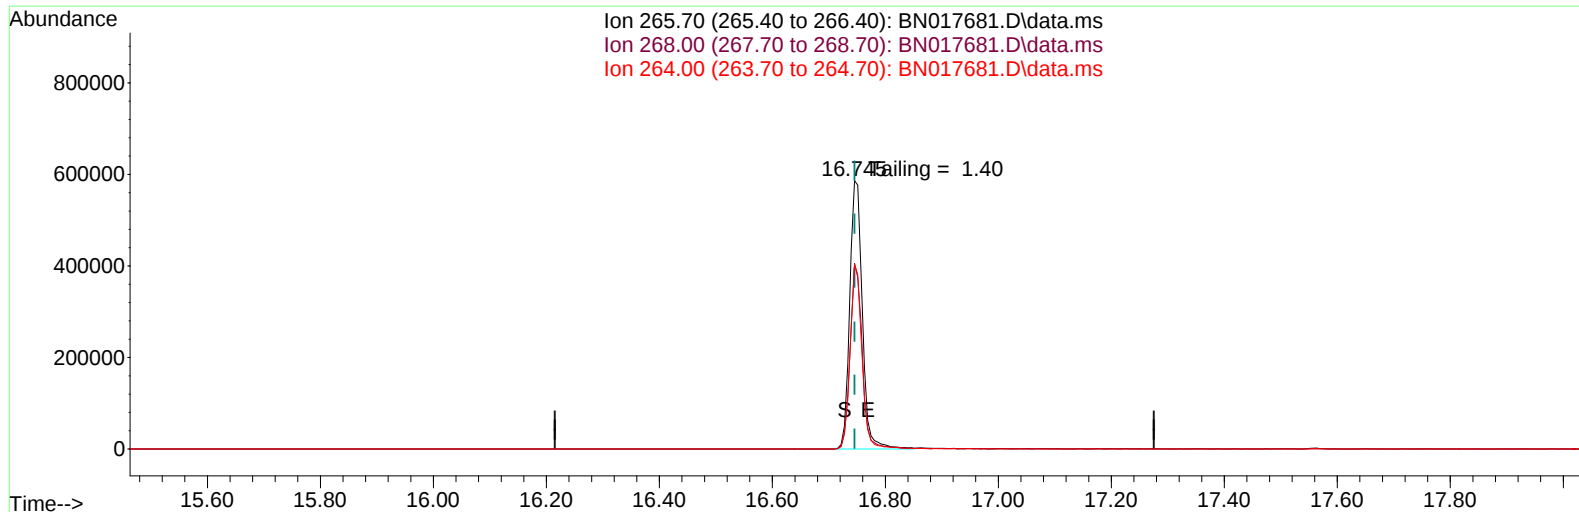

TIC: BN017681.D\data.ms

(70) Pentachlorophenol (C)

16.745min (0.000) 27823.06 ng




response 911386

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.18
264.00	61.60	68.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120221\
 Data File : BN017681.D
 Acq On : 02 Dec 2021 13:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 03 03:30:42 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 03 03:30:36 2021
 Response via : Initial Calibration

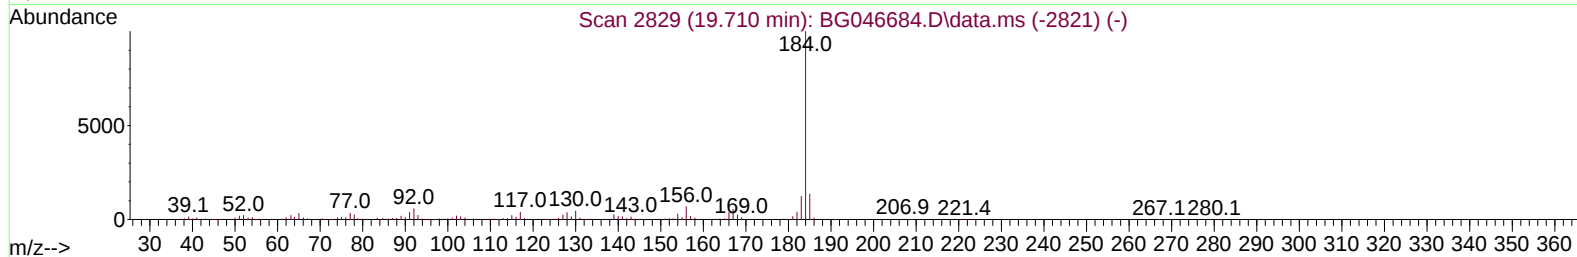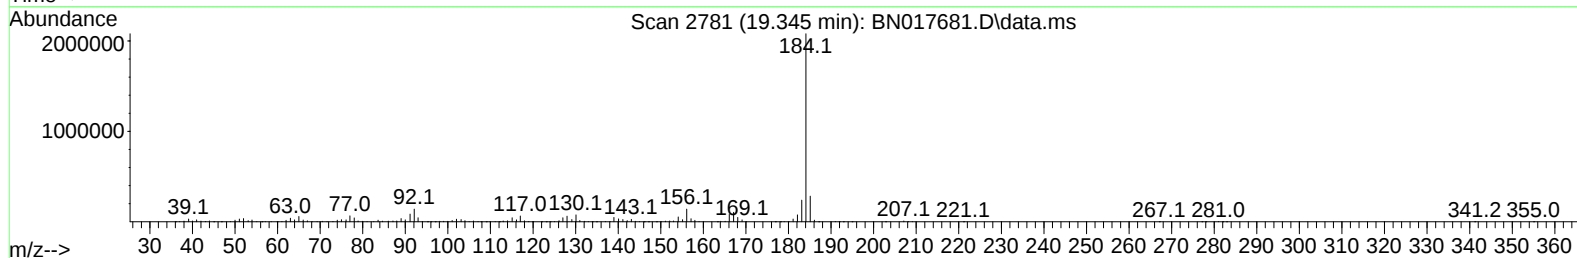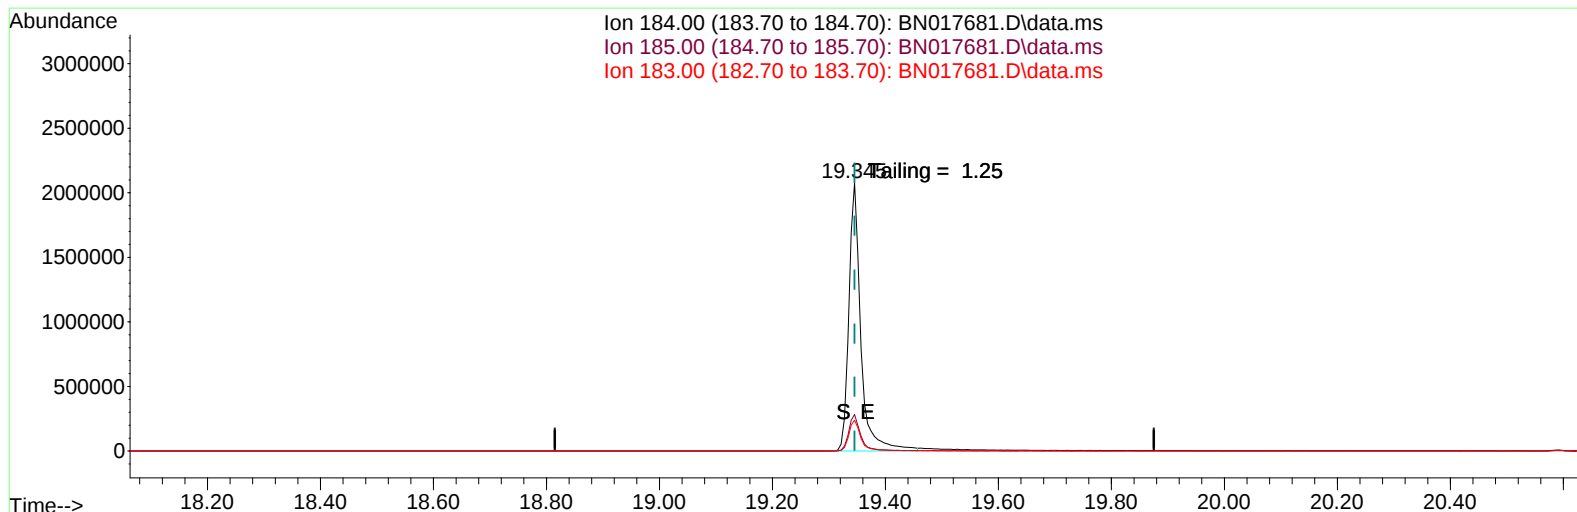

TIC: BN017681.D\data.ms

(77) Benzidine

19.345min (0.000) 0.00 ng

response 3147451

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.60
183.00	13.20	11.51
0.00	0.00	0.00