
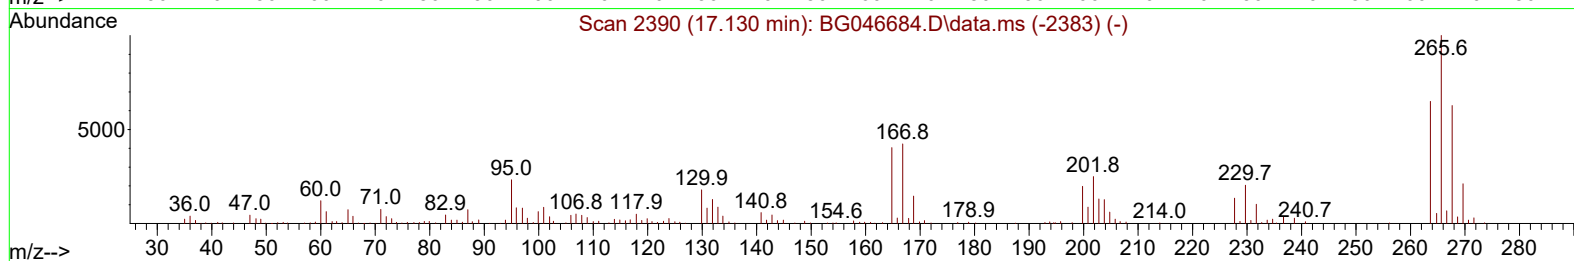
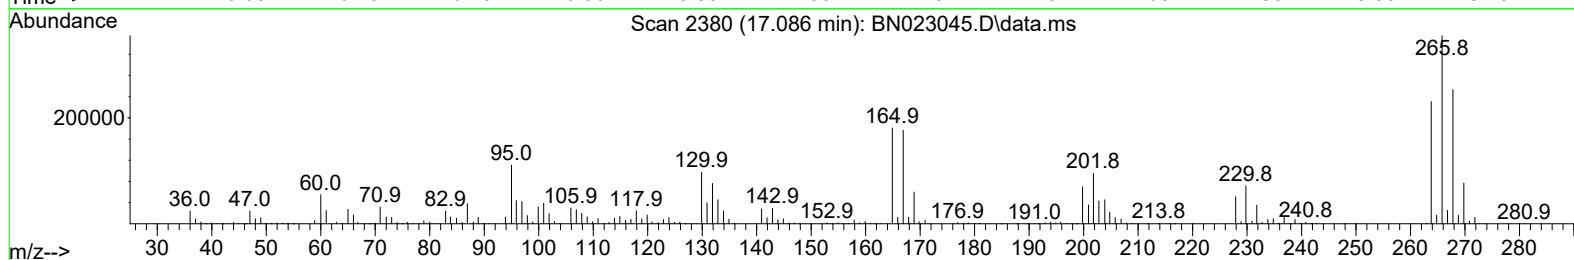


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120222\
Data File : BN023045.D
Acq On : 02 Dec 2022 12:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 01:34:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 05 01:34:14 2022
Response via : Initial Calibration

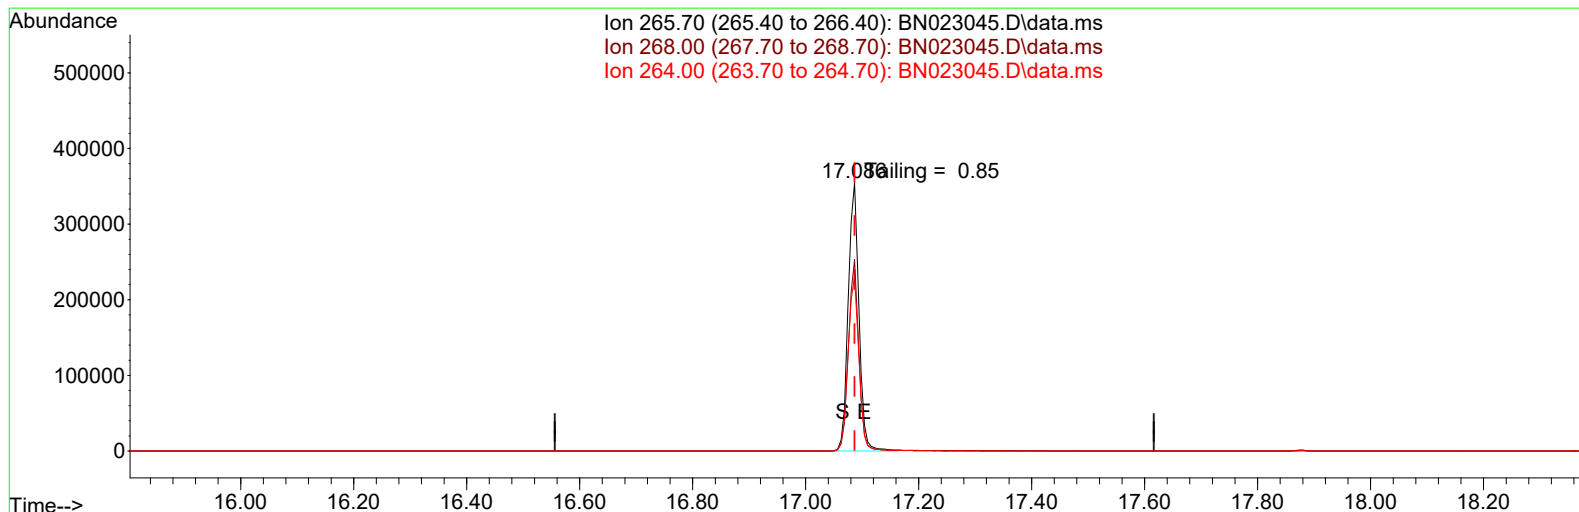

TIC: BN023045.D\data.ms

(70) Pentachlorophenol (C)




17.086min (0.000) 16272.58 ng

response 470586

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	71.33
264.00	61.60	65.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120222\
Data File : BN023045.D
Acq On : 02 Dec 2022 12:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 01:34:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 05 01:34:14 2022
Response via : Initial Calibration

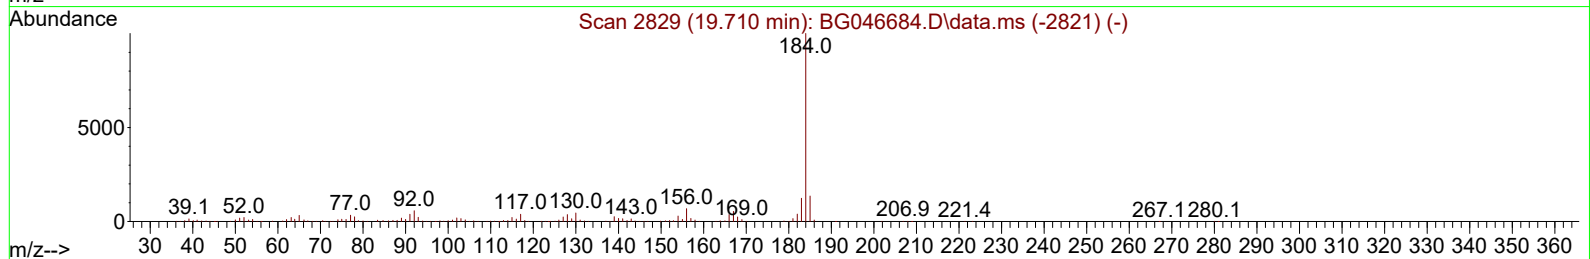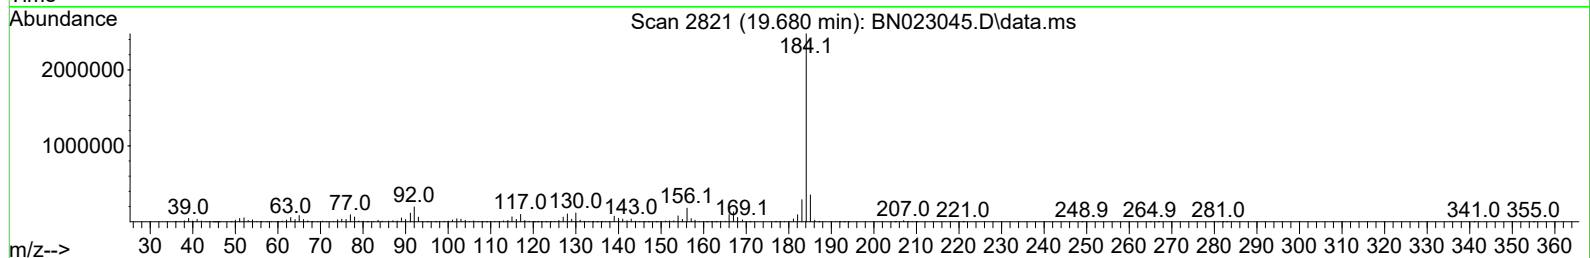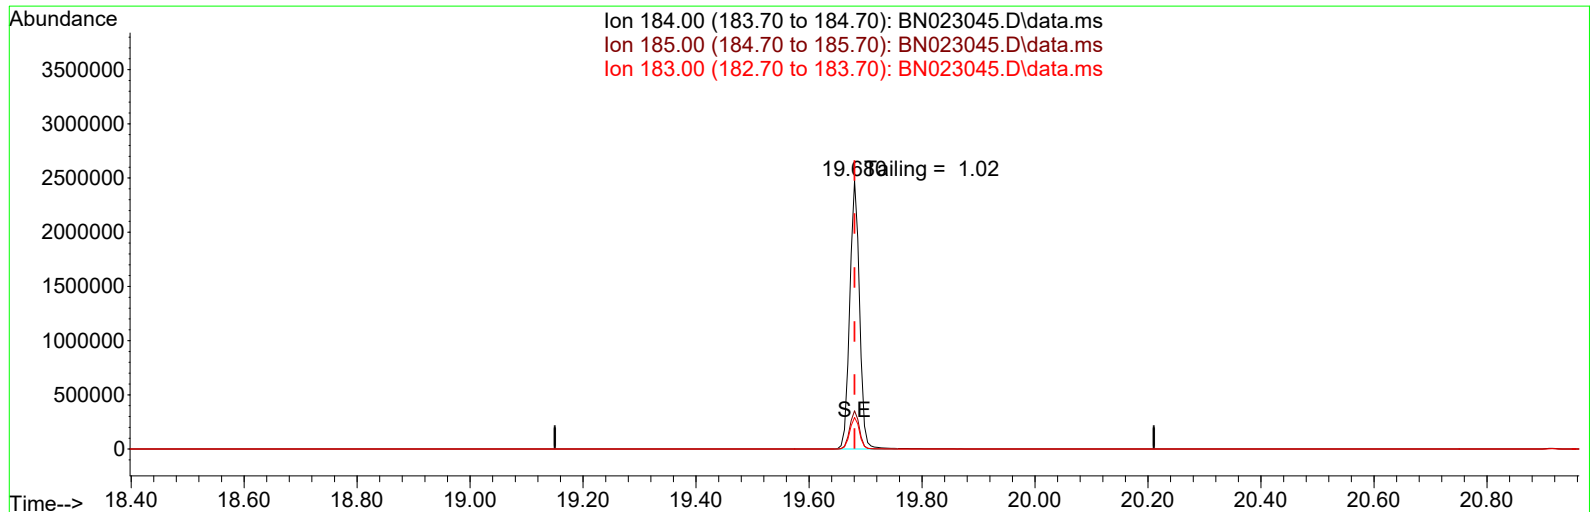

TIC: BN023045.D\data.ms

(77) Benzidine**19.680min (0.000) 294089.64 ng****response 2982524**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.28
183.00	13.20	11.76
0.00	0.00	0.00