

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120222\
 Data File : BN023047.D
 Acq On : 02 Dec 2022 14:31
 Operator : CG/JU
 Sample : PB149383BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB149383BL

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 12/05/2022
 Supervised By : Jagrut Upadhyay 12/05/2022

Quant Time: Dec 05 00:33:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 02:30:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.049	152	6802	0.400	ng	0.00
7) Naphthalene-d8	10.861	136	17940	0.400	ng	-0.01
13) Acenaphthene-d10	14.687	164	8641	0.400	ng	0.00
19) Phenanthrene-d10	17.439	188	16742	0.400	ng	# 0.00
29) Chrysene-d12	21.625	240	9396	0.400	ng	# 0.00
35) Perylene-d12	24.106	264	6766	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.586	112	6472	0.366	ng	0.00
5) Phenol-d6	7.190	99	8082	0.359	ng	-0.01
8) Nitrobenzene-d5	9.206	82	5115m	0.367	ng	-0.01
11) 2-Methylnaphthalene-d10	12.450	152	11856	0.305	ng	0.00
14) 2,4,6-Tribromophenol	16.173	330	1249	0.299	ng	-0.01
15) 2-Fluorobiphenyl	13.319	172	15626	0.395	ng	0.00
27) Fluoranthene-d10	19.464	212	13803	0.304	ng	0.00
31) Terphenyl-d14	20.058	244	9382	0.425	ng	0.00

Target Compounds Qvalue

 (#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120222\
Data File : BN023047.D
Acq On : 02 Dec 2022 14:31
Operator : CG/JU
Sample : PB149383BL
Misc :
ALS Vial : 3 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
PB149383BL

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 12/05/2022
Supervised By :Jagrut Upadhyay 12/05/2022


Quant Time: Dec 05 00:33:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 02 02:30:10 2022
Response via : Initial Calibration

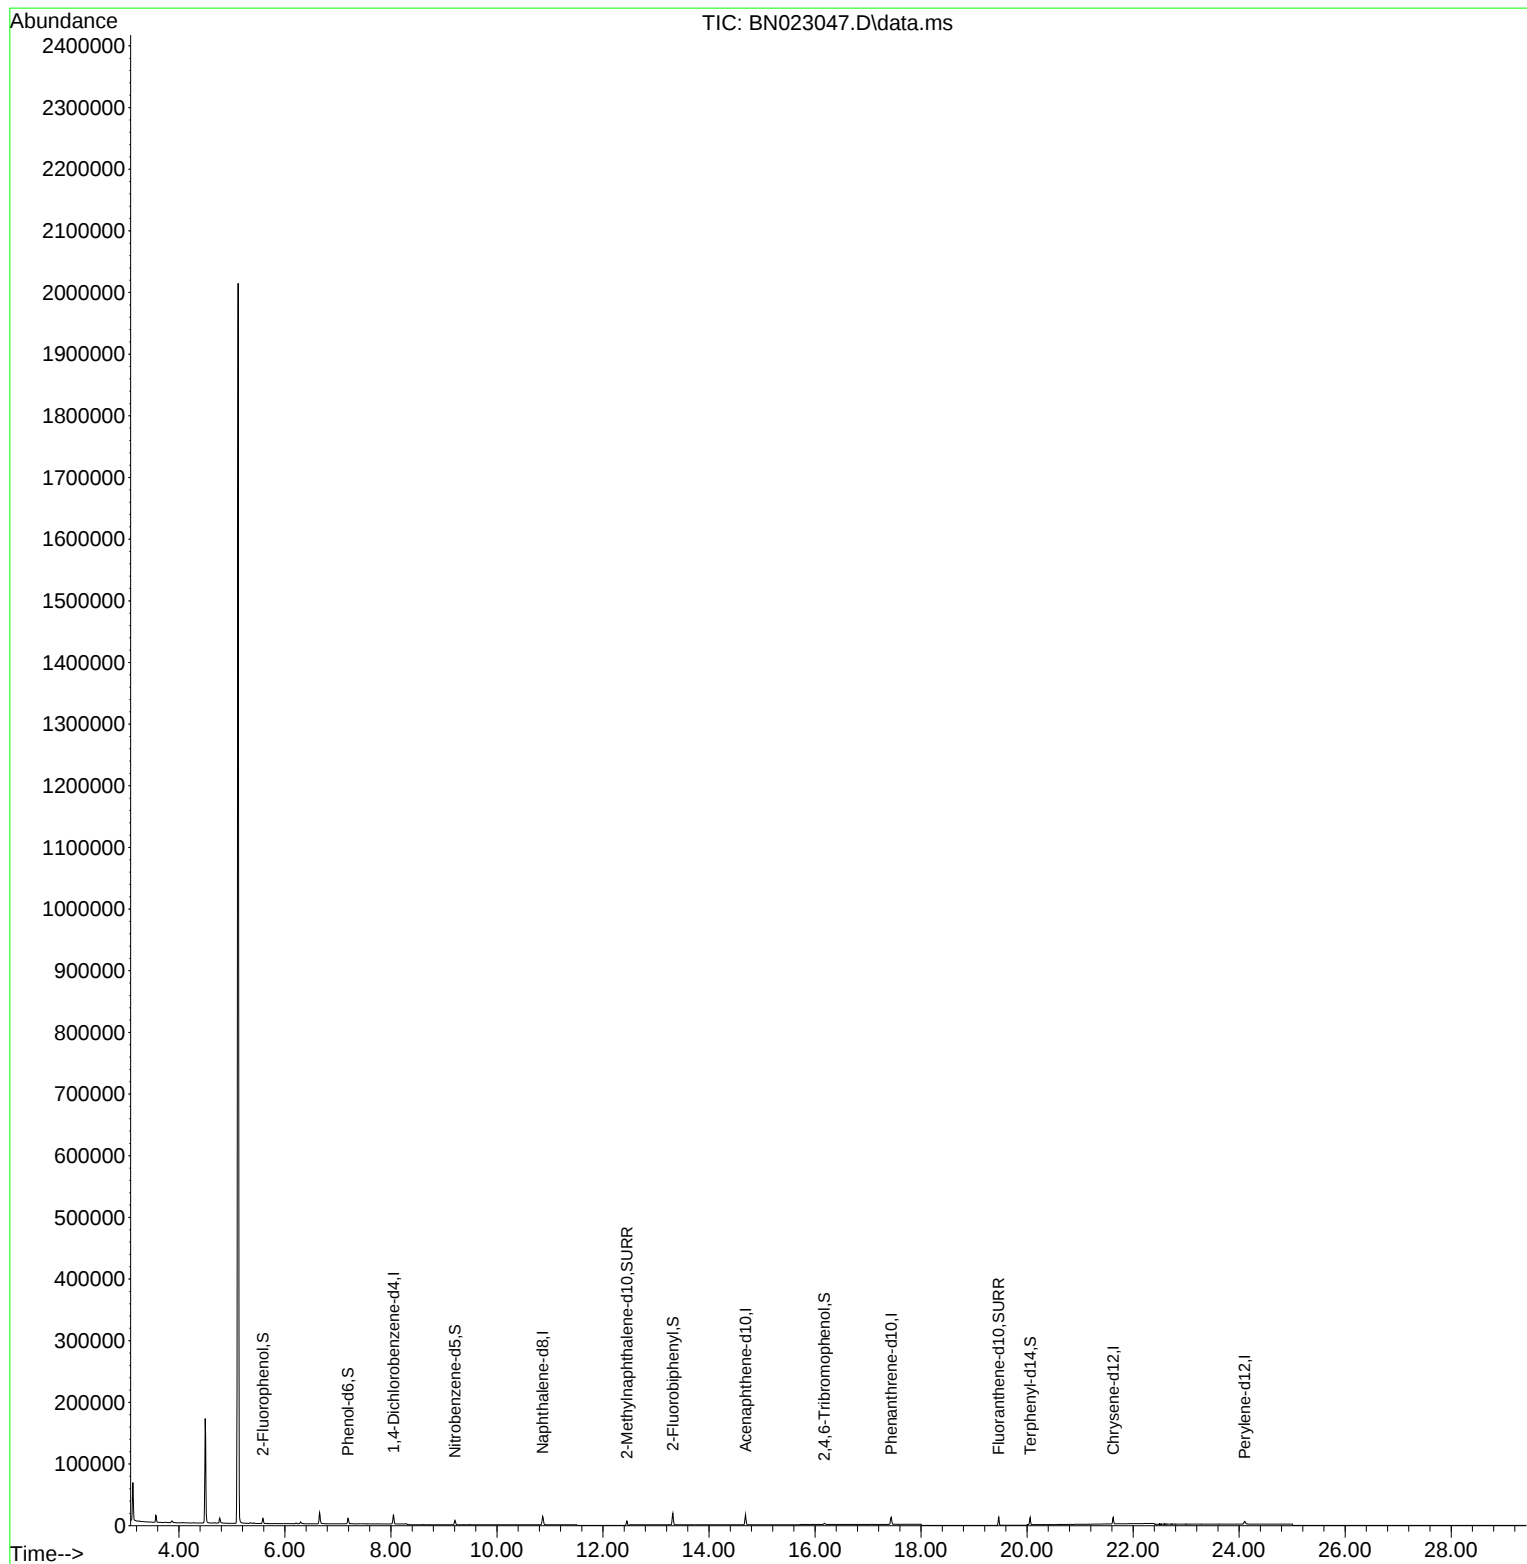

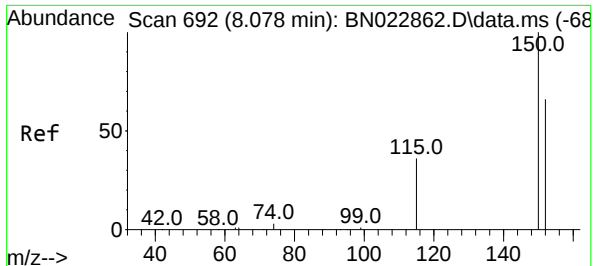

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.049 min Scan# 688
Delta R.T. -0.008 min
Lab File: BN023047.D
Acq: 02 Dec 2022 14:31




Instrument :
BNA_N
ClientSampleId :
PB149383BL

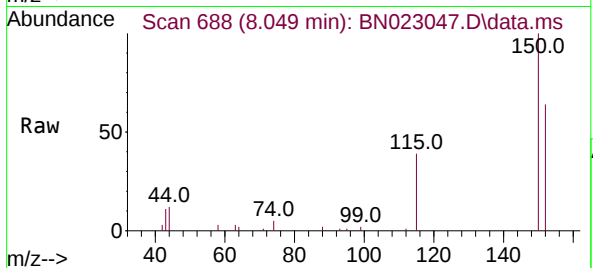


Tgt Ion:152 Resp: 6802
Ion Ratio Lower Upper
152 100
150 155.2 121.2 181.8
115 60.2 46.2 69.4

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 12/05/2022
Supervised By :Jagrut Upadhyay 12/05/2022

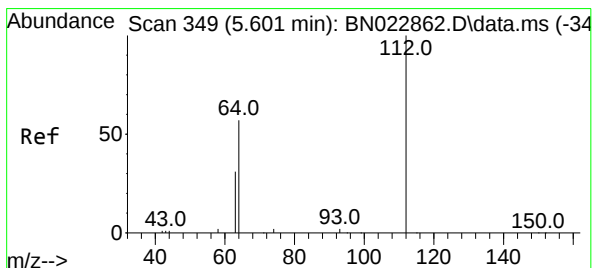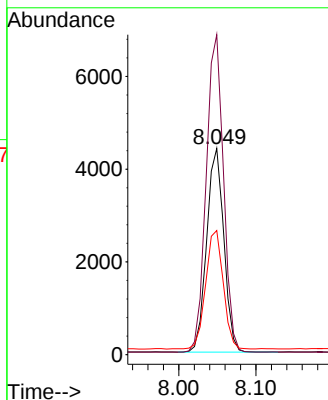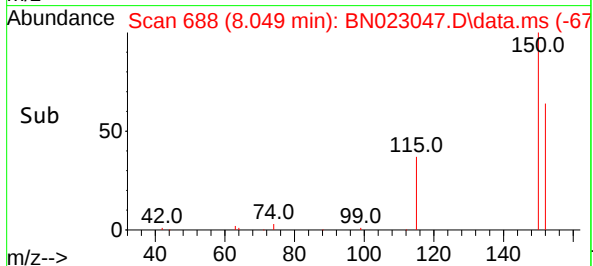


#4
2-Fluorophenol
Concen: 0.366 ng
RT: 5.586 min Scan# 347
Delta R.T. -0.007 min
Lab File: BN023047.D
Acq: 02 Dec 2022 14:31

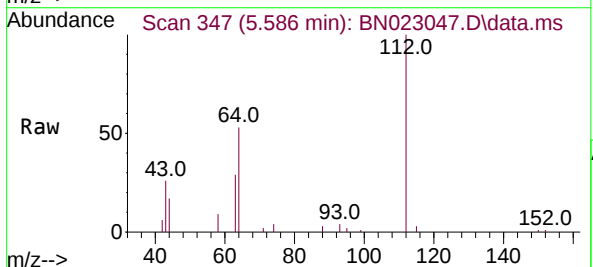

Tgt Ion:112 Resp: 6472
Ion Ratio Lower Upper
112 100
64 55.6 43.4 65.2
63 30.8 23.4 35.2

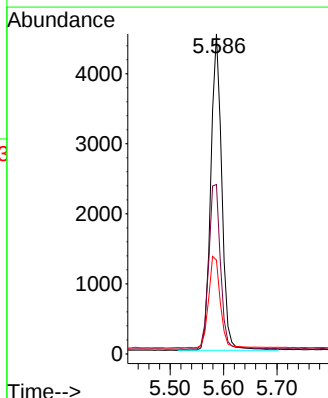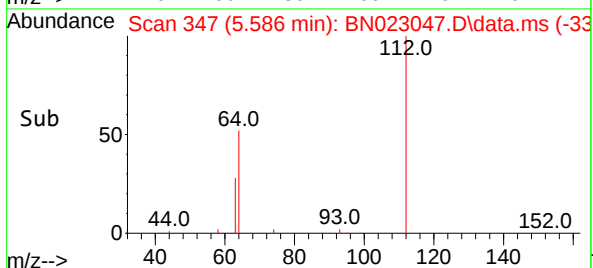

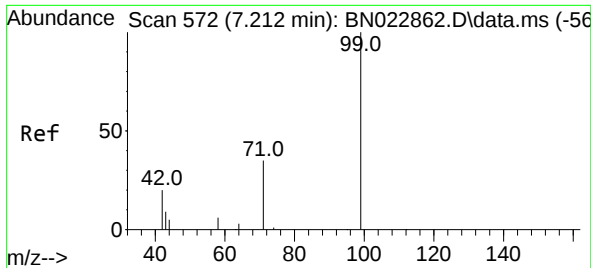





#5
Phenol-d6
Concen: 0.359 ng
RT: 7.190 min Scan# 50
Delta R.T. -0.015 min
Lab File: BN023047.D
Acq: 02 Dec 2022 14:31

Instrument :
BNA_N
ClientSampleId :
PB149383BL

Tgt Ion: 99 Resp: 8082
Ion Ratio Lower Upper
99 100
42 20.8 16.0 24.0
71 34.8 26.8 40.2




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/05/2022
Supervised By :Jagrut Upadhyay 12/05/2022

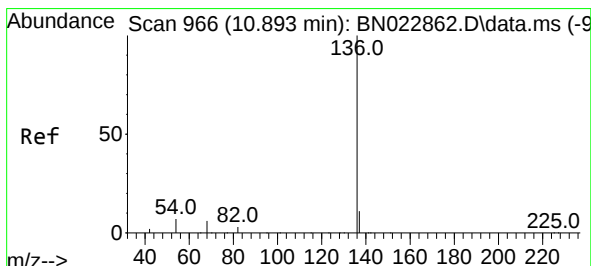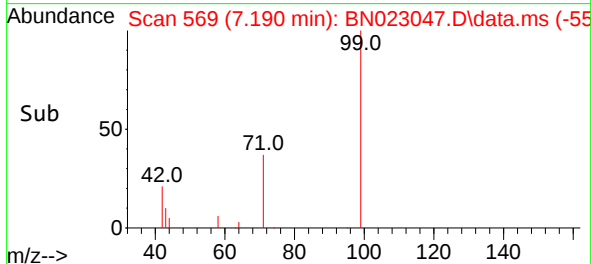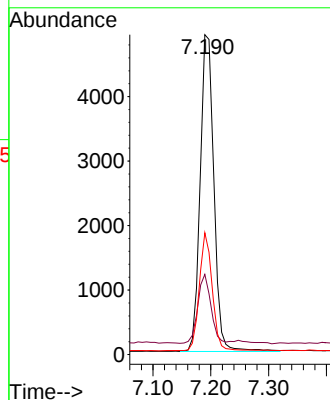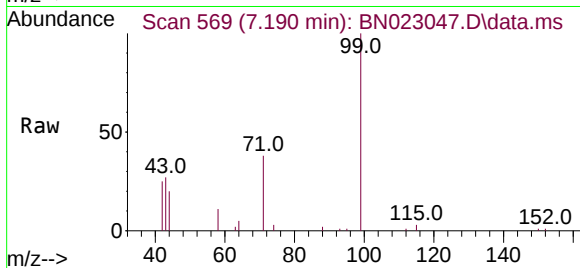

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.861 min Scan# 963
Delta R.T. -0.011 min
Lab File: BN023047.D
Acq: 02 Dec 2022 14:31


Tgt Ion:136 Resp: 17940
Ion Ratio Lower Upper
136 100
137 11.0 9.0 13.4
54 9.7 6.6 9.8
68 7.1 5.5 8.3

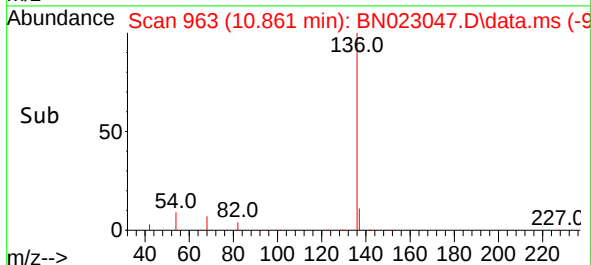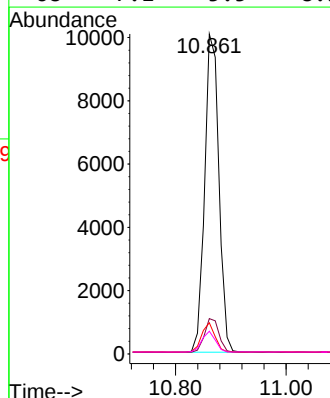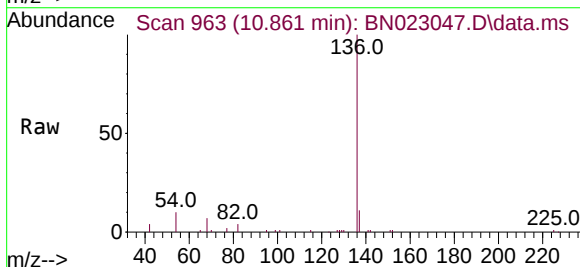

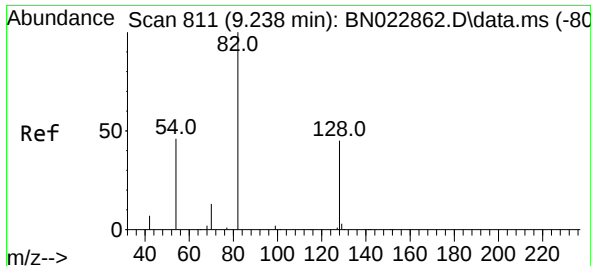

#8
Nitrobenzene-d5
Concen: 0.367 ng m
RT: 9.206 min Scan# 808
Delta R.T. -0.011 min
Lab File: BN023047.D
Acq: 02 Dec 2022 14:31




Instrument :
BNA_N
ClientSampleId :
PB149383BL

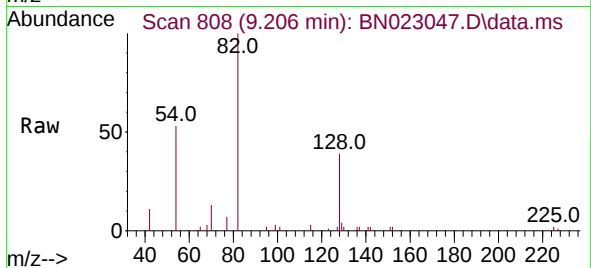

Tgt Ion: 82 Resp: 5115
Ion Ratio Lower Upper
82 100
128 38.9 36.6 54.8
54 53.0 38.5 57.7




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/05/2022
Supervised By :Jagrut Upadhyay 12/05/2022

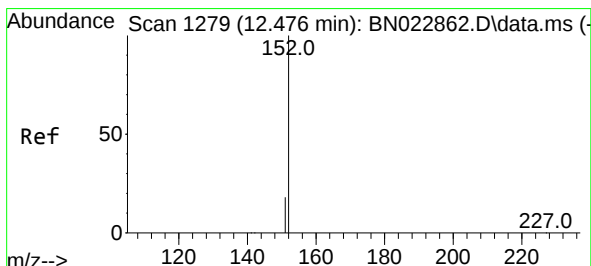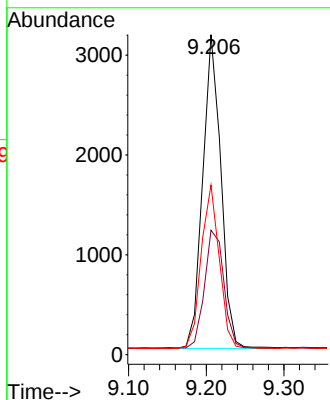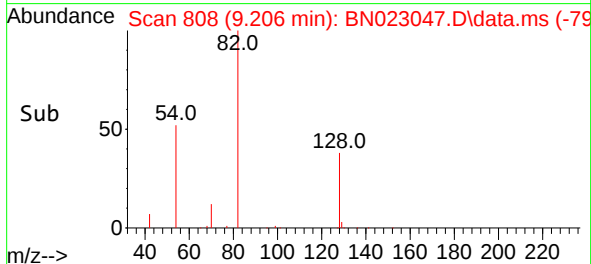

#11
2-Methylnaphthalene-d10
Concen: 0.305 ng
RT: 12.450 min Scan# 1272
Delta R.T. -0.008 min
Lab File: BN023047.D
Acq: 02 Dec 2022 14:31


Tgt Ion:152 Resp: 11856
Ion Ratio Lower Upper
152 100
151 20.7 18.6 27.8

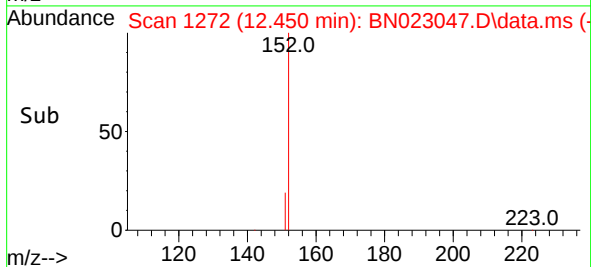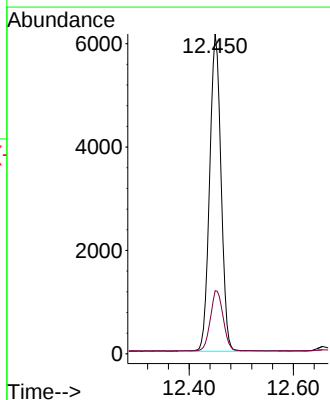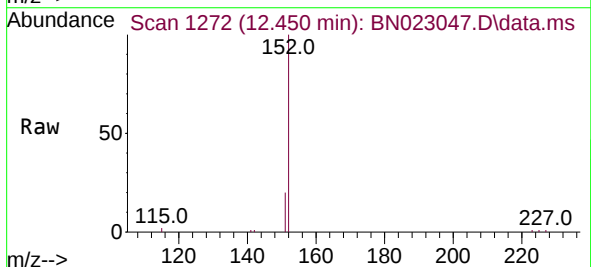

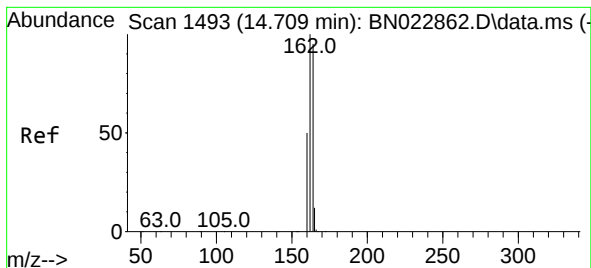

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.687 min Scan# 1493
Delta R.T. -0.000 min
Lab File: BN023047.D
Acq: 02 Dec 2022 14:31




Instrument :
BNA_N
ClientSampleId :
PB149383BL

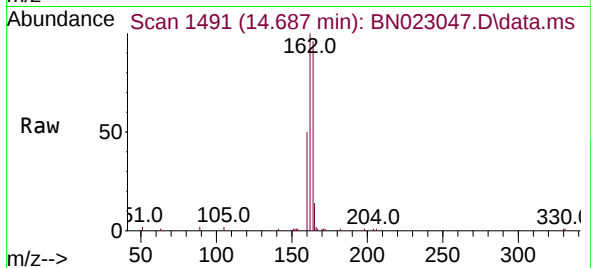


Tgt Ion:164 Resp: 864
Ion Ratio Lower Upper
164 100
162 104.5 84.2 126.4
160 52.6 42.5 63.7

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 12/05/2022
Supervised By :Jagrut Upadhyay 12/05/2022

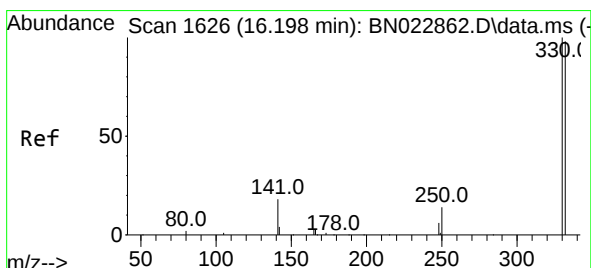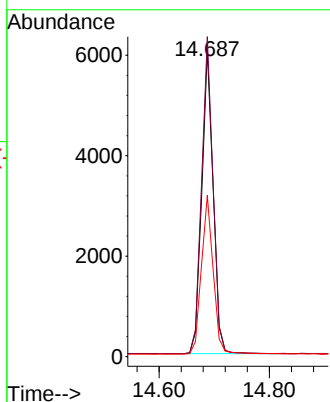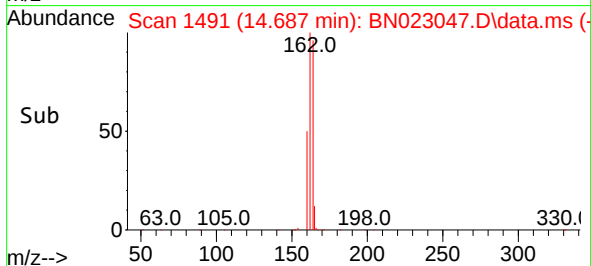


#14
2,4,6-Tribromophenol
Concen: 0.299 ng
RT: 16.173 min Scan# 1624
Delta R.T. -0.013 min
Lab File: BN023047.D
Acq: 02 Dec 2022 14:31

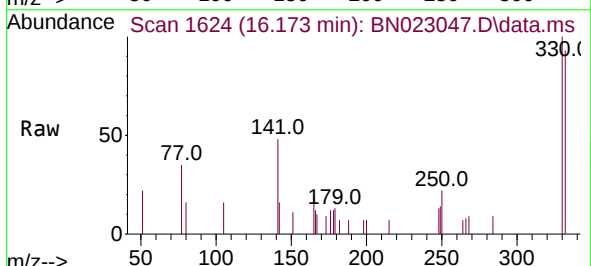

Tgt Ion:330 Resp: 1249
Ion Ratio Lower Upper
330 100
332 94.2 76.5 114.7
141 45.9 32.6 48.8

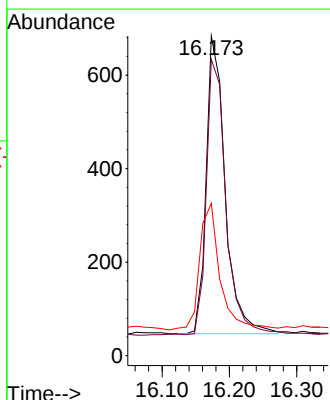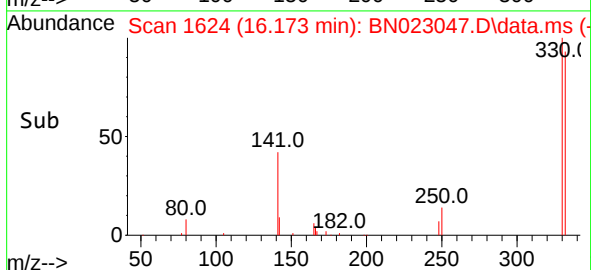

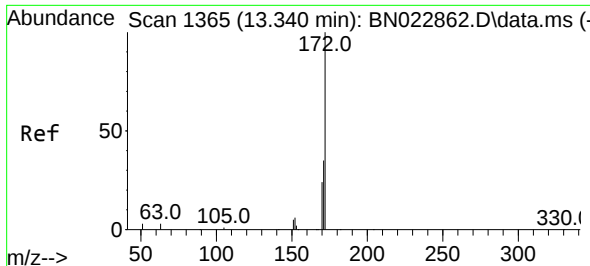


#15
2-Fluorobiphenyl
Concen: 0.395 ng
RT: 13.319 min Scan# 1363
Delta R.T. -0.000 min
Lab File: BN023047.D
Acq: 02 Dec 2022 14:31

Instrument :

BNA_N

ClientSampleId :

PB149383BL



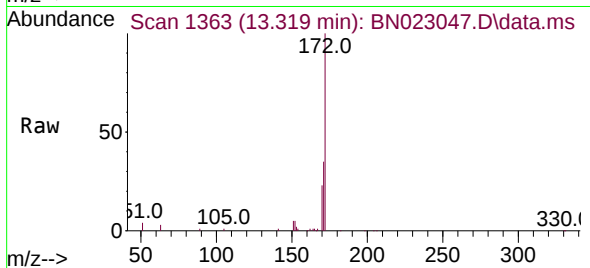


Tgt Ion:172 Resp: 15626
Ion Ratio Lower Upper
172 100
171 34.7 28.2 42.4
170 23.1 19.3 28.9


Manual Integrations

APPROVED



Reviewed By :Christian Giraldo 12/05/2022
Supervised By :Jagrut Upadhyay 12/05/2022

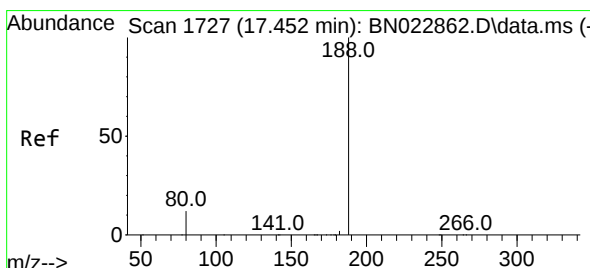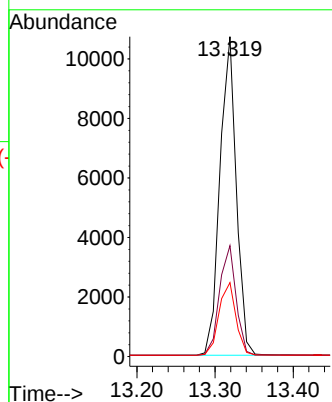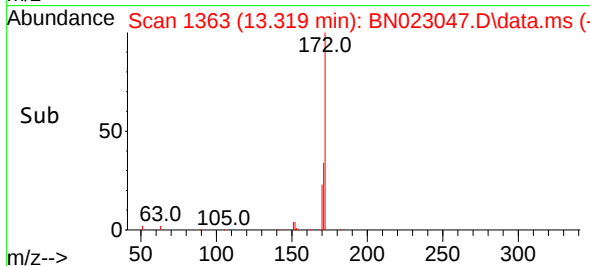


#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.439 min Scan# 1726
Delta R.T. -0.000 min
Lab File: BN023047.D
Acq: 02 Dec 2022 14:31

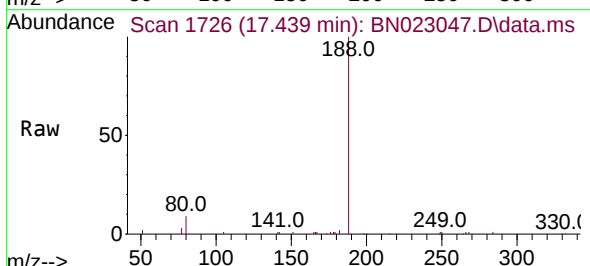


Tgt Ion:188 Resp: 16742
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.8 10.3 15.5

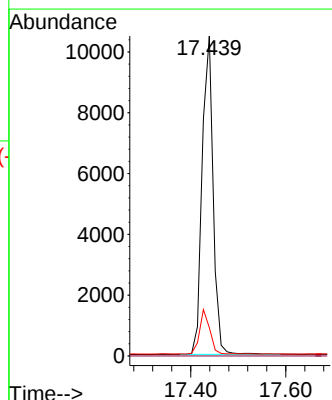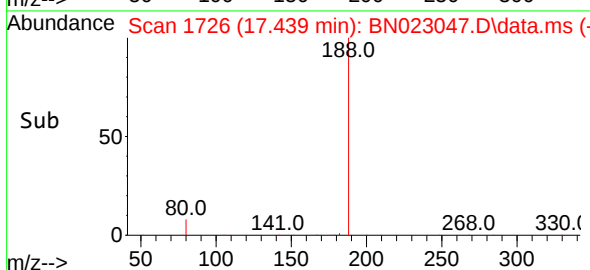

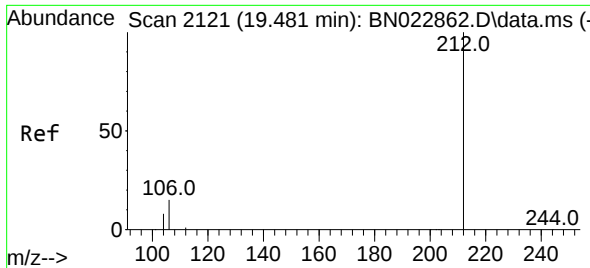

#27
Fluoranthene-d10
Concen: 0.304 ng
RT: 19.464 min Scan# 2117
Delta R.T. -0.000 min
Lab File: BN023047.D
Acq: 02 Dec 2022 14:31




Instrument :
BNA_N
ClientSampleId :
PB149383BL

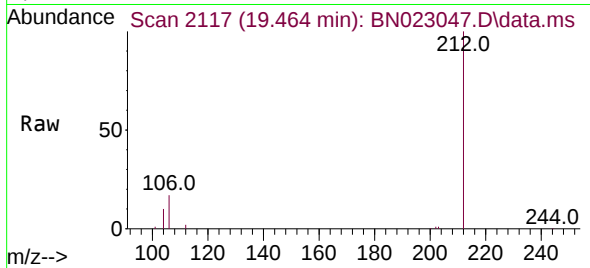


Tgt Ion:212 Resp: 13803
Ion Ratio Lower Upper
212 100
106 16.4 12.3 18.5
104 9.8 7.0 10.4

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 12/05/2022
Supervised By :Jagrut Upadhyay 12/05/2022

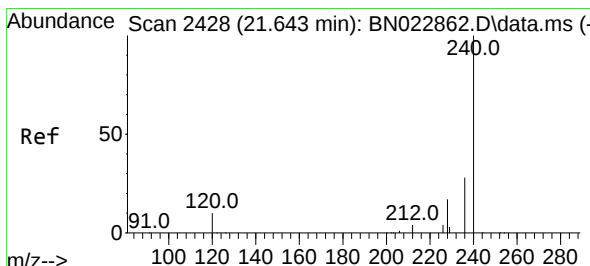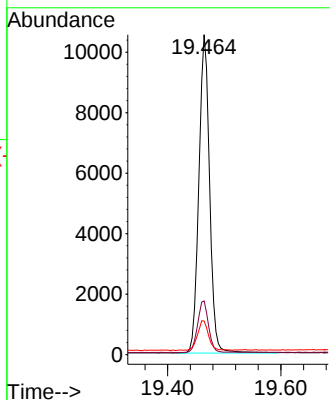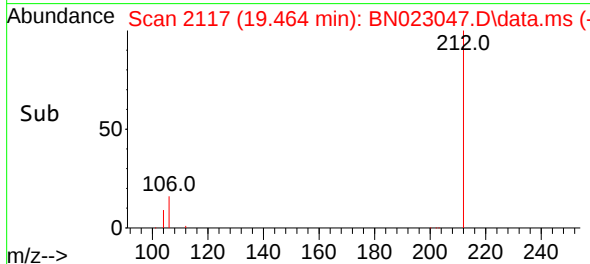


#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.625 min Scan# 2426
Delta R.T. 0.009 min
Lab File: BN023047.D
Acq: 02 Dec 2022 14:31

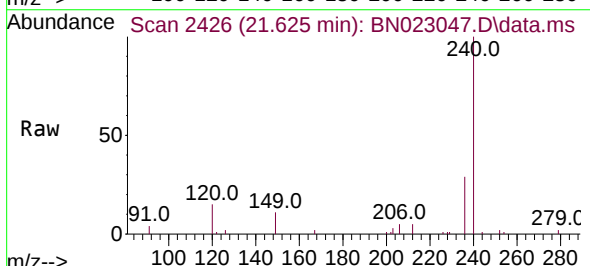

Tgt Ion:240 Resp: 9396
Ion Ratio Lower Upper
240 100
120 15.3 9.2 13.8#
236 28.7 22.6 34.0

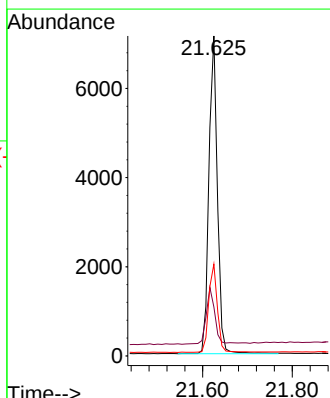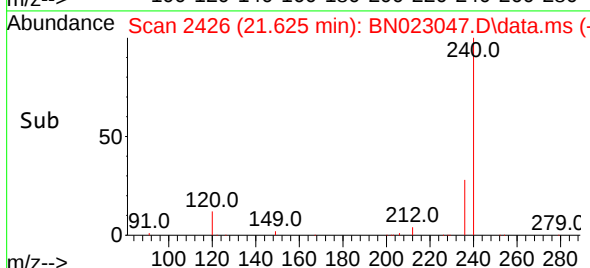

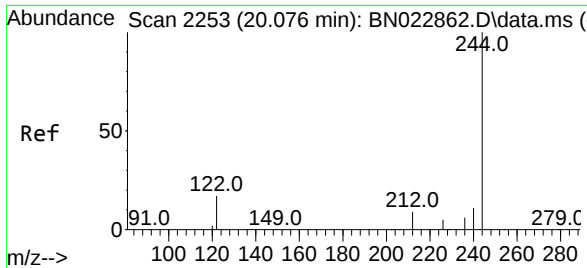


#31
 Terphenyl-d14
 Concen: 0.425 ng
 RT: 20.058 min Scan# 211
 Delta R.T. -0.000 min
 Lab File: BN023047.D
 Acq: 02 Dec 2022 14:31

Instrument :

BNA_N

ClientSampleId :

PB149383BL



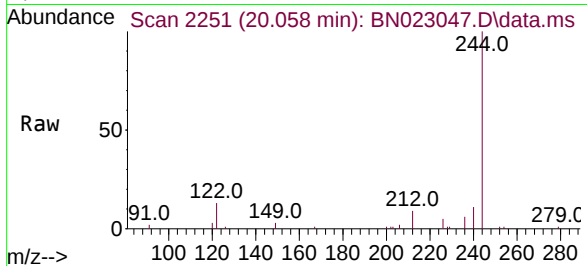


Tgt Ion:244 Resp: 9382
 Ion Ratio Lower Upper
 244 100
 212 9.2 7.9 11.9
 122 13.3 13.9 20.9


Manual Integrations

APPROVED

Reviewed By :Christian Giraldo 12/05/2022
 Supervised By :Jagrut Upadhyay 12/05/2022

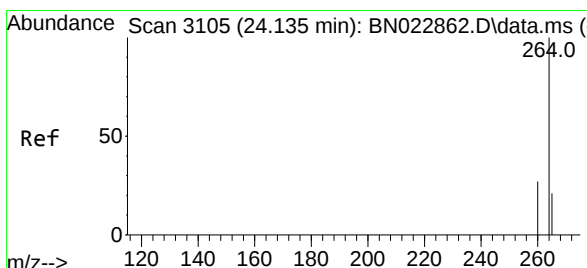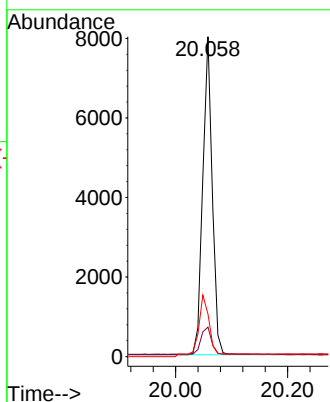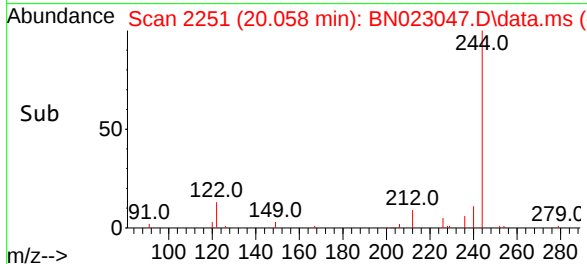

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.106 min Scan# 3095
 Delta R.T. 0.003 min
 Lab File: BN023047.D
 Acq: 02 Dec 2022 14:31

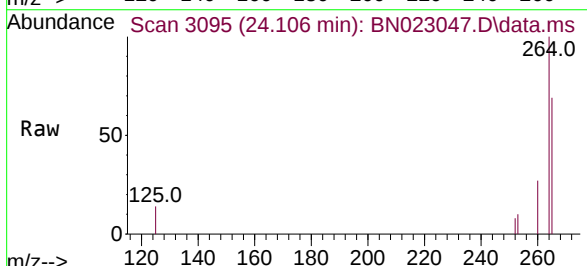

Tgt Ion:264 Resp: 6766
 Ion Ratio Lower Upper
 264 100
 260 27.3 21.7 32.5
 265 69.2 31.0 46.4

