

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120222\
 Data File : BN023053.D
 Acq On : 02 Dec 2022 18:57
 Operator : CG/JU
 Sample : N5852-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RW9-PT-OUT-03-12012022

Quant Time: Dec 05 00:35:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 02:30:10 2022
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 12/05/2022
 Supervised By :Jagrut Upadhyay 12/05/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.057	152	4570	0.400	ng	0.00
7) Naphthalene-d8	10.872	136	12494	0.400	ng	0.00
13) Acenaphthene-d10	14.688	164	6184	0.400	ng	0.00
19) Phenanthrene-d10	17.439	188	11769	0.400	ng	# 0.00
29) Chrysene-d12	21.625	240	6294	0.400	ng	# 0.00
35) Perylene-d12	24.103	264	4767	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.594	112	1252	0.105	ng	0.00
5) Phenol-d6	7.204	99	953	0.063	ng	0.00
8) Nitrobenzene-d5	9.217	82	3317m	0.342	ng	0.00
11) 2-Methylnaphthalene-d10	12.458	152	5592	0.206	ng	0.00
14) 2,4,6-Tribromophenol	16.186	330	699	0.234	ng	0.00
15) 2-Fluorobiphenyl	13.319	172	10553	0.373	ng	0.00
27) Fluoranthene-d10	19.465	212	8636	0.270	ng	0.00
31) Terphenyl-d14	20.058	244	8303	0.562	ng	0.00

Target Compounds Qvalue

 (#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120222\
Data File : BN023053.D
Acq On : 02 Dec 2022 18:57
Operator : CG/JU
Sample : N5852-03
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
RW9-PT-OUT-03-12012022

Quant Time: Dec 05 00:35:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 02 02:30:10 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/05/2022
Supervised By :Jagrut Upadhyay 12/05/2022

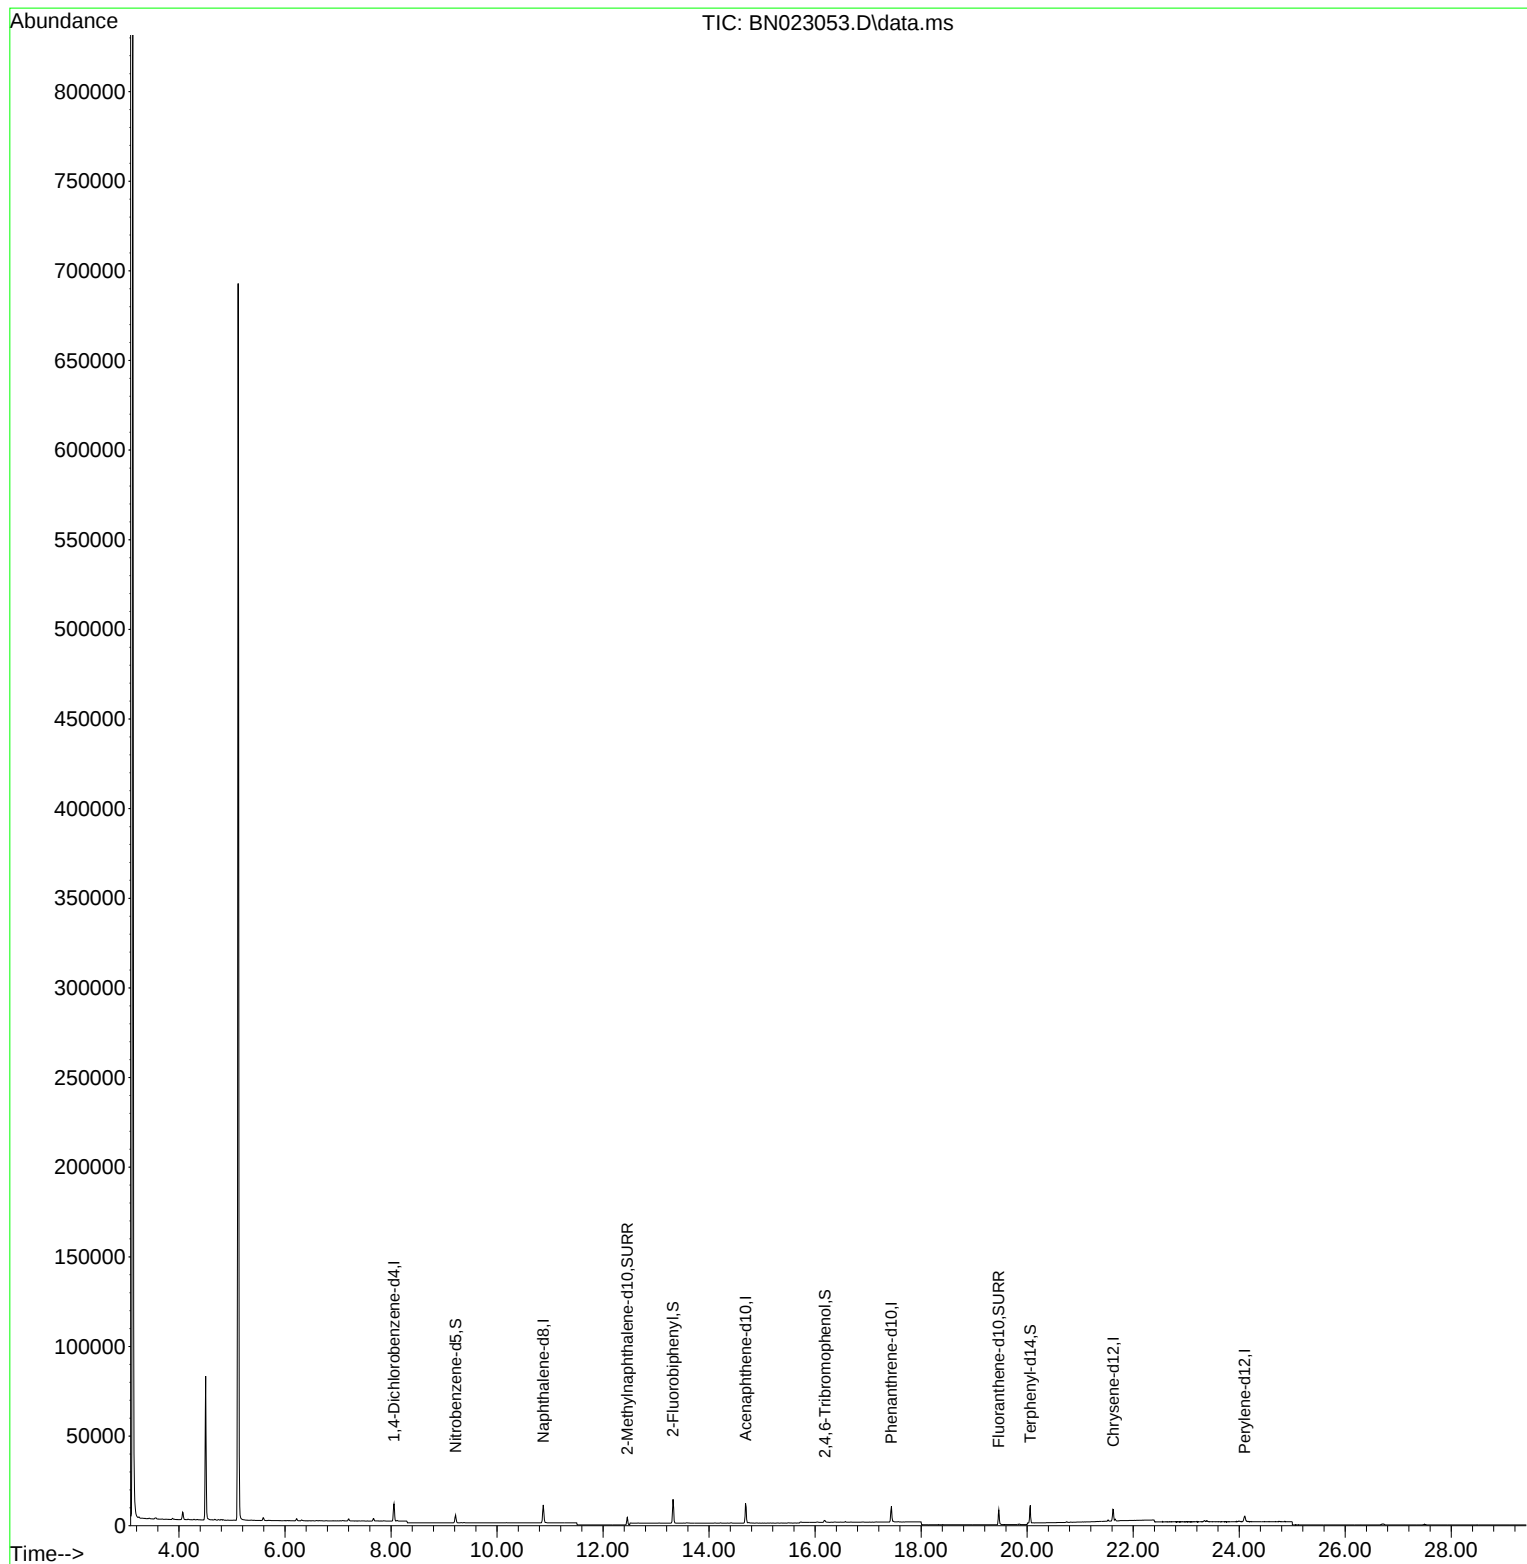

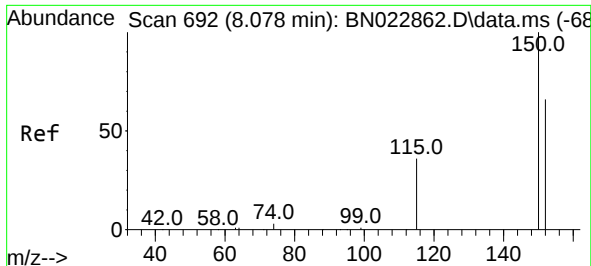

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.057 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN023053.D
Acq: 02 Dec 2022 18:57




Instrument :
BNA_N
ClientSampleId :
RW9-PT-OUT-03-12012022

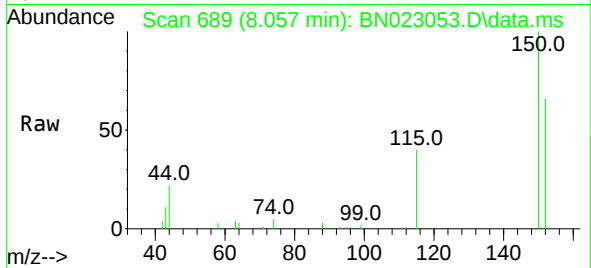

Tgt Ion:152 Resp: 4570
Ion Ratio Lower Upper
152 100
150 152.4 121.2 181.8
115 61.0 46.2 69.4




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/05/2022
Supervised By :Jagrut Upadhyay 12/05/2022

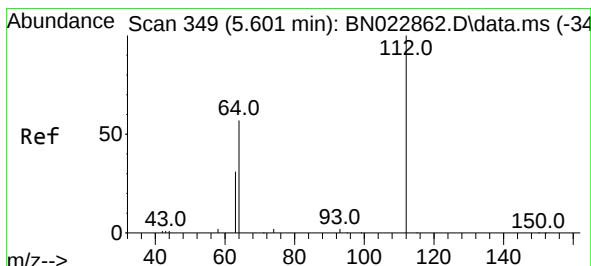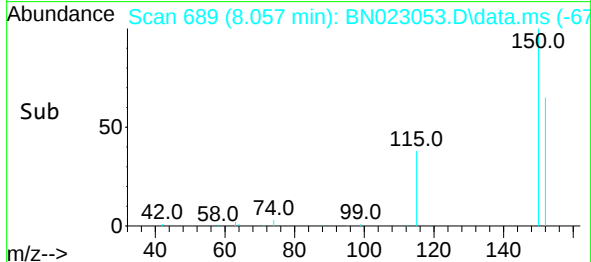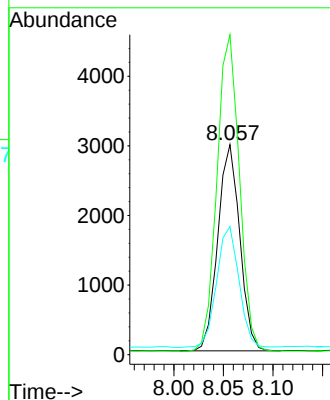

#4
2-Fluorophenol
Concen: 0.105 ng
RT: 5.594 min Scan# 348
Delta R.T. -0.000 min
Lab File: BN023053.D
Acq: 02 Dec 2022 18:57


Tgt Ion:112 Resp: 1252
Ion Ratio Lower Upper
112 100
64 57.6 43.4 65.2
63 32.9 23.4 35.2

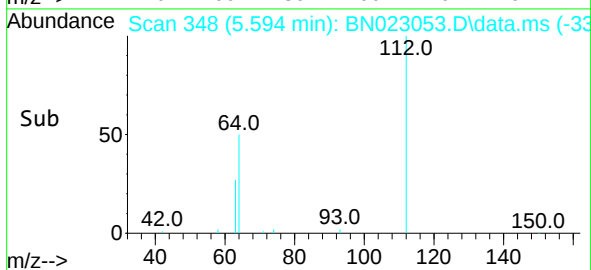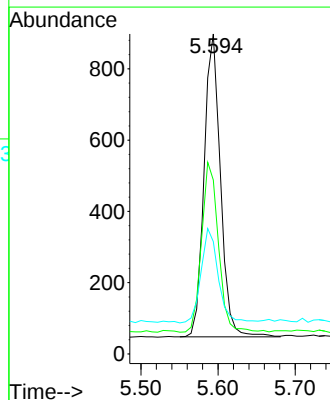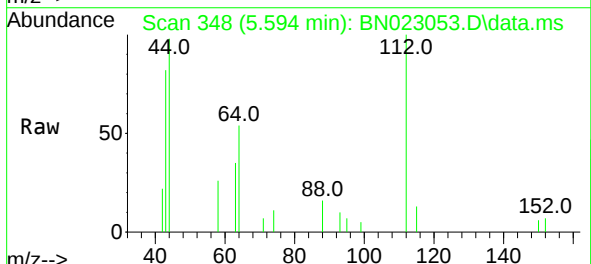

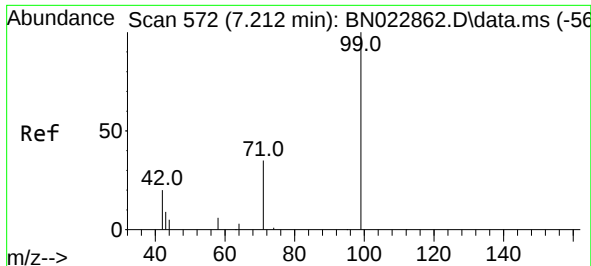

#5
Phenol-d6
Concen: 0.063 ng
RT: 7.204 min Scan# 571
Delta R.T. -0.000 min
Lab File: BN023053.D
Acq: 02 Dec 2022 18:57




Instrument :
BNA_N
ClientSampleId :
RW9-PT-OUT-03-12012022

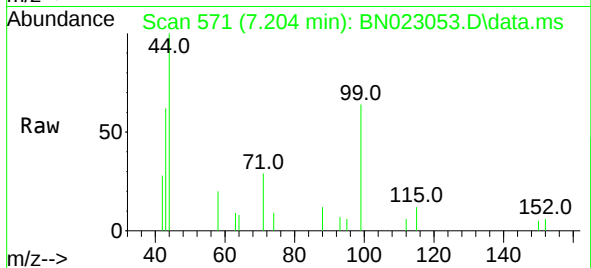

Tgt Ion: 99 Resp: 95
Ion Ratio Lower Upper
99 100
42 25.3 16.0 24.0
71 40.1 26.8 40.2




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/05/2022
Supervised By :Jagrut Upadhyay 12/05/2022

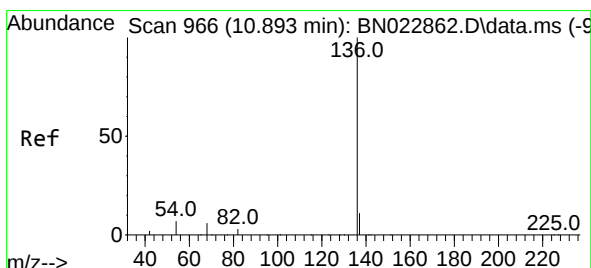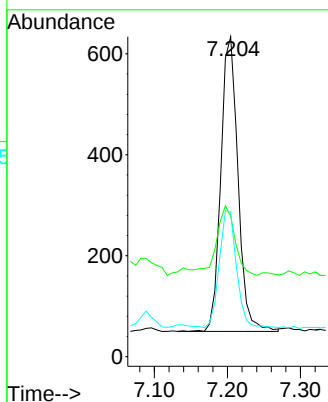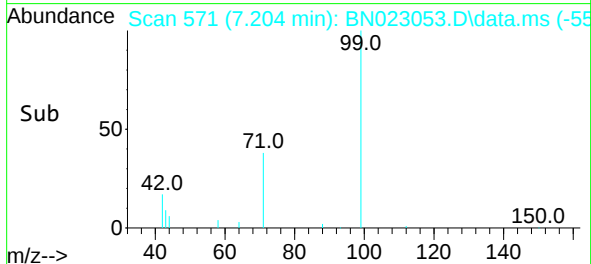

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.872 min Scan# 964
Delta R.T. -0.000 min
Lab File: BN023053.D
Acq: 02 Dec 2022 18:57


Tgt Ion:136 Resp: 12494
Ion Ratio Lower Upper
136 100
137 11.4 9.0 13.4
54 9.1 6.6 9.8
68 6.9 5.5 8.3

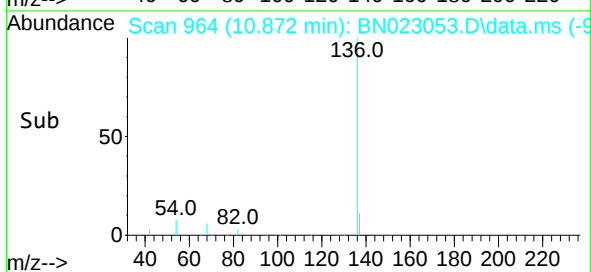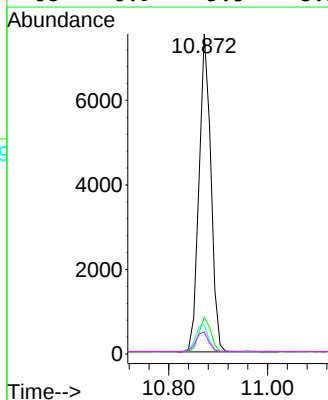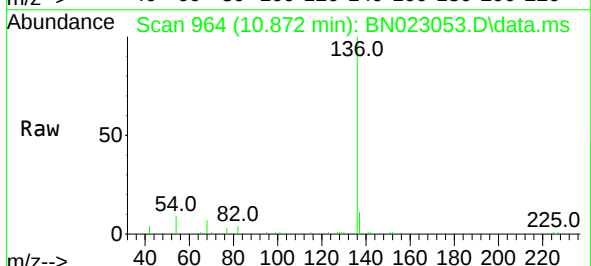

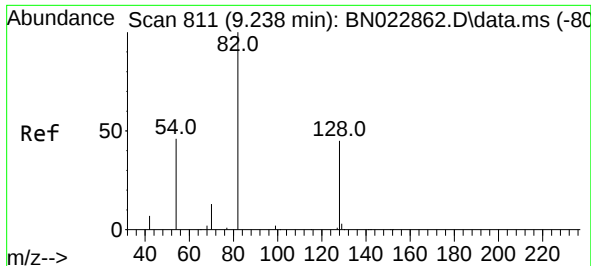

#8
Nitrobenzene-d5
Concen: 0.342 ng m
RT: 9.217 min Scan# 809
Delta R.T. -0.000 min
Lab File: BN023053.D
Acq: 02 Dec 2022 18:57




Instrument :
BNA_N
ClientSampleId :
RW9-PT-OUT-03-12012022

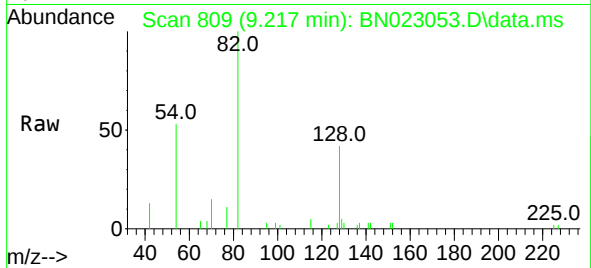

Tgt Ion: 82 Resp: 331
Ion Ratio Lower Upper
82 100
128 41.5 36.6 54.8
54 53.0 38.5 57.7




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/05/2022
Supervised By :Jagrut Upadhyay 12/05/2022

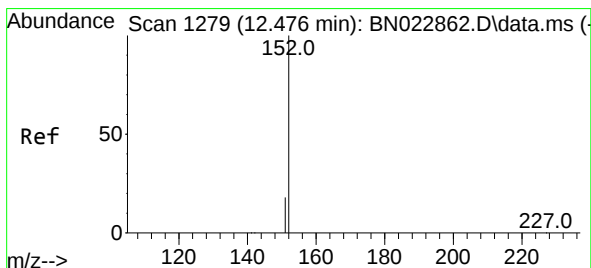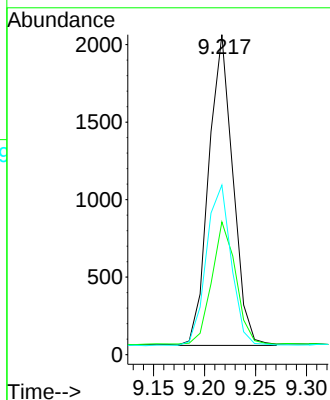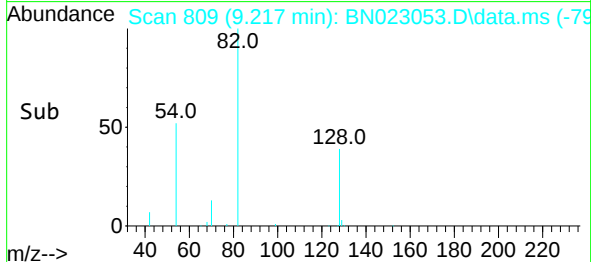

#11
2-Methylnaphthalene-d10
Concen: 0.206 ng
RT: 12.458 min Scan# 1274
Delta R.T. -0.000 min
Lab File: BN023053.D
Acq: 02 Dec 2022 18:57


Tgt Ion:152 Resp: 5592
Ion Ratio Lower Upper
152 100
151 22.9 18.6 27.8

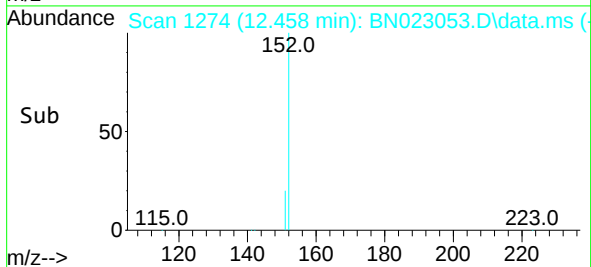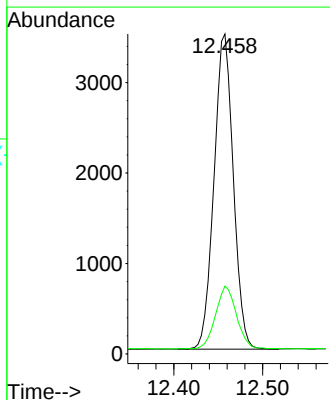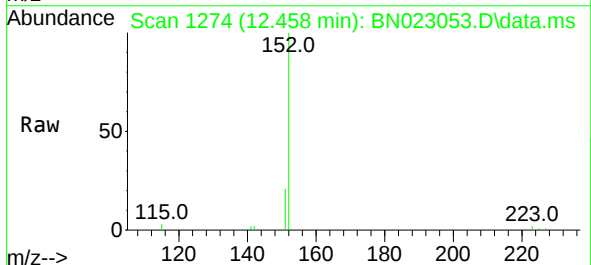

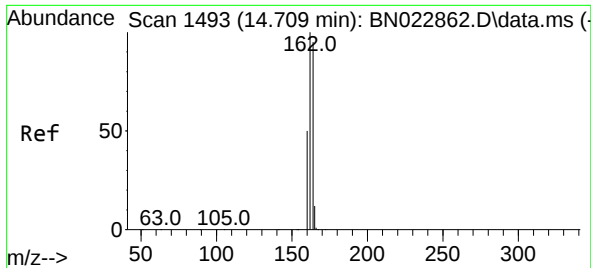

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.688 min Scan# 1491
Delta R.T. -0.000 min
Lab File: BN023053.D
Acq: 02 Dec 2022 18:57




Instrument : BNA_N
ClientSampleId : RW9-PT-OUT-03-12012022

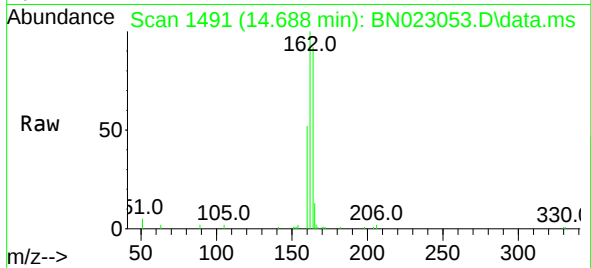


Tgt Ion:164 Resp: 6184
Ion Ratio Lower Upper
164 100
162 108.3 84.2 126.4
160 56.7 42.5 63.7

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 12/05/2022
Supervised By :Jagrut Upadhyay 12/05/2022

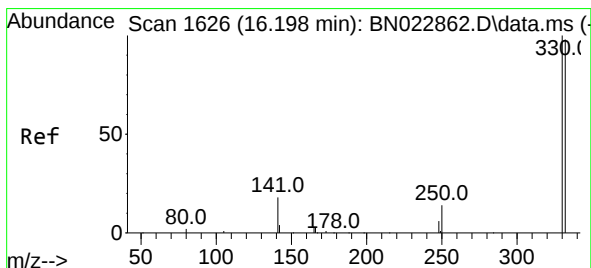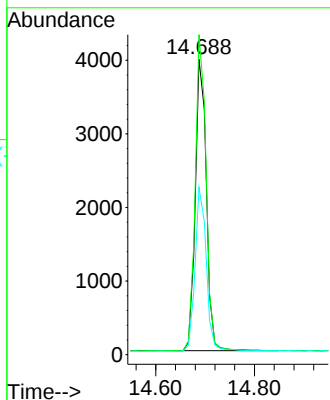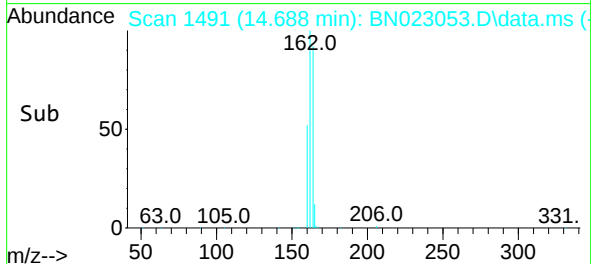


#14
2,4,6-Tribromophenol
Concen: 0.234 ng
RT: 16.186 min Scan# 1625
Delta R.T. -0.000 min
Lab File: BN023053.D
Acq: 02 Dec 2022 18:57

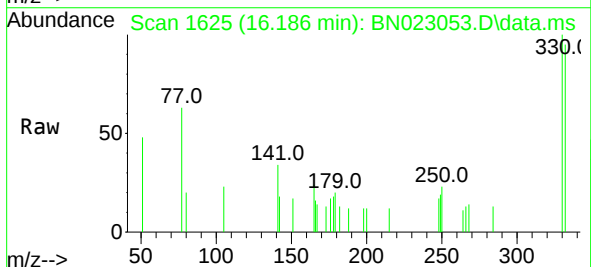


Tgt Ion:330 Resp: 699
Ion Ratio Lower Upper
330 100
332 95.9 76.5 114.7
141 43.2 32.6 48.8

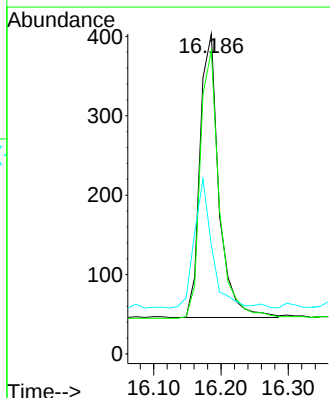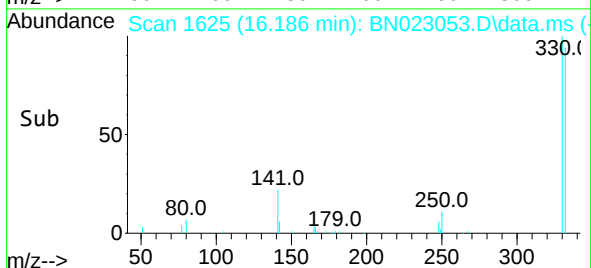

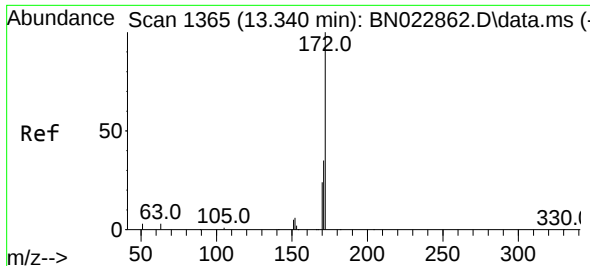

#15
2-Fluorobiphenyl
Concen: 0.373 ng
RT: 13.319 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN023053.D
Acq: 02 Dec 2022 18:57




Instrument :
BNA_N
ClientSampleId :
RW9-PT-OUT-03-12012022

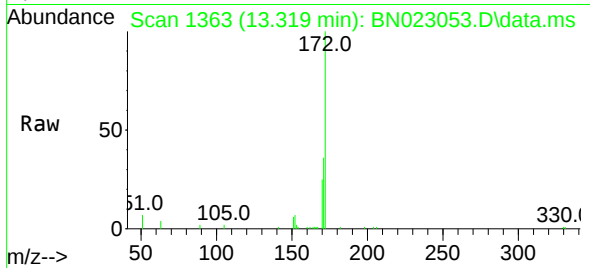


Tgt Ion:172 Resp: 1055
Ion Ratio Lower Upper
172 100
171 35.6 28.2 42.4
170 24.8 19.3 28.9

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 12/05/2022
Supervised By :Jagrut Upadhyay 12/05/2022

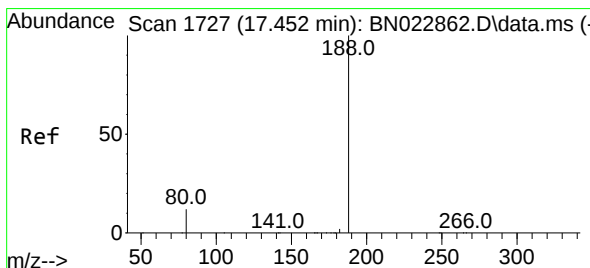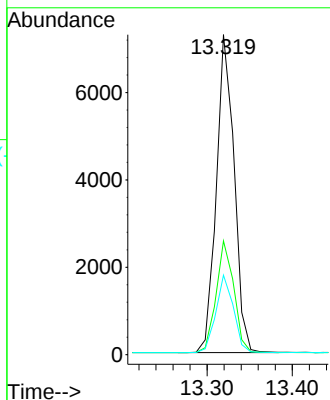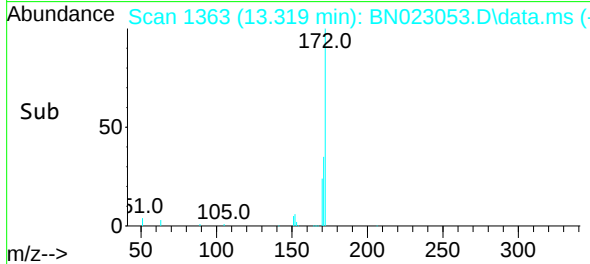


#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.439 min Scan# 1726
Delta R.T. -0.000 min
Lab File: BN023053.D
Acq: 02 Dec 2022 18:57

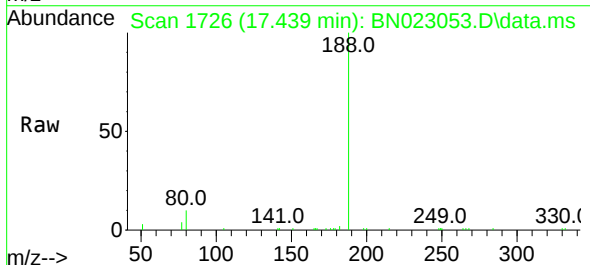


Tgt Ion:188 Resp: 11769
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.3 10.3 15.5#

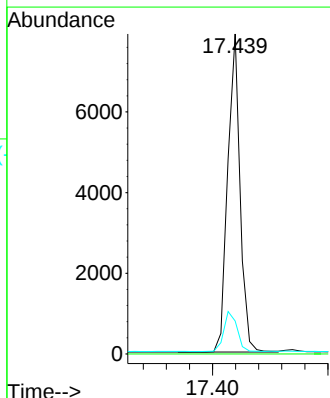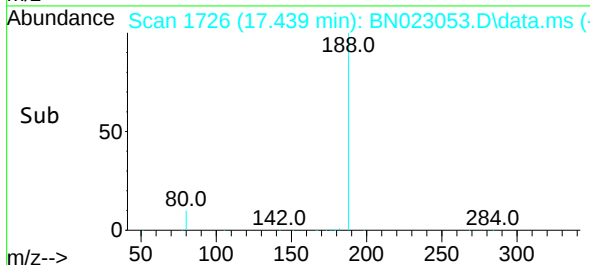

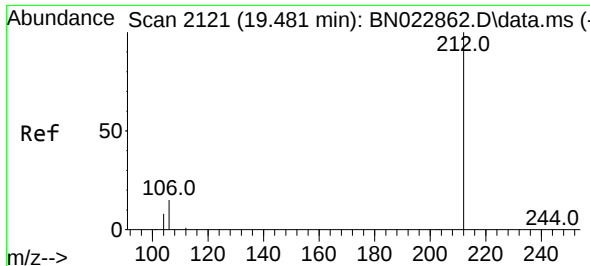

#27
Fluoranthene-d10
Concen: 0.270 ng
RT: 19.465 min Scan# 2117
Delta R.T. -0.000 min
Lab File: BN023053.D
Acq: 02 Dec 2022 18:57




Instrument :
BNA_N
ClientSampleId :
RW9-PT-OUT-03-12012022

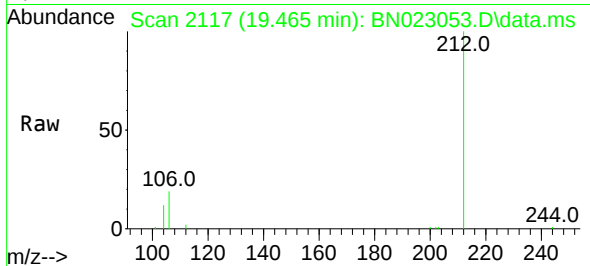

Tgt Ion:212 Resp: 8630
Ion Ratio Lower Upper
212 100
106 17.6 12.3 18.5
104 10.9 7.0 10.4




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/05/2022
Supervised By :Jagrut Upadhyay 12/05/2022

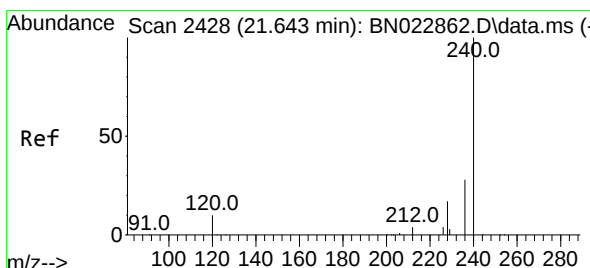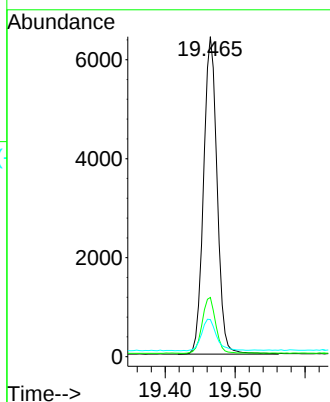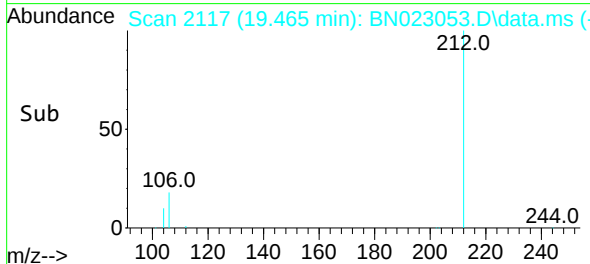

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.625 min Scan# 2426
Delta R.T. 0.009 min
Lab File: BN023053.D
Acq: 02 Dec 2022 18:57


Tgt Ion:240 Resp: 6294
Ion Ratio Lower Upper
240 100
120 15.6 9.2 13.8#
236 29.7 22.6 34.0

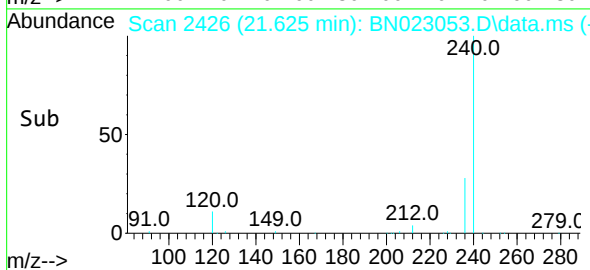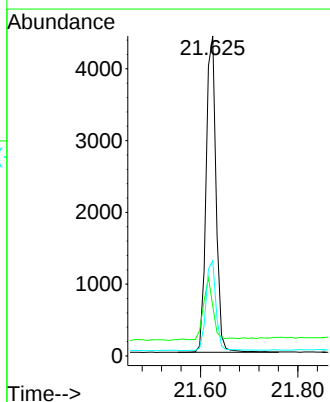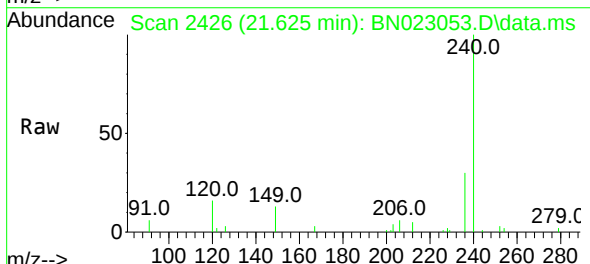

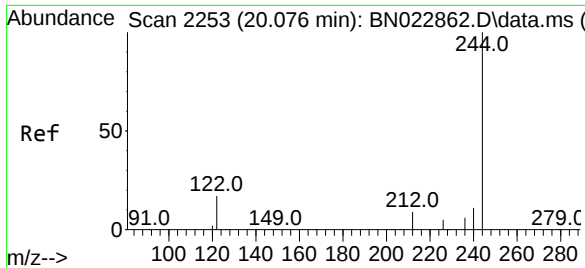

#31
 Terphenyl-d14
 Concen: 0.562 ng
 RT: 20.058 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN023053.D
 Acq: 02 Dec 2022 18:57




Instrument :
 BNA_N
 ClientSampleId :
 RW9-PT-OUT-03-12012022

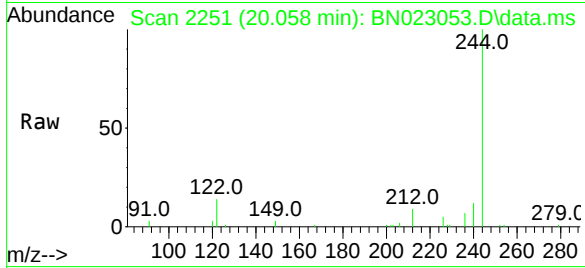

Tgt Ion:244 Resp: 830
 Ion Ratio Lower Upper
 244 100
 212 9.0 7.9 11.9
 122 13.6 13.9 20.9

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 12/05/2022
 Supervised By :Jagrut Upadhyay 12/05/2022

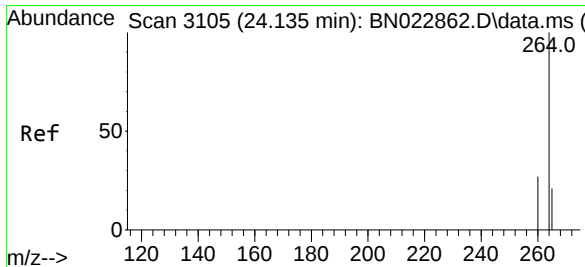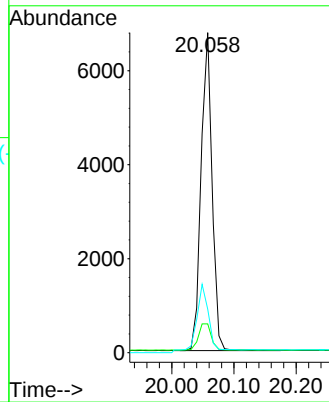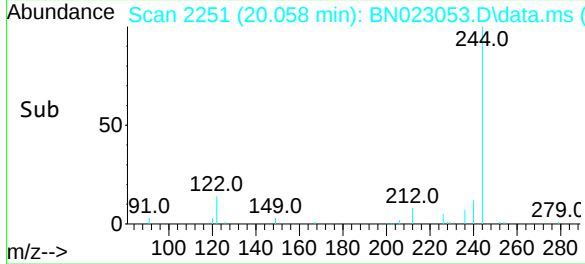

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.103 min Scan# 3094
 Delta R.T. -0.000 min
 Lab File: BN023053.D
 Acq: 02 Dec 2022 18:57

Tgt Ion:264 Resp: 4767
 Ion Ratio Lower Upper
 264 100
 260 29.0 21.7 32.5
 265 81.7 31.0 46.4

