
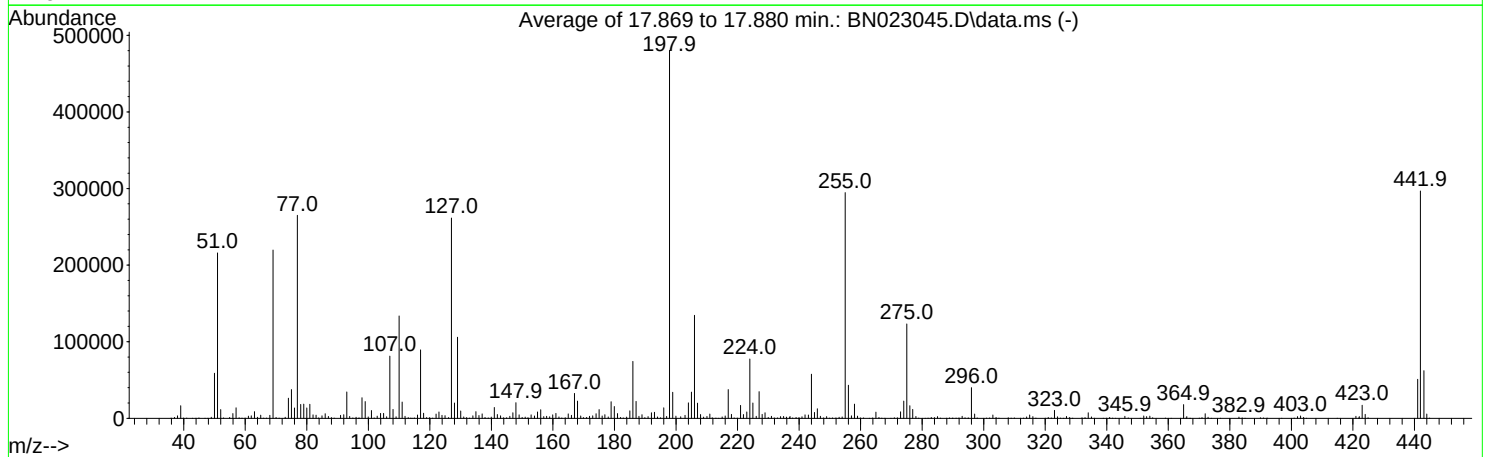


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120222\
 Data File : BN023045.D
 Acq On : 02 Dec 2022 12:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 02 02:30:10 2022

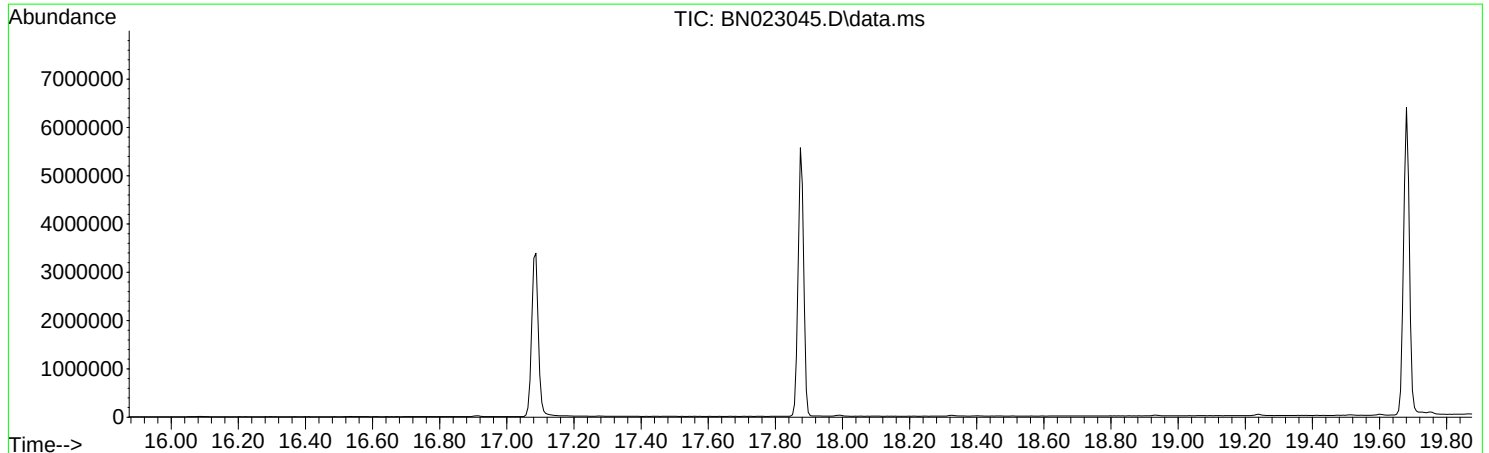




AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	215829	PASS
68	69	0.00	2	1.8	3913	PASS
69	198	0.00	100	45.7	219648	PASS
70	69	0.00	2	0.5	1091	PASS
127	198	10	80	54.4	261461	PASS
197	198	0.00	2	0.5	2480	PASS
198	198	100	100	100.0	480320	PASS
199	198	5	9	7.1	33893	PASS
275	198	10	60	25.6	123096	PASS
365	198	1	100	3.7	17850	PASS
441	198	0.01	100	10.6	50963	PASS
442	442	50	100	100.0	296725	PASS
443	442	15	24	20.9	62064	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120222\
 Data File : BN023045.D
 Acq On : 02 Dec 2022 12:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 05 01:34:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 05 01:34:14 2022
 Response via : Initial Calibration

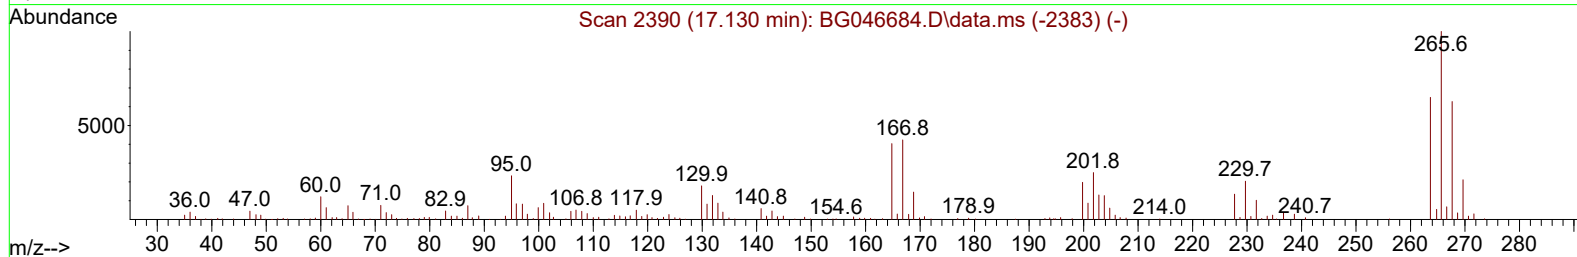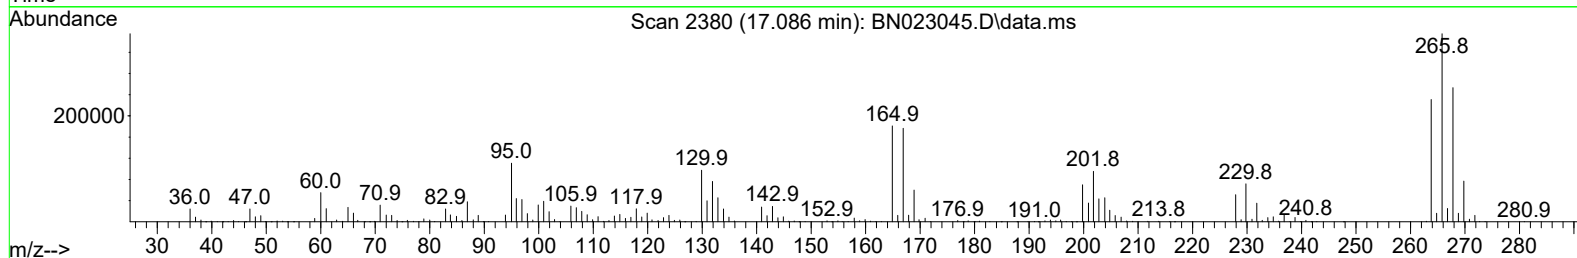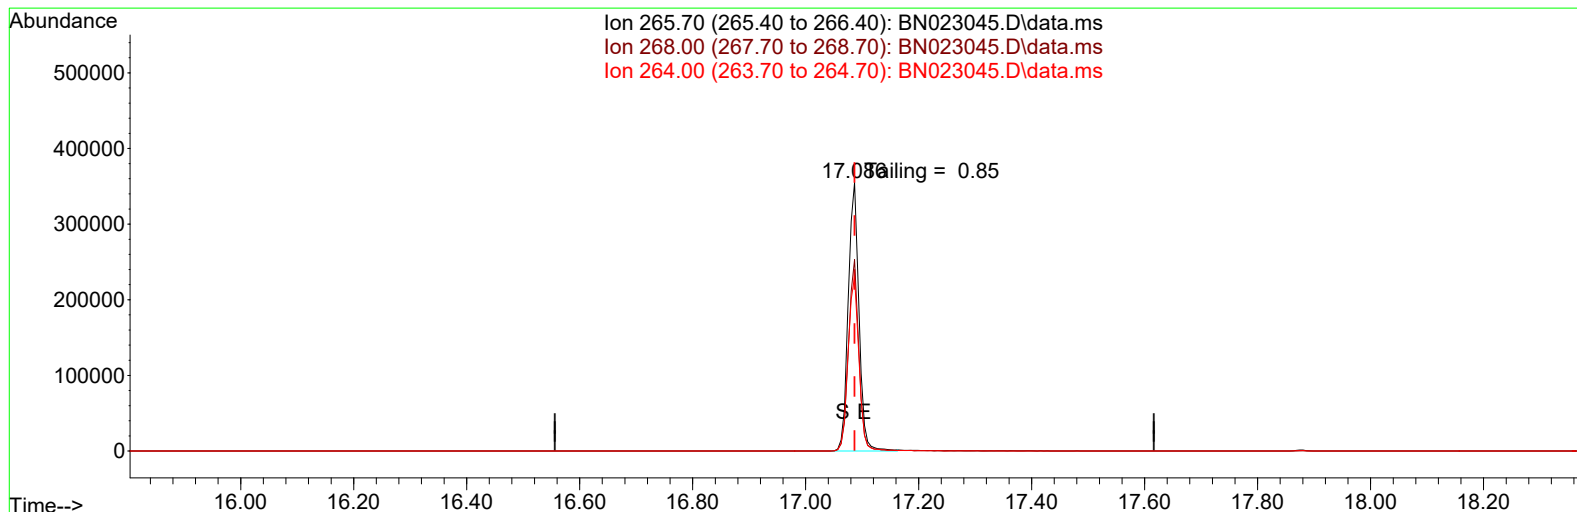

TIC: BN023045.D\data.ms

(70) Pentachlorophenol (C)

17.086min (0.000) 16272.58 ng




response 470586

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	71.33
264.00	61.60	65.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120222\
Data File : BN023045.D
Acq On : 02 Dec 2022 12:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 05 01:34:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 05 01:34:14 2022
Response via : Initial Calibration

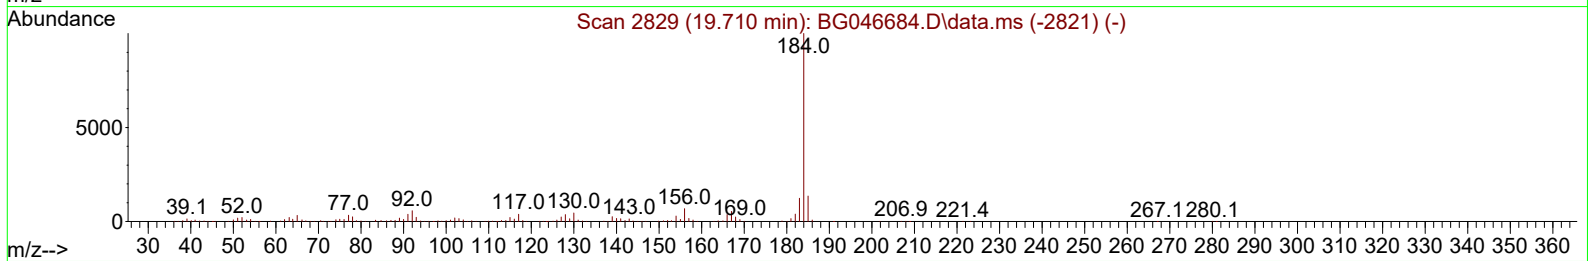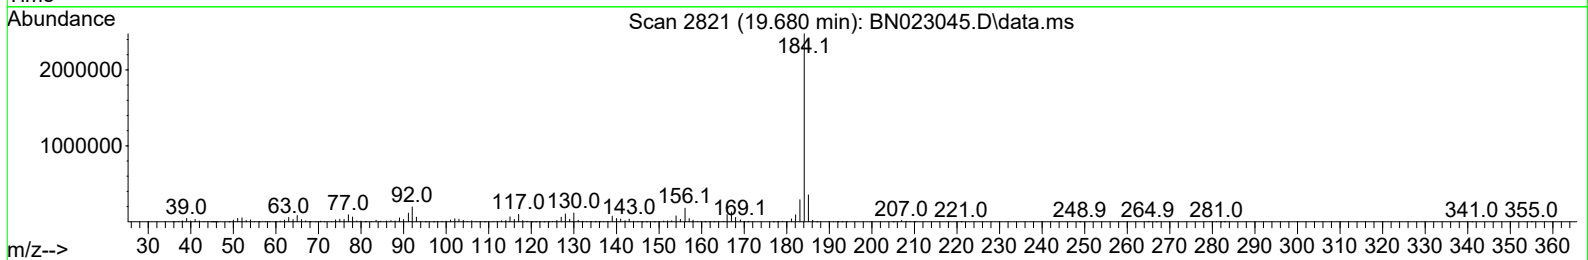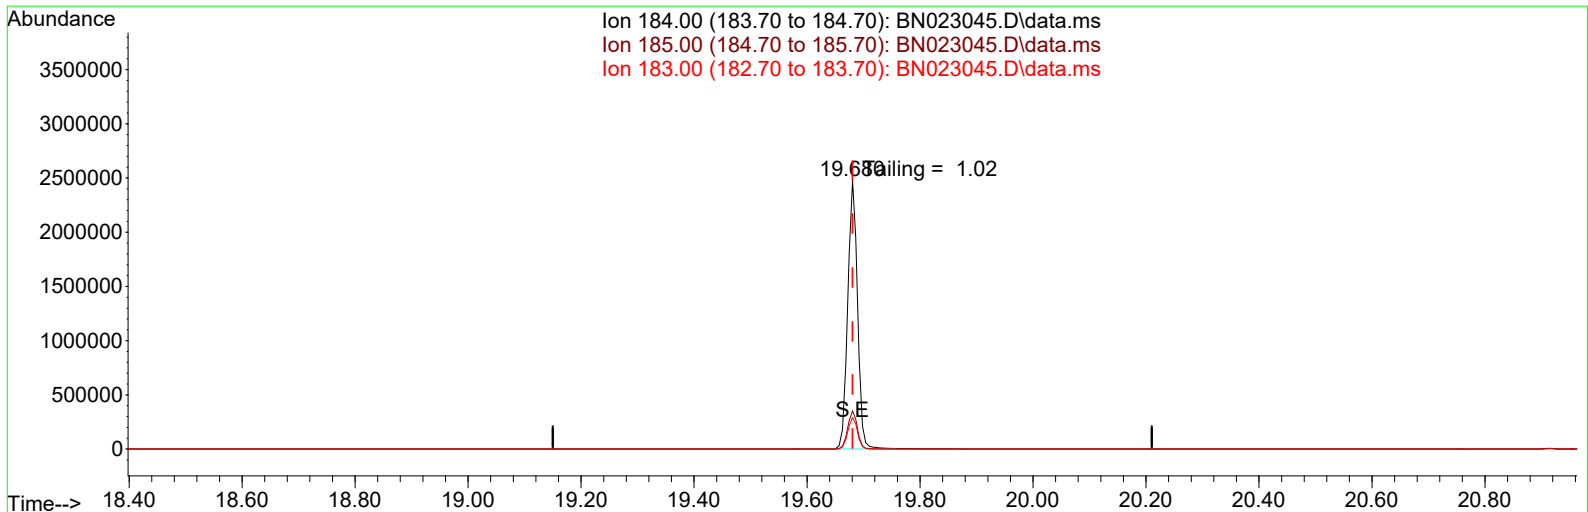

TIC: BN023045.D\data.ms

(77) Benzidine

19.680min (0.000) 294089.64 ng

response 2982524

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.28
183.00	13.20	11.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/2/2022	BNA_N	<u>BN023045.D</u>
Compound Name	Response	Retention Time
DDT	1547267	20.916
DDD	20969	20.469
DDE	1303	19.963
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22272	1569539	1.42

Instrument :
BNA_N
ClientSampleId :
DFTPP