

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120224\
 Data File : BN035391.D
 Acq On : 02 Dec 2024 19:35
 Operator : RC/JU
 Sample : PB165114BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK114

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035391.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.964	9	13	24	rVB	18453	24482	0.90%	0.098%
2	3.340	73	77	95	rBV	215563	334087	12.23%	1.337%
3	3.646	124	129	134	rVB2	2822	4353	0.16%	0.017%
4	6.505	608	615	626	rBV	312997	468183	17.14%	1.873%
5	6.663	636	642	650	rBV	249201	377977	13.84%	1.512%
6	6.840	666	672	683	rVB	320370	498149	18.24%	1.993%
7	7.299	744	750	759	rBV	302710	461613	16.90%	1.847%
8	8.016	865	872	884	rBV	427300	636528	23.31%	2.547%
9	8.440	937	944	952	rBV	307994	468754	17.16%	1.875%
10	9.152	1058	1065	1074	rBV	272878	419107	15.34%	1.677%
11	9.681	1149	1155	1169	rBV	420549	702303	25.71%	2.810%
12	10.052	1209	1218	1226	rBV	427044	691566	25.32%	2.767%
13	10.199	1236	1243	1252	rBV	420259	690597	25.28%	2.763%
14	11.651	1483	1490	1496	rBV2	6062	11876	0.43%	0.048%
15	13.393	1779	1786	1798	rBV	864058	1212280	44.38%	4.850%
16	13.645	1822	1829	1839	rBV	972462	1406996	51.51%	5.629%
17	13.963	1876	1883	1892	rVB	762506	1100396	40.29%	4.403%
18	14.193	1916	1922	1943	rBV	337904	546567	20.01%	2.187%
19	14.969	2048	2054	2065	rBV	1290857	1790350	65.55%	7.163%
20	15.104	2071	2077	2090	rBV	368527	484098	17.72%	1.937%
21	15.210	2092	2095	2102	rVB	4975	6518	0.24%	0.026%
22	16.728	2347	2353	2362	rVB	1081003	1432432	52.45%	5.731%
23	16.828	2363	2370	2381	rVV	1475322	2023180	74.07%	8.095%
24	17.969	2560	2564	2565	rBV2	3732	3908	0.14%	0.016%
25	18.128	2586	2591	2594	rBV7	2150	3465	0.13%	0.014%
26	18.704	2685	2689	2693	rBV2	16779	22763	0.83%	0.091%
27	18.781	2698	2702	2707	rVB	16351	22602	0.83%	0.090%
28	19.151	2758	2765	2771	rBV	1844966	2513415	92.02%	10.056%
29	20.980	3070	3076	3084	rBV	1347444	1793393	65.66%	7.175%
30	22.304	3298	3301	3308	rVB6	22922	34272	1.25%	0.137%
31	22.963	3410	3413	3419	rVB3	27186	43222	1.58%	0.173%
32	23.474	3491	3500	3512	rBV	1276911	2731286	100.00%	10.928%
33	23.651	3522	3530	3540	rBV	858642	1873649	68.60%	7.496%
34	23.733	3540	3544	3554	rVB3	40674	87885	3.22%	0.352%
35	24.639	3695	3698	3709	rVB6	33978	71448	2.62%	0.286%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120224\
Data File : BN035391.D
Acq On : 02 Dec 2024 19:35
Operator : RC/JU
Sample : PB165114BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK114

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 24993700

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120224\
Data File : BN035391.D
Acq On : 02 Dec 2024 19:35
Operator : RC/JU
Sample : PB165114BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK114

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

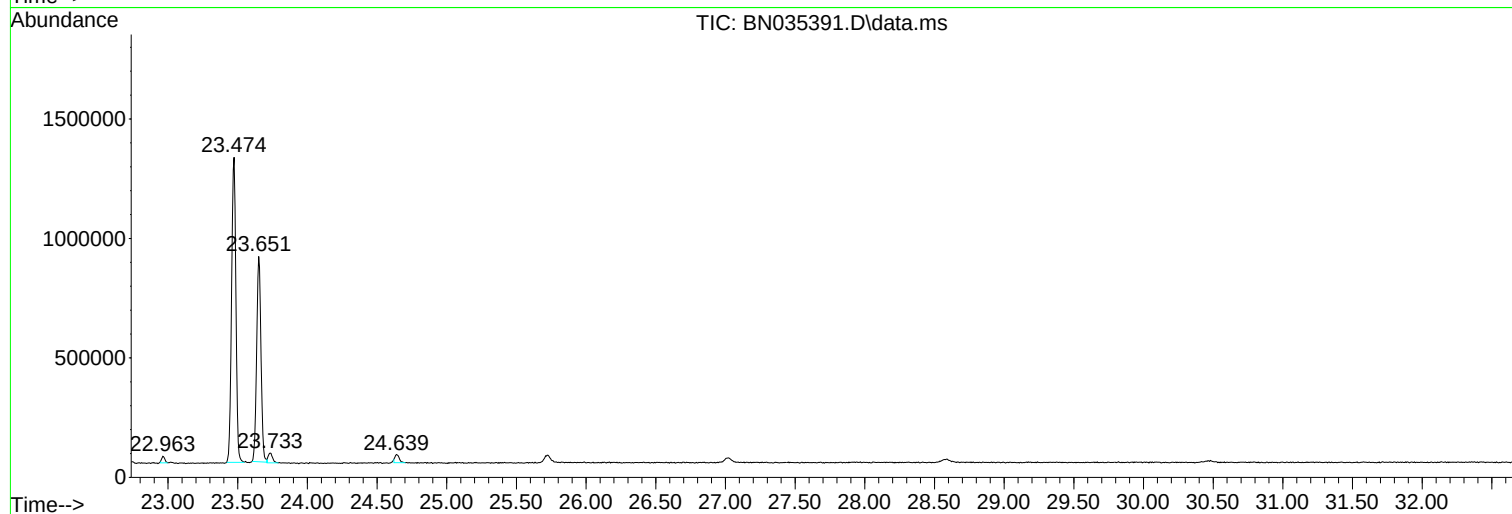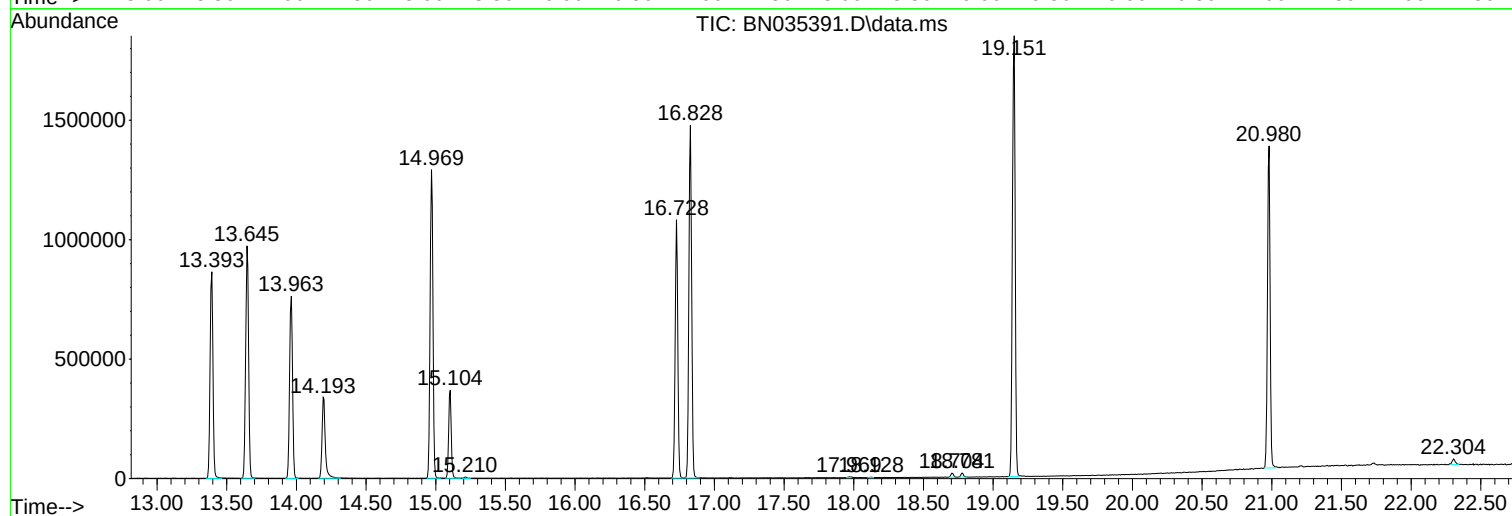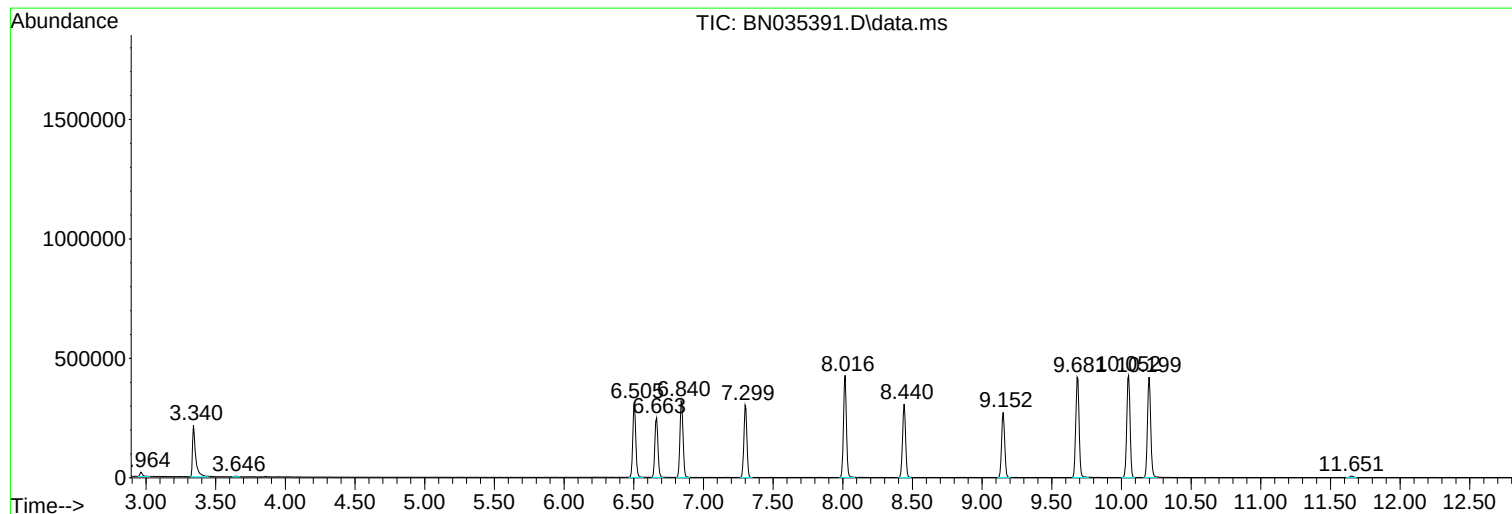

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120224\
Data File : BN035391.D
Acq On : 02 Dec 2024 19:35
Operator : RC/JU
Sample : PB165114BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK114

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120224\
Data File : BN035391.D
Acq On : 02 Dec 2024 19:35
Operator : RC/JU
Sample : PB165114BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK114

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc