

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120224\
 Data File : BN035394.D
 Acq On : 02 Dec 2024 21:32
 Operator : RC/JU
 Sample : PB165141BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK141

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.964	9	13	21	rVB	15131	19325	0.77%	0.090%
2	3.340	73	77	97	rBV	177569	279840	11.20%	1.301%
3	3.640	124	128	136	rBV	4350	6463	0.26%	0.030%
4	6.505	608	615	627	rVB	264317	399609	15.99%	1.858%
5	6.664	636	642	656	rVB	208062	317865	12.72%	1.478%
6	6.840	666	672	681	rVB	278930	417283	16.70%	1.941%
7	7.299	744	750	759	rBV	245232	360862	14.44%	1.678%
8	8.016	865	872	886	rBV	356396	539601	21.60%	2.509%
9	8.440	937	944	952	rBV	258509	387230	15.50%	1.801%
10	9.152	1058	1065	1075	rVB	224045	348029	13.93%	1.619%
11	9.681	1148	1155	1170	rBV	374316	599436	23.99%	2.788%
12	10.046	1209	1217	1224	rBV	337227	554887	22.21%	2.580%
13	10.199	1234	1243	1255	rBV	362028	582179	23.30%	2.707%
14	11.657	1484	1491	1498	rVB	4674	8519	0.34%	0.040%
15	13.393	1779	1786	1799	rBV	770197	1076588	43.09%	5.007%
16	13.646	1822	1829	1840	rBV	837763	1234184	49.39%	5.740%
17	13.963	1876	1883	1893	rBV	612086	908051	36.34%	4.223%
18	14.193	1916	1922	1941	rBV	298629	470431	18.83%	2.188%
19	14.969	2048	2054	2066	rVB	1165285	1600279	64.04%	7.442%
20	15.098	2071	2076	2086	rBV	320719	418276	16.74%	1.945%
21	15.210	2091	2095	2102	rVB2	3931	4795	0.19%	0.022%
22	16.510	2314	2316	2324	rVB3	1524	2501	0.10%	0.012%
23	16.728	2347	2353	2361	rVB	909055	1197301	47.92%	5.568%
24	16.828	2363	2370	2379	rBV	1322155	1849181	74.01%	8.600%
25	18.704	2684	2689	2695	rBV2	15383	20687	0.83%	0.096%
26	18.775	2695	2701	2707	rBV	14571	20939	0.84%	0.097%
27	19.145	2758	2764	2779	rBV	1672064	2271402	90.90%	10.563%
28	20.975	3070	3075	3084	rBV	1111816	1492043	59.71%	6.939%
29	22.033	3251	3255	3261	rVB3	32229	49081	1.96%	0.228%
30	22.963	3410	3413	3420	rVB4	21948	36311	1.45%	0.169%
31	23.469	3491	3499	3514	rBV2	1122240	2498714	100.00%	11.620%
32	23.651	3522	3530	3539	rBV	705350	1531235	61.28%	7.121%




Sum of corrected areas: 21503127

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120224\
Data File : BN035394.D
Acq On : 02 Dec 2024 21:32
Operator : RC/JU
Sample : PB165141BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK141

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

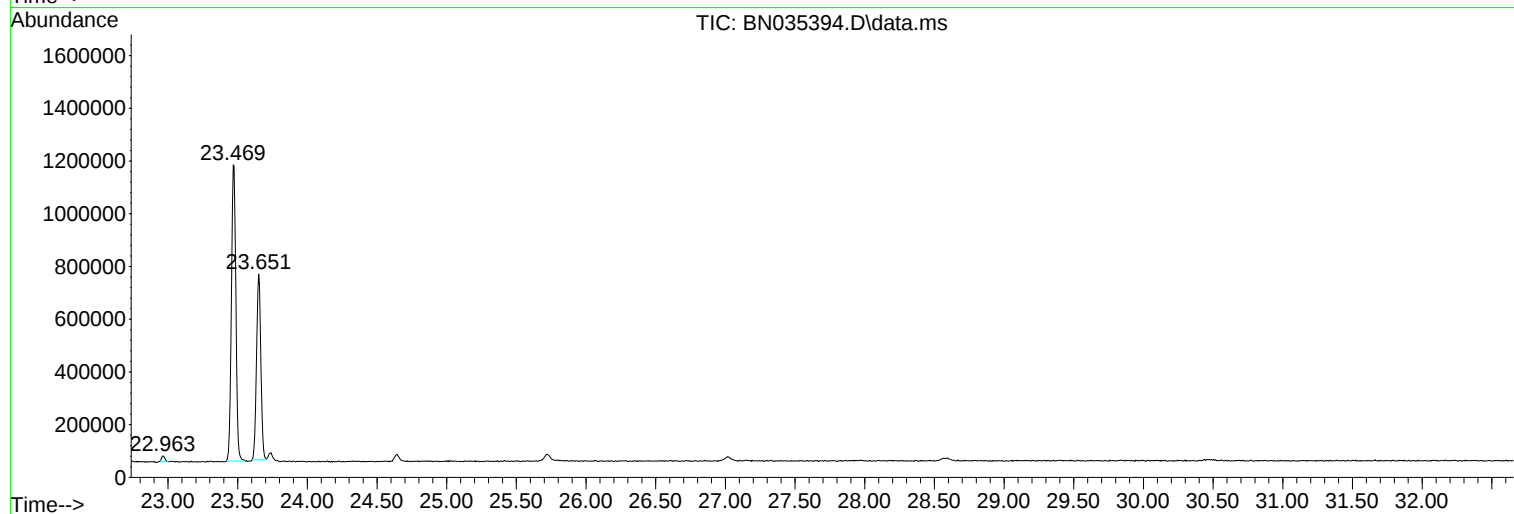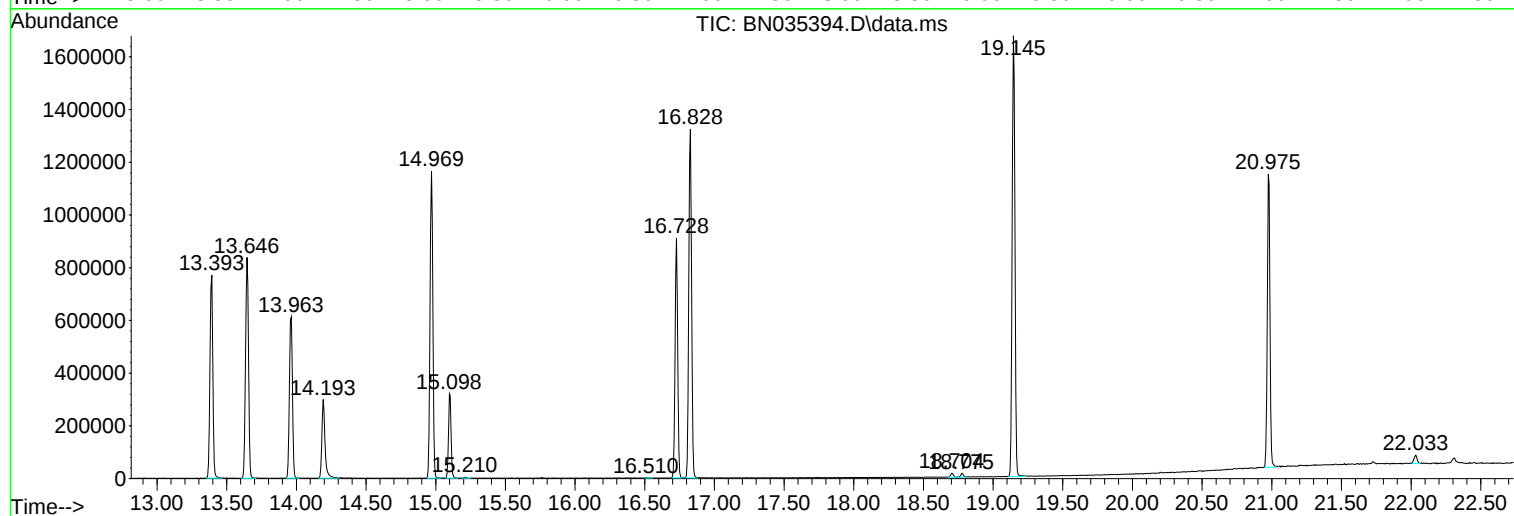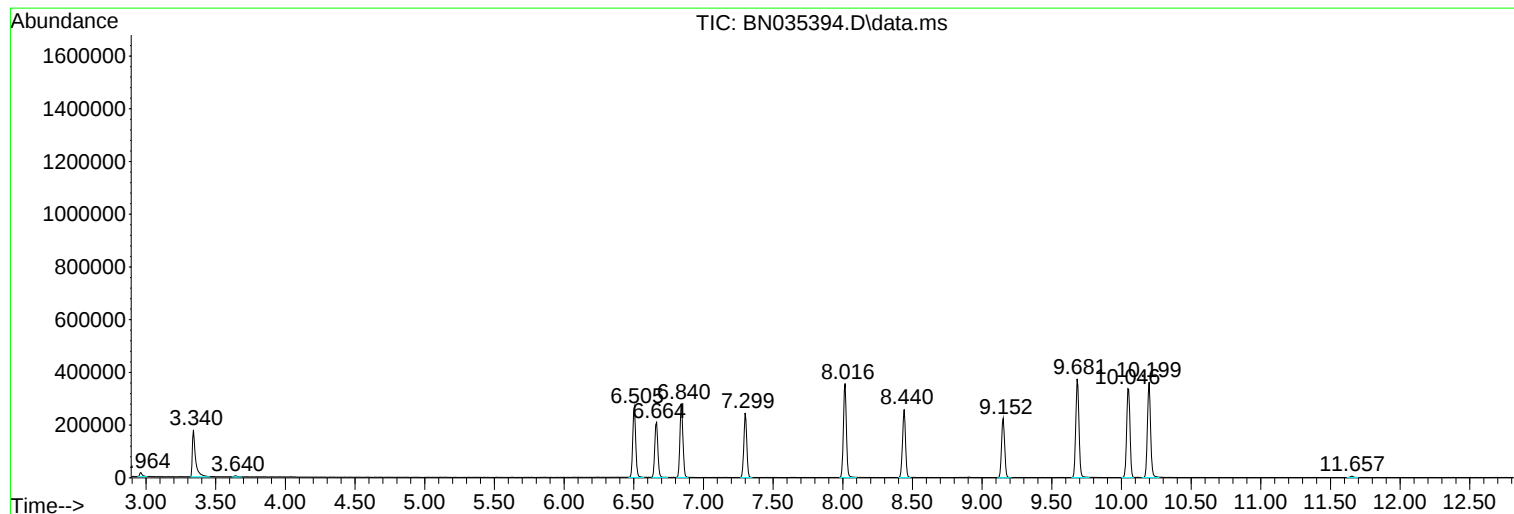

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120224\
Data File : BN035394.D
Acq On : 02 Dec 2024 21:32
Operator : RC/JU
Sample : PB165141BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK141

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120224\
Data File : BN035394.D
Acq On : 02 Dec 2024 21:32
Operator : RC/JU
Sample : PB165141BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK141

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc