


2,4,6-Tribromophenol

Response Ratio

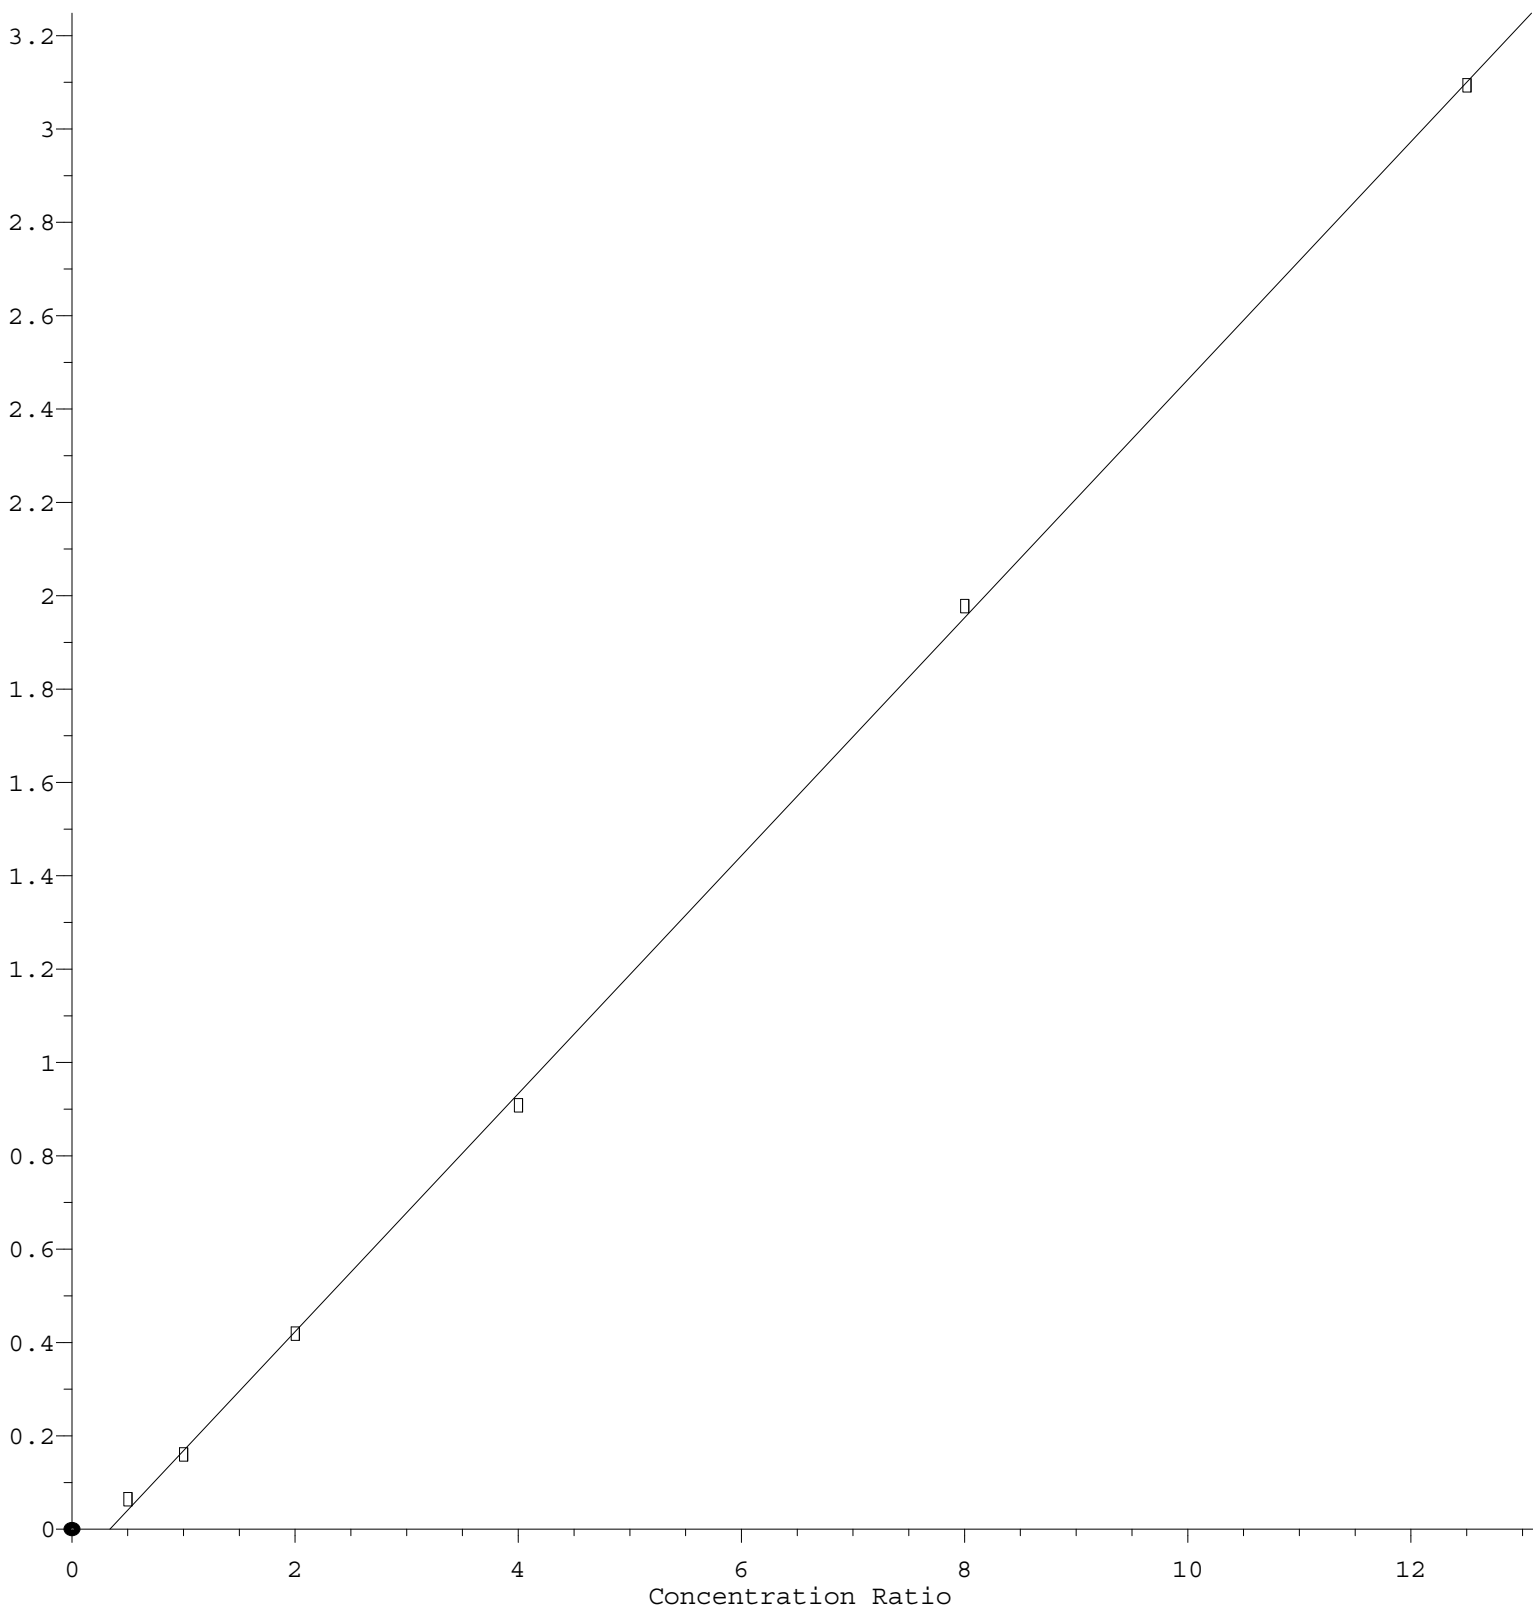


$$\text{Response} = 2.549\text{e-}001 * \text{Amt} - 8.570\text{e-}002$$

Coef of Det (r^2) = 0.999737 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN120321.M


Calibration Table Last Updated: Fri Dec 03 23:07:38 2021

4,6-Dinitro-2-methylphenol

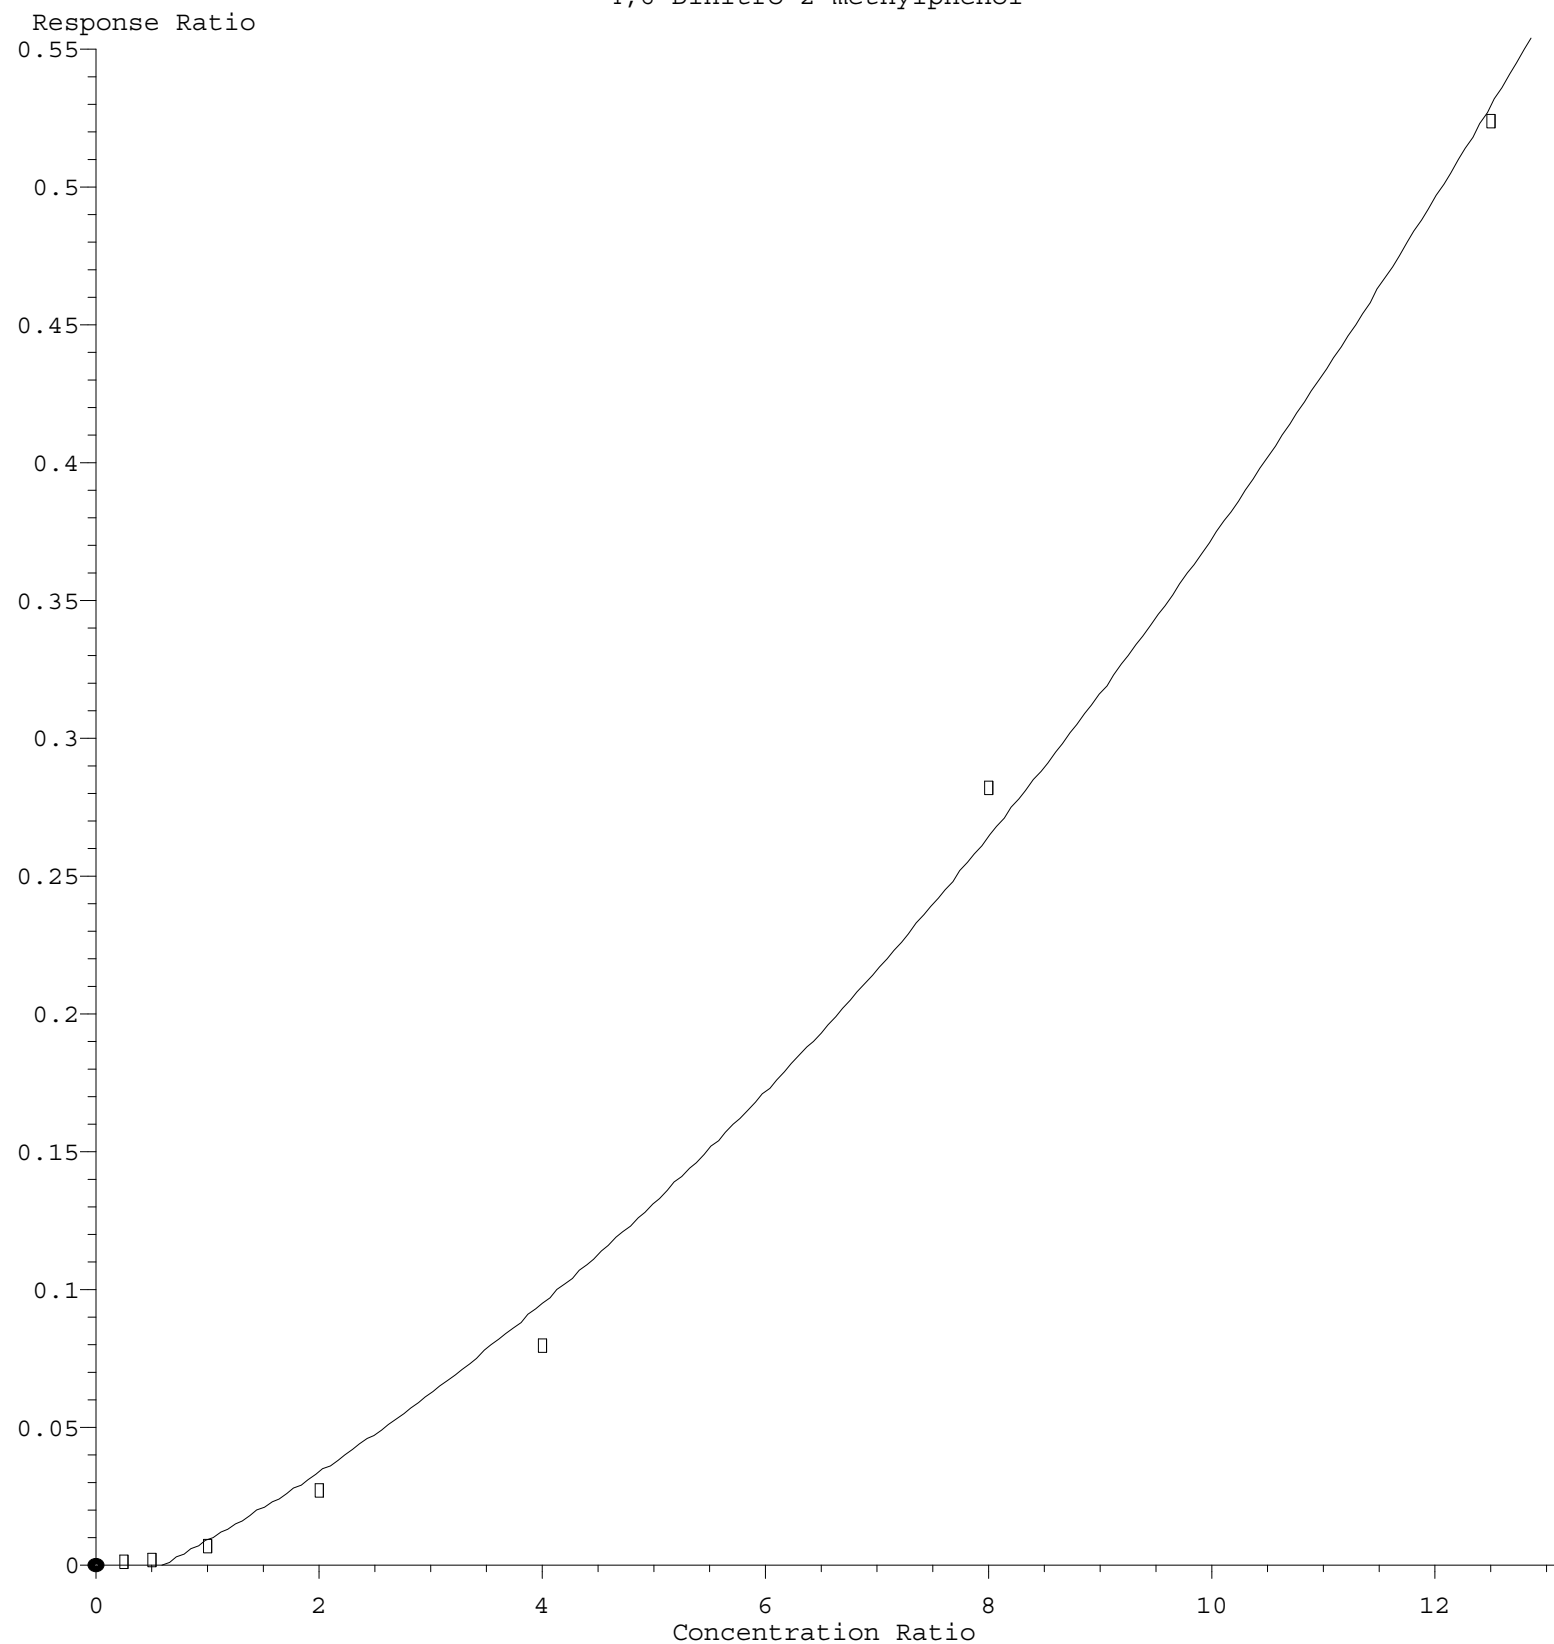

$R = 1.953e-003 A^2 + 1.889e-002 A - 1.181e-002$
 Coef of Det (r^2) = 0.997027 Curve Fit: Quadratic
 Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN120321.M
 Calibration Table Last Updated: Fri Dec 03 23:07:38 2021


Atrazine

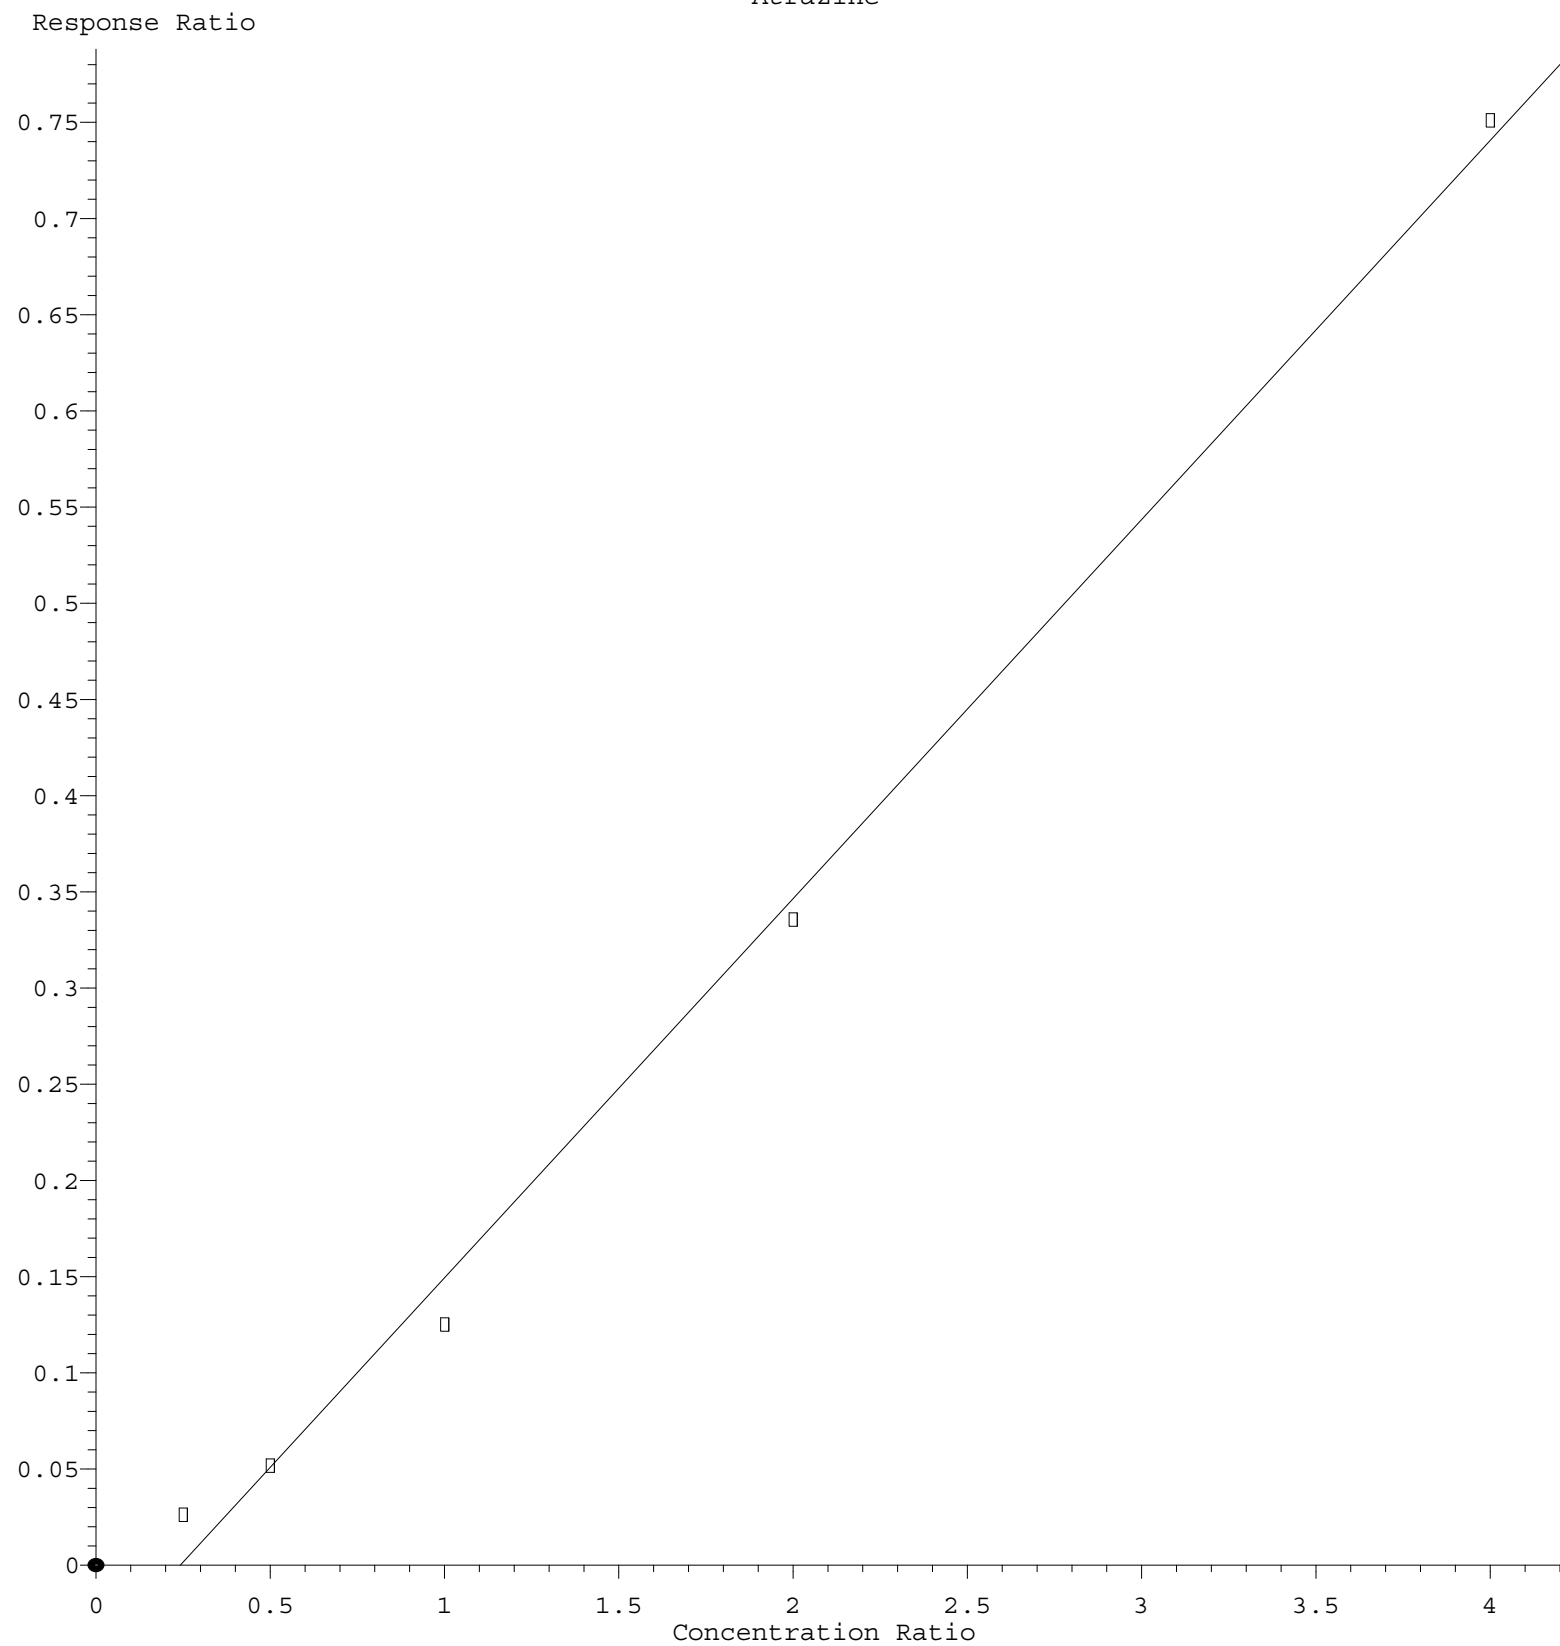

Response = 1.972e-001 * Amt - 4.771e-002
 Coef of Det (r^2) = 0.996092 Curve Fit: Linear
 Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN120321.M
 Calibration Table Last Updated: Fri Dec 03 23:07:38 2021

Pentachlorophenol

Response Ratio

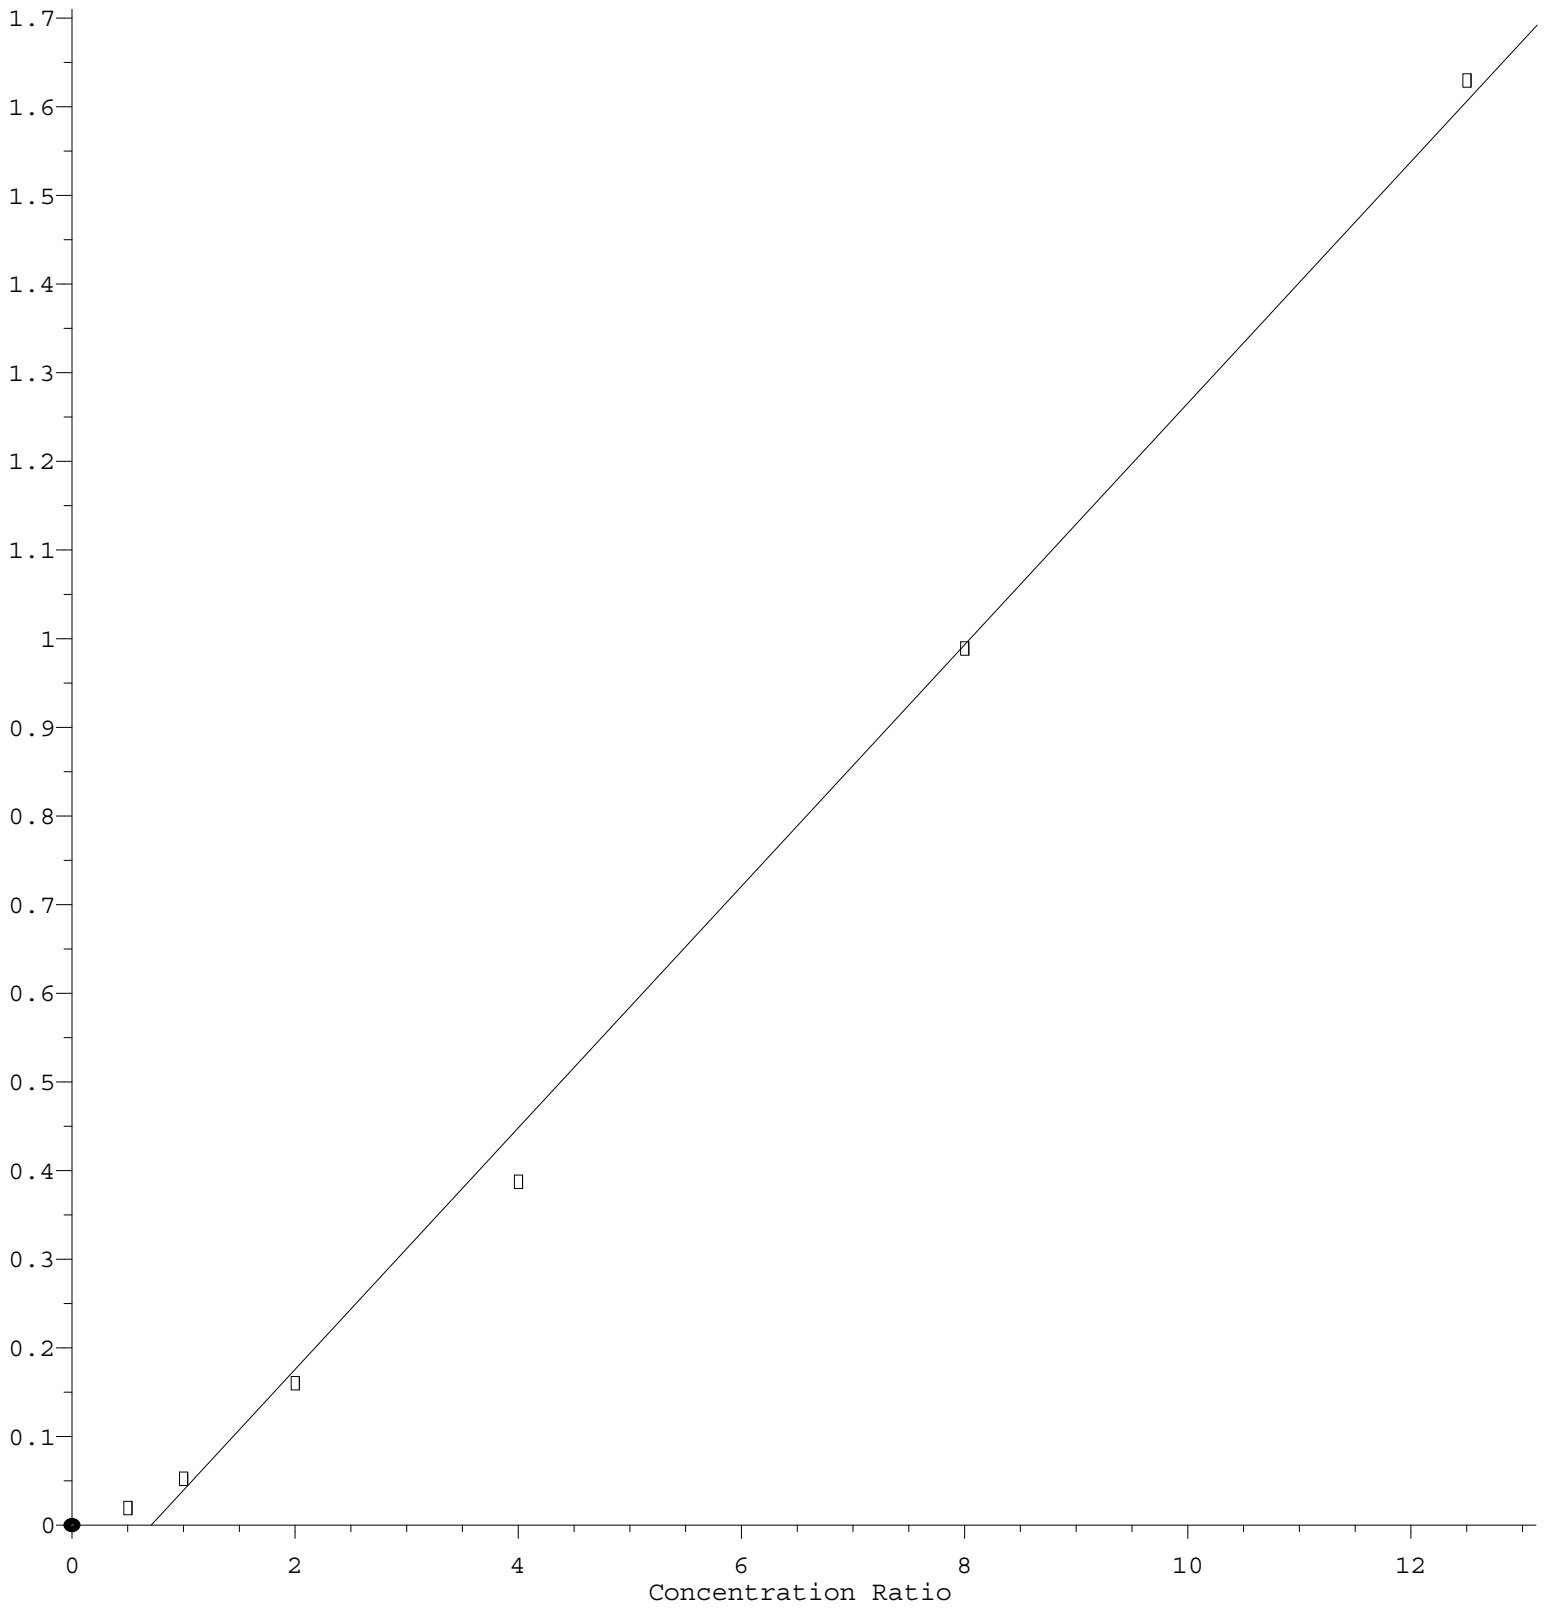

$$\text{Response} = 1.363\text{e-}001 * \text{Amt} - 9.637\text{e-}002$$


Coef of Det (r^2) = 0.996625 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN120321.M

Calibration Table Last Updated: Fri Dec 03 23:07:38 2021

Dibenzo (a,h) anthracene

Response Ratio

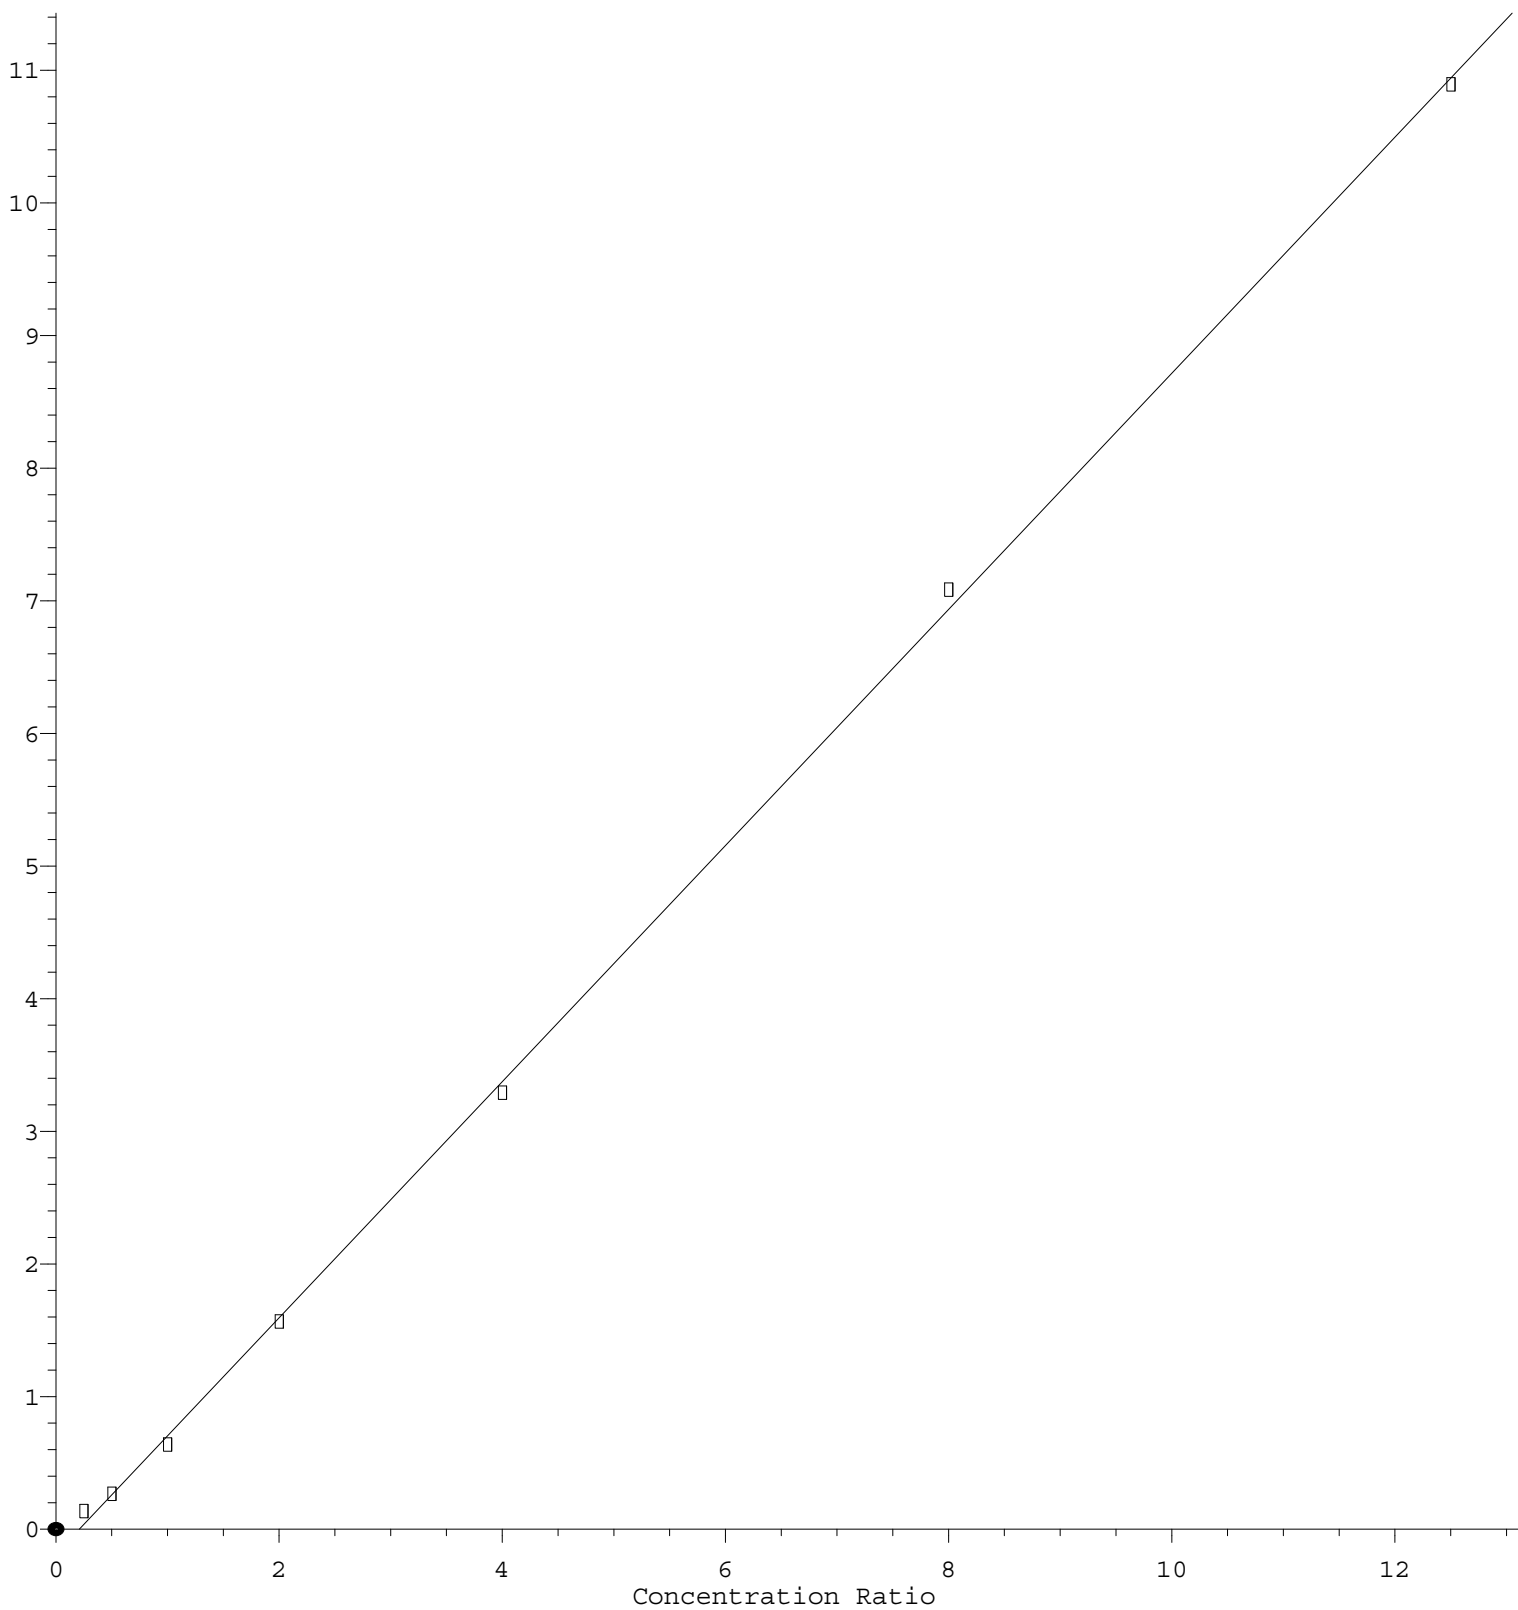

$$\text{Response} = 8.905\text{e-}001 * \text{Amt} - 1.828\text{e-}001$$

Coef of Det (r^2) = 0.999541 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN120321.M

Calibration Table Last Updated: Fri Dec 03 23:07:38 2021