

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120324\
 Data File : BN035401.D
 Acq On : 03 Dec 2024 10:09
 Operator : RC/JU
 Sample : PB165141BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK141

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035401.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.963	9	13	24	rVB	20445	28777	0.84%	0.096%
2	3.340	73	77	98	rBV	234407	394157	11.51%	1.317%
3	3.640	124	128	135	rBV2	5685	9255	0.27%	0.031%
4	6.504	608	615	627	rVB	353349	556794	16.26%	1.860%
5	6.657	635	641	651	rVB	284384	441133	12.88%	1.474%
6	6.840	666	672	682	rVB	390100	585275	17.09%	1.955%
7	7.298	744	750	760	rVB	335142	505259	14.76%	1.688%
8	8.010	865	871	884	rBV	472579	749736	21.90%	2.505%
9	8.440	937	944	951	rBV	361959	550969	16.09%	1.841%
10	9.151	1058	1065	1074	rBV	310420	486307	14.20%	1.625%
11	9.681	1148	1155	1168	rBV	526694	841635	24.58%	2.812%
12	10.045	1210	1217	1225	rBV	468028	777307	22.70%	2.597%
13	10.198	1235	1243	1258	rBV	472454	797193	23.28%	2.663%
14	11.651	1484	1490	1497	rVB	7149	11854	0.35%	0.040%
15	13.392	1779	1786	1800	rBV	1008174	1460691	42.66%	4.880%
16	13.645	1822	1829	1844	rBV2	1155209	1700332	49.66%	5.680%
17	13.957	1876	1882	1890	rBV	843575	1247630	36.44%	4.168%
18	14.192	1915	1922	1935	rBV	436716	647145	18.90%	2.162%
19	14.969	2047	2054	2063	rBV	1536015	2176056	63.55%	7.270%
20	15.098	2070	2076	2088	rBV	440435	588277	17.18%	1.965%
21	15.210	2091	2095	2099	rVB	5116	6463	0.19%	0.022%
22	15.757	2186	2188	2195	rVB3	2854	3808	0.11%	0.013%
23	16.727	2347	2353	2363	rBV	1174476	1602923	46.81%	5.355%
24	16.827	2363	2370	2382	rBV	1767003	2487012	72.63%	8.308%
25	18.704	2685	2689	2693	rVB2	21218	27660	0.81%	0.092%
26	18.774	2697	2701	2708	rVV	20020	26195	0.77%	0.088%
27	19.145	2758	2764	2773	rBV	2128135	3023572	88.30%	10.101%
28	20.980	3070	3076	3085	rBV2	1474530	2000551	58.43%	6.683%
29	22.033	3251	3255	3260	rVB	41988	62070	1.81%	0.207%
30	22.304	3298	3301	3311	rVB2	38105	60741	1.77%	0.203%
31	22.968	3409	3414	3420	rVB	46230	81817	2.39%	0.273%
32	23.474	3491	3500	3516	rBV2	1553254	3424122	100.00%	11.439%
33	23.651	3522	3530	3539	rBV	986369	2141186	62.53%	7.153%
34	23.733	3540	3544	3553	rVB3	69148	148792	4.35%	0.497%
35	24.639	3693	3698	3707	rVB3	55226	128553	3.75%	0.429%
36	25.721	3877	3882	3895	rVB3	53304	152330	4.45%	0.509%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120324\
Data File : BN035401.D
Acq On : 03 Dec 2024 10:09
Operator : RC/JU
Sample : PB165141BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK141

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 29933577

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120324\
Data File : BN035401.D
Acq On : 03 Dec 2024 10:09
Operator : RC/JU
Sample : PB165141BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK141

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

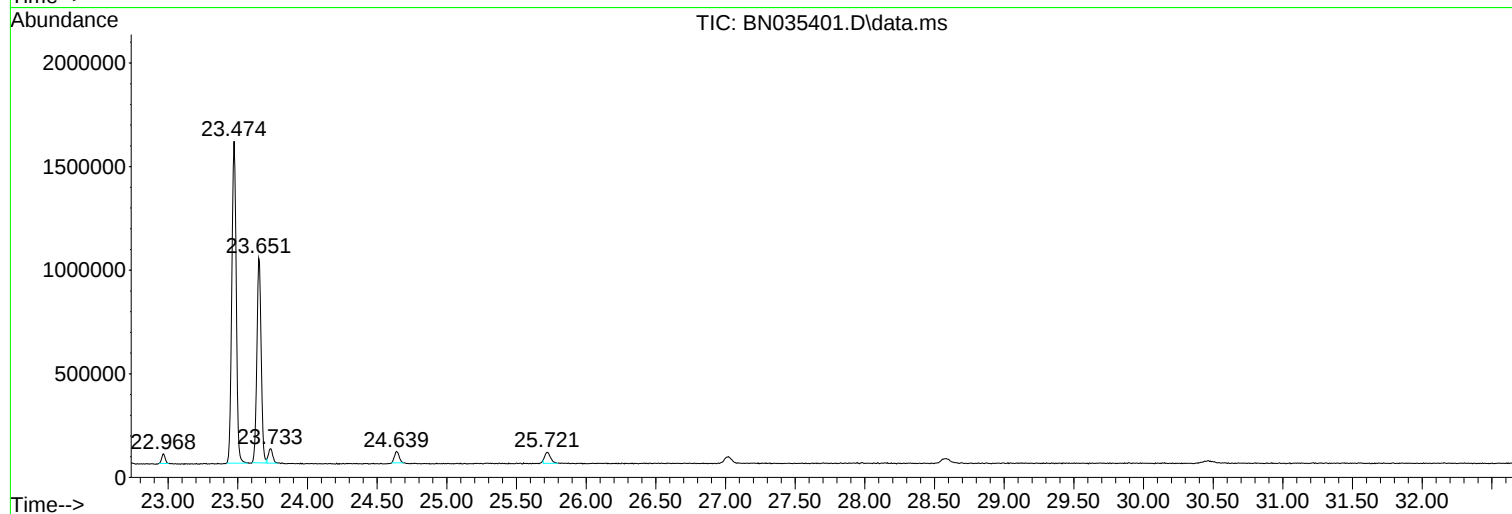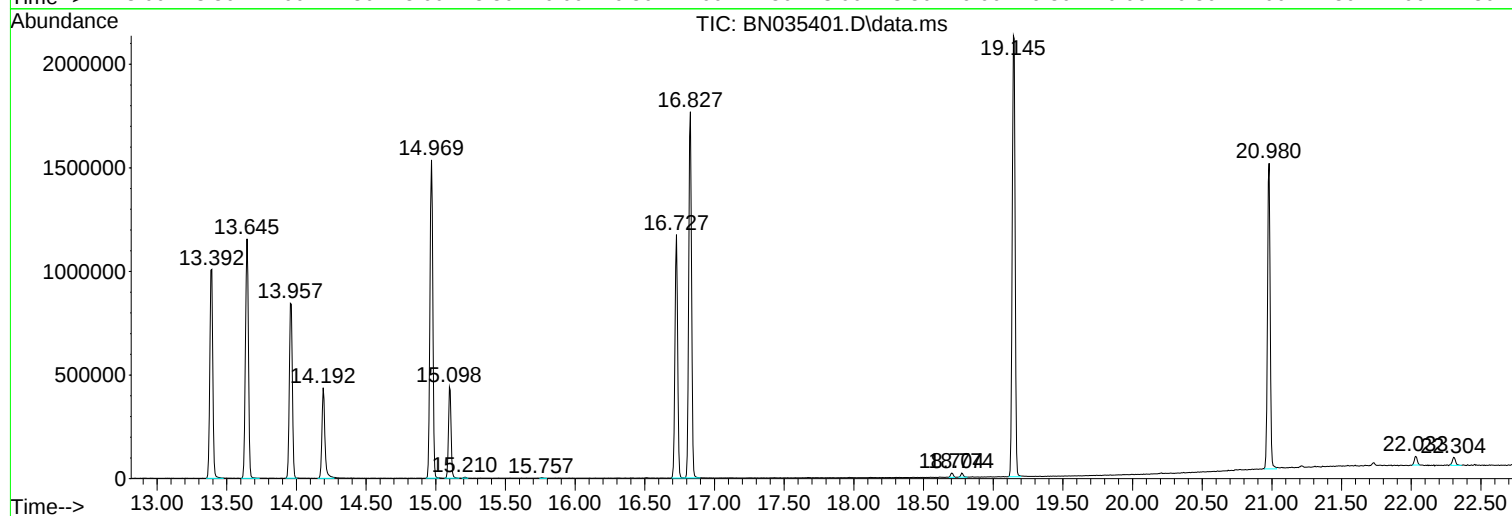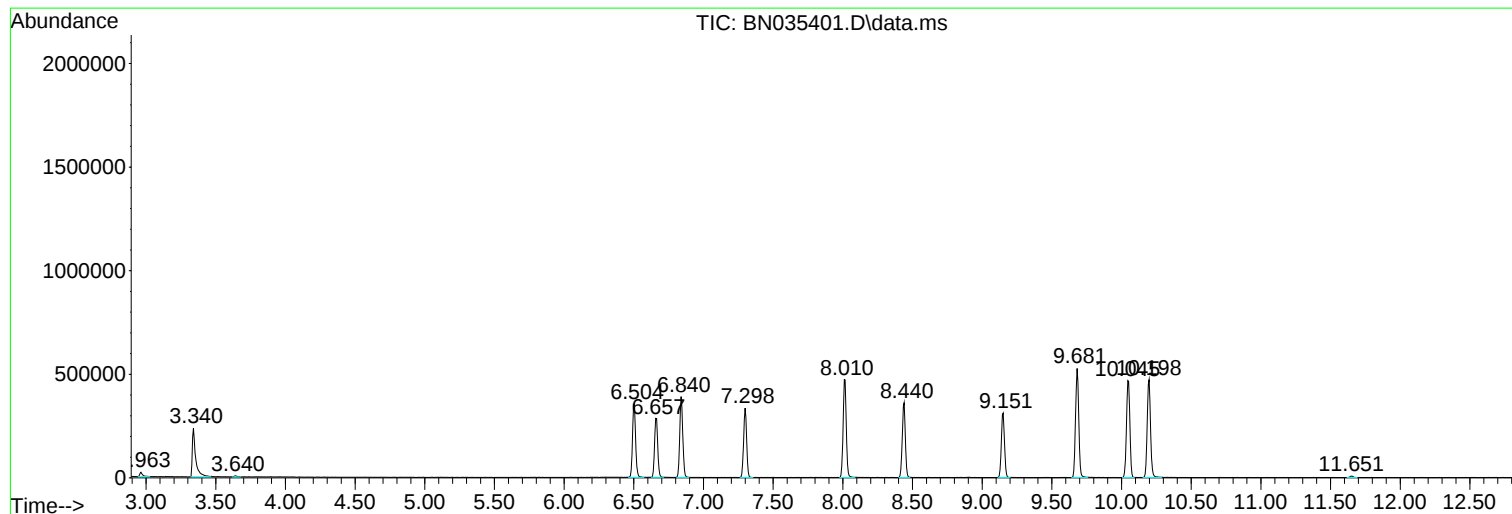

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120324\
Data File : BN035401.D
Acq On : 03 Dec 2024 10:09
Operator : RC/JU
Sample : PB165141BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK141

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120324\
Data File : BN035401.D
Acq On : 03 Dec 2024 10:09
Operator : RC/JU
Sample : PB165141BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK141

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc