


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120419\
 Data File : BN008835.D
 Acq On : 04 Dec 2019 10:44
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN120419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 04 15:42:09 2019

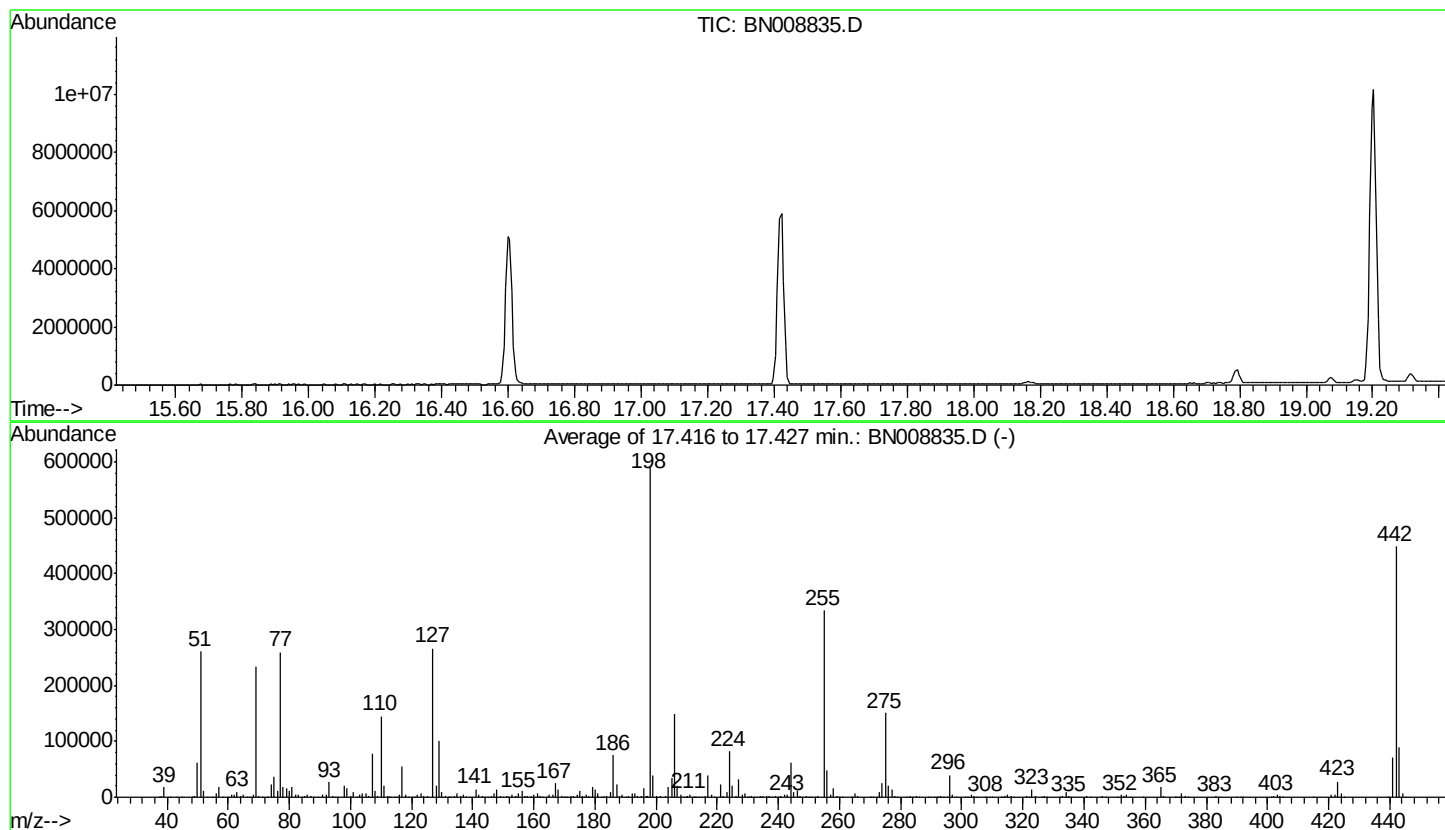

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	260575	PASS
68	69	0.00	2	2.0	4630	PASS
69	198	0.00	100	39.4	233788	PASS
70	69	0.00	2	0.5	1277	PASS
127	198	10	80	45.0	267008	PASS
197	198	0.00	2	0.3	1690	PASS
198	198	100	100	100.0	593706	PASS
199	198	5	9	6.7	39490	PASS
275	198	10	60	25.3	150229	PASS
365	198	1	100	3.0	17698	PASS
441	198	0.01	100	12.1	72109	PASS
442	198	50	100	75.6	448597	PASS
443	442	15	24	19.9	89274	PASS