
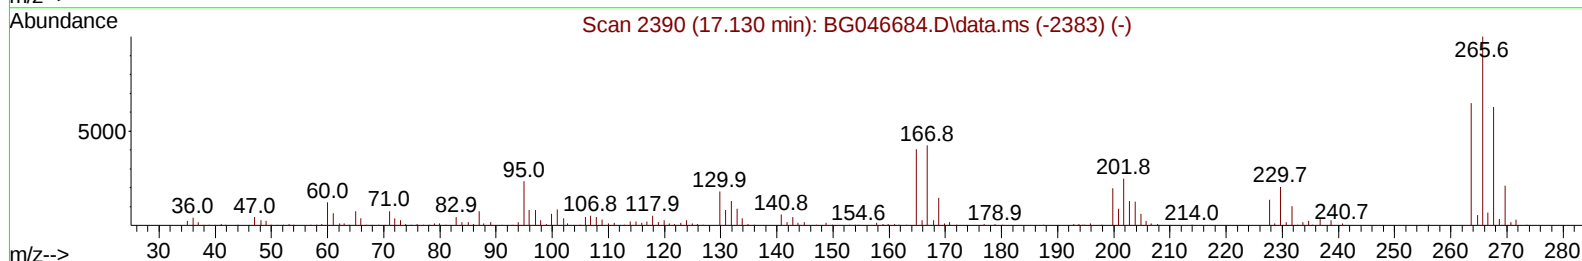
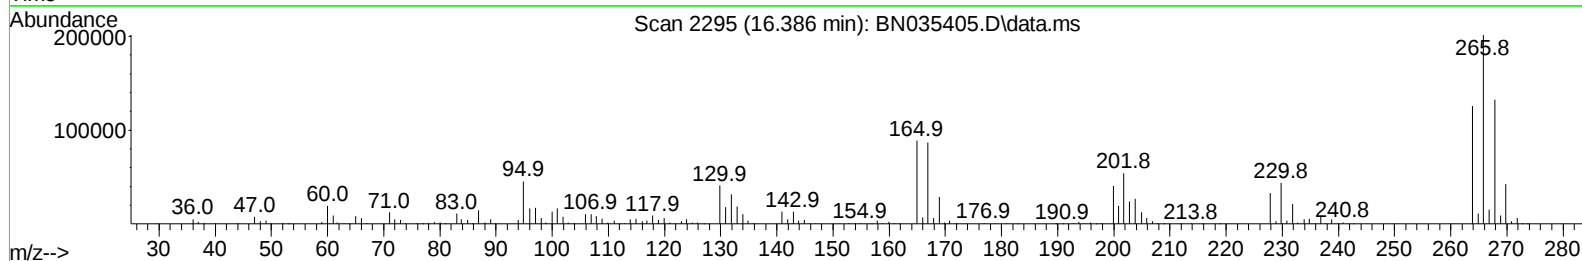


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120424\
Data File : BN035405.D
Acq On : 03 Dec 2024 15:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 23:08:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 23:08:29 2024
Response via : Initial Calibration

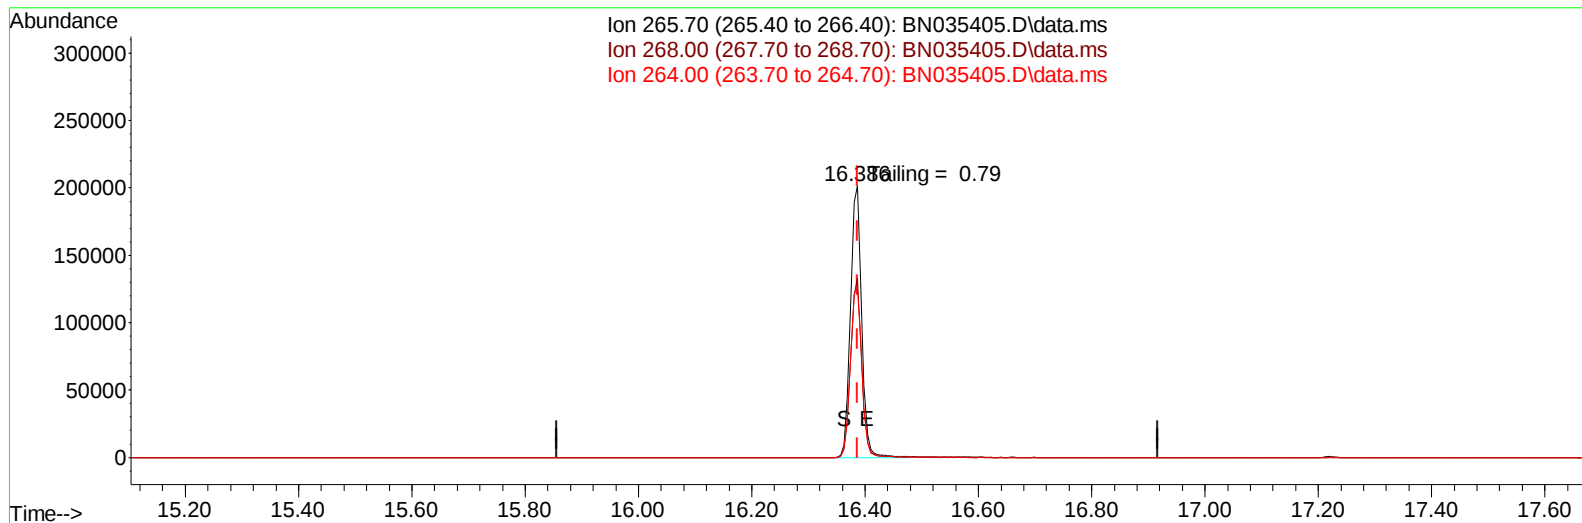




TIC: BN035405.D\data.ms

(70) Pentachlorophenol (C)**16.386min (0.000) 30135.06 ng****response 280007**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.85
264.00	61.60	62.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120424\
Data File : BN035405.D
Acq On : 03 Dec 2024 15:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 23:08:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 23:08:29 2024
Response via : Initial Calibration

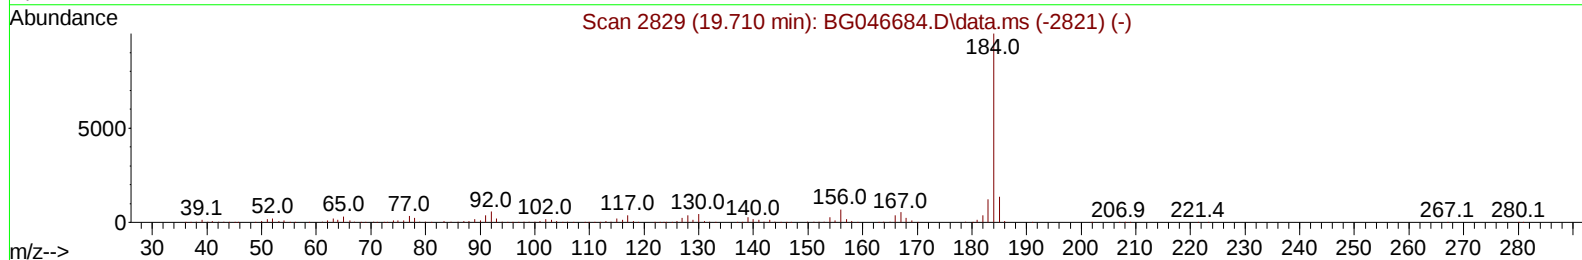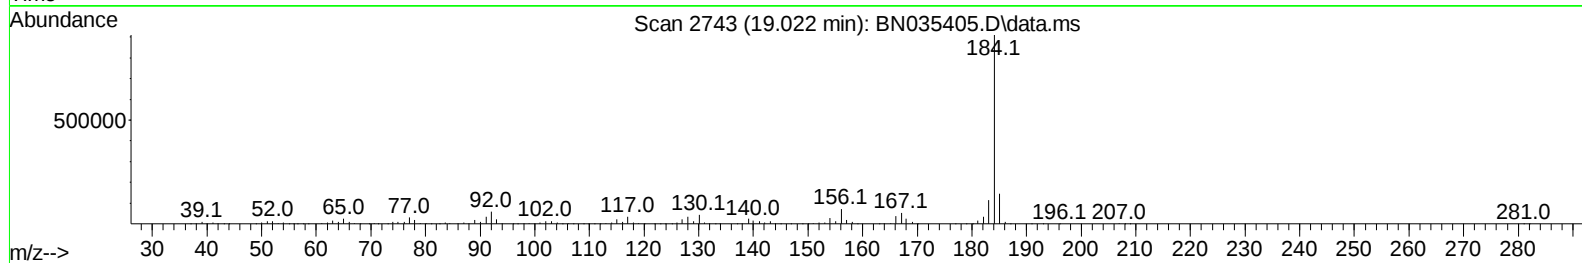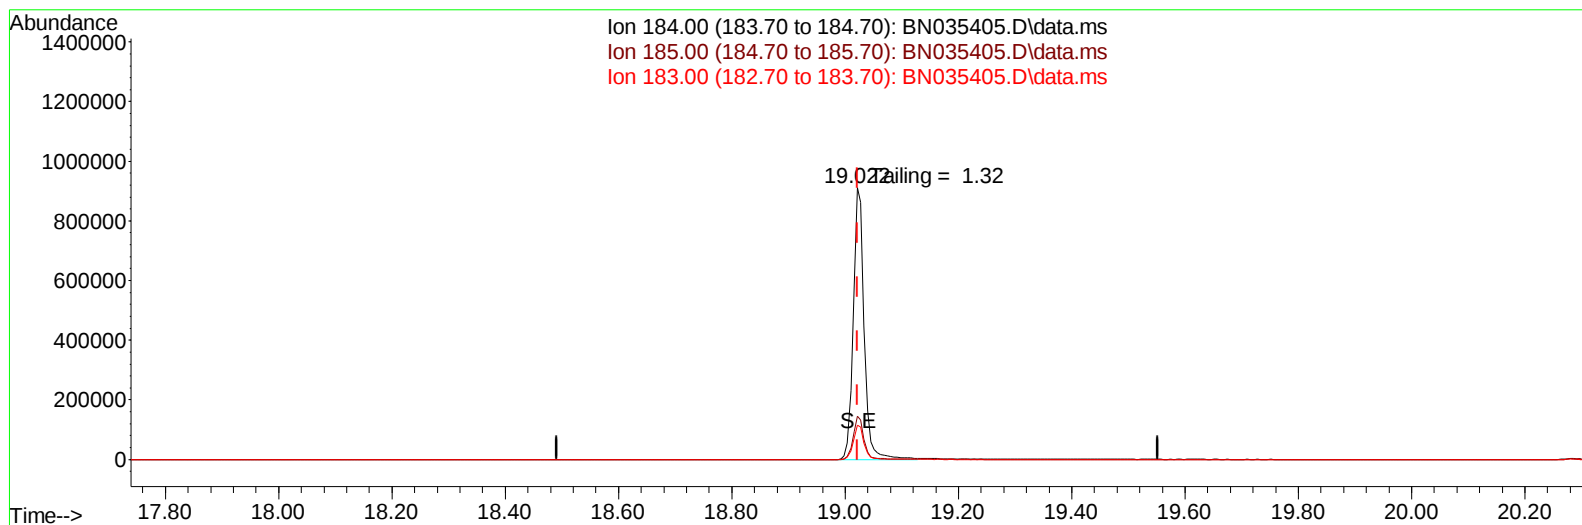

TIC: BN035405.D\data.ms

(77) Benzidine

19.022min (0.000) 0.00 ng

response 1239645

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.96
183.00	13.20	12.61
0.00	0.00	0.00