


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120424\
Data File : BN035405.D
Acq On : 03 Dec 2024 15:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 27 23:03:24 2024

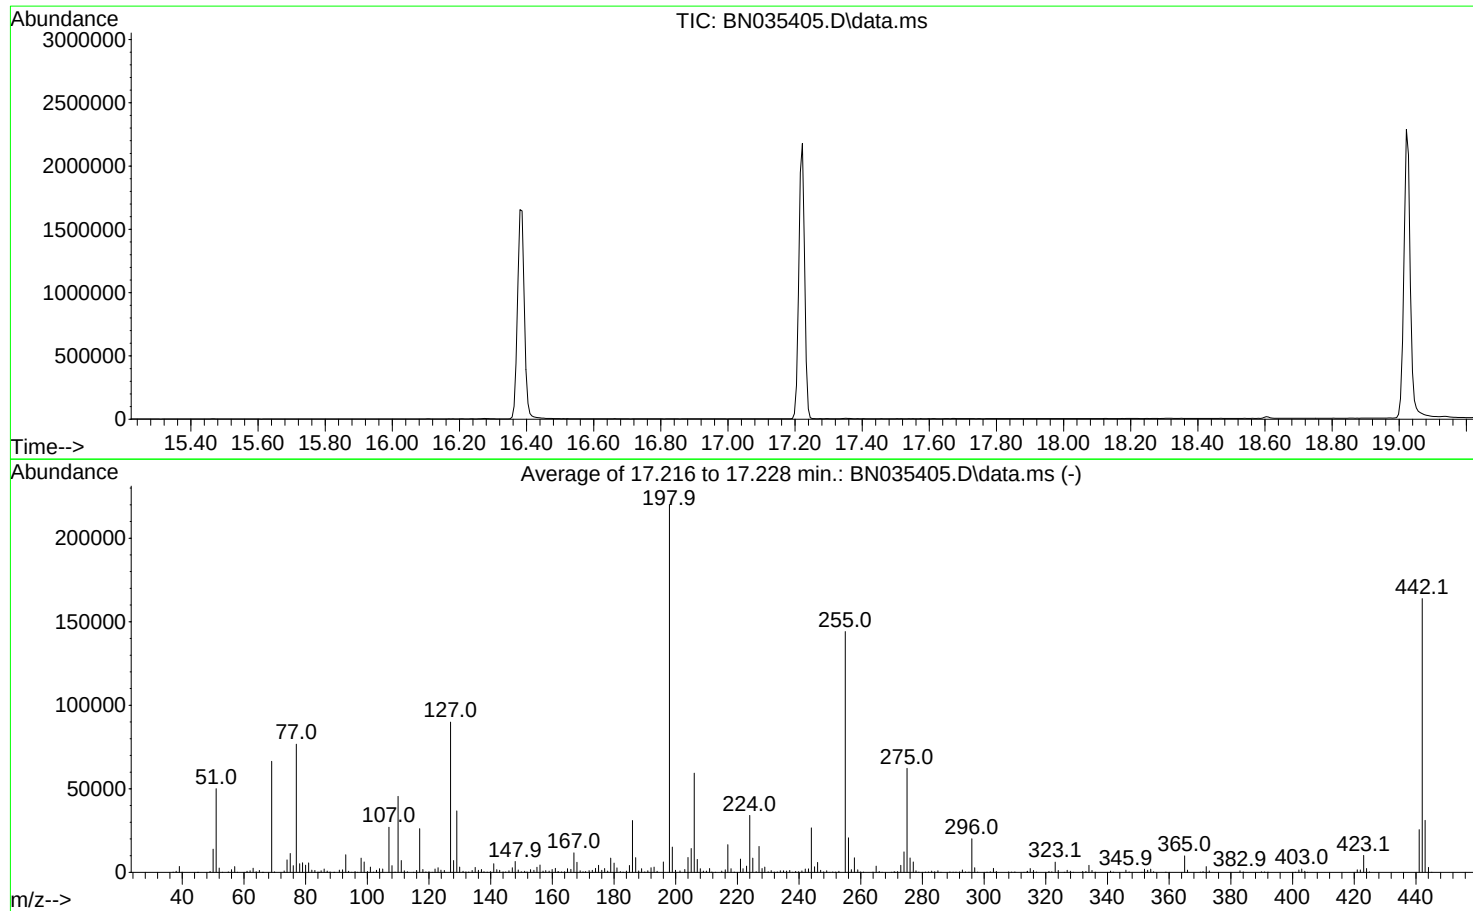

AutoFind: Scans 2436, 2437, 2438; Background Corrected with Scan 2429

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	22.8	50112	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.2	66499	PASS
70	69	0.00	2	0.4	295	PASS
127	198	10	80	40.9	89949	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	220181	PASS
199	198	5	9	6.9	15167	PASS
275	198	10	60	28.3	62245	PASS
365	198	1	100	4.5	9919	PASS
441	198	0.01	100	11.6	25605	PASS
442	442	50	100	100.0	163819	PASS
443	442	15	24	19.0	31133	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/4/2024	BNA_N	<u>BN035405.D</u>
Compound Name	Response	Retention Time
DDT	674620	20.286
DDD	16934	19.833
DDE	1155	19.322
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18089	692709	2.61

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120424\
Data File : BN035405.D
Acq On : 03 Dec 2024 15:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 03 23:08:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 23:08:29 2024
Response via : Initial Calibration

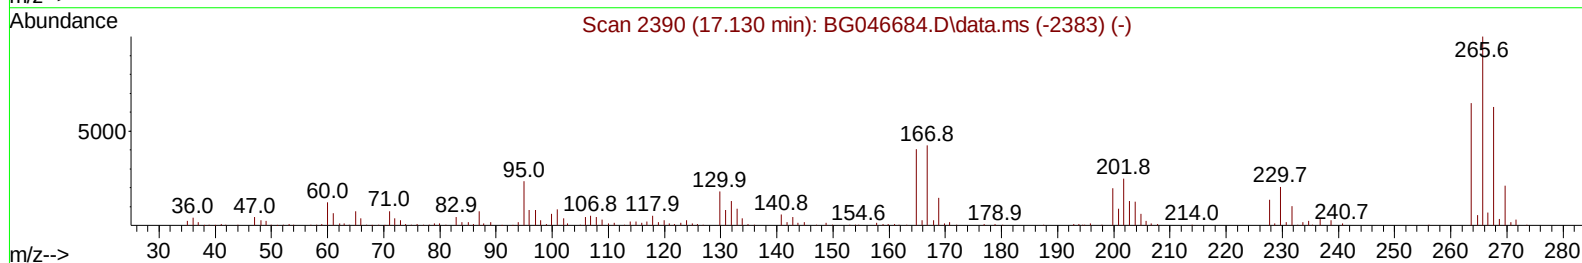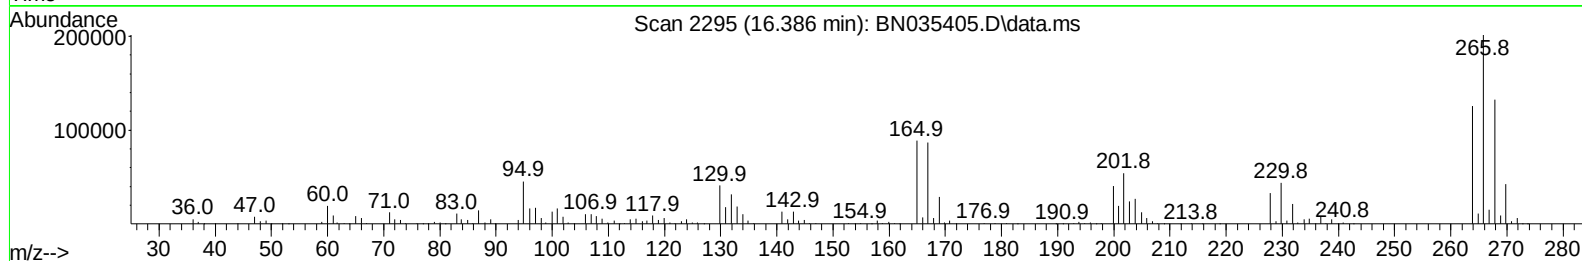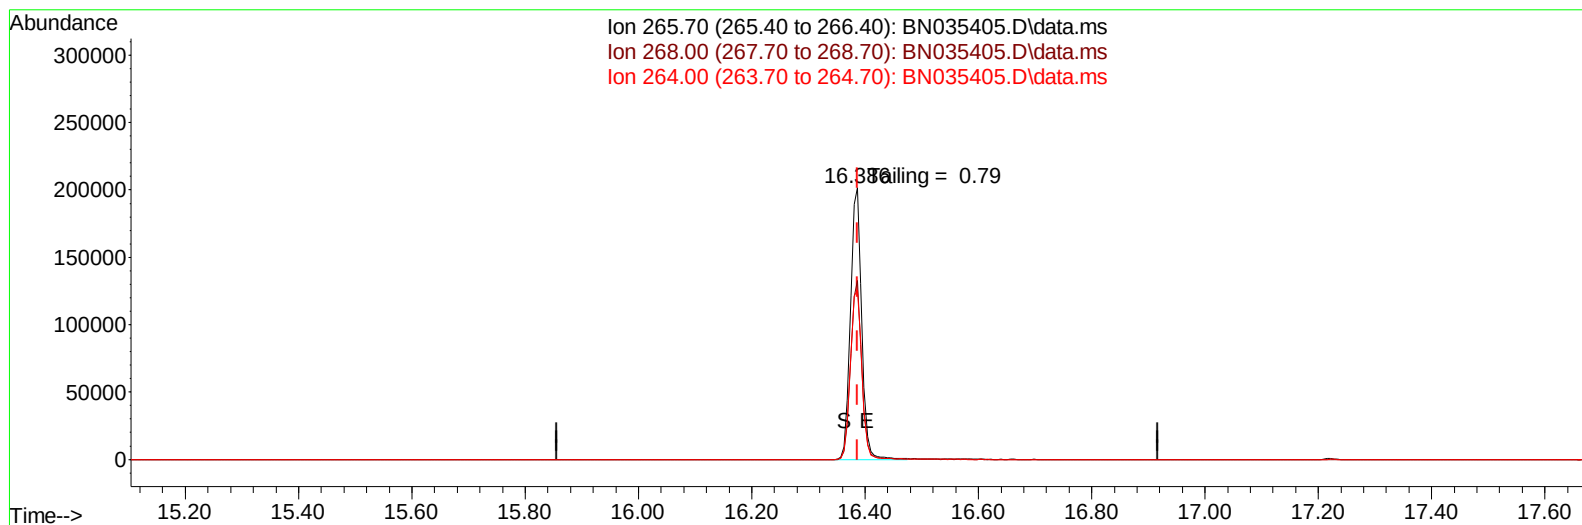

TIC: BN035405.D\data.ms

(70) Pentachlorophenol (C)

16.386min (0.000) 30135.06 ng




response 280007

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.85
264.00	61.60	62.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120424\
Data File : BN035405.D
Acq On : 03 Dec 2024 15:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 03 23:08:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 23:08:29 2024
Response via : Initial Calibration

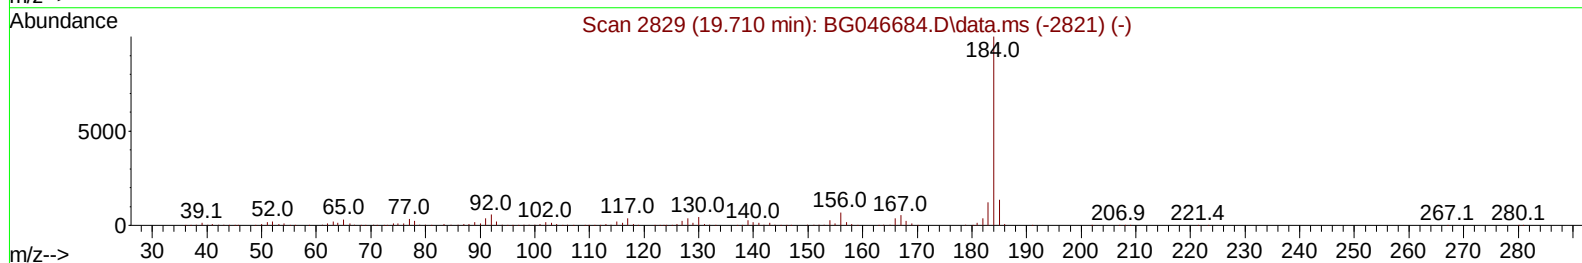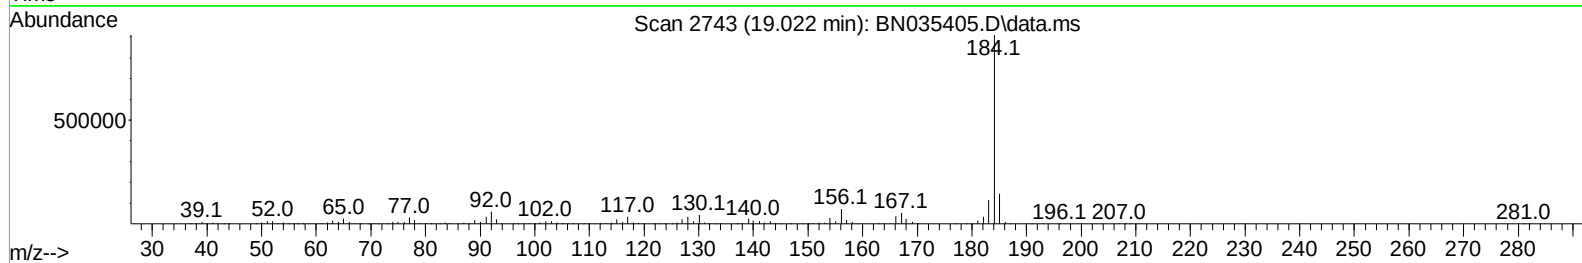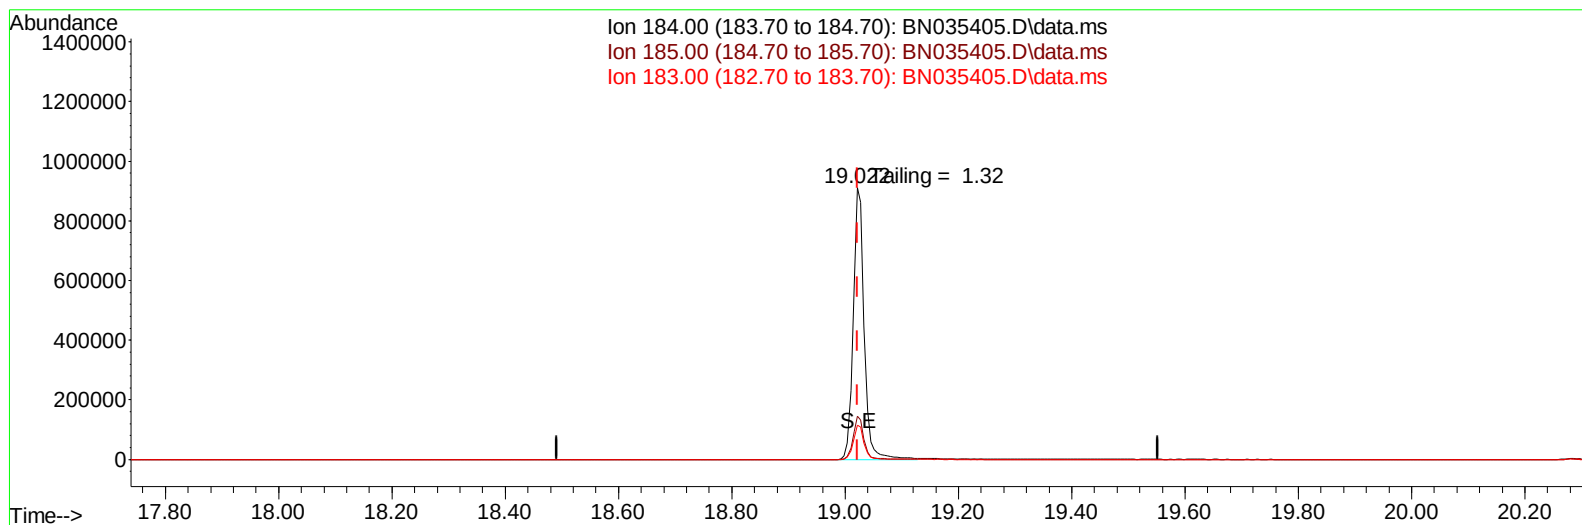

TIC: BN035405.D\data.ms

(77) Benzidine

19.022min (0.000) 0.00 ng

response 1239645

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.96
183.00	13.20	12.61
0.00	0.00	0.00