

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120524\
 Data File : BN035416.D
 Acq On : 04 Dec 2024 09:45
 Operator : RC/JU
 Sample : PB165168BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK168

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035416.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.964	9	13	22	rBV	18479	26517	0.87%	0.097%
2	3.340	73	77	94	rBV	222324	370539	12.10%	1.358%
3	3.640	124	128	138	rVB	5769	8905	0.29%	0.033%
4	6.499	608	614	625	rVB	338064	515952	16.85%	1.891%
5	6.658	635	641	654	rVB	283795	414582	13.54%	1.519%
6	6.840	666	672	682	rBV	366497	540308	17.65%	1.980%
7	7.299	744	750	758	rBV	322831	483073	15.78%	1.770%
8	8.011	864	871	880	rBV	462993	698032	22.80%	2.558%
9	8.434	936	943	953	rBV	324070	503921	16.46%	1.847%
10	9.146	1057	1064	1073	rBV	283744	442878	14.47%	1.623%
11	9.681	1147	1155	1166	rBV	476997	776592	25.37%	2.846%
12	10.046	1210	1217	1225	rVB	460516	739552	24.16%	2.710%
13	10.193	1235	1242	1256	rBV	438604	740161	24.18%	2.712%
14	11.646	1484	1489	1497	rVB	6323	11410	0.37%	0.042%
15	13.387	1779	1785	1796	rBV	980040	1335329	43.62%	4.893%
16	13.646	1822	1829	1841	rBV	1058491	1566195	51.16%	5.739%
17	13.957	1876	1882	1892	rBV	828668	1189944	38.87%	4.361%
18	14.193	1915	1922	1935	rBV	366485	571177	18.66%	2.093%
19	14.969	2047	2054	2066	rBV	1434959	2017589	65.91%	7.393%
20	15.098	2071	2076	2086	rVV	408293	530194	17.32%	1.943%
21	15.204	2090	2094	2099	rBV4	5008	6830	0.22%	0.025%
22	16.728	2346	2353	2360	rBV	1140069	1572847	51.38%	5.764%
23	16.828	2363	2370	2388	rVB	1650126	2333164	76.21%	8.550%
24	18.704	2685	2689	2694	rVB2	19146	23491	0.77%	0.086%
25	18.775	2697	2701	2710	rVB	17839	23776	0.78%	0.087%
26	19.145	2758	2764	2774	rBV	2110426	2856207	93.30%	10.467%
27	20.975	3070	3075	3088	rBV	1373869	1897360	61.98%	6.953%
28	22.033	3251	3255	3262	rVB2	42081	60267	1.97%	0.221%
29	23.469	3491	3499	3516	rBV2	1383417	3061319	100.00%	11.218%
30	23.651	3522	3530	3539	rBV	882828	1970784	64.38%	7.222%




Sum of corrected areas: 27288895

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120524\
Data File : BN035416.D
Acq On : 04 Dec 2024 09:45
Operator : RC/JU
Sample : PB165168BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK168

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

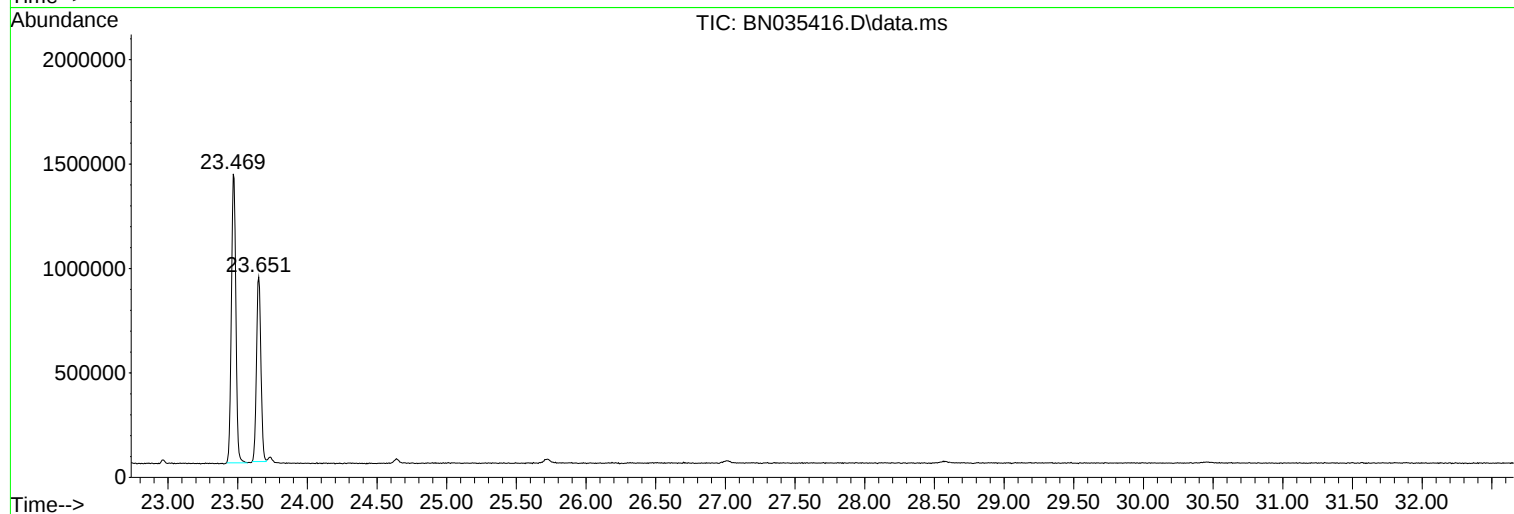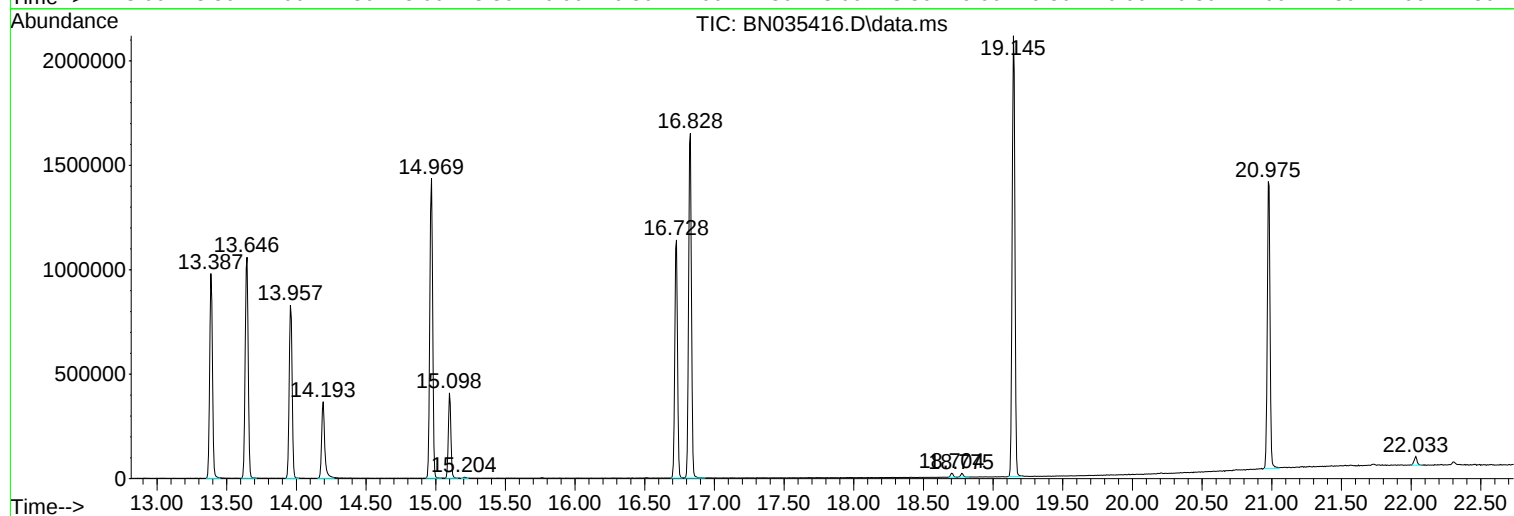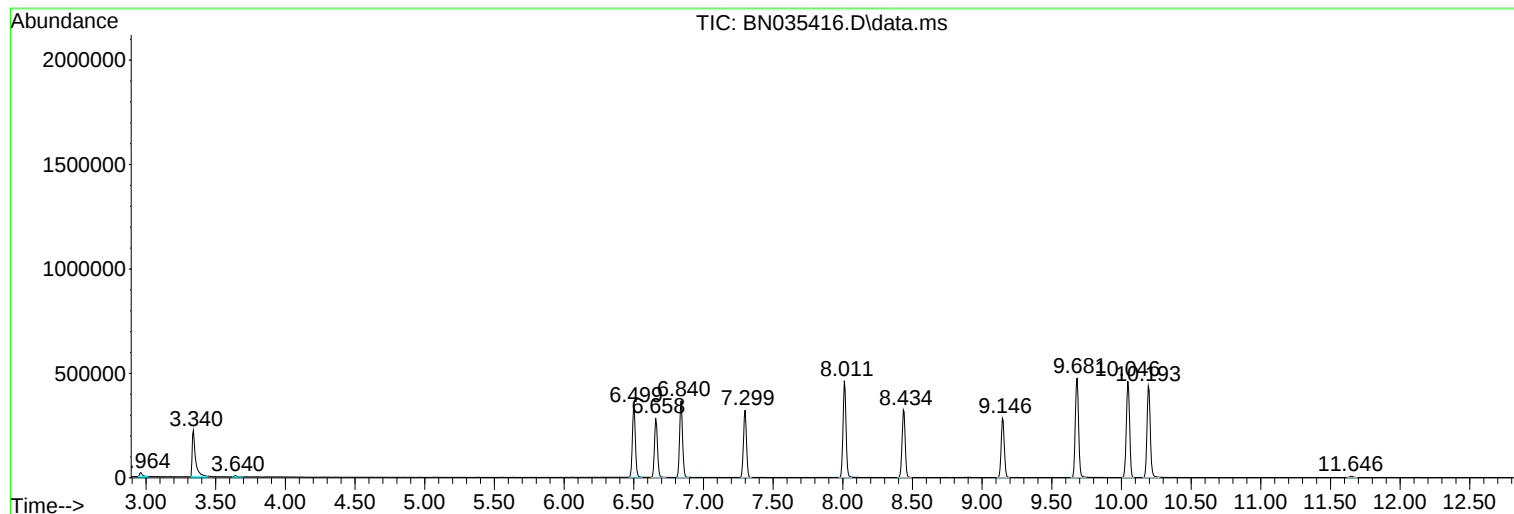

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120524\
Data File : BN035416.D
Acq On : 04 Dec 2024 09:45
Operator : RC/JU
Sample : PB165168BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK168

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120524\
Data File : BN035416.D
Acq On : 04 Dec 2024 09:45
Operator : RC/JU
Sample : PB165168BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK168

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc