

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120524\
 Data File : BN035417.D
 Acq On : 04 Dec 2024 10:24
 Operator : RC/JU
 Sample : PB165173BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK173

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.964	9	13	20	rVB	18860	23421	0.74%	0.083%
2	3.340	73	77	97	rBV	230727	381797	12.08%	1.361%
3	3.640	124	128	136	rBV	5770	7820	0.25%	0.028%
4	6.499	608	614	626	rVB	343233	532014	16.83%	1.896%
5	6.658	635	641	651	rBV	283707	424930	13.45%	1.514%
6	6.840	666	672	683	rBV	380201	560275	17.73%	1.997%
7	7.299	744	750	758	rBV	329824	492737	15.59%	1.756%
8	8.010	865	871	886	rBV	469343	722900	22.87%	2.576%
9	8.434	936	943	952	rBV	334043	521976	16.52%	1.860%
10	9.146	1058	1064	1071	rBV	294594	459021	14.52%	1.636%
11	9.681	1148	1155	1167	rBV	513905	798515	25.27%	2.846%
12	10.046	1210	1217	1225	rBV	463998	742868	23.51%	2.647%
13	10.199	1235	1243	1257	rBV	445955	765605	24.22%	2.728%
14	11.651	1484	1490	1496	rBV3	7023	11576	0.37%	0.041%
15	13.387	1779	1785	1799	rBV	1042472	1406297	44.50%	5.011%
16	13.645	1822	1829	1839	rBV	1099298	1603505	50.74%	5.714%
17	13.957	1876	1882	1894	rBV	858105	1208198	38.23%	4.305%
18	14.192	1916	1922	1940	rBV	394864	608629	19.26%	2.169%
19	14.969	2047	2054	2063	rBV	1489856	2096582	66.34%	7.471%
20	15.098	2070	2076	2085	rBV	433389	564856	17.87%	2.013%
21	15.210	2091	2095	2101	rVB	5695	7132	0.23%	0.025%
22	15.763	2184	2189	2193	rBV5	2323	3559	0.11%	0.013%
23	16.728	2346	2353	2363	rBV	1127369	1578551	49.95%	5.625%
24	16.828	2363	2370	2380	rBV	1667722	2414908	76.41%	8.606%
25	18.704	2685	2689	2695	rVB	19977	26048	0.82%	0.093%
26	18.775	2696	2701	2706	rVV	18725	24041	0.76%	0.086%
27	19.145	2758	2764	2776	rBV	2153584	2916719	92.29%	10.394%
28	20.974	3070	3075	3089	rBV	1410977	1889545	59.79%	6.733%
29	22.027	3251	3254	3262	rVB2	40006	57636	1.82%	0.205%
30	22.963	3410	3413	3418	rVB3	20118	29182	0.92%	0.104%
31	23.474	3491	3500	3517	rVB2	1414149	3160431	100.00%	11.262%
32	23.651	3521	3530	3539	rBV	912430	2021041	63.95%	7.202%




Sum of corrected areas: 28062315

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120524\
Data File : BN035417.D
Acq On : 04 Dec 2024 10:24
Operator : RC/JU
Sample : PB165173BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

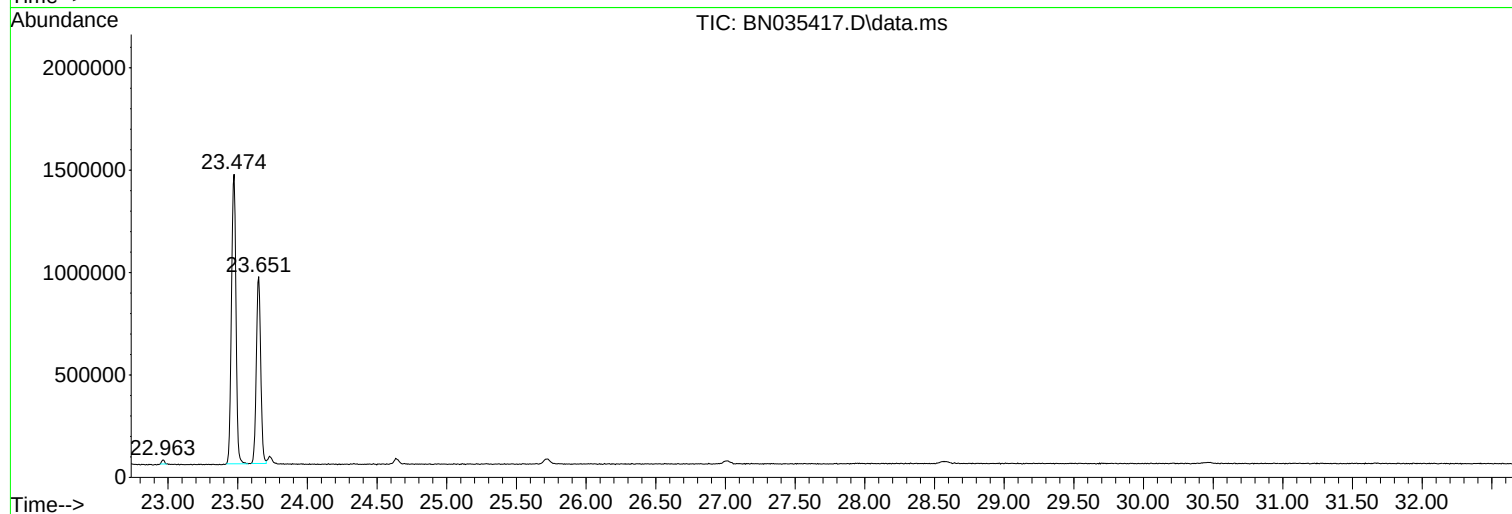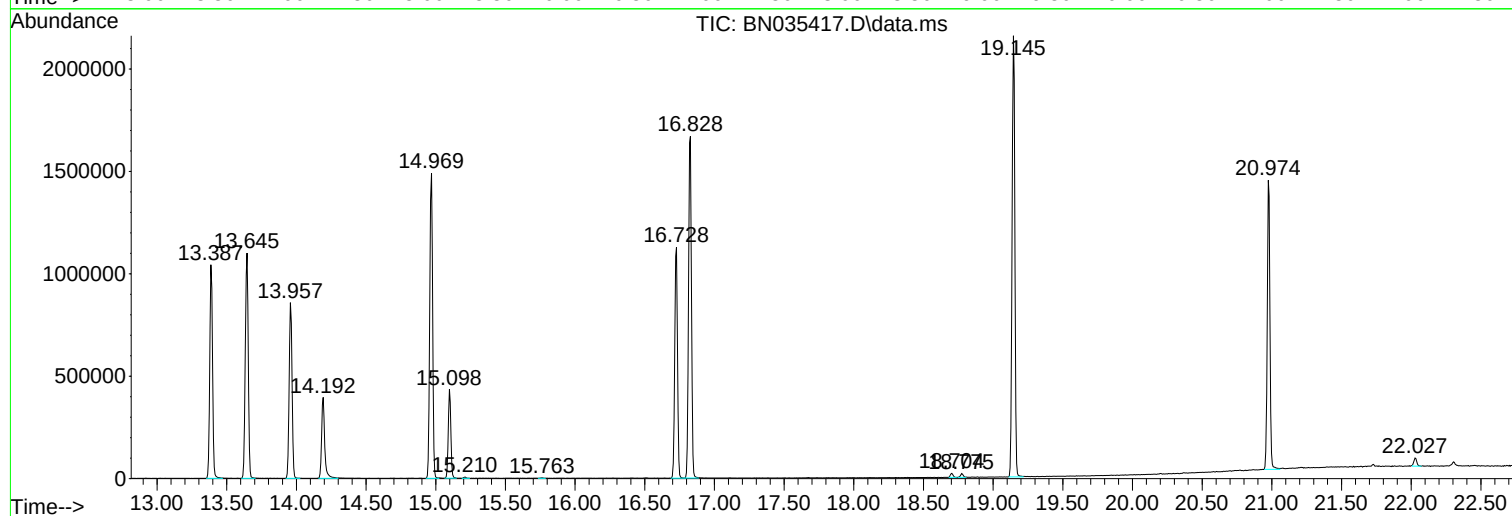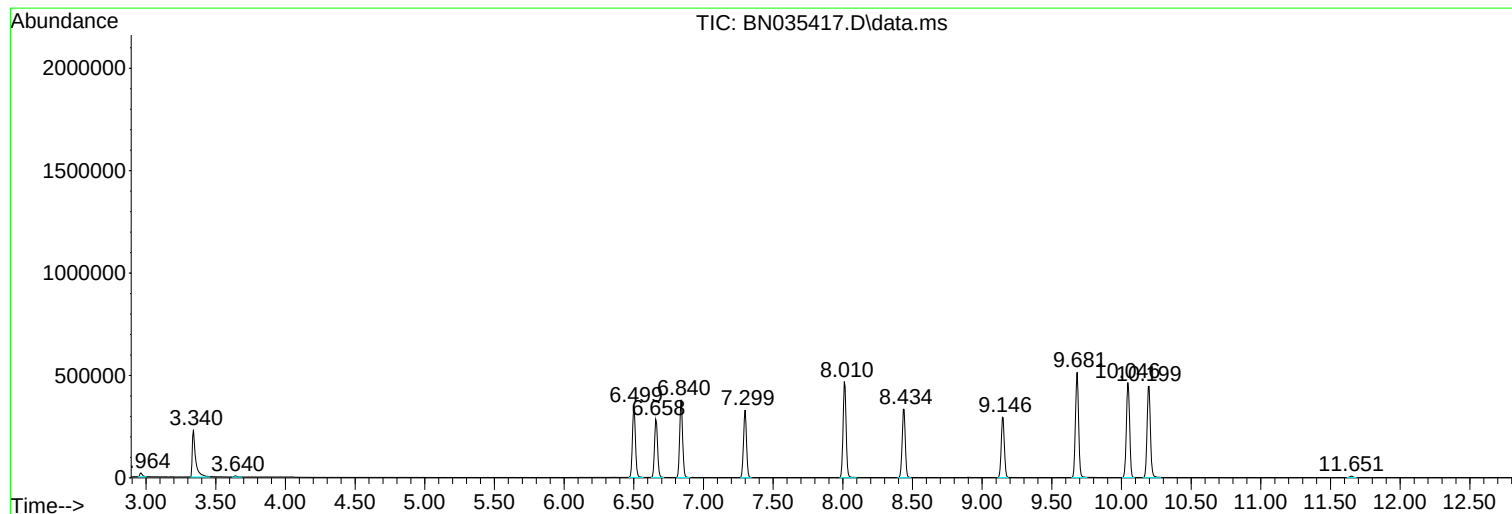

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120524\
Data File : BN035417.D
Acq On : 04 Dec 2024 10:24
Operator : RC/JU
Sample : PB165173BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120524\
Data File : BN035417.D
Acq On : 04 Dec 2024 10:24
Operator : RC/JU
Sample : PB165173BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc