

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120524\
 Data File : BN035421.D
 Acq On : 04 Dec 2024 13:38
 Operator : RC/JU
 Sample : PB165149BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK149

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	9	12	20	rBV	17544	25666	0.88%	0.099%
2	3.340	73	77	93	rBV	210733	345085	11.79%	1.336%
3	3.640	125	128	131	rBV	4356	5308	0.18%	0.021%
4	6.499	608	614	631	rVB	320553	486580	16.62%	1.884%
5	6.658	634	641	653	rBV	255366	385247	13.16%	1.491%
6	6.840	666	672	682	rBV	342439	506329	17.30%	1.960%
7	7.299	744	750	757	rBV	298236	443919	15.17%	1.719%
8	8.011	865	871	883	rBV	425036	648530	22.16%	2.511%
9	8.440	936	944	952	rBV	302967	470310	16.07%	1.821%
10	9.152	1058	1065	1075	rVB	260565	412315	14.09%	1.596%
11	9.681	1148	1155	1166	rBV	457911	718881	24.56%	2.783%
12	10.046	1208	1217	1226	rBV	419314	681503	23.28%	2.638%
13	10.199	1235	1243	1259	rBV	407827	688465	23.52%	2.665%
14	11.652	1485	1490	1496	rBV	6101	10551	0.36%	0.041%
15	13.387	1779	1785	1799	rBV	918924	1283018	43.83%	4.967%
16	13.646	1822	1829	1842	rBV	989914	1458647	49.83%	5.647%
17	13.957	1876	1882	1896	rBV	777196	1104784	37.74%	4.277%
18	14.193	1915	1922	1939	rBV	347882	543115	18.55%	2.103%
19	14.969	2047	2054	2067	rBV	1408287	1897293	64.82%	7.345%
20	15.098	2071	2076	2091	rVV	391047	493852	16.87%	1.912%
21	15.210	2091	2095	2100	rVB3	4061	5282	0.18%	0.020%
22	15.757	2184	2188	2193	rBV4	2440	3599	0.12%	0.014%
23	16.728	2346	2353	2363	rBV	1043977	1425630	48.70%	5.519%
24	16.828	2363	2370	2385	rVB2	1516278	2190053	74.82%	8.479%
25	18.704	2684	2689	2693	rVB2	18157	24112	0.82%	0.093%
26	18.775	2696	2701	2707	rBV	17490	23454	0.80%	0.091%
27	19.145	2758	2764	2776	rBV	1981098	2648678	90.49%	10.254%
28	20.975	3070	3075	3087	rBV2	1289538	1756724	60.02%	6.801%
29	22.033	3251	3255	3261	rVB2	37286	54597	1.87%	0.211%
30	22.304	3298	3301	3308	rVB5	27832	45544	1.56%	0.176%
31	22.963	3409	3413	3422	rVB2	36828	66510	2.27%	0.257%
32	23.469	3490	3499	3514	rBV2	1317795	2927096	100.00%	11.332%
33	23.651	3521	3530	3539	rBV	843955	1845845	63.06%	7.146%
34	23.733	3540	3544	3551	rVB	53931	104168	3.56%	0.403%
35	24.633	3693	3697	3707	rVB4	41612	99457	3.40%	0.385%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120524\
Data File : BN035421.D
Acq On : 04 Dec 2024 13:38
Operator : RC/JU
Sample : PB165149BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK149

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 25830147

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120524\
Data File : BN035421.D
Acq On : 04 Dec 2024 13:38
Operator : RC/JU
Sample : PB165149BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK149

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

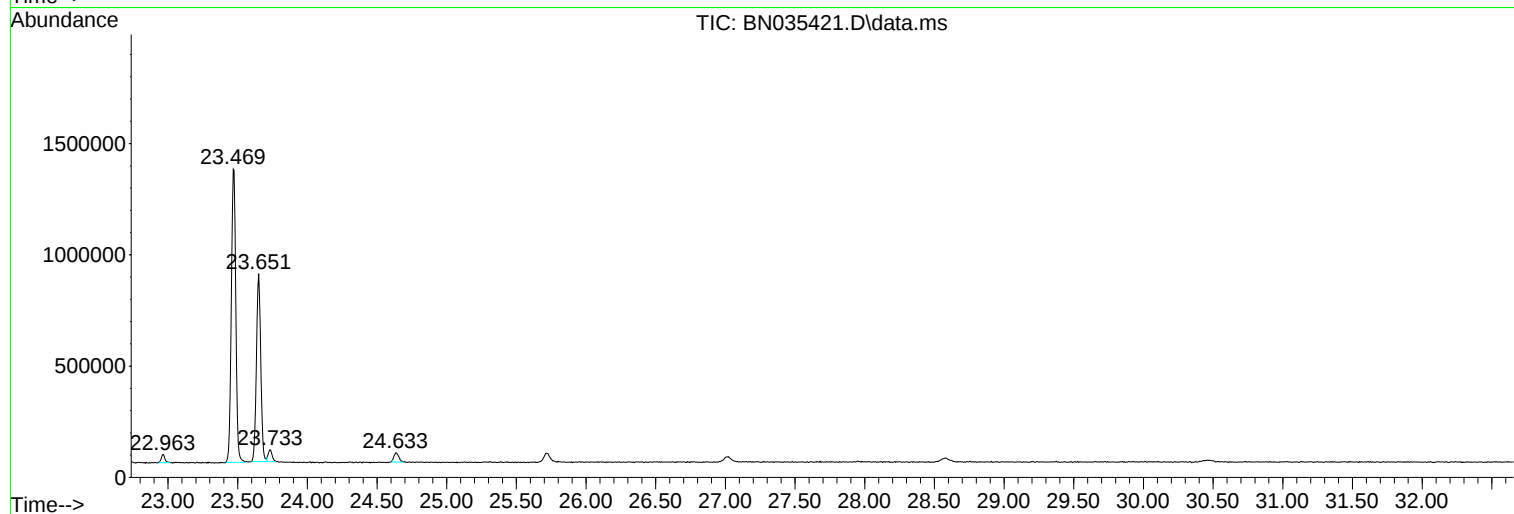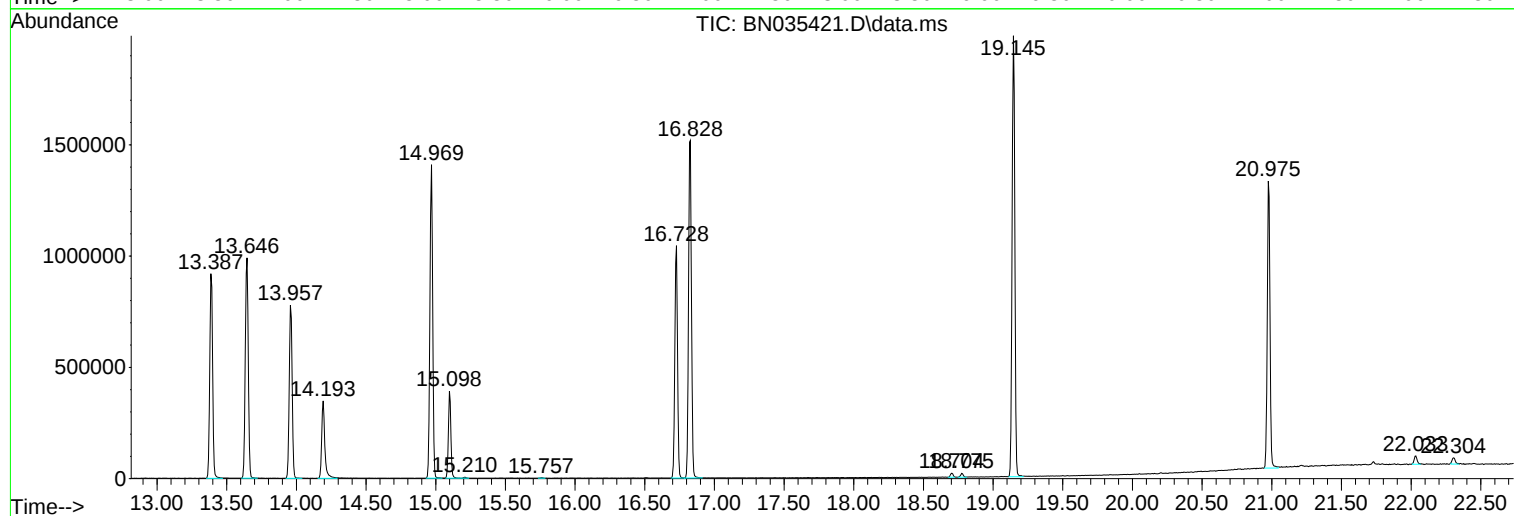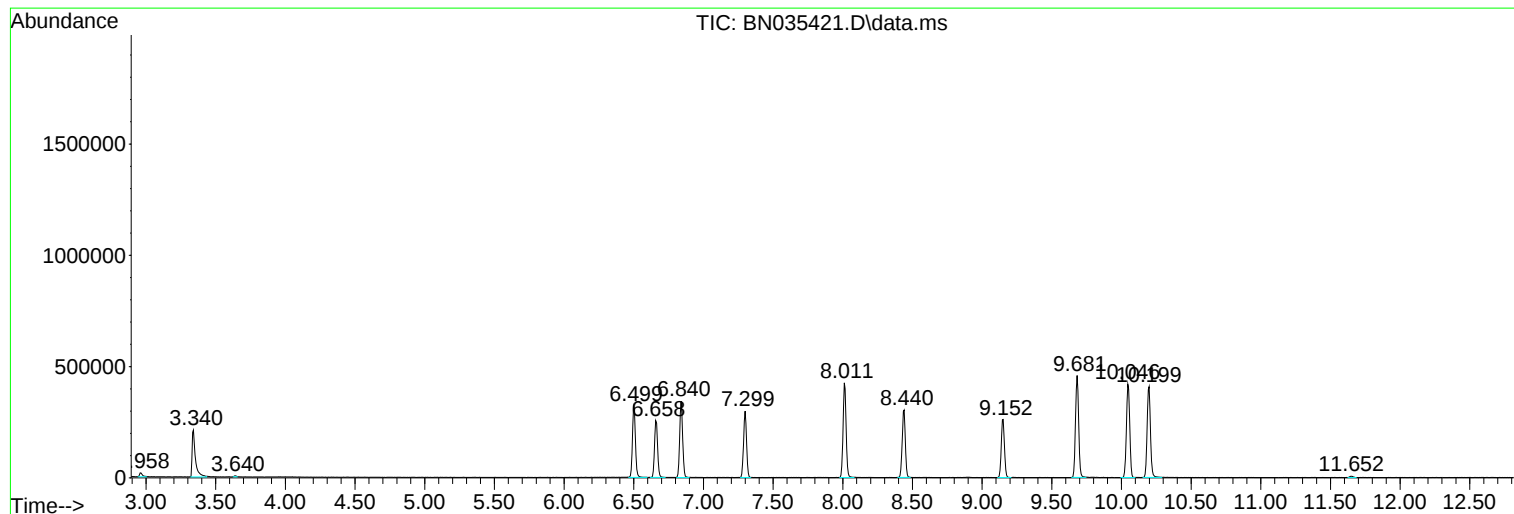

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120524\
Data File : BN035421.D
Acq On : 04 Dec 2024 13:38
Operator : RC/JU
Sample : PB165149BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK149

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120524\
Data File : BN035421.D
Acq On : 04 Dec 2024 13:38
Operator : RC/JU
Sample : PB165149BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK149

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc