

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
 Data File : BN012895.D
 Acq On : 06 Dec 2020 00:25
 Operator : CG/JU
 Sample : L4864-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BB0

Quant Time: Dec 07 01:02:39 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 07 01:01:09 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	876	0.40	ng/ul	0.00
2) Naphthalene-d8	10.16	136	3541	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.06	164	2149	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.82
16) Chrysene-d12	21.04	240	3848	0.40	ng/ul	0.00
20) Perylene-d12	23.14	264	4393	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.76	152	2041	0.39	ng/ul	0.00
14) Fluoranthene-d10	18.86	212	4616	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.23	202	1098	0.060	ng/ul#	1
23) Benzo(a)pyrene	23.01	252	2416	0.128	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
Data File : BN012895.D
Acq On : 06 Dec 2020 00:25
Operator : CG/JU
Sample : L4864-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BB0

Quant Time: Dec 07 01:02:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 01:01:09 2020
Response via : Initial Calibration

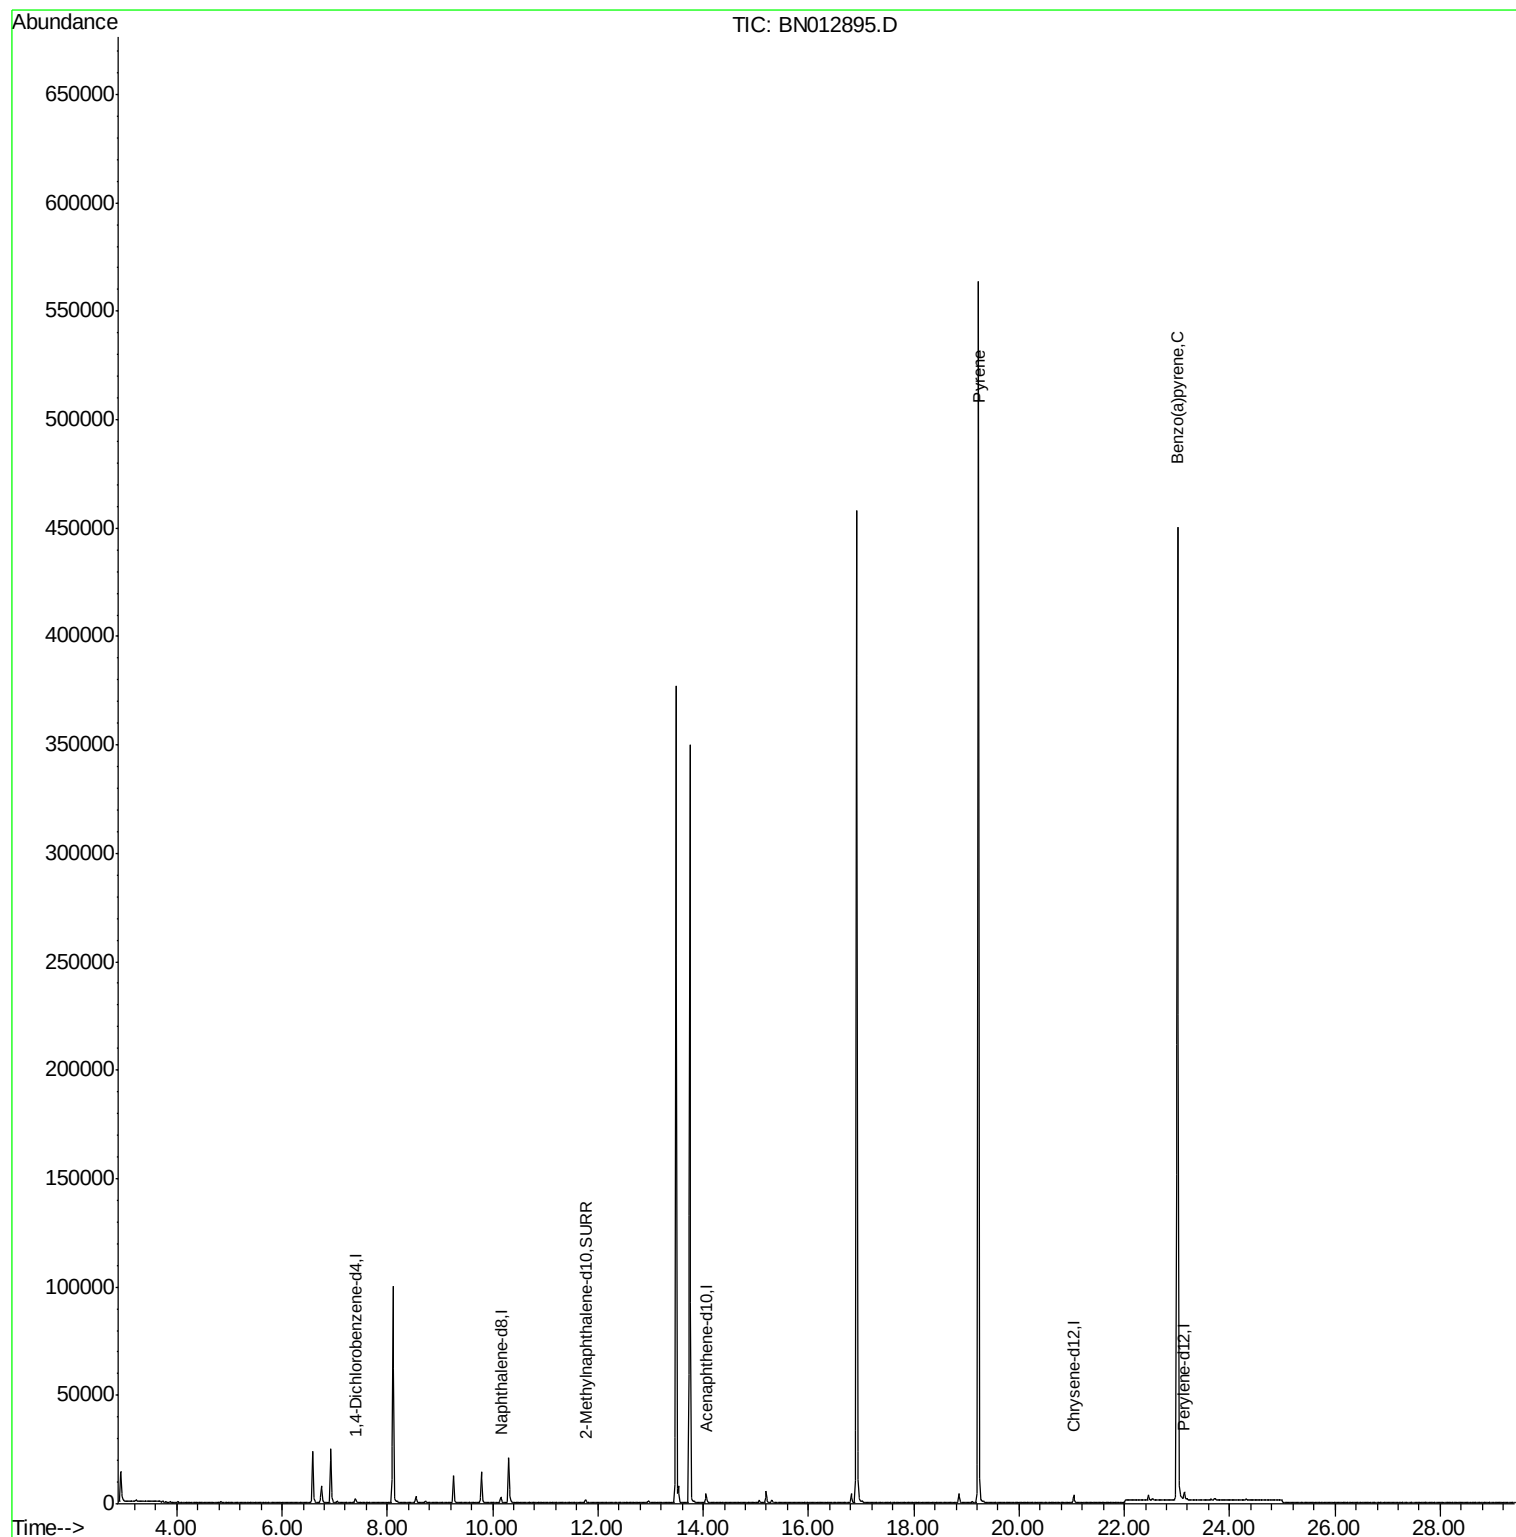

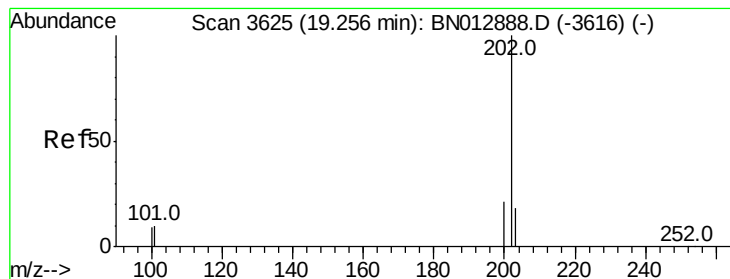

#17

Pvrene

Concen: 0.060 ng/ul

RT: 19.23 min Scan# 3619

Delta R.T. -0.03 min

Lab File: BN012895.D

Acq: 06 Dec 2020 00:25

Instrument :

BNA_N

ClientSampleId :

C0BB0


Tot Ion:202 Resp: 1098

Ion Ratio Lower Upper

202 100

101 205.5 9.1 13.7#




100 1427.1 7.5 11.3#

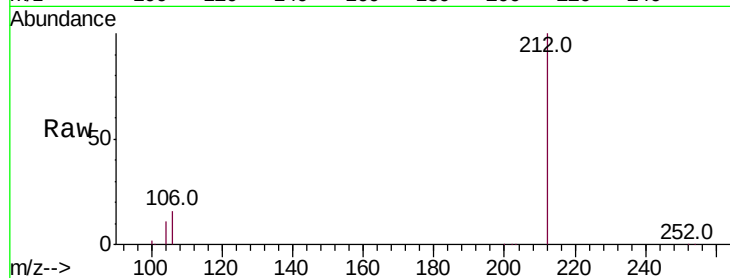

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

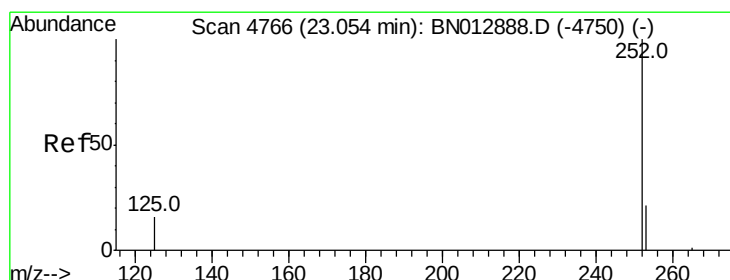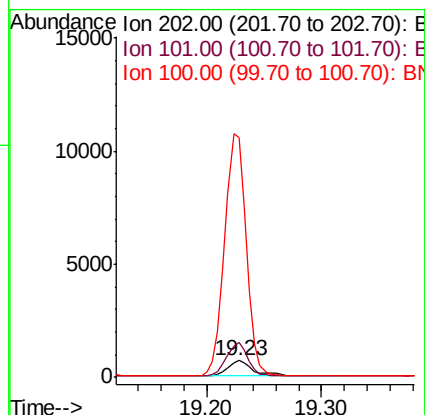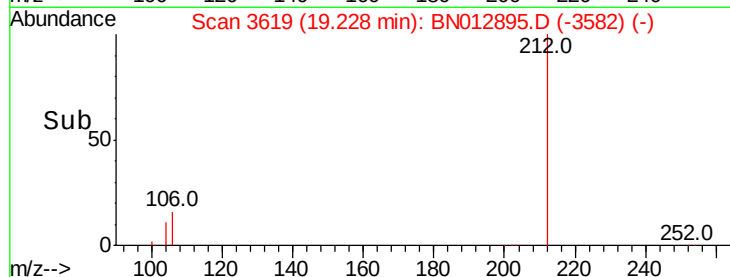

#23

Benzo(a)pyrene

Concen: 0.128 ng/ul

RT: 23.01 min Scan# 4751

Delta R.T. -0.04 min

Lab File: BN012895.D

Acq: 06 Dec 2020 00:25


Tgt Ion:252 Resp: 2416

Ion Ratio Lower Upper

252 100

253 45.1 26.5 39.7#

125 36.2 14.2 21.2#

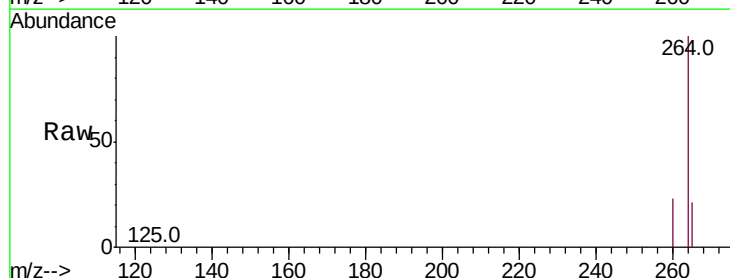

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

