

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
 Data File : BN012903.D
 Acq On : 06 Dec 2020 05:53
 Operator : CG/JU
 Sample : L4864-12
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BD8

Quant Time: Dec 07 02:18:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 07 02:16:16 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	814	0.40	ng/ul	0.00
2) Naphthalene-d8	10.15	136	3206	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.06	164	1934	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.82
16) Chrysene-d12	21.04	240	3708	0.40	ng/ul	0.00
20) Perylene-d12	23.14	264	4131	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.76	152	1741	0.37	ng/ul	0.00
14) Fluoranthene-d10	18.86	212	4289	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.23	202	886	0.051	ng/ul#	1
23) Benzo(a)pyrene	23.01	252	2181	0.123	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
Data File : BN012903.D
Acq On : 06 Dec 2020 05:53
Operator : CG/JU
Sample : L4864-12
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BD8

Quant Time: Dec 07 02:18:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 02:16:16 2020
Response via : Initial Calibration

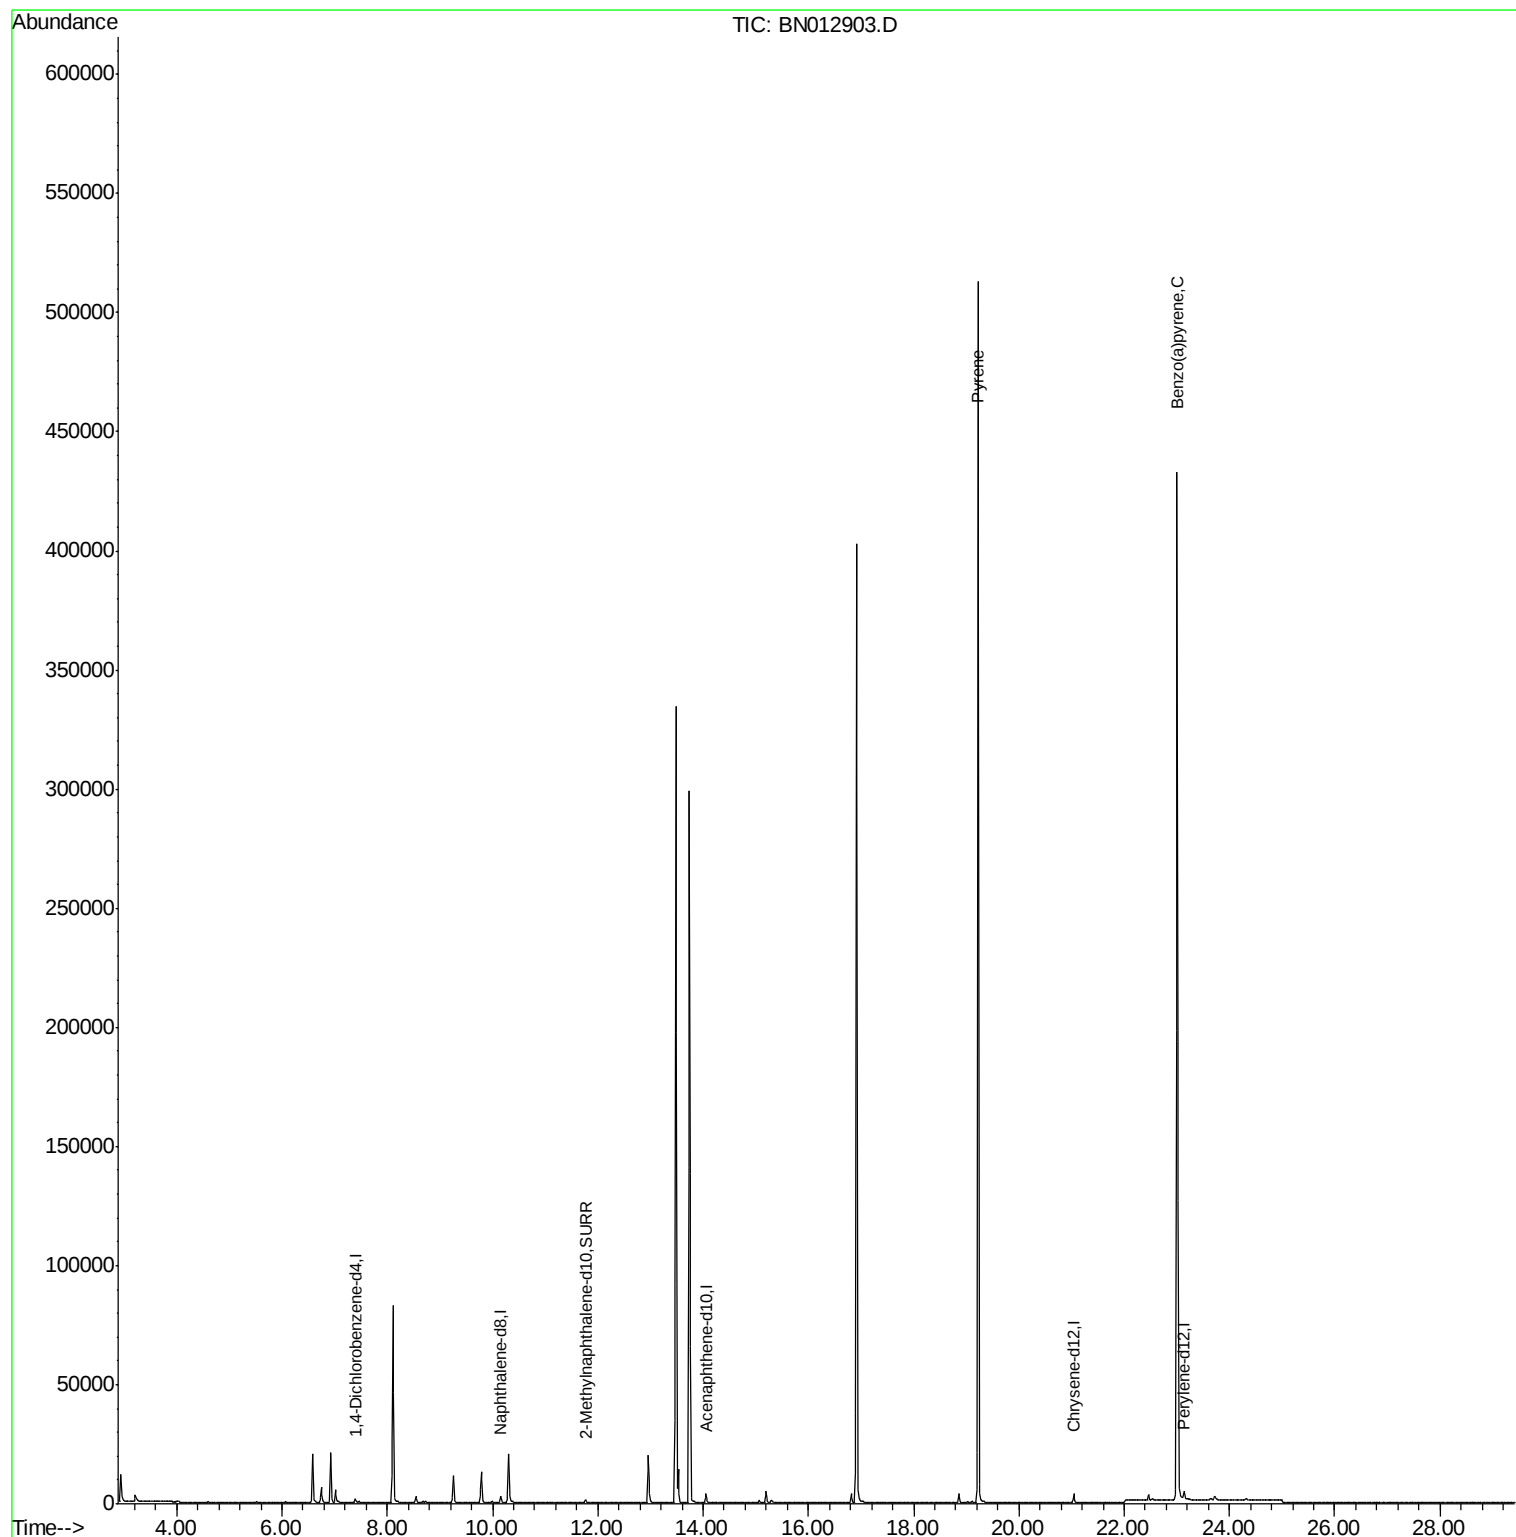


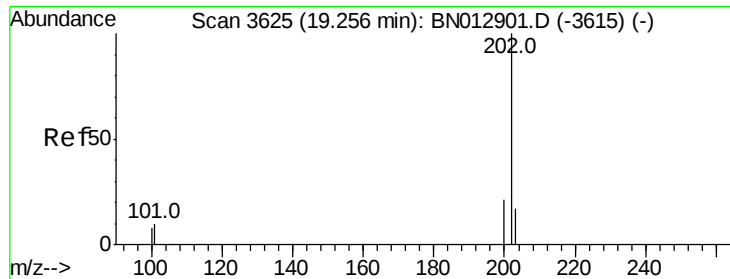




#17
Pvrene
Concen: 0.051 ng/ul
RT: 19.23 min Scan# 3619
Delta R.T. -0.03 min
Lab File: BN012903.D
Acq: 06 Dec 2020 05:53

Instrument :
BNA_N
ClientSampleId :
C0BD8

Tot Ion:202 Resp: 886
Ion Ratio Lower Upper
202 100
101 201.7 9.1 13.7#
100 1391.2 7.5 11.3#

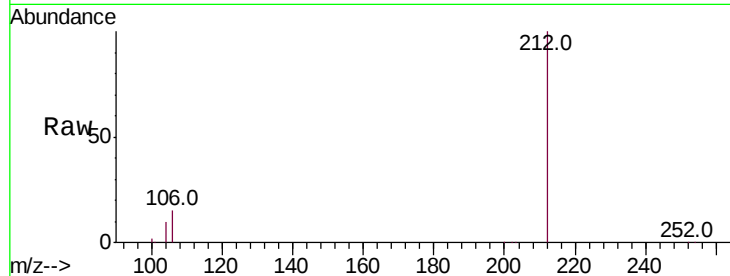


Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

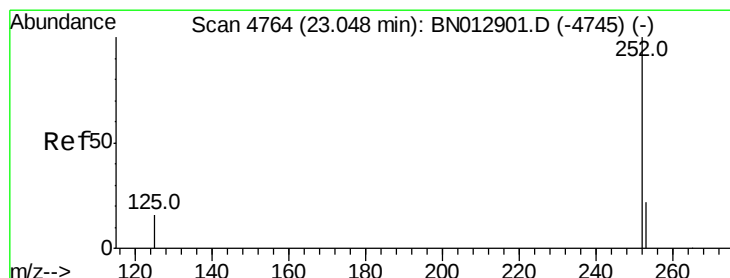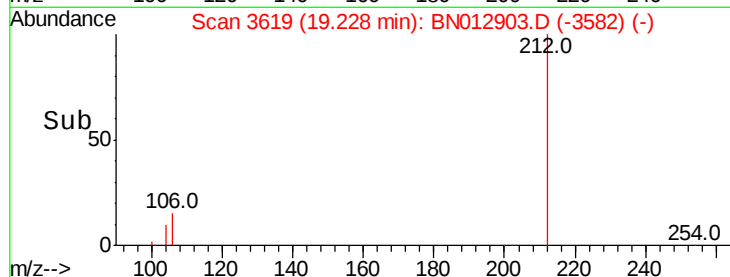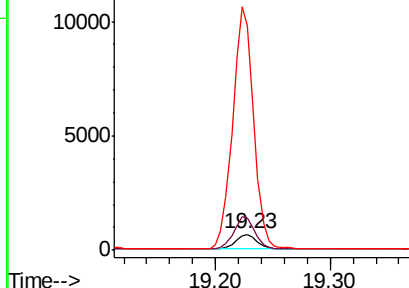

#23
Benzo(a)pyrene
Concen: 0.123 ng/ul
RT: 23.01 min Scan# 4751
Delta R.T. -0.04 min
Lab File: BN012903.D
Acq: 06 Dec 2020 05:53

Tgt Ion:252 Resp: 2181
Ion Ratio Lower Upper
252 100
253 43.3 26.5 39.7#
125 36.1 14.2 21.2#

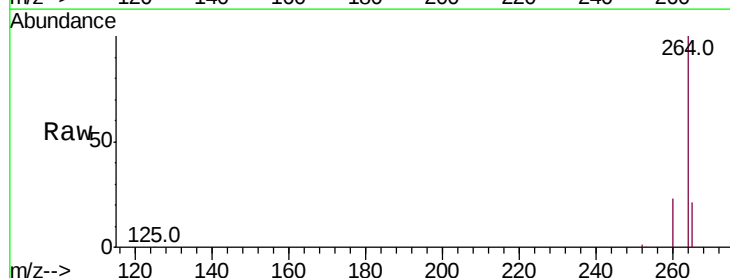

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

