

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
 Data File : BN012908.D
 Acq On : 06 Dec 2020 08:53
 Operator : CG/JU
 Sample : L4859-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B25

Quant Time: Dec 07 02:18:35 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 07 02:16:16 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1295	0.40	ng/ul	0.00
2) Naphthalene-d8	10.15	136	5191	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.06	164	3060	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.81	188	6696	0.40	ng/ul	0.00
16) Chrysene-d12	21.03	240	5919	0.40	ng/ul	0.00
20) Perylene-d12	23.14	264	6245	0.40	ng/ul	0.00

System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.76	152	1180	0.15	ng/ul	0.00
14) Fluoranthene-d10	18.86	212	2930	0.16	ng/ul	0.00


Target Compounds				Ovalue		
11) Pentachlorophenol	16.48	266	53	0.027	ng/ul	87
12) Phenanthrene	16.85	178	4122	0.184	ng/ul	99
13) Anthracene	16.95	178	774	0.041	ng/ul#	90
15) Fluoranthene	18.89	202	12079	0.453	ng/ul	97
17) Pyrene	19.25	202	12015	0.430	ng/ul	98
18) Benzo(a)anthracene	21.02	228	5486	0.224	ng/ul	98
19) Chrysene	21.07	228	6550	0.242	ng/ul	98
21) Benzo(b)fluoranthene	22.52	252	12988	0.450	ng/ul	96
22) Benzo(k)fluoranthene	22.52	252	12966	0.406	ng/ul	97
23) Benzo(a)pyrene	22.96	252	2587	0.097	ng/ul	97
24) Indeno(1,2,3-cd)pyrene	25.20	276	4381	0.124	ng/ul#	95
25) Dibenzo(a,h)anthracene	25.20	278	1096	0.039	ng/ul#	64
26) Benzo(g,h,i)perylene	25.82	276	4035	0.127	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
Data File : BN012908.D
Acq On : 06 Dec 2020 08:53
Operator : CG/JU
Sample : L4859-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B25

Quant Time: Dec 07 02:18:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 02:16:16 2020
Response via : Initial Calibration




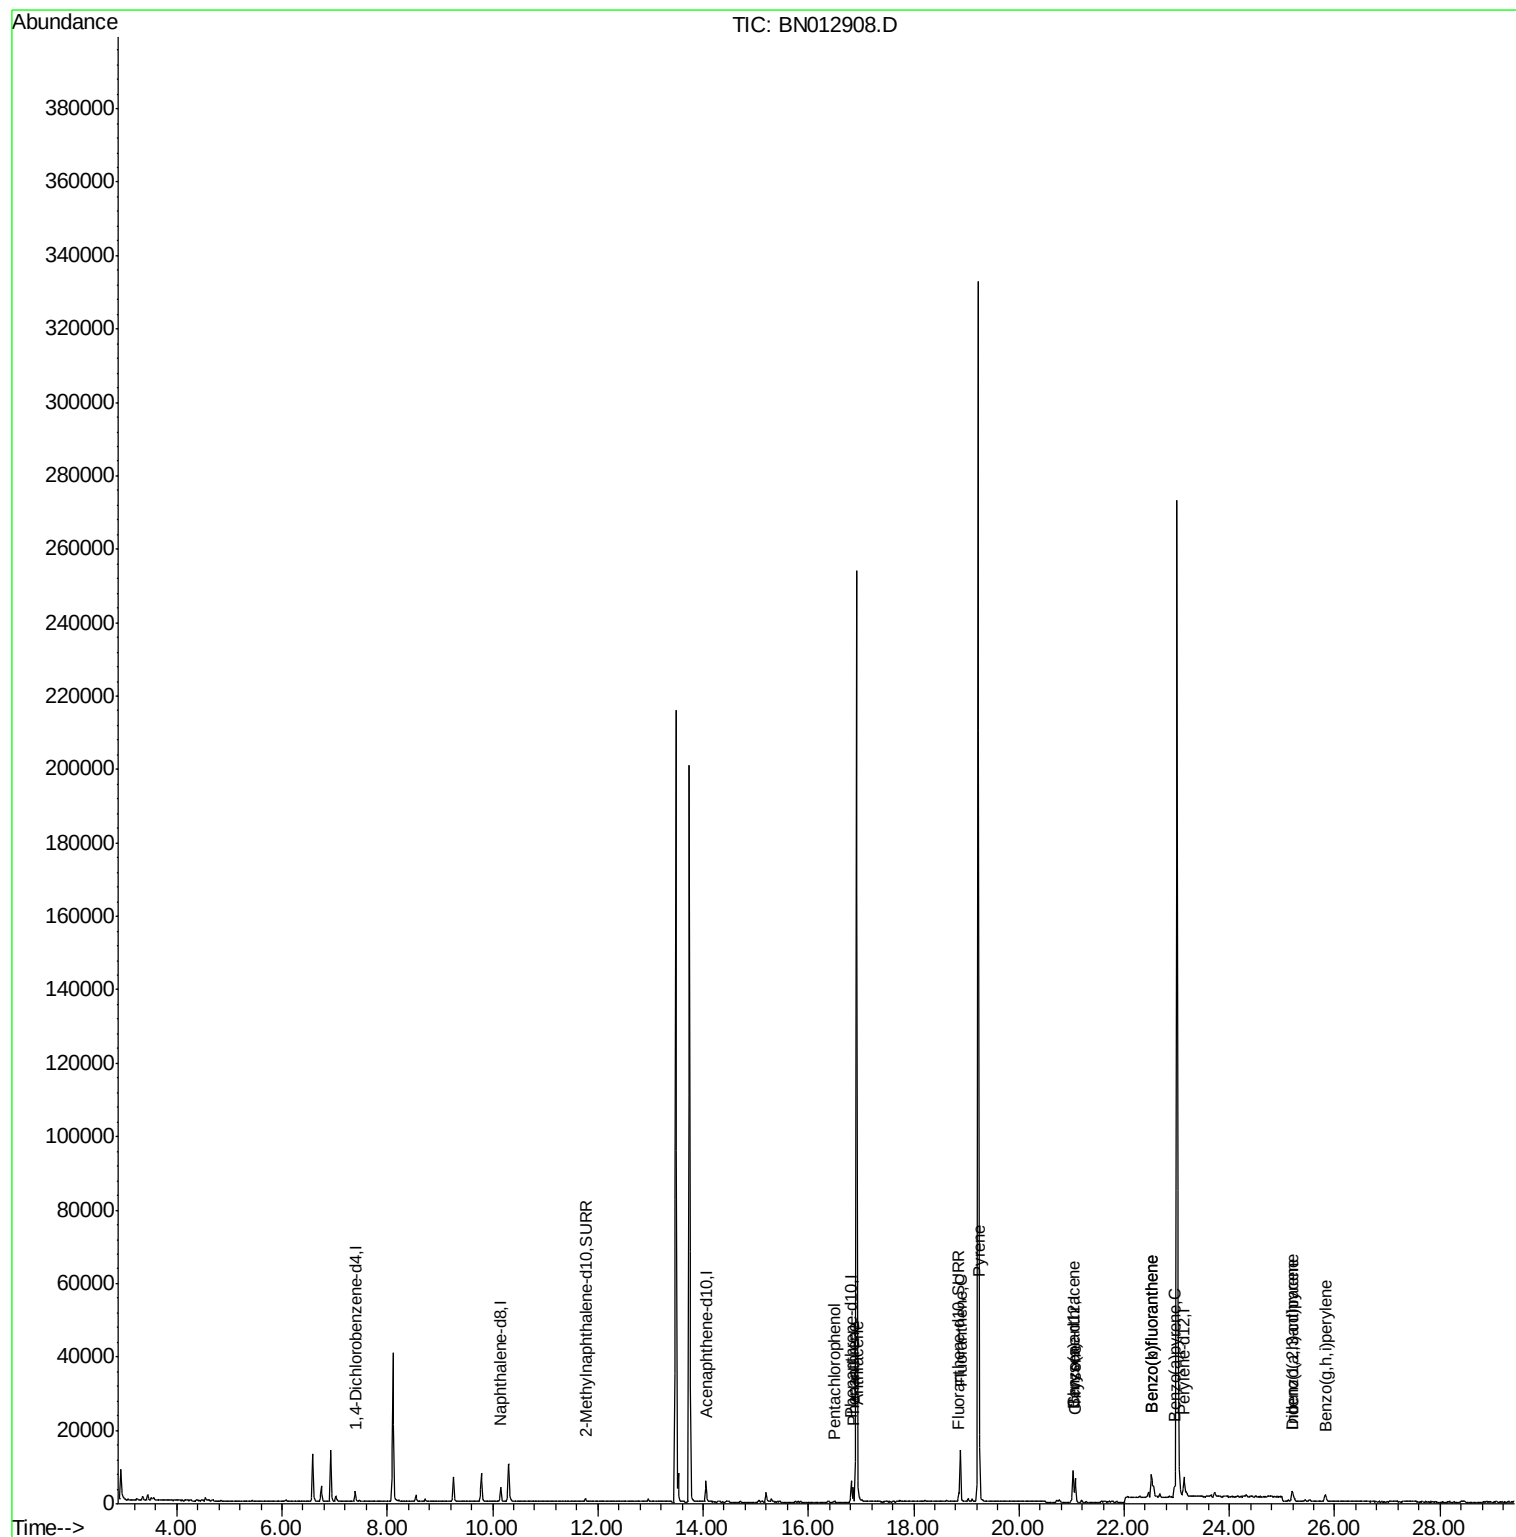


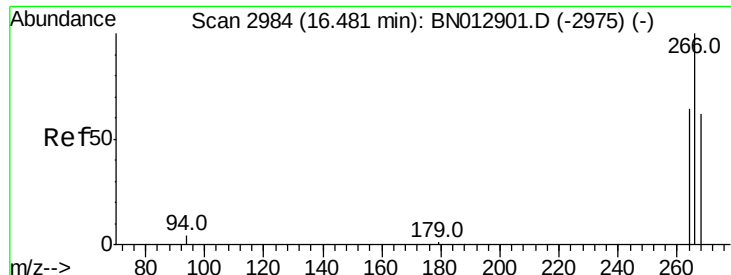

#11
 Pentachlorophenol
 Concen: 0.027 ng/ul
 RT: 16.48 min Scan# 2983
 Delta R.T. -0.00 min
 Lab File: BN012908.D
 Acq: 06 Dec 2020 08:53




Instrument :
 BNA_N
 ClientSampleId :
 C0B25


Tot Ion:266 Resp: 53
 Ion Ratio Lower Upper
 266 100
 264 73.6 51.5 77.3
 268 81.1 56.0 84.0

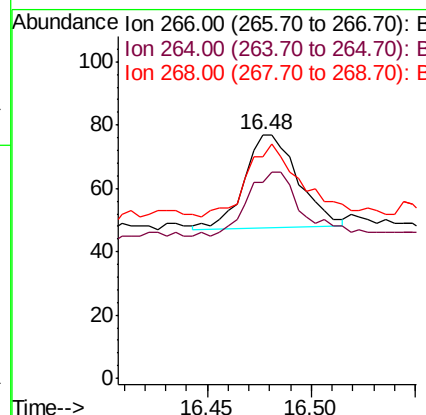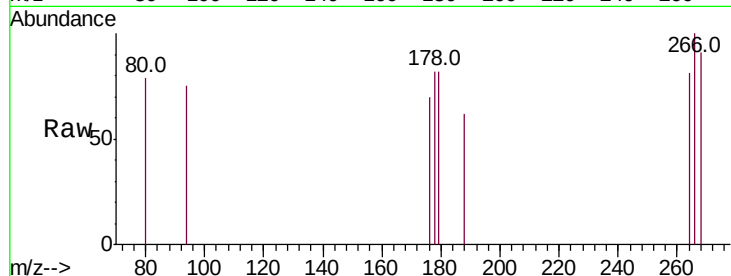

#12
 Phenanthrene
 Concen: 0.184 ng/ul
 RT: 16.85 min Scan# 3072
 Delta R.T. -0.00 min
 Lab File: BN012908.D
 Acq: 06 Dec 2020 08:53

Tgt Ion:178 Resp: 4122
 Ion Ratio Lower Upper
 178 100
 179 17.3 13.6 20.4
 176 20.3 16.4 24.6

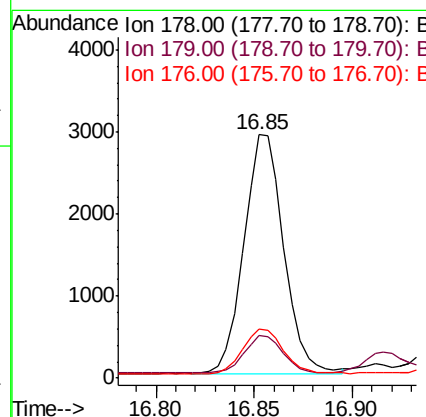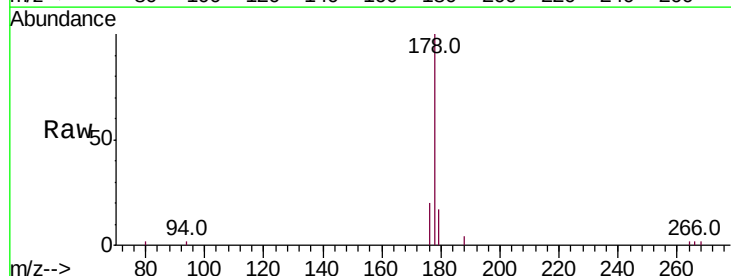



#13

Anthracene

Concen: 0.041 ng/ul

RT: 16.95 min Scan# 3094

Delta R.T. -0.01 min

Lab File: BN012908.D

Acq: 06 Dec 2020 08:53

Instrument :

BNA_N

ClientSampleId :

C0B25


Tot Ion:178 Resp: 774

Ion Ratio Lower Upper

178 100

179 25.0 14.6 21.8#




176 24.0 17.1 25.7

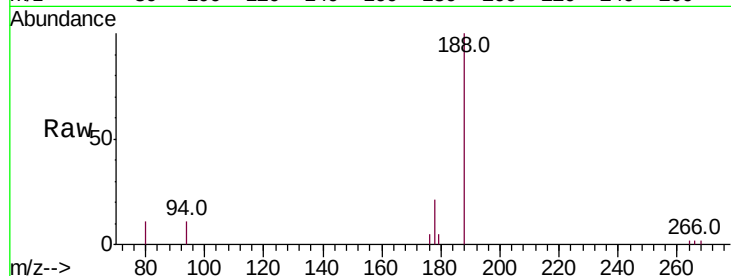

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

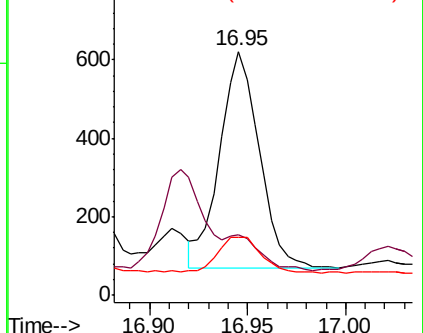

#15

Fluoranthene

Concen: 0.453 ng/ul

RT: 18.89 min Scan# 3546

Delta R.T. 0.00 min

Lab File: BN012908.D

Acq: 06 Dec 2020 08:53


Tgt Ion:202 Resp: 12079

Ion Ratio Lower Upper

202 100

101 9.7 0.0 30.6



100 7.2 0.0 28.7




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B



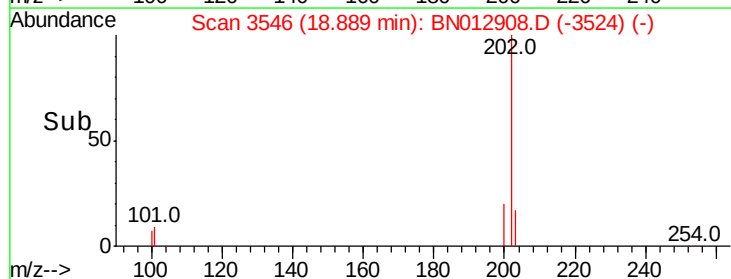
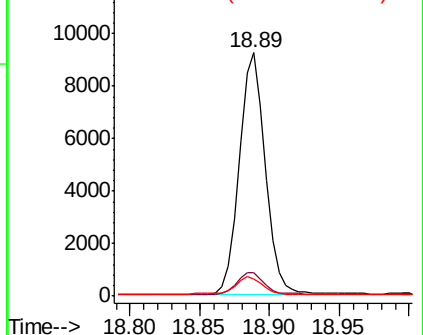


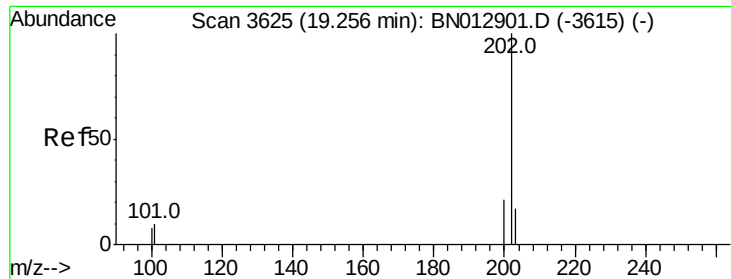

#17
Pvrene
Concen: 0.430 ng/ul
RT: 19.25 min Scan# 3624
Delta R.T. -0.00 min
Lab File: BN012908.D
Acq: 06 Dec 2020 08:53




Instrument :
BNA_N
ClientSampleId :
C0B25


Tot Ion:202 Resp: 12015
Ion Ratio Lower Upper
202 100
101 11.9 9.1 13.7
100 10.6 7.5 11.3

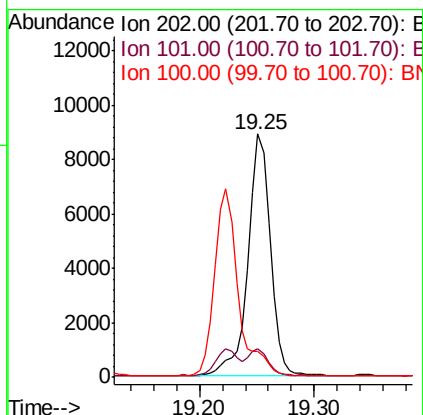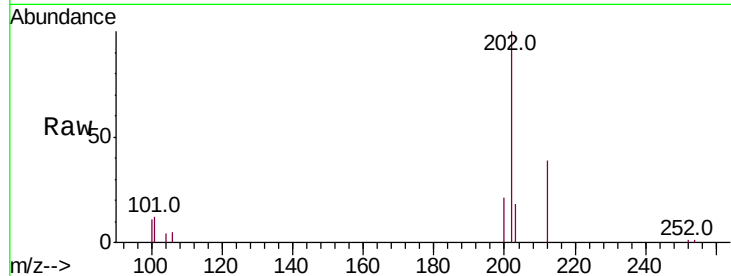

#18
Benzo(a)anthracene
Concen: 0.224 ng/ul
RT: 21.02 min Scan# 4070
Delta R.T. -0.00 min
Lab File: BN012908.D
Acq: 06 Dec 2020 08:53

Tgt Ion:228 Resp: 5486
Ion Ratio Lower Upper
228 100
229 21.6 16.3 24.5
226 28.6 23.4 35.2

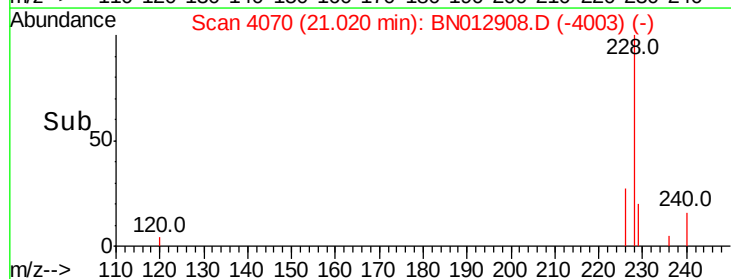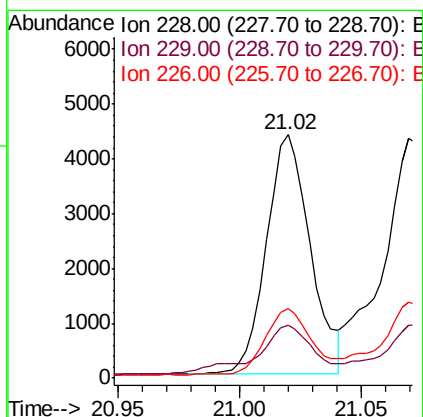

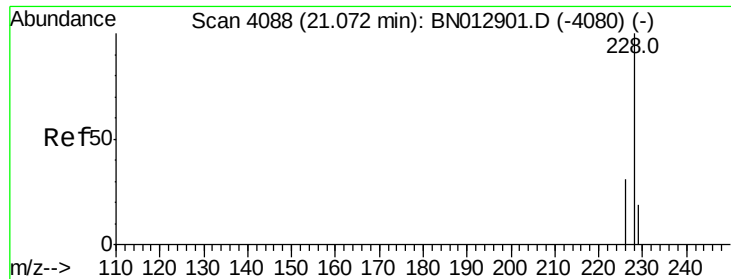

#19

Chrysene

Concen: 0.242 ng/ul

RT: 21.07 min Scan# 4087

Delta R.T. -0.00 min

Lab File: BN012908.D

Acq: 06 Dec 2020 08:53

Instrument :

BNA_N

ClientSampleId :

C0B25


Tot Ion:228 Resp: 6550

Ion Ratio Lower Upper

228 100

226 31.6 25.0 37.6




229 22.3 16.4 24.6



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

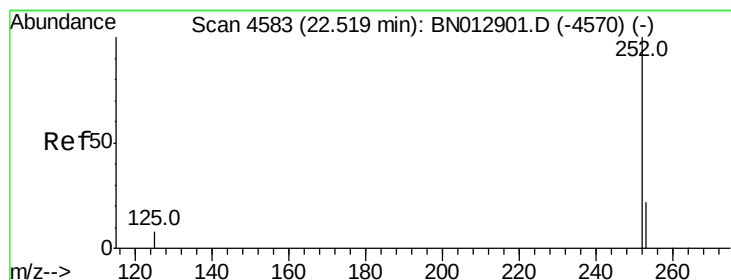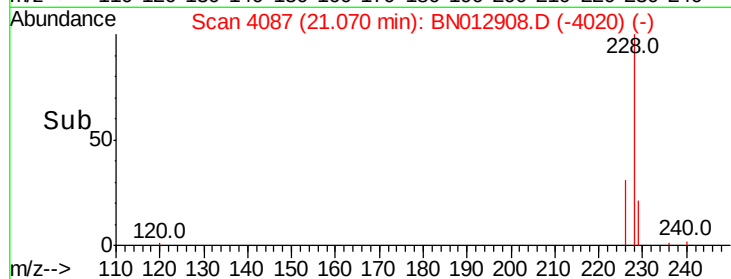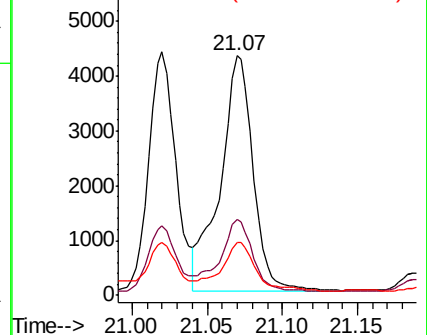

#21

Benzo(b)fluoranthene

Concen: 0.450 ng/ul

RT: 22.52 min Scan# 4583

Delta R.T. 0.00 min

Lab File: BN012908.D

Acq: 06 Dec 2020 08:53


Tgt Ion:252 Resp: 12988

Ion Ratio Lower Upper

252 100

253 28.3 0.0 59.6



125 16.1 0.0 26.0

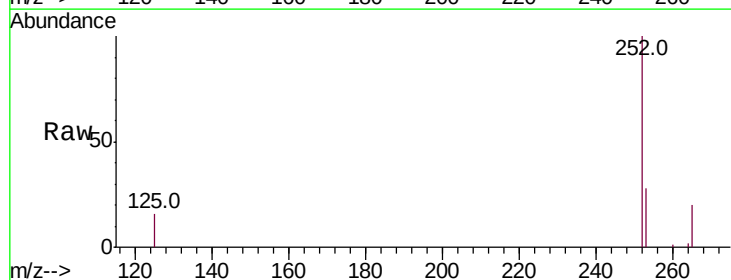


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

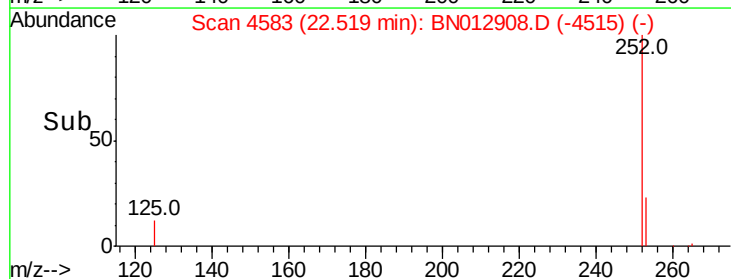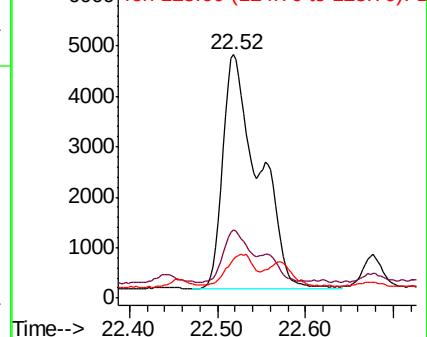

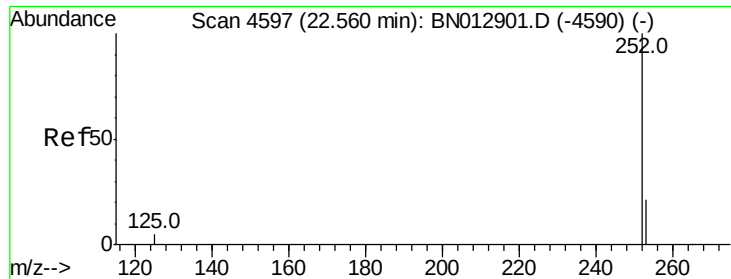

#22

Benzo(k)fluoranthene

Concen: 0.406 ng/ul

RT: 22.52 min Scan# 4583

Delta R.T. -0.04 min

Lab File: BN012908.D

Acq: 06 Dec 2020 08:53

Instrument :

BNA_N

ClientSampleId :

C0B25


Tot Ion:252 Resp: 12966

Ion Ratio Lower Upper




252 100

253 28.3 23.4 35.2

125 16.1 11.1 16.7

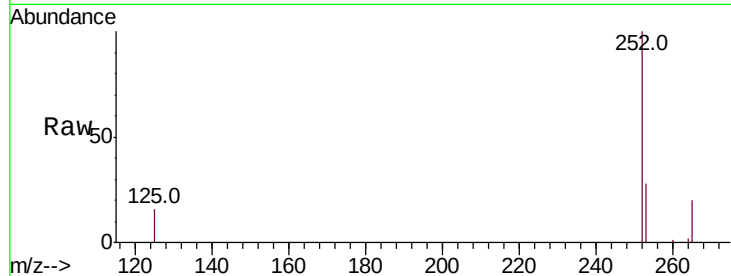

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

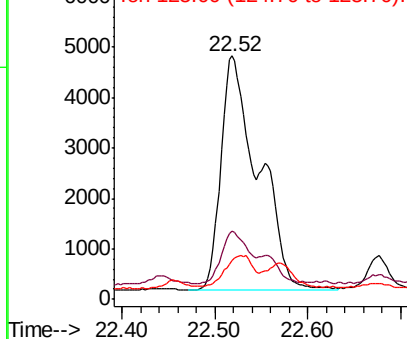

#23

Benzo(a)pyrene

Concen: 0.097 ng/ul

RT: 22.96 min Scan# 4733

Delta R.T. -0.09 min

Lab File: BN012908.D

Acq: 06 Dec 2020 08:53


Tgt Ion:252 Resp: 2587

Ion Ratio Lower Upper



252 100


253 31.7 26.5 39.7

125 19.5 14.2 21.2



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

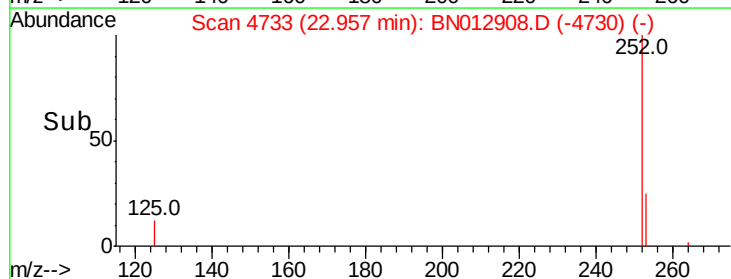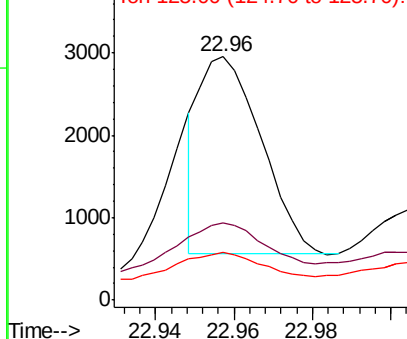



#24

Indeno(1,2,3-cd)pyrene

Concen: 0.124 ng/ul

RT: 25.20 min Scan# 5490

Delta R.T. -0.00 min

Lab File: BN012908.D

Acq: 06 Dec 2020 08:53

Instrument :

BNA_N

ClientSampleId :

C0B25


Tot Ion:276 Resp: 4381

Ion Ratio Lower Upper

276 100

138 22.3 16.2 24.2




227 0.1 0.0 0.0#

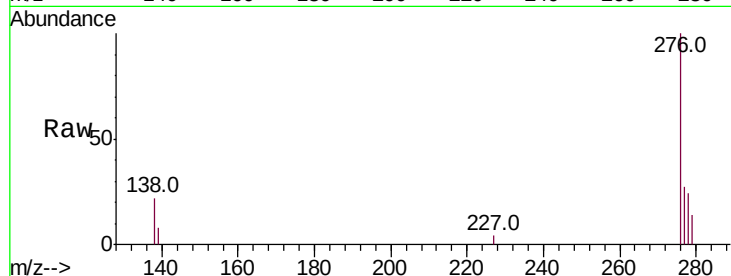

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E

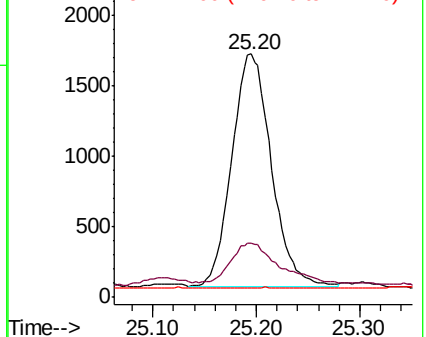

#25

Dibenzo(a,h)anthracene

Concen: 0.039 ng/ul

RT: 25.20 min Scan# 5492

Delta R.T. -0.01 min

Lab File: BN012908.D

Acq: 06 Dec 2020 08:53


Tgt Ion:278 Resp: 1096

Ion Ratio Lower Upper

278 100

139 33.4 14.5 21.7#



279 54.1 26.3 39.5#




Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

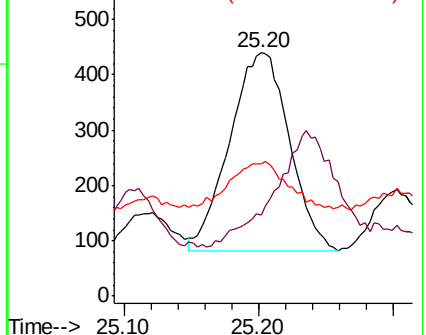



#26

Benzo(a,h,i)perylene

Concen: 0.127 ng/ul

RT: 25.82 min Scan# 5677

Delta R.T. -0.01 min

Lab File: BN012908.D

Acq: 06 Dec 2020 08:53

Instrument :

BNA_N

ClientSampleId :

C0B25


Tot Ion:276 Resp: 4035

Ion Ratio Lower Upper

276 100

138 23.2 16.3 24.5

277 27.8 21.8 32.6

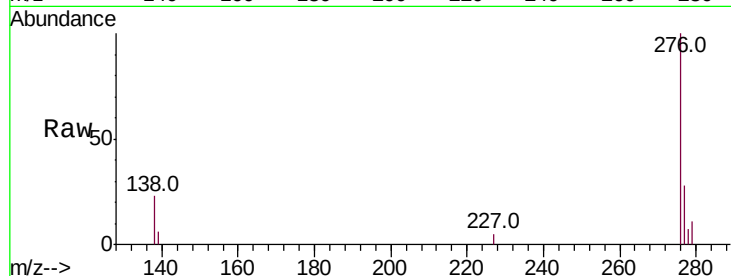

Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

