

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
 Data File : BN012910.D
 Acq On : 06 Dec 2020 10:05
 Operator : CG/JU
 Sample : L4859-09
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BE2

Quant Time: Dec 07 02:18:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 07 02:16:16 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1335	0.40	ng/ul	0.00
2) Naphthalene-d8	10.16	136	5463	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.05	164	3324	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.82
16) Chrysene-d12	21.04	240	6466	0.40	ng/ul	0.00
20) Perylene-d12	23.13	264	6859	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.76	152	2570	0.32	ng/ul	0.00
14) Fluoranthene-d10	18.85	212	6219	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.23	202	1494	0.049	ng/ul#	1
23) Benzo(a)pyrene	23.01	252	3094	0.105	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
Data File : BN012910.D
Acq On : 06 Dec 2020 10:05
Operator : CG/JU
Sample : L4859-09
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BE2

Quant Time: Dec 07 02:18:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 02:16:16 2020
Response via : Initial Calibration




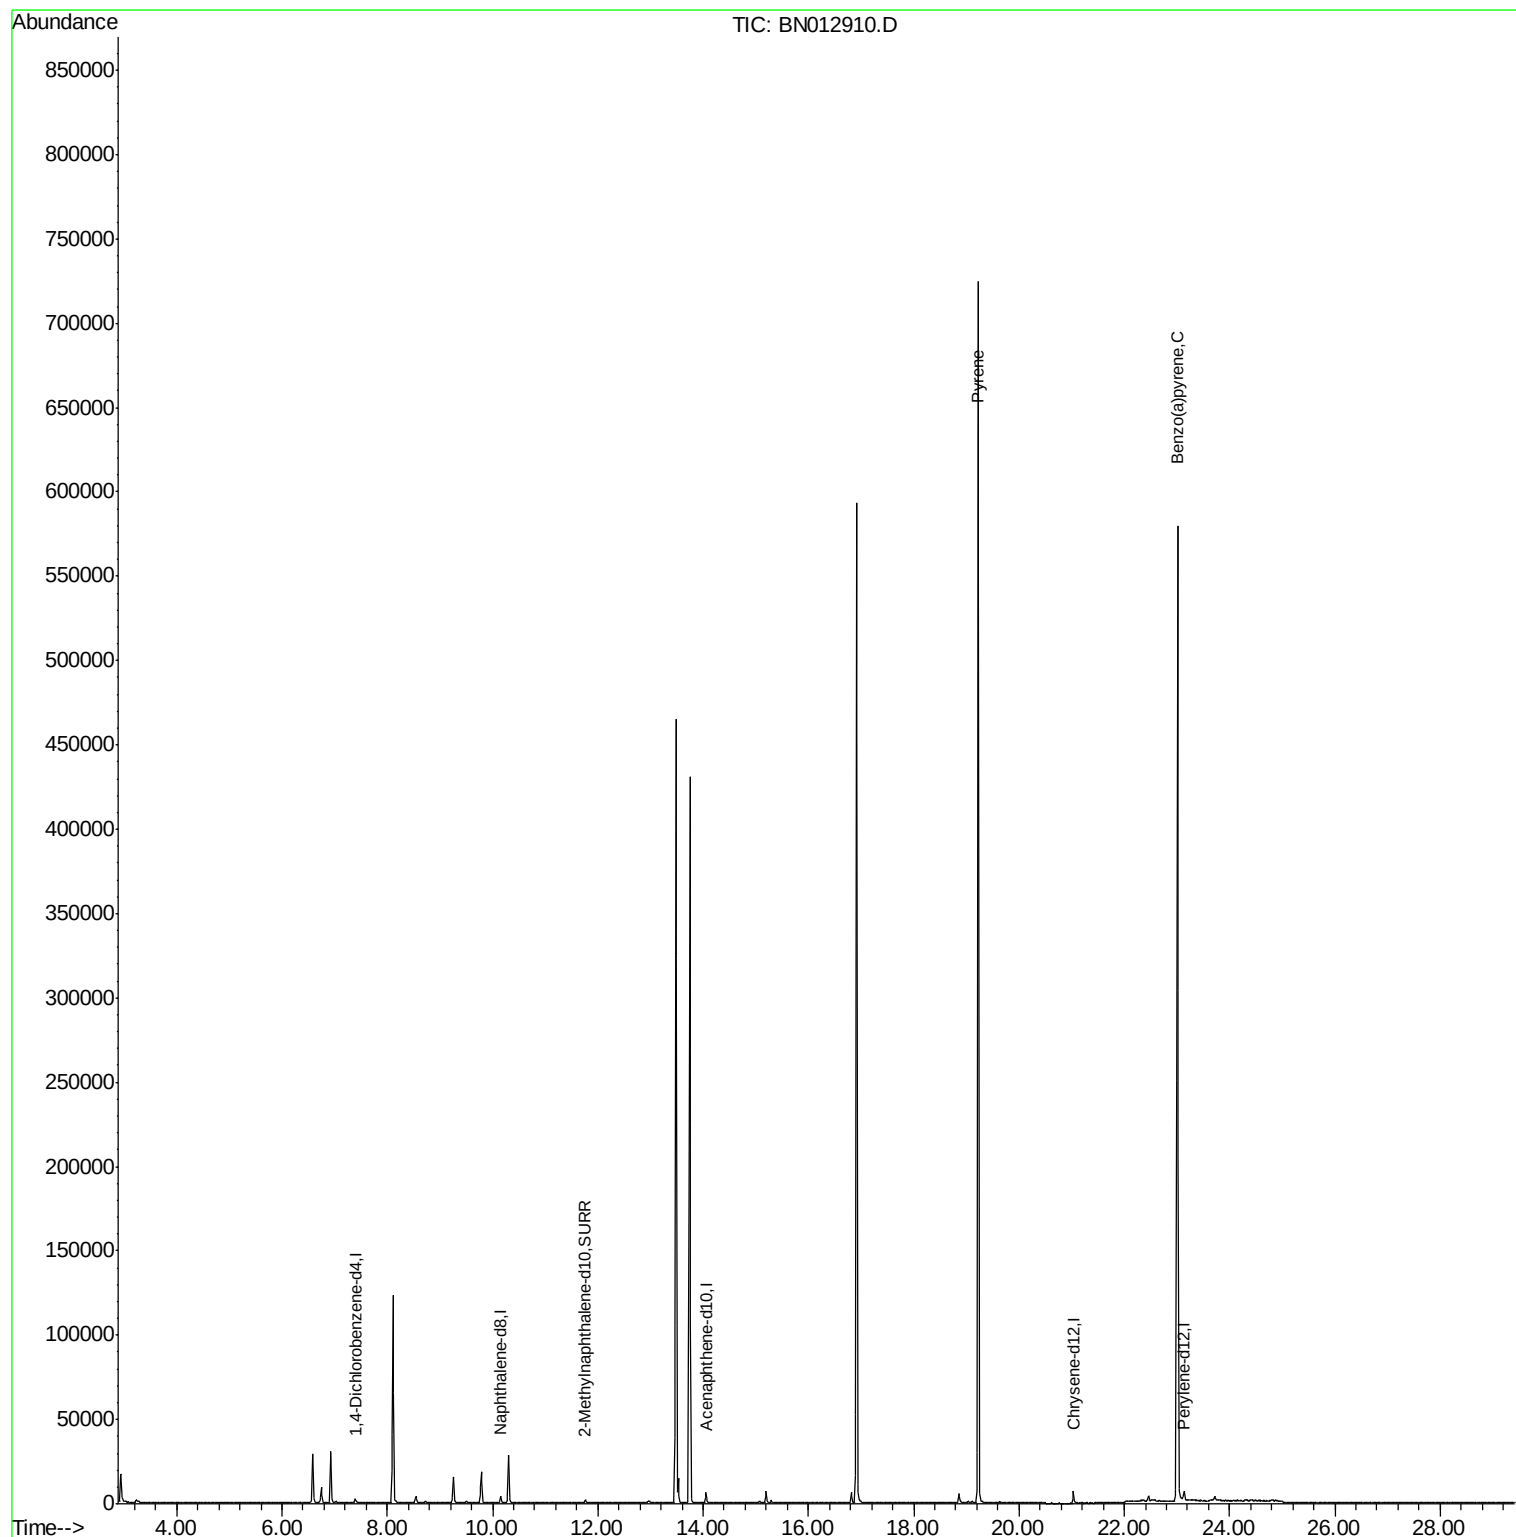


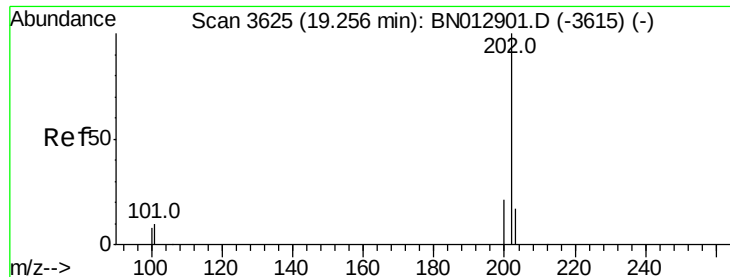

#17
Pvrene
Concen: 0.049 ng/ul
RT: 19.23 min Scan# 3619
Delta R.T. -0.03 min
Lab File: BN012910.D
Acq: 06 Dec 2020 10:05

Instrument :
BNA_N
ClientSampleId :
C0BE2

Tot Ion:202 Resp: 1494
Ion Ratio Lower Upper
202 100
101 189.9 9.1 13.7#
100 1360.2 7.5 11.3#

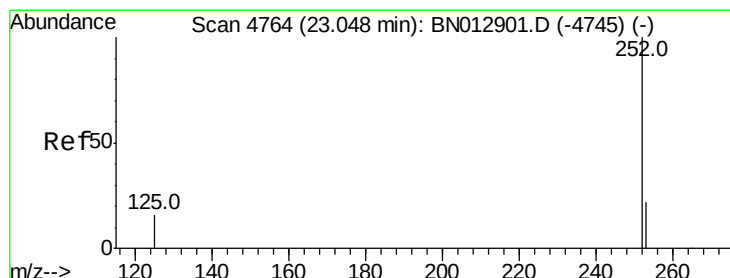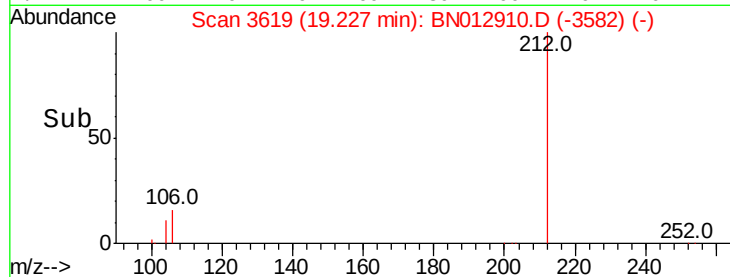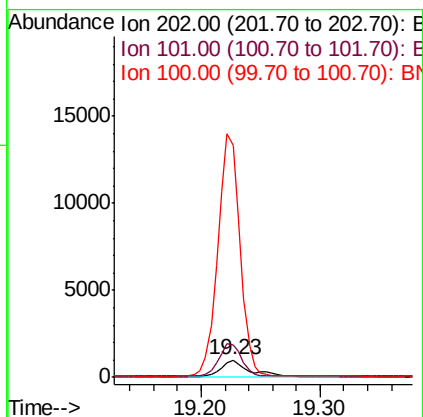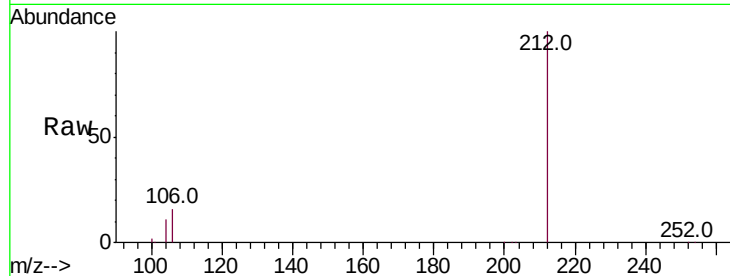

#23
Benzo(a)pyrene
Concen: 0.105 ng/ul
RT: 23.01 min Scan# 4751
Delta R.T. -0.04 min
Lab File: BN012910.D
Acq: 06 Dec 2020 10:05

Tgt Ion:252 Resp: 3094
Ion Ratio Lower Upper
252 100
253 39.9 26.5 39.7#
125 34.5 14.2 21.2#

