

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
 Data File : BN012913.D
 Acq On : 06 Dec 2020 11:53
 Operator : CG/JU
 Sample : L4859-19
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BD1

Quant Time: Dec 07 02:18:58 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 07 02:16:16 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1419	0.40	ng/ul	0.00
2) Naphthalene-d8	10.15	136	5698	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.06	164	3623	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.82
16) Chrysene-d12	21.04	240	6920	0.40	ng/ul	0.00
20) Perylene-d12	23.14	264	7089	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.76	152	3075	0.36	ng/ul	0.00
14) Fluoranthene-d10	18.86	212	7334	0.00	ng/ul	0.00
Target Compounds				Ovalue		
9) Fluorene	15.06	166	1397	0.087	ng/ul#	16
17) Pyrene	19.23	202	1808	0.055	ng/ul#	1
23) Benzo(a)pyrene	23.01	252	3514	0.115	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
Data File : BN012913.D
Acq On : 06 Dec 2020 11:53
Operator : CG/JU
Sample : L4859-19
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BD1

Quant Time: Dec 07 02:18:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 02:16:16 2020
Response via : Initial Calibration

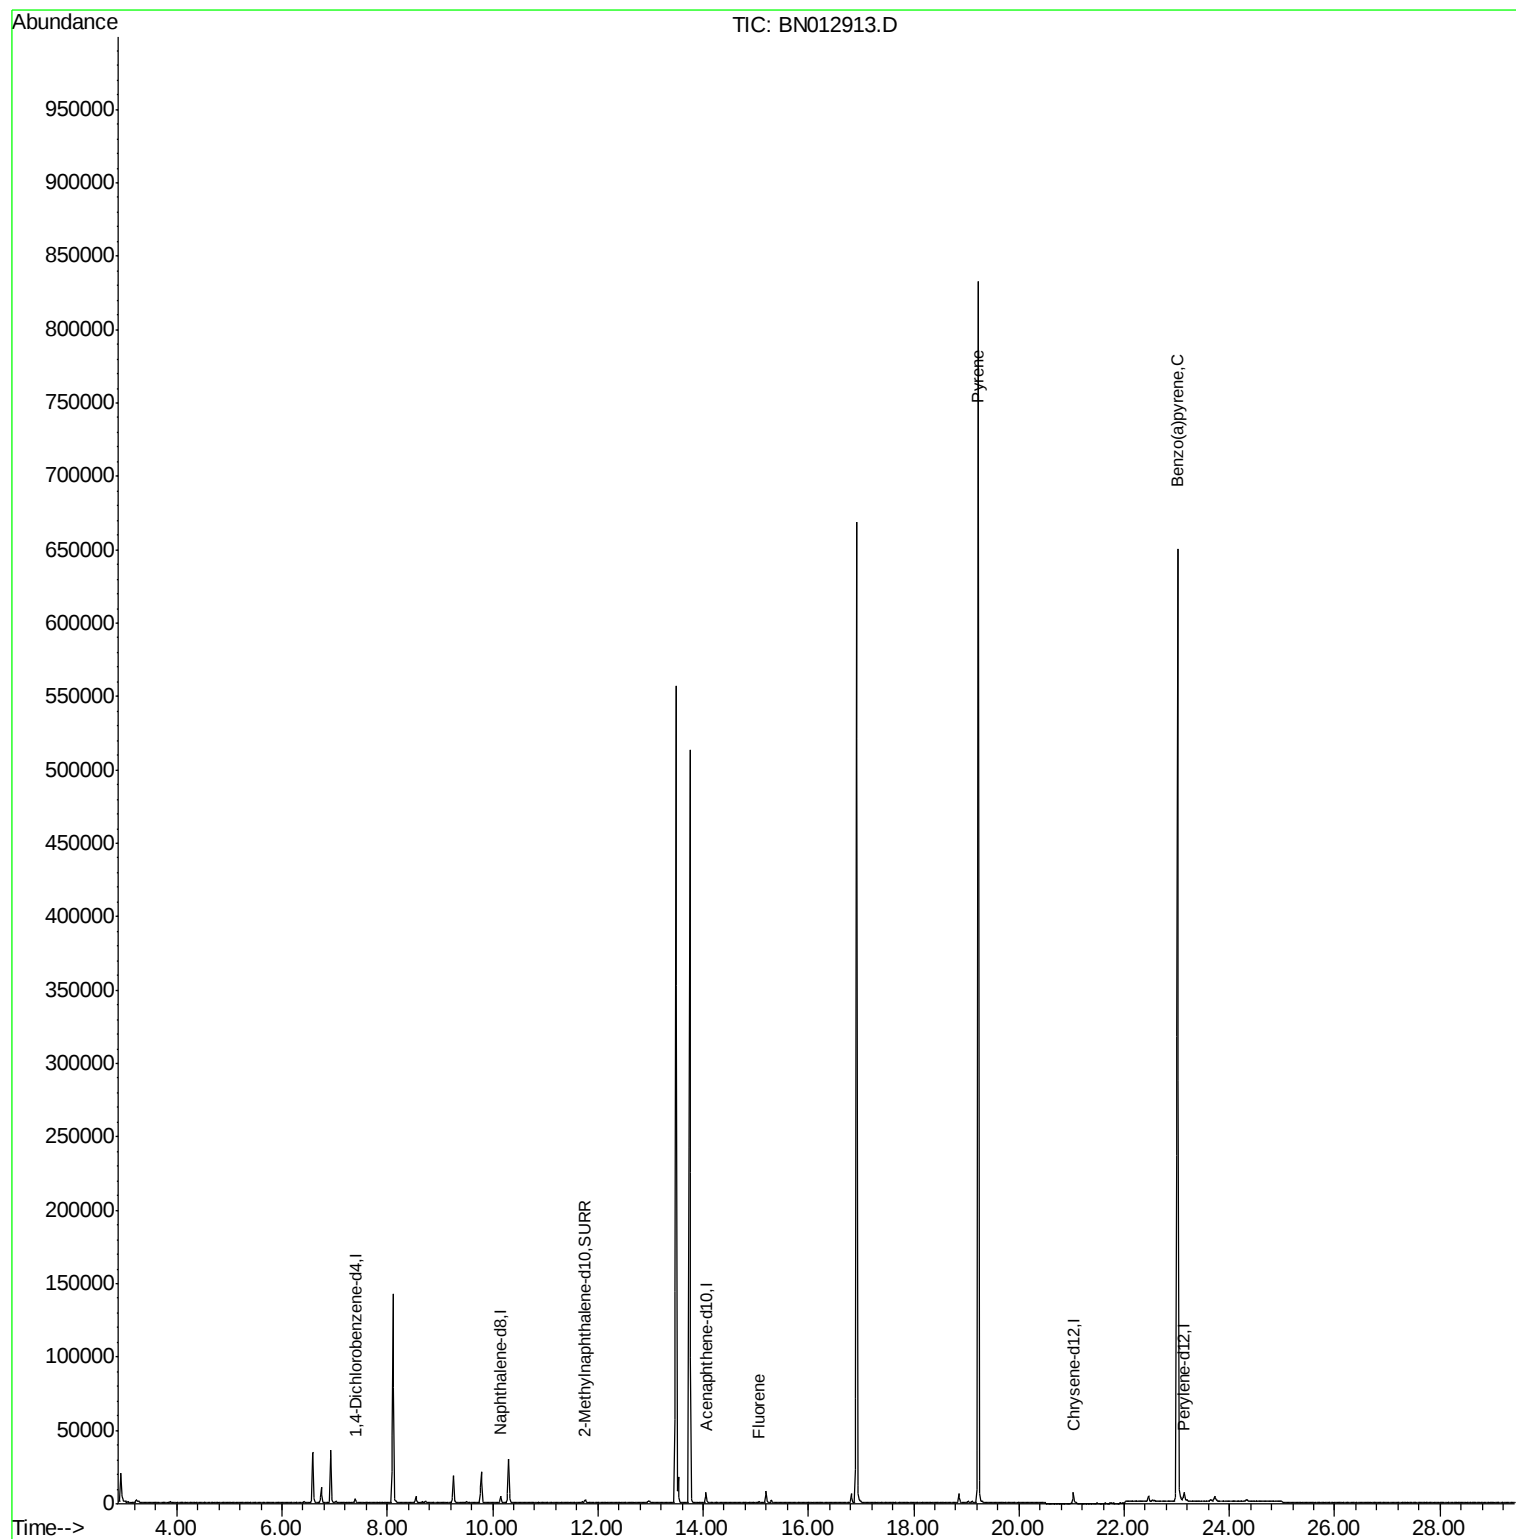

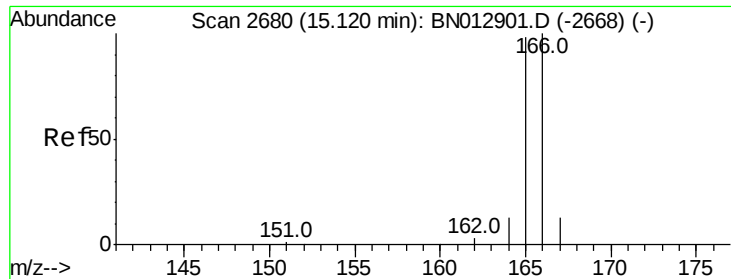

#9

Fluorene

Concen: 0.087 ng/ul

RT: 15.06 min Scan# 2668

Delta R.T. -0.06 min

Lab File: BN012913.D

Acq: 06 Dec 2020 11:53

Instrument :

BNA_N

ClientSampleId :

C0BD1


Tot Ion:166 Resp: 1397

Ion Ratio Lower Upper

166 100

165 9.3 79.8 119.8#




167 38.2 13.8 20.8#

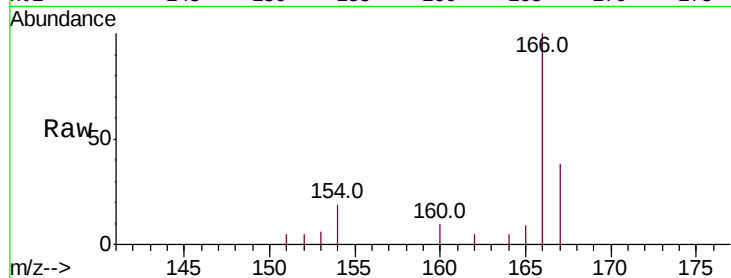

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

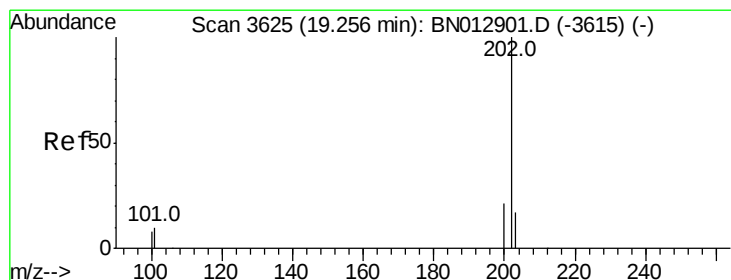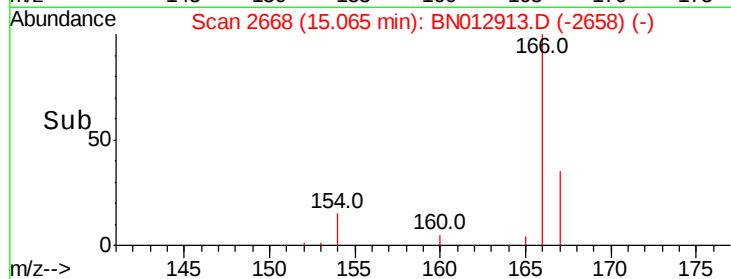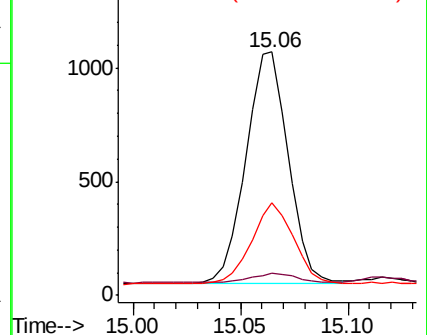

#17

Pyrene

Concen: 0.055 ng/ul

RT: 19.23 min Scan# 3619

Delta R.T. -0.03 min

Lab File: BN012913.D

Acq: 06 Dec 2020 11:53


Tgt Ion:202 Resp: 1808

Ion Ratio Lower Upper

202 100

101 198.9 9.1 13.7#



100 1423.8 7.5 11.3#

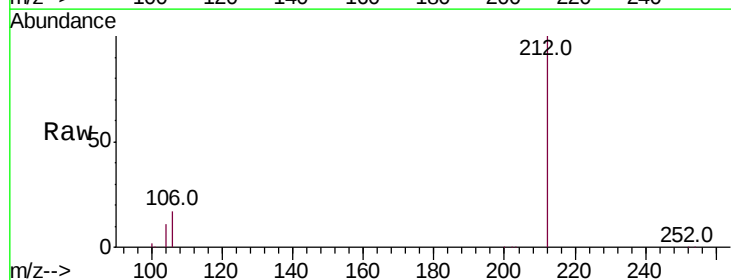


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

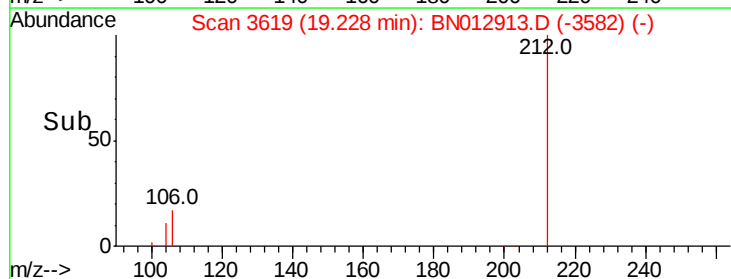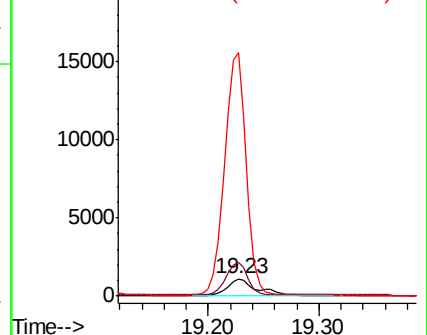

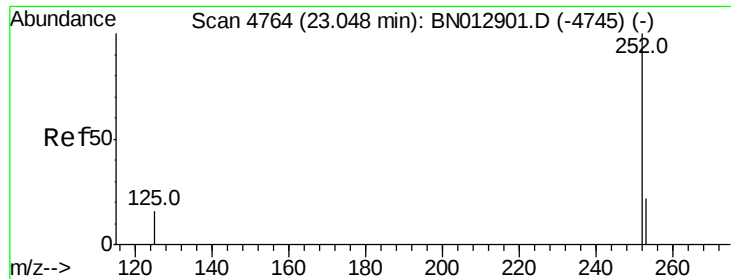

#23

Benzo(a)pyrene

Concen: 0.115 ng/ul

RT: 23.01 min Scan# 4751

Delta R.T. -0.04 min

Lab File: BN012913.D

Acq: 06 Dec 2020 11:53

Instrument :

BNA_N

ClientSampleId :

C0BD1


Tot Ion: 252 Resp: 3514

Ion Ratio Lower Upper

252 100

253 39.2 26.5 39.7

125 34.0 14.2 21.2#

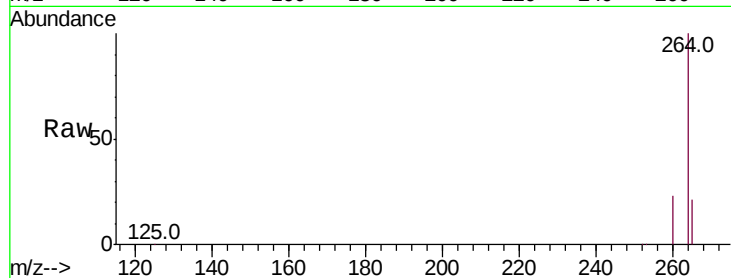

Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

