


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
Data File : BN012891.D
Acq On : 05 Dec 2020 21:59
Operator : CG/JU
Sample : L4864-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BA7

Manual Integrations
APPROVED

mohammad
12/7/2020 2:10:05 PM

Quant Time: Dec 07 01:24:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 01:01:09 2020
Response via : Initial Calibration

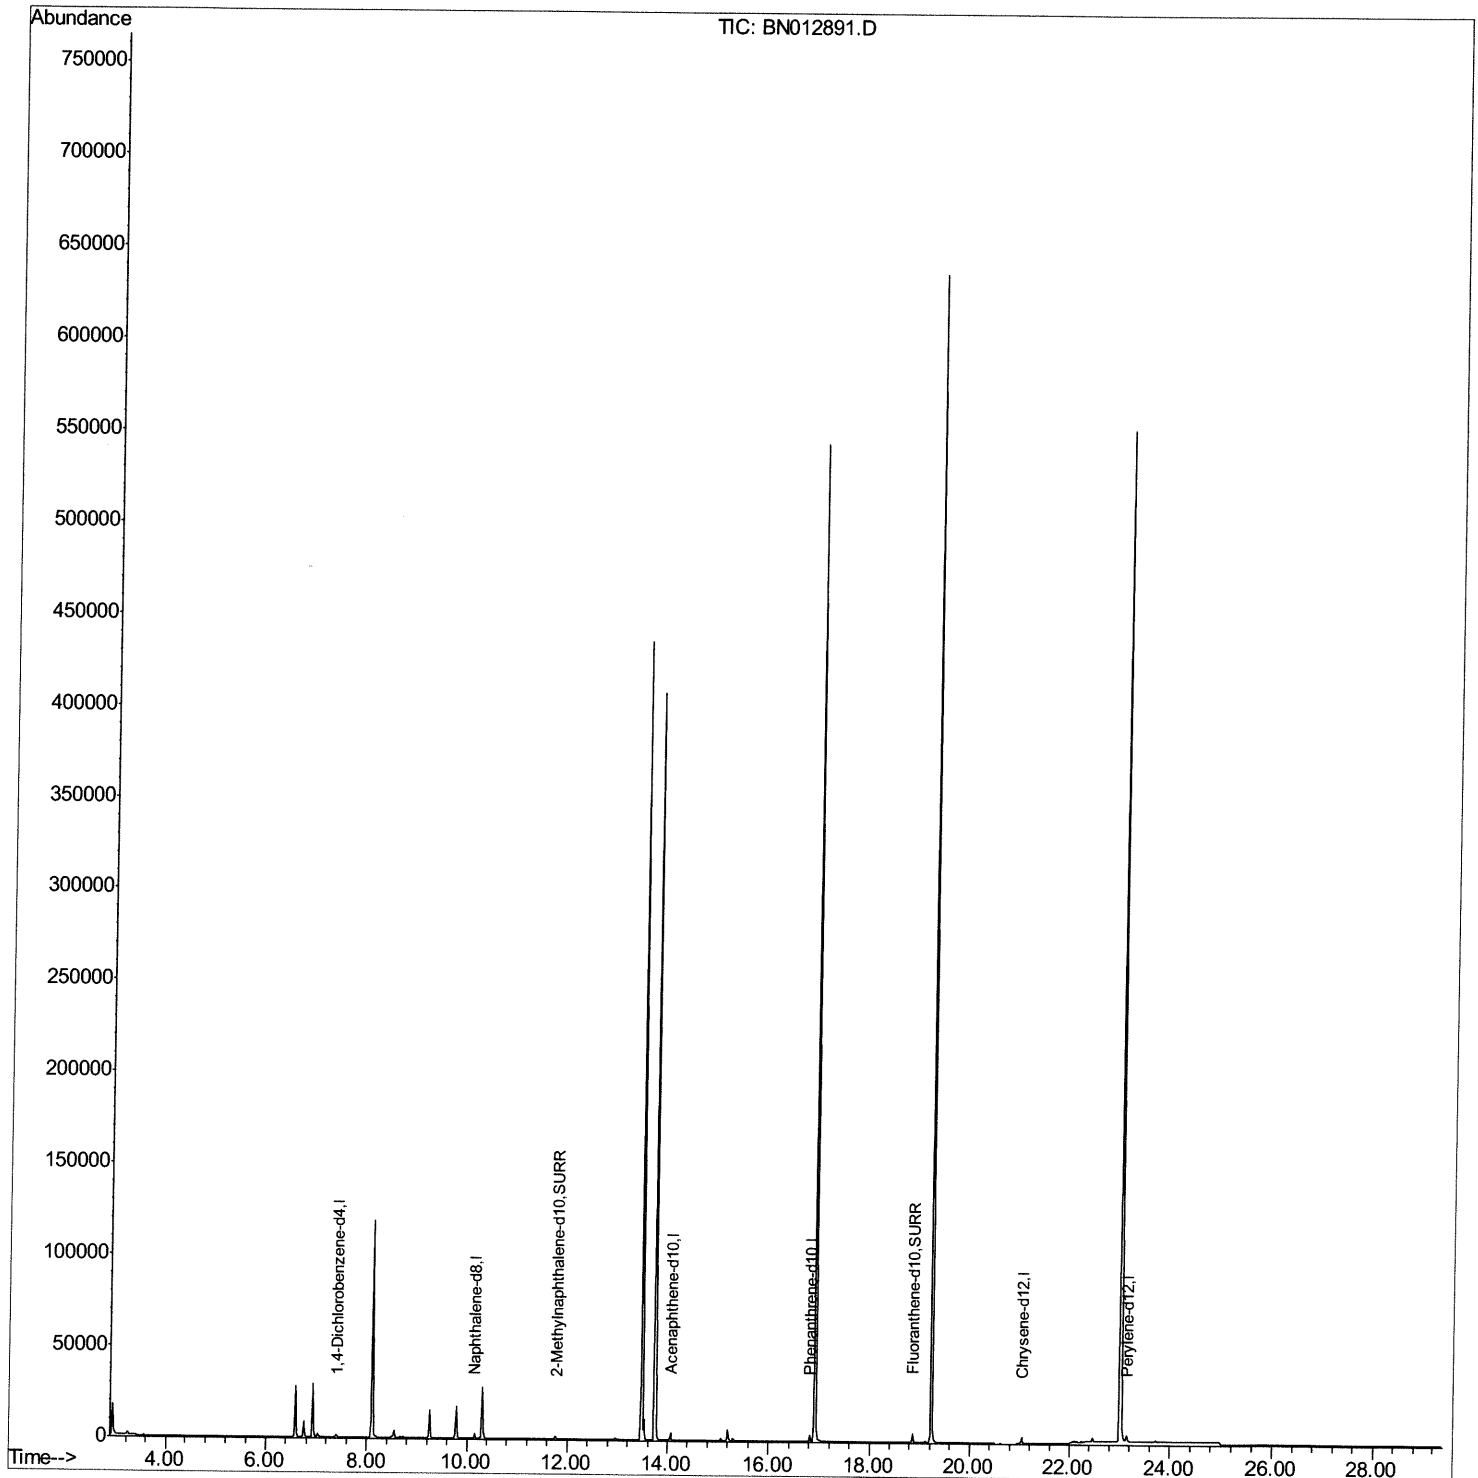

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
Data File : BN012891.D
Acq On : 05 Dec 2020 21:59
Operator : CG/JU
Sample : L4864-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BA7

Manual Integrations
APPROVED

mohammad
12/7/2020 2:10:05 PM

Quant Time: Dec 07 01:02:21 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 01:01:09 2020
Response via : Initial Calibration

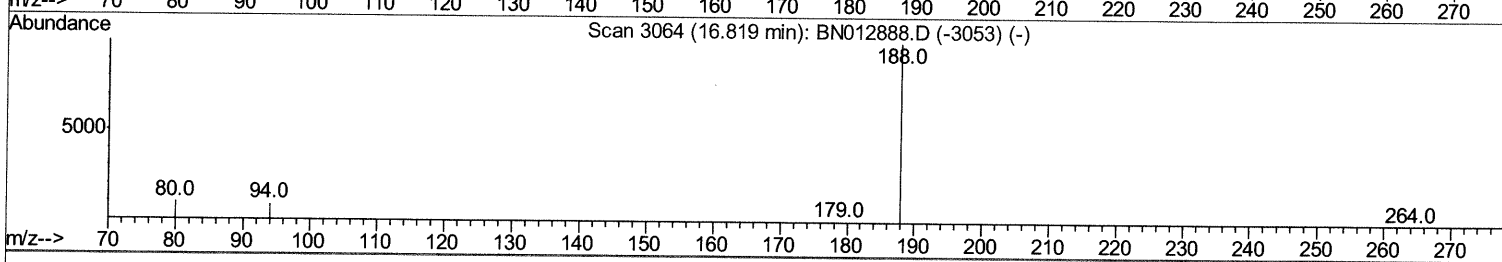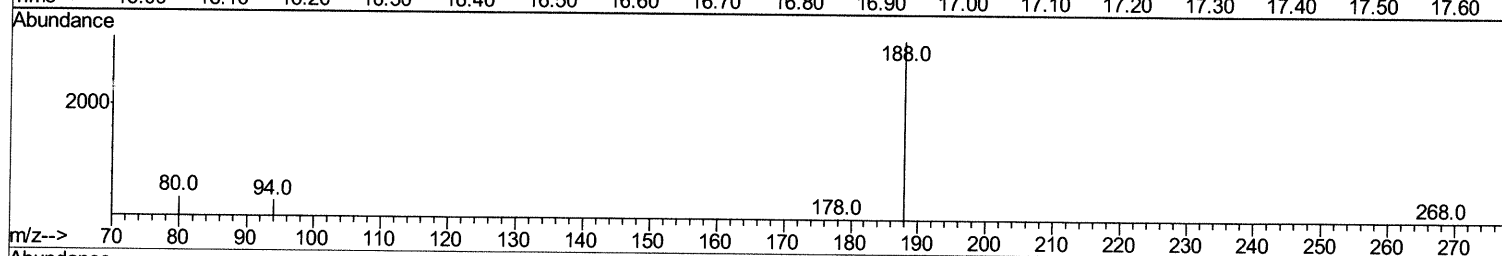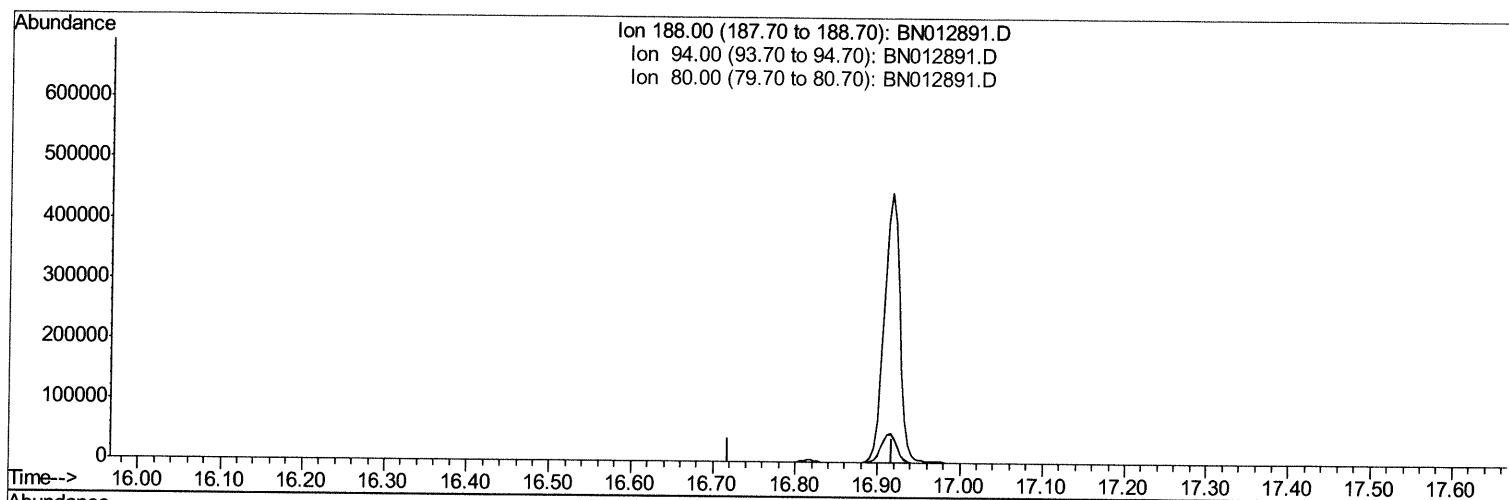

TIC: BN012891.D

(10) Phenanthrene-d10 (I)

16.819min (-16.819) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.40	0.00#
80.00	12.40	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
 Data File : BN012891.D
 Acq On : 05 Dec 2020 21:59
 Operator : CG/JU
 Sample : L4864-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BA7

Manual Integrations
 APPROVED

mohammad
 12/7/2020 2:10:05 PM

Quant Time: Dec 07 01:02:21 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 07 01:01:09 2020
 Response via : Initial Calibration

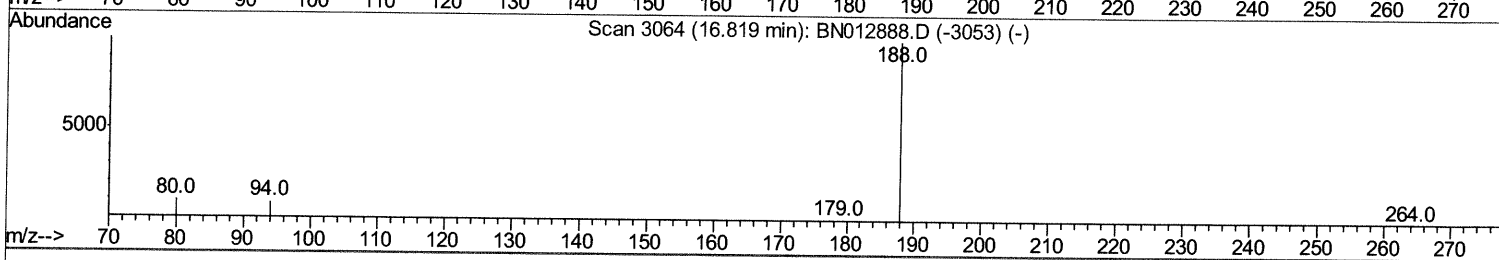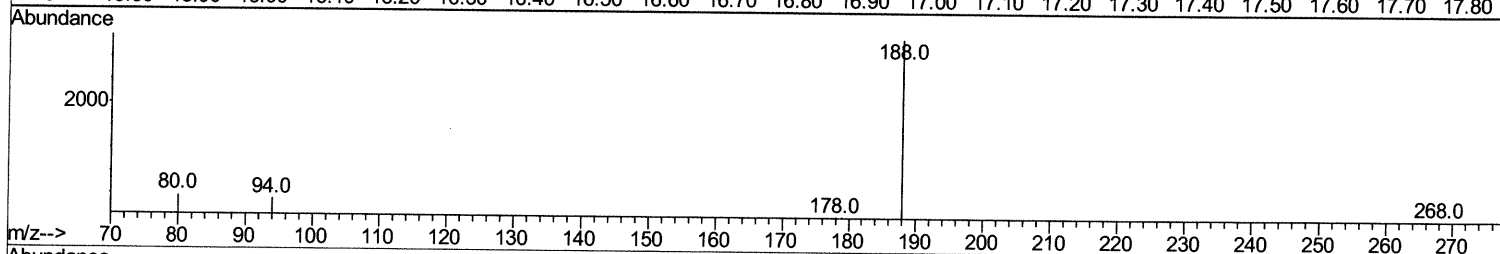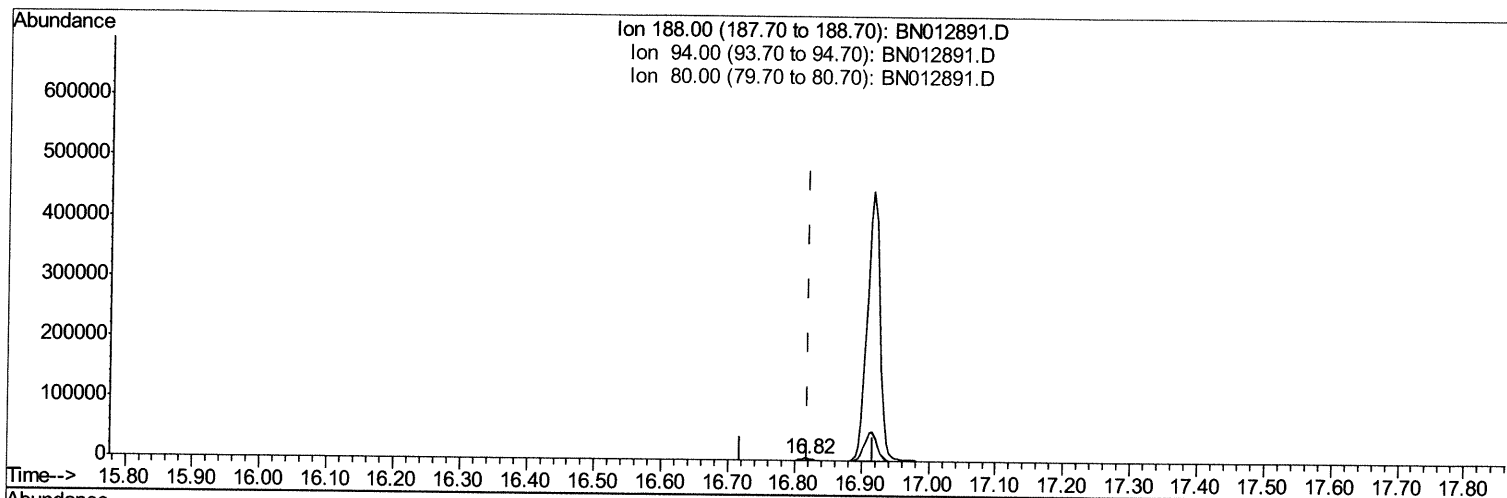

TIC: BN012891.D

(10) Phenanthrene-d10 (I)

16.819min (0.000) 0.40ng/ul m 12/04/2024

response 4342

Ion	Exp%	Act%
188.00	100	100
94.00	11.40	9.88
80.00	12.40	11.65
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
 Data File : BN012891.D
 Acq On : 05 Dec 2020 21:59
 Operator : CG/JU
 Sample : L4864-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BA7

Manual Integrations
 APPROVED

mohammad
 12/7/2020 2:10:05 PM

Quant Time: Dec 07 01:24:17 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 07 01:01:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	808	0.40	ng/ul	0.00
2) Naphthalene-d8	10.16	136	3209	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.06	164	2044	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.82	188	4342m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.04	240	3757	0.40	ng/ul	0.00
20) Perylene-d12	23.14	264	4186	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.76	152	2395	0.50	ng/ul	0.00
14) Fluoranthene-d10	18.86	212	5555	0.47	ng/ul	0.00

12/6/20 DV

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed