


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
Data File : BN012909.D
Acq On : 06 Dec 2020 09:29
Operator : CG/JU
Sample : L4859-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BB6

Manual Integrations
APPROVED

mohammad
12/7/2020 2:10:59 PM

Quant Time: Dec 07 02:48:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 02:16:16 2020
Response via : Initial Calibration

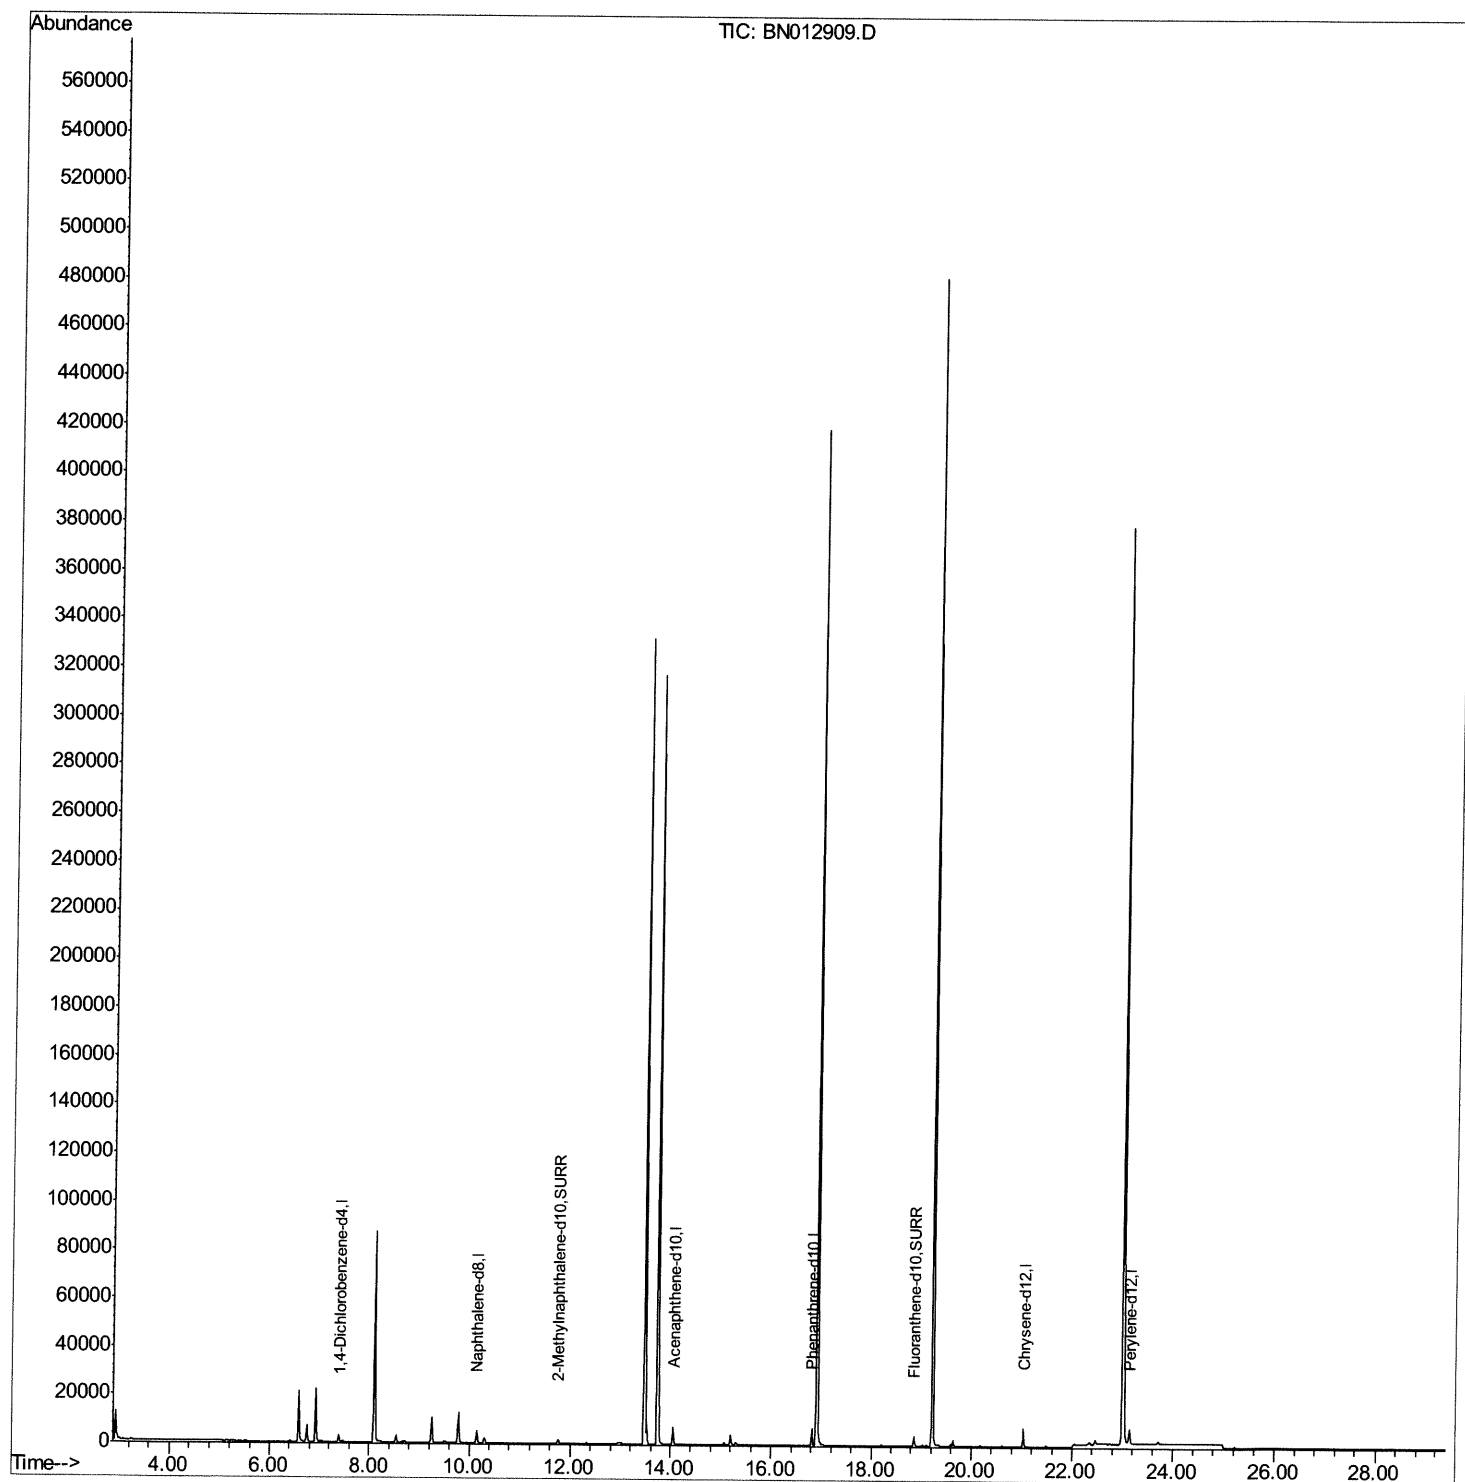

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
Data File : BN012909.D
Acq On : 06 Dec 2020 09:29
Operator : CG/JU
Sample : L4859-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BB6

Manual Integrations
APPROVED

mohammad
12/7/2020 2:10:59 PM

Quant Time: Dec 07 02:18:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 02:16:16 2020
Response via : Initial Calibration

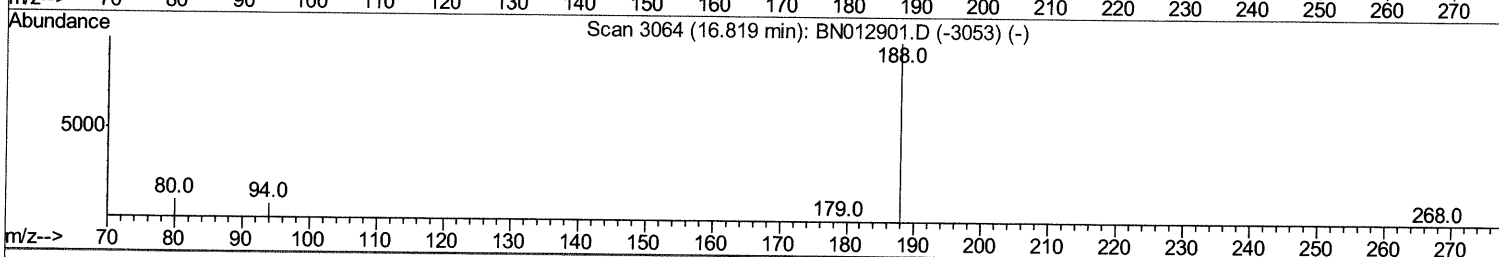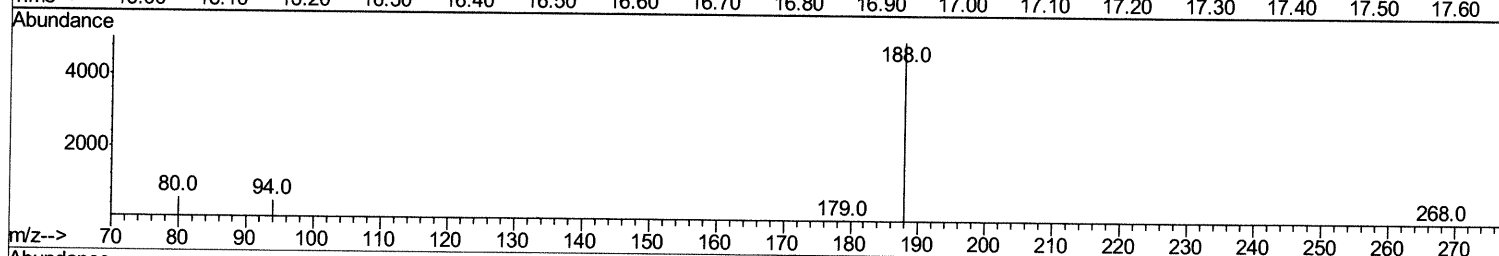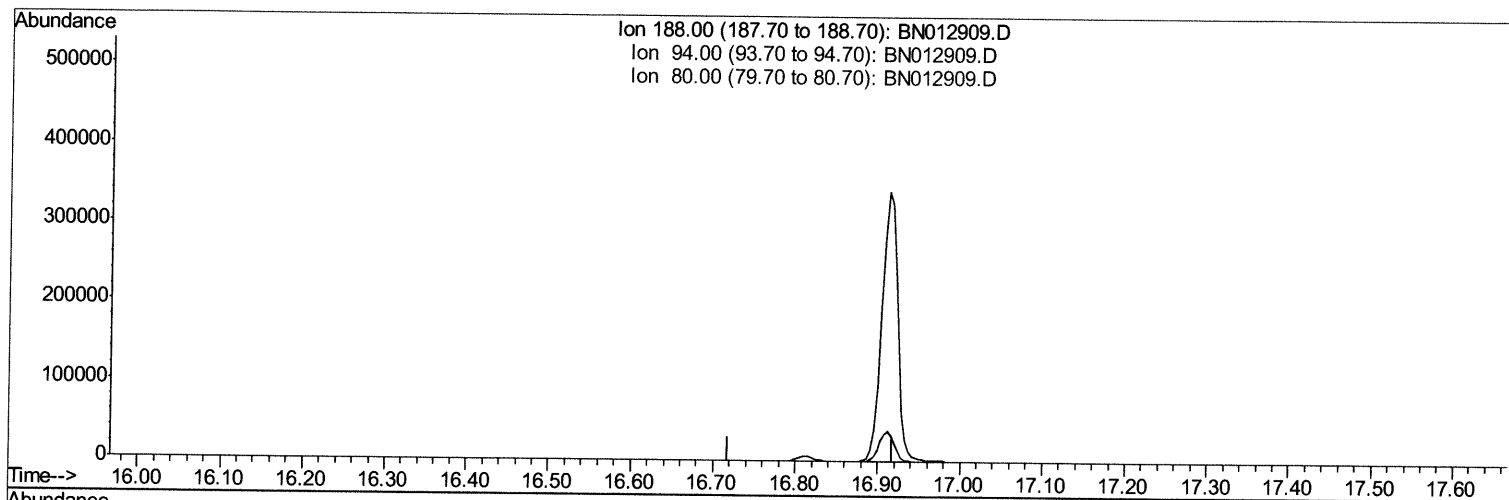

TIC: BN012909.D

(10) Phenanthrene-d10 (I)

16.819min (-16.819) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.40	0.00#
80.00	12.40	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
Data File : BN012909.D
Acq On : 06 Dec 2020 09:29
Operator : CG/JU
Sample : L4859-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BB6

Manual Integrations
APPROVED

mohammad
12/7/2020 2:10:59 PM

Quant Time: Dec 07 02:18:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 02:16:16 2020
Response via : Initial Calibration

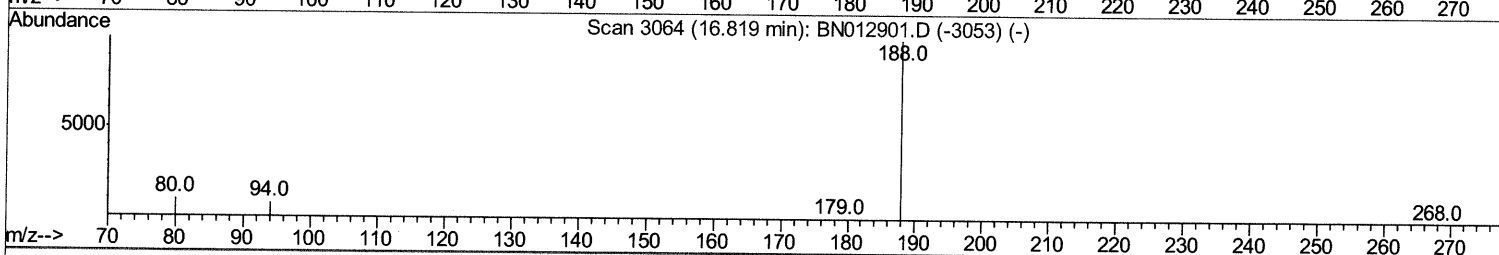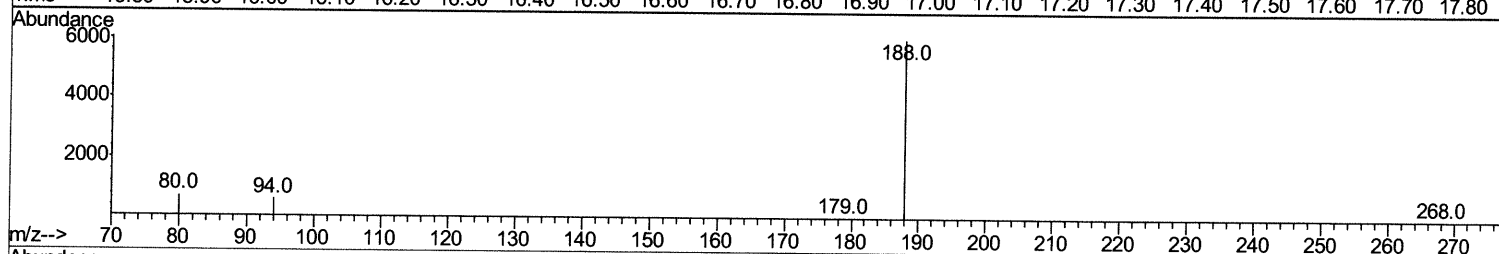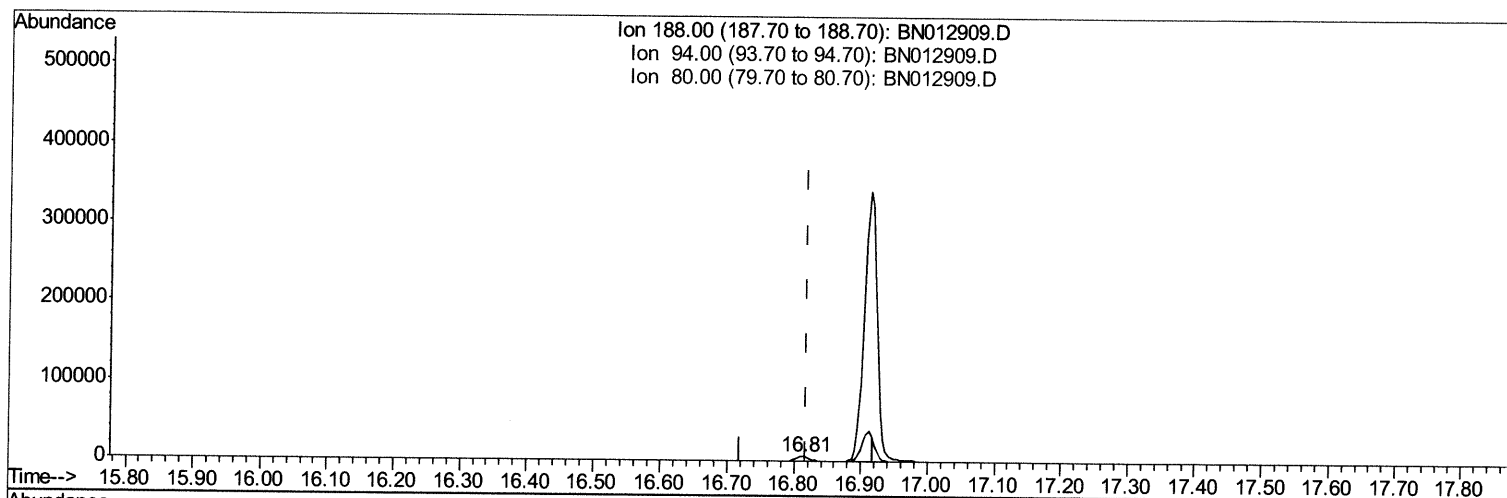

TIC: BN012909.D

(10) Phenanthrene-d10 (I)

16.814min (-0.004) 0.40ng/ul m 12/09/2020

response 8262

Ion	Exp%	Act%
188.00	100	100
94.00	11.40	10.00
80.00	12.40	11.71
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
Data File : BN012909.D
Acq On : 06 Dec 2020 09:29
Operator : CG/JU
Sample : L4859-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BB6

Manual Integrations
APPROVED

mohammad
12/7/2020 2:10:59 PM

Quant Time: Dec 07 02:48:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 02:16:16 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1526	0.40	ng/ul	0.00
2) Naphthalene-d8	10.15	136	6253	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.06	164	3754	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.81	188	8262m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.04	240	6945	0.40	ng/ul	0.00
20) Perylene-d12	23.14	264	7322	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.76	152	1850	0.20	ng/ul	0.00
14) Fluoranthene-d10	18.86	212	4280	0.19	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed