


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
Data File : BN012910.D
Acq On : 06 Dec 2020 10:05
Operator : CG/JU
Sample : L4859-09
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BE2

Manual Integrations
APPROVED

mohammad
12/7/2020 2:11:01 PM

Quant Time: Dec 07 02:51:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 02:16:16 2020
Response via : Initial Calibration

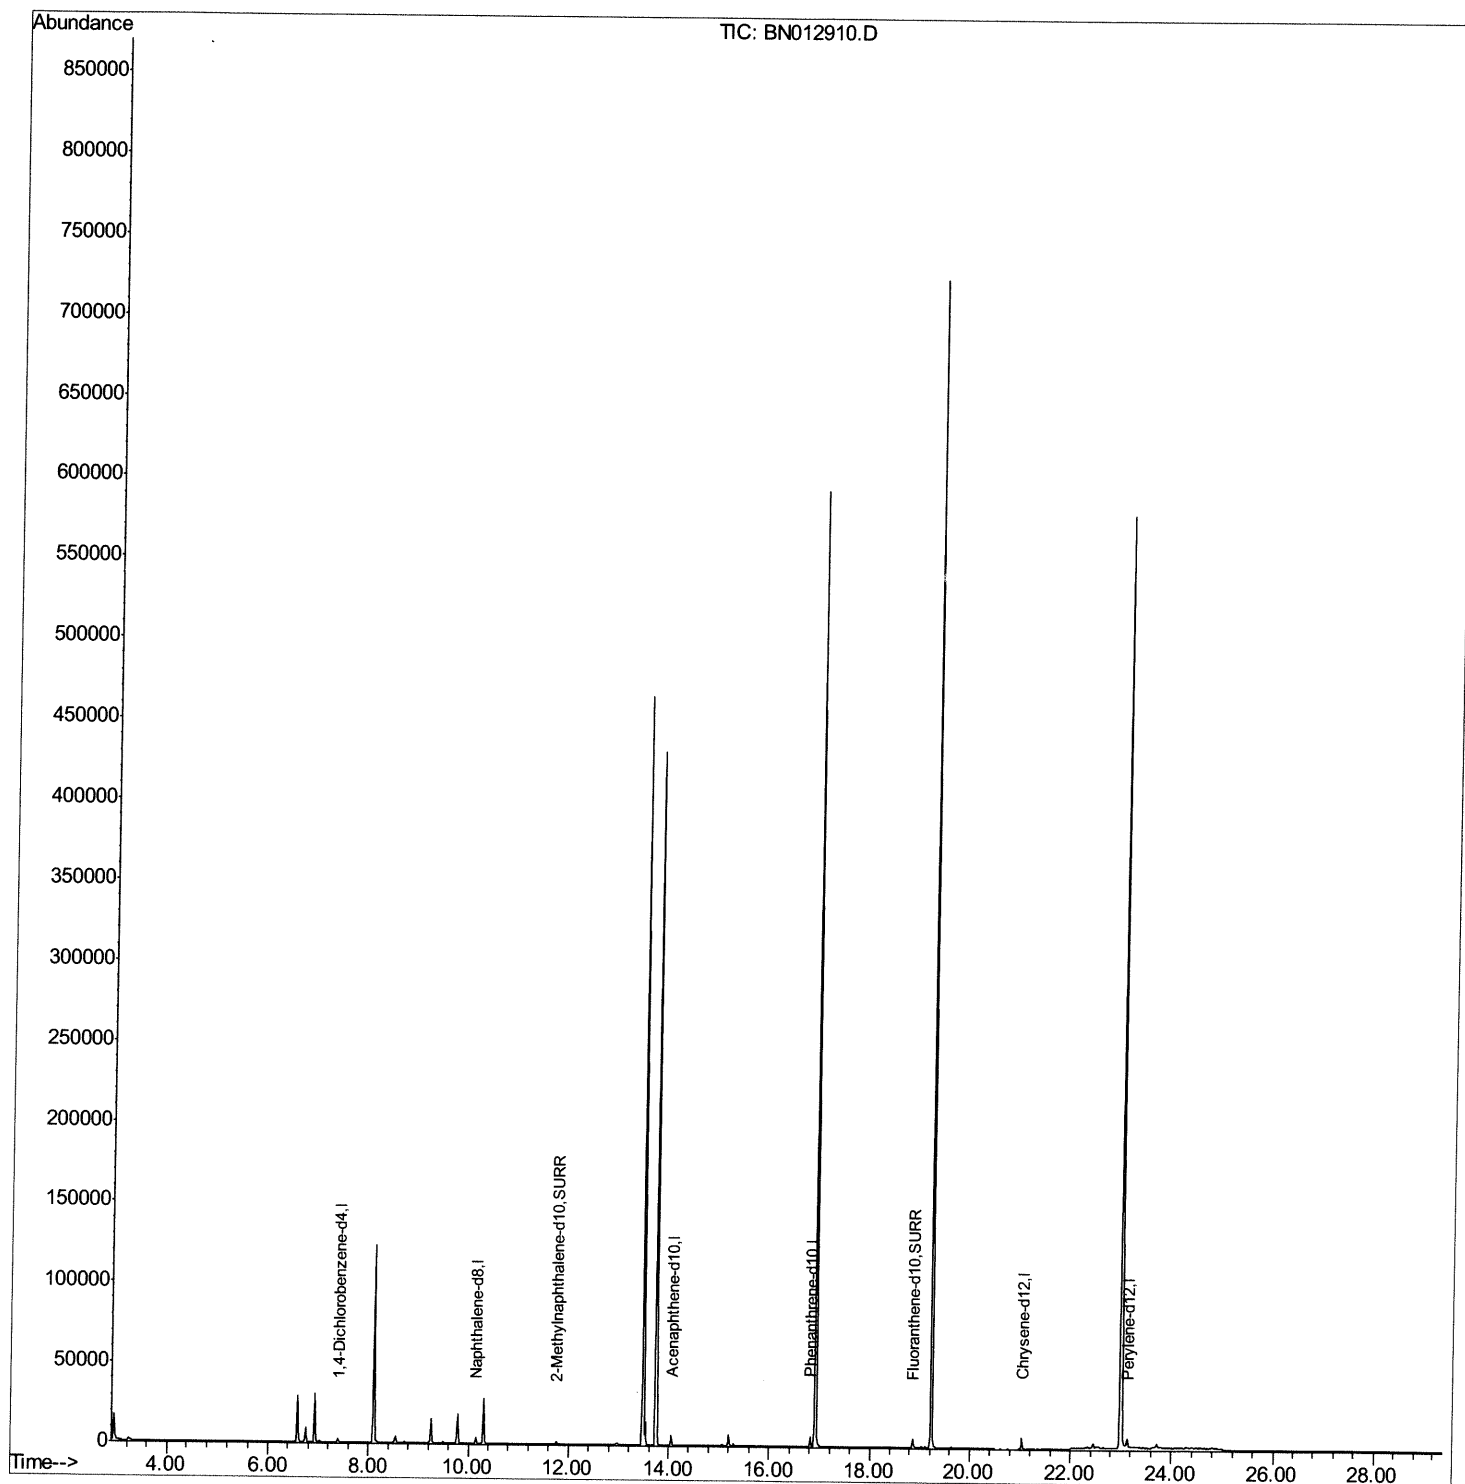

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
 Data File : BN012910.D
 Acq On : 06 Dec 2020 10:05
 Operator : CG/JU
 Sample : L4859-09
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 C0BE2

Manual Integrations
APPROVED

mohammad
 12/7/2020 2:11:01 PM

Quant Time: Dec 07 02:18:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 07 02:16:16 2020
 Response via : Initial Calibration

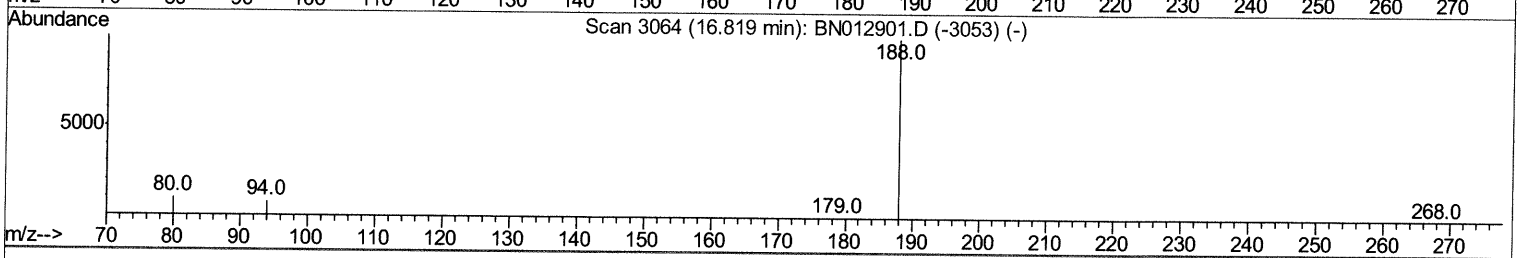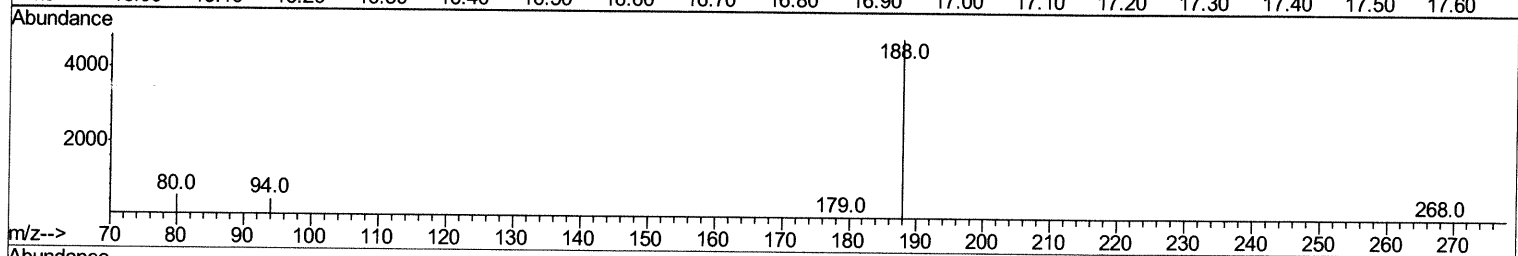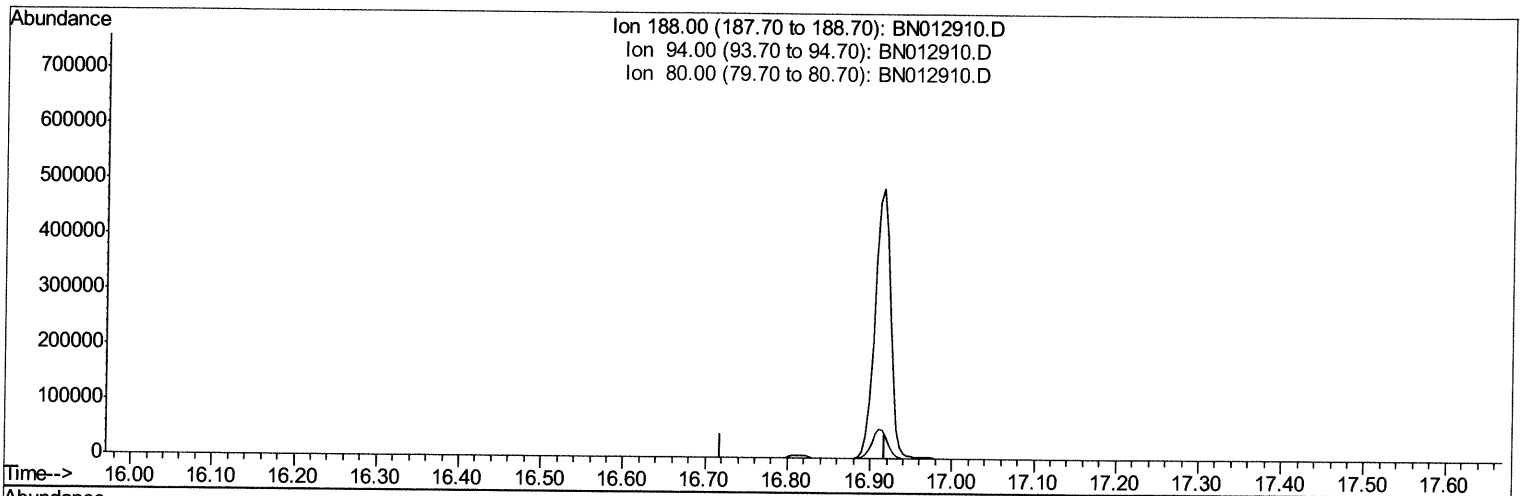

TIC: BN012910.D

(10) Phenanthrene-d10 (I)

16.819min (-16.819) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.40	0.00#
80.00	12.40	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
Data File : BN012910.D
Acq On : 06 Dec 2020 10:05
Operator : CG/JU
Sample : L4859-09
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BE2

Manual Integrations
APPROVED

mohammad
12/7/2020 2:11:01 PM

Quant Time: Dec 07 02:18:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 02:16:16 2020
Response via : Initial Calibration

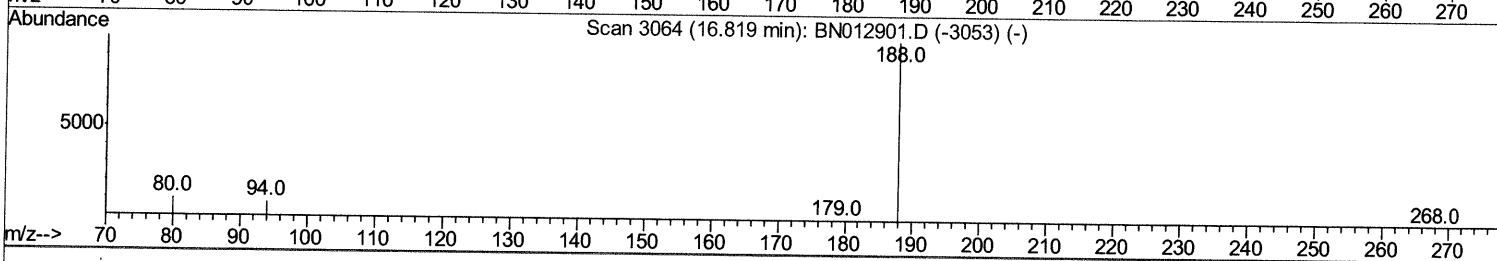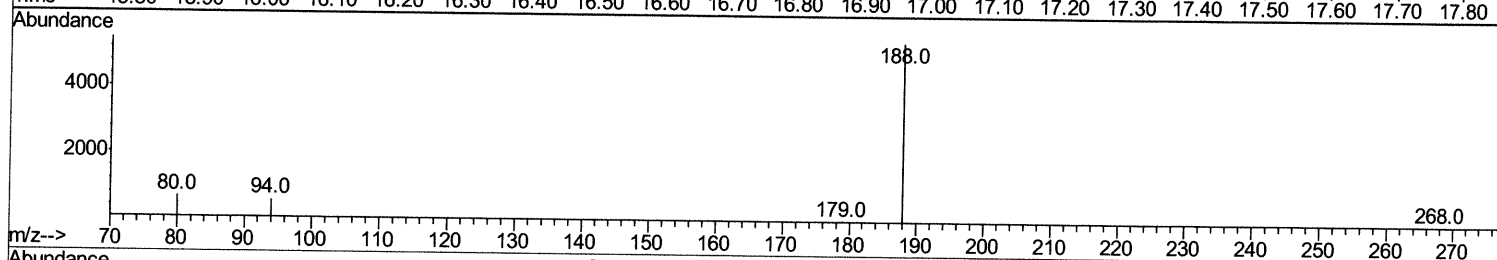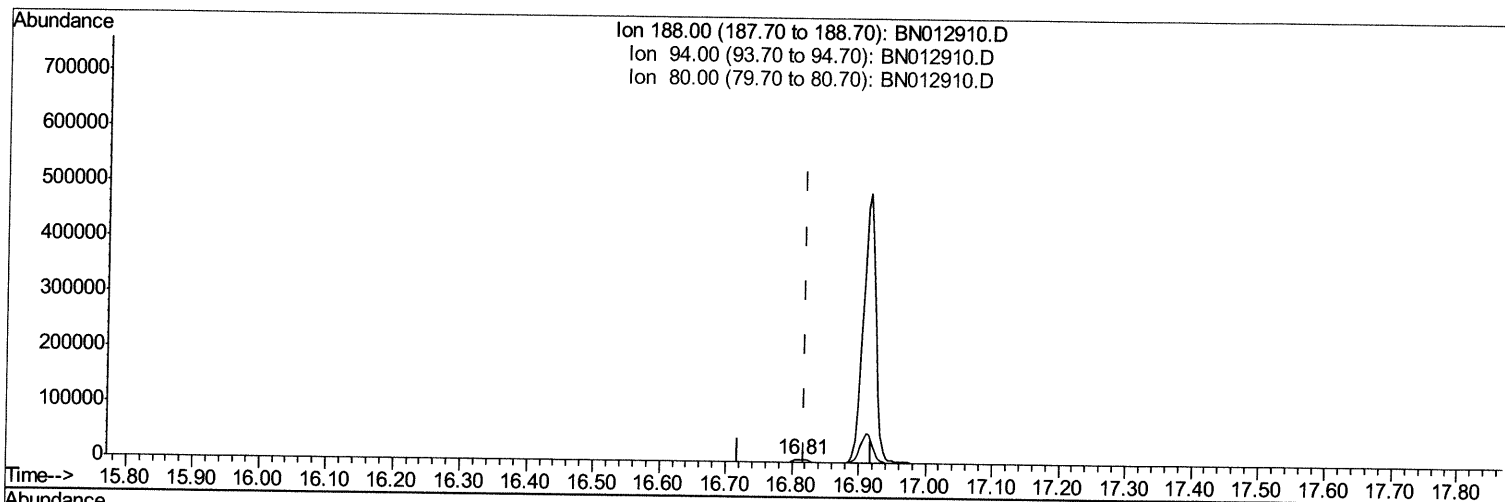

TIC: BN012910.D

(10) Phenanthrene-d10 (I)

16.813min (-0.005) 0.40ng/ul m 12/09/20 JU

response 7367

Ion	Exp%	Act%
188.00	100	100
94.00	11.40	10.55
80.00	12.40	12.17
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
 Data File : BN012910.D
 Acq On : 06 Dec 2020 10:05
 Operator : CG/JU
 Sample : L4859-09
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BE2

Manual Integrations
 APPROVED

mohammad
 12/7/2020 2:11:01 PM

Quant Time: Dec 07 02:51:17 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 07 02:16:16 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1335	0.40	ng/ul	0.00
2) Naphthalene-d8	10.16	136	5463	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.05	164	3324	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.81	188	7367m>	0.40	ng/ul>	0.00(2109/2020)
16) Chrysene-d12	21.04	240	6466	0.40	ng/ul	0.00
20) Perylene-d12	23.13	264	6859	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.76	152	2570	0.32	ng/ul	0.00
14) Fluoranthene-d10	18.85	212	6219	0.31	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed