

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
 Data File : BN012900.D
 Acq On : 06 Dec 2020 03:28
 Operator : CG/JU
 Sample : L4864-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BD4

Manual Integrations
 APPROVED

mohammad
 12/7/2020 2:10:32 PM

Quant Time: Dec 07 01:47:50 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 07 01:01:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	875	0.40	ng/ul	0.00
2) Naphthalene-d8	10.16	136	3410	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.06	164	2099	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.81	188	4535m	0.40	ng/ul	0.00
16) Chrysene-d12	21.04	240	4021	0.40	ng/ul	0.00
20) Perylene-d12	23.14	264	4712	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.76	152	1933	0.38	ng/ul	0.00
14) Fluoranthene-d10	18.86	212	4659	0.38	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	16.48	266	73	0.056	ng/ul	Ovalue 87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120620\
Data File : BN012900.D
Acq On : 06 Dec 2020 03:28
Operator : CG/JU
Sample : L4864-08
Misc :
ALS Vial : 14 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
C0BD4

Manual Integrations
APPROVED

mohammad
12/7/2020 2:10:32 PM

Quant Time: Dec 07 01:47:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 01:01:09 2020
Response via : Initial Calibration

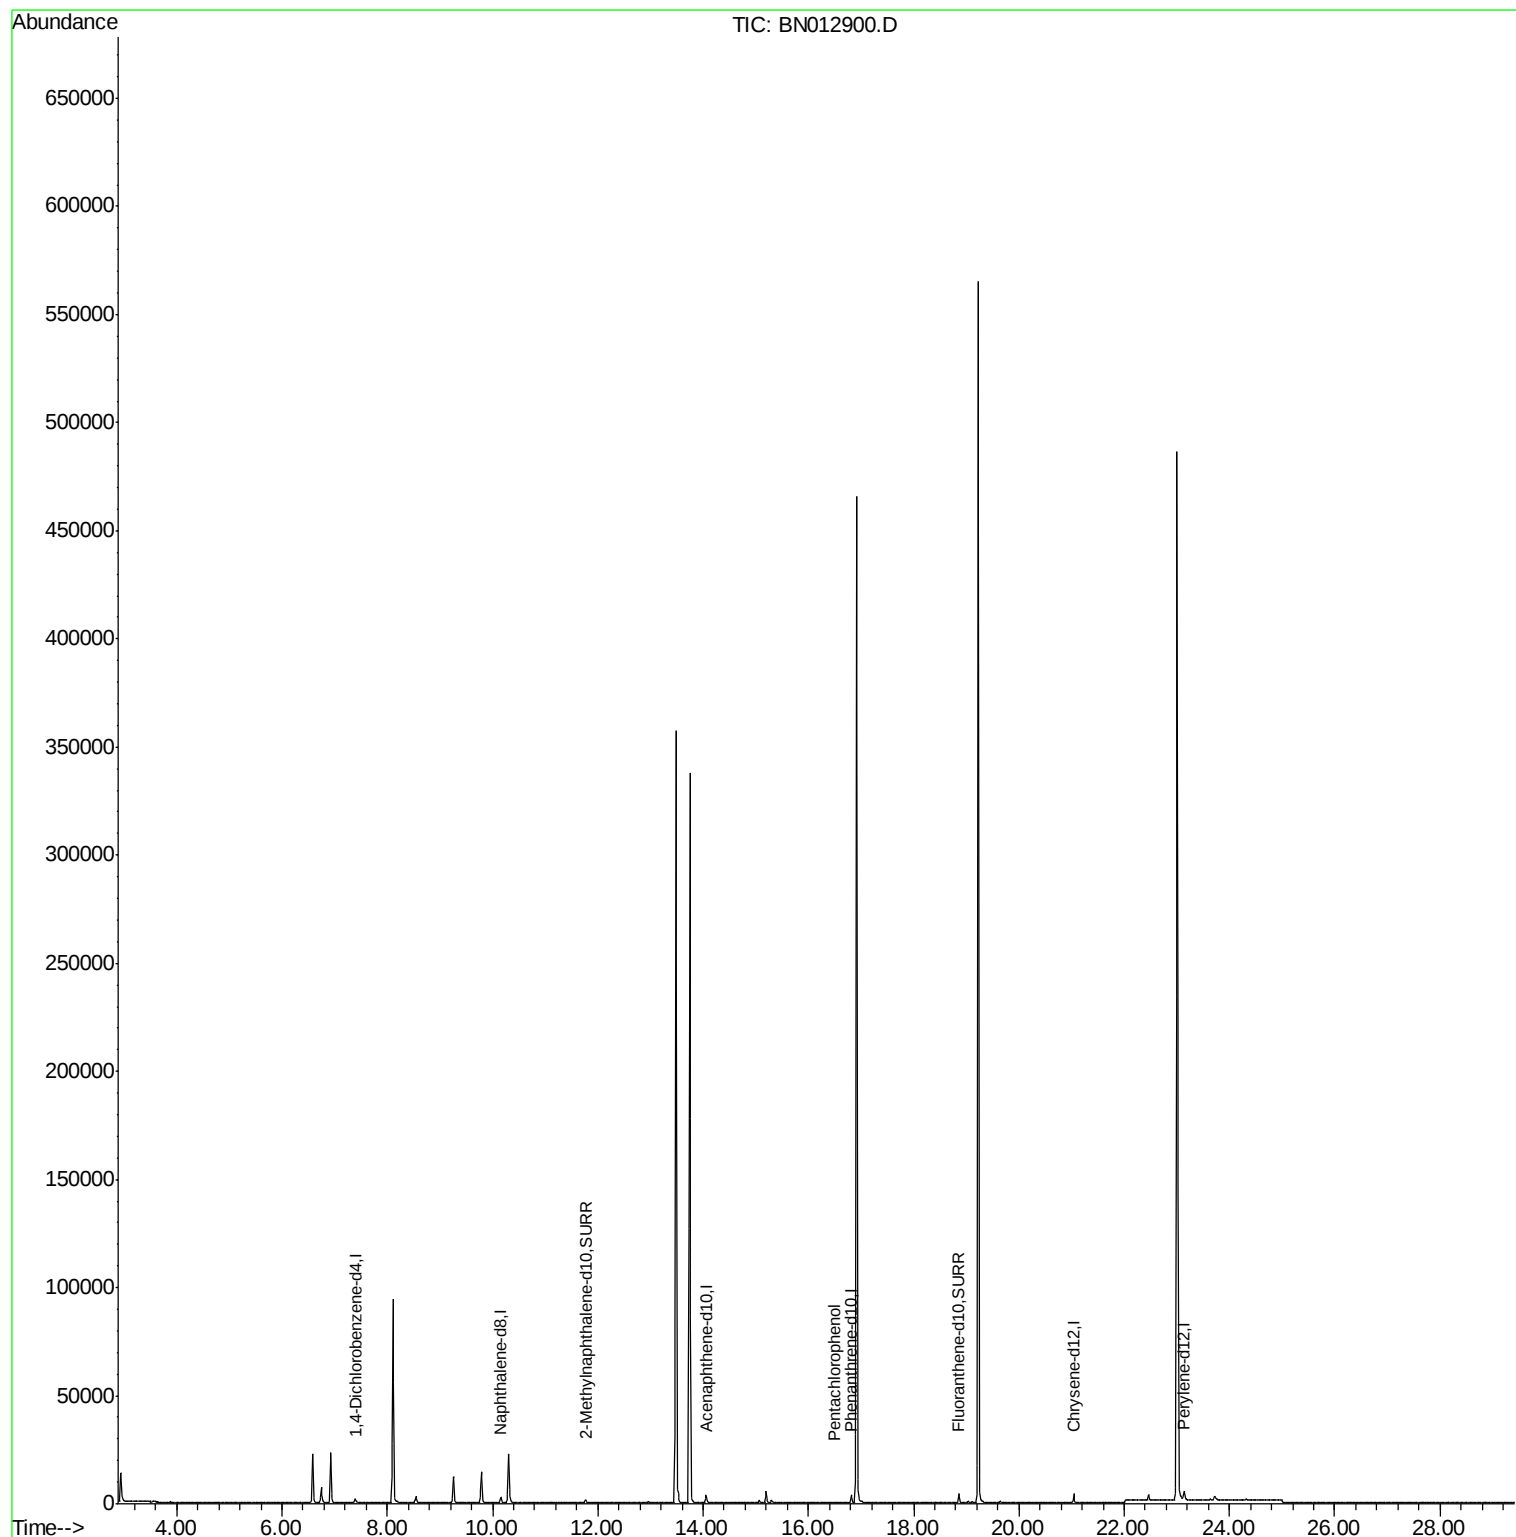

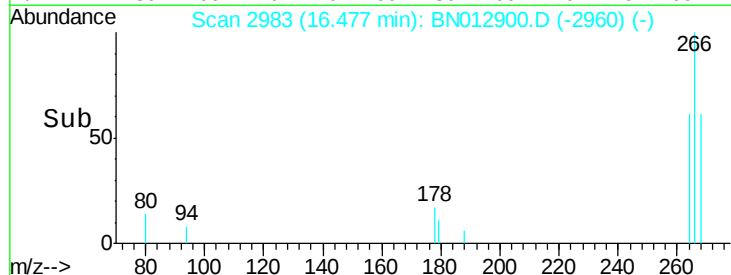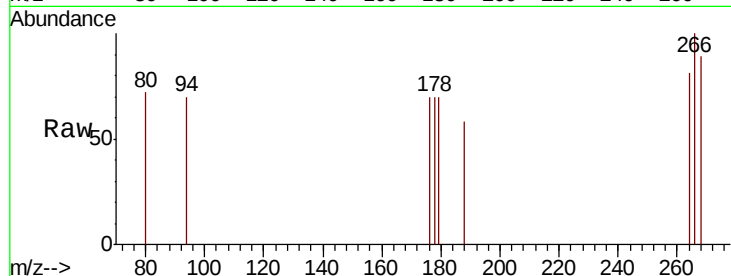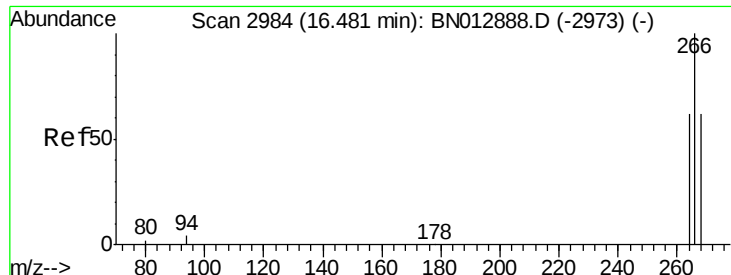

#11
 Pentachlorophenol
 Concen: 0.056 ng/ul
 RT: 16.48 min Scan# 2983
 Delta R.T. -0.00 min
 Lab File: BN012900.D
 Acq: 06 Dec 2020 03:28

Instrument :
 BNA_N
 ClientSampleId :
 C0BD4

Tot Ion:	266	Resp:	73
Ion Ratio	Lower	Upper	
266	100		
264	56.2	51.5	77.3
268	57.5	56.0	84.0

Manual Integrations
 APPROVED

mohammad
 12/7/2020 2:10:32 PM

