
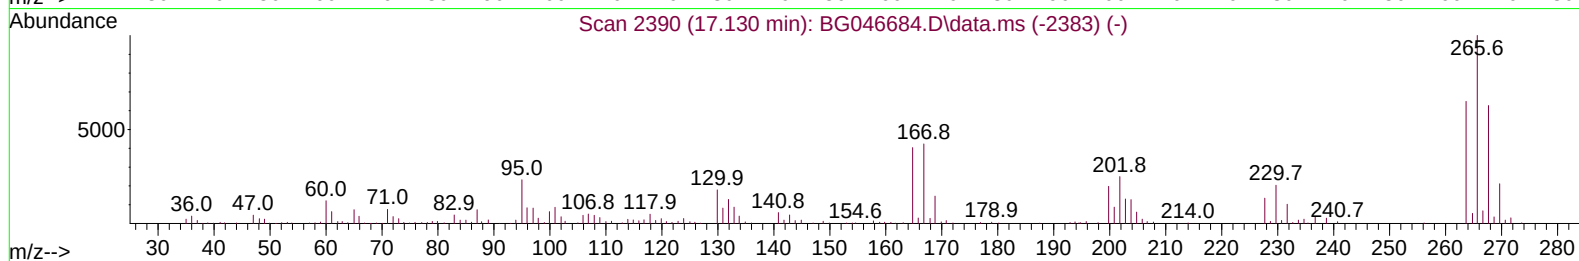
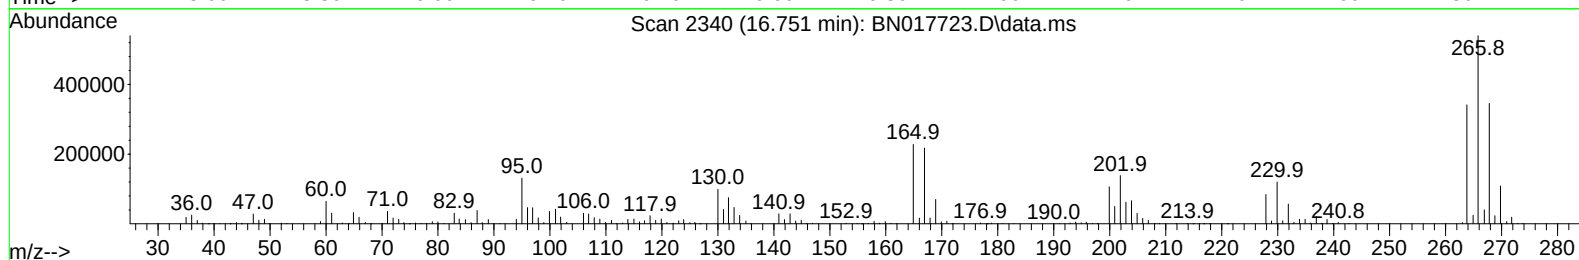


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120621\
Data File : BN017723.D
Acq On : 06 Dec 2021 10:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 15:11:44 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 06 15:11:38 2021
Response via : Initial Calibration

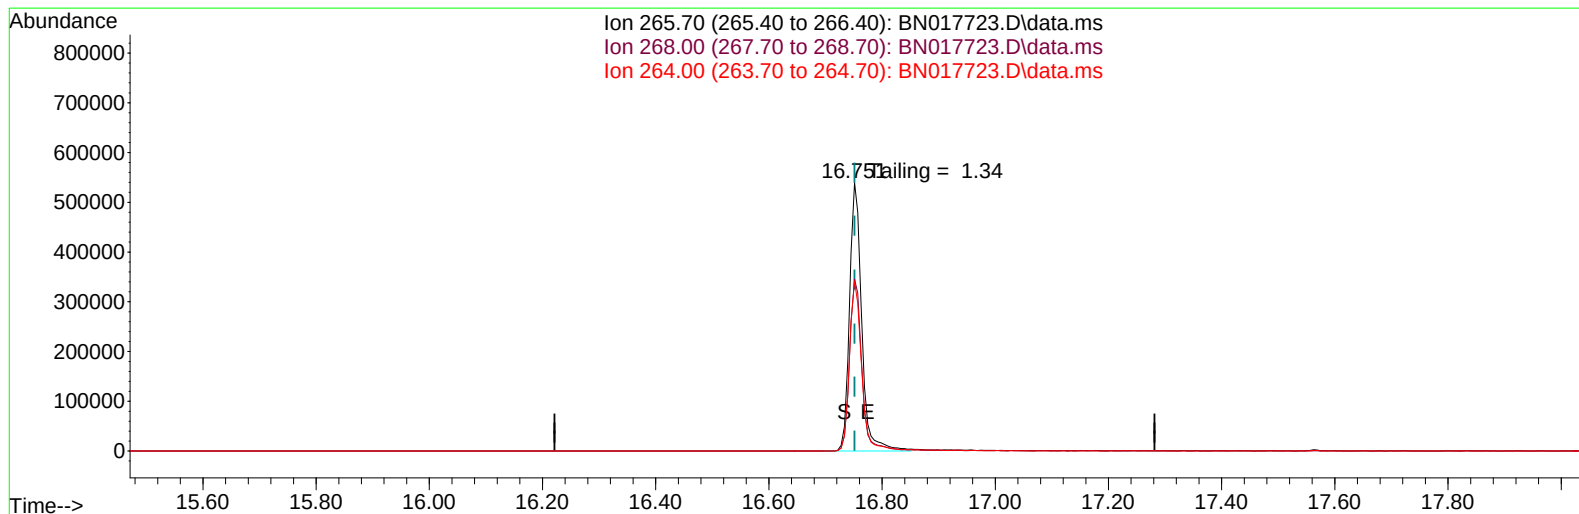

TIC: BN017723.D\data.ms

(70) Pentachlorophenol (C)




16.751min (0.000) 24899.13 ng

response 811114

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.05
264.00	61.60	63.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120621\
Data File : BN017723.D
Acq On : 06 Dec 2021 10:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 15:11:44 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 06 15:11:38 2021
Response via : Initial Calibration

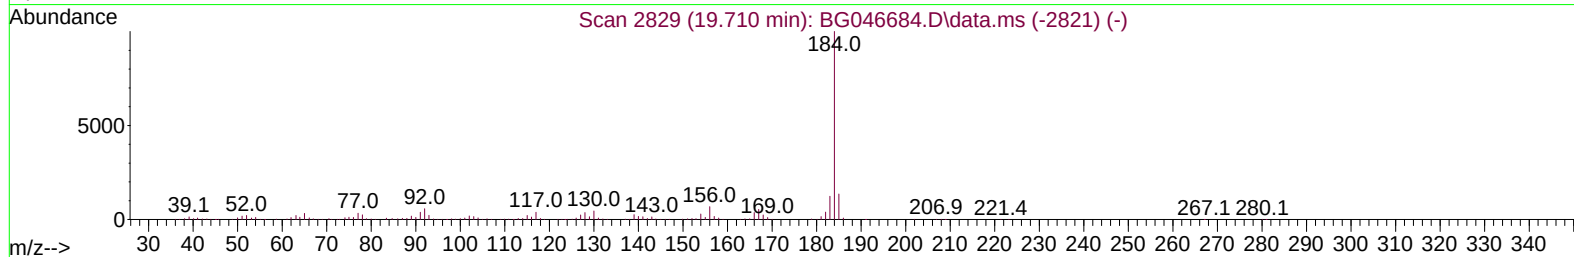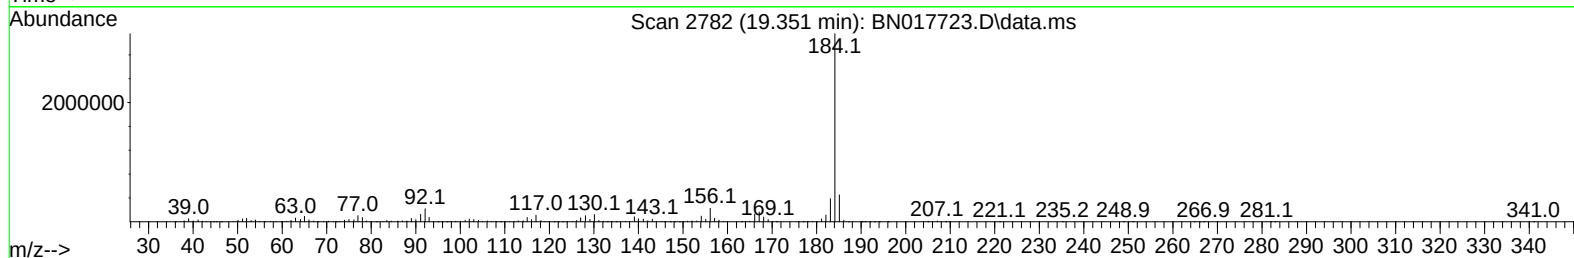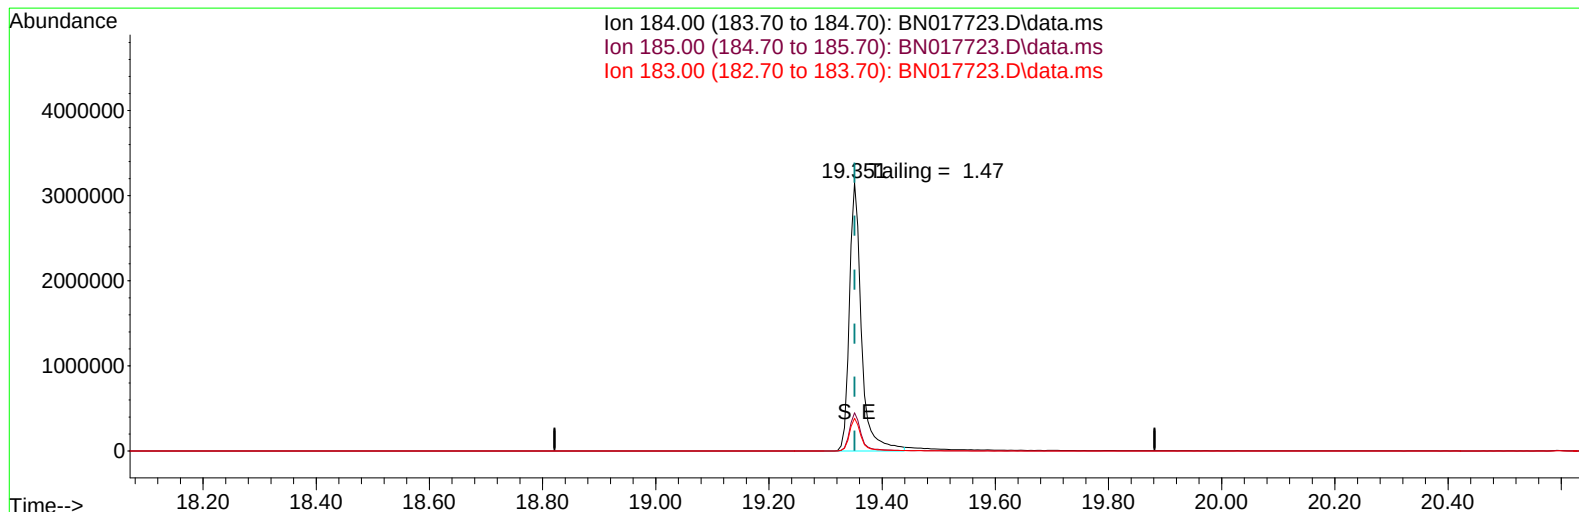

TIC: BN017723.D\data.ms

(77) Benzidine**19.351min (0.000) 693772.14 ng****response 4854573**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.29
183.00	13.20	12.26
0.00	0.00	0.00