

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120621\
 Data File : BN017750.D
 Acq On : 07 Dec 2021 04:21
 Operator : CG/JU
 Sample : M4917-06RE
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DUP120121RE

Quant Time: Dec 07 06:53:45 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN120621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 06 15:58:05 2021
 Response via : Initial Calibration


Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/07/2021
 Supervised By :Sohil Jodhani 12/10/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.771	152	18981	0.400	ng	0.02
7) Naphthalene-d8	10.545	136	76866	0.400	ng	# 0.01
13) Acenaphthene-d10	14.373	164	134238	0.400	ng	# 0.00
19) Phenanthrene-d10	17.117	188	114078	0.400	ng	# 0.00
29) Chrysene-d12	21.304	240	118641	0.400	ng	# 0.00
35) Perylene-d12	23.617	264	110285	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.410	112	33264	0.817	ng	0.06
5) Phenol-d6	6.959	99	7303	0.167	ng	0.03
8) Nitrobenzene-d5	8.910	82	74681m	1.437	ng	0.01
11) 2-Methylnaphthalene-d10	12.130	152	49303	0.350	ng	0.00
14) 2,4,6-Tribromophenol	15.870	330	19415	0.368	ng	0.00
15) 2-Fluorobiphenyl	13.003	172	92131	0.185	ng	0.00
27) Fluoranthene-d10	19.160	212	159097	0.414	ng	0.00
31) Terphenyl-d14	19.755	244	154903	0.509	ng	0.00
Target Compounds						Qvalue
9) Naphthalene	10.608	128	24570632	128.912	ng	# 91
10) Hexachlorobutadiene	10.925	225	9	0.000	ng	# 18
12) 2-Methylnaphthalene	12.219	142	10429688	79.765	ng	# 94
17) Acenaphthene	14.436	154	358302	1.027	ng	# 77
18) Fluorene	15.426	166	802264	1.793	ng	# 94
21) 4-Bromophenyl-phenylether	16.290	248	995	0.015	ng	# 1
22) Hexachlorobenzene	16.460	284	120	0.001	ng	# 42
24) Pentachlorophenol	16.789	266	525	0.191	ng	# 81
25) Phenanthrene	17.166	178	1158790	3.855	ng	# 98
26) Anthracene	17.251	178	35736	0.136	ng	# 76
28) Fluoranthene	19.189	202	33396	0.092	ng	# 93
30) Pyrene	19.547	202	39687	0.089	ng	# 91
32) Benzo(a)anthracene	21.293	228	3019	0.008	ng	# 1
33) Chrysene	21.347	228	3309	0.009	ng	# 1
34) Bis(2-ethylhexyl)phtha...	21.230	149	45672	0.244	ng	# 92
36) Indeno(1,2,3-cd)pyrene	25.982	276	1010	0.004	ng	# 53
37) Benzo(b)fluoranthene	22.919	252	1918	0.005	ng	# 1
38) Benzo(k)fluoranthene	22.963	252	1031	0.003	ng	# 1
39) Benzo(a)pyrene	23.518	252	1553	0.005	ng	# 1
40) Dibenzo(a,h)anthracene	26.003	278	590	0.004	ng	# 1
41) Benzo(g,h,i)perylene	26.711	276	865	0.004	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.771 min Scan# 41
 Delta R.T. 0.019 min
 Lab File: BN017750.D
 Acq: 07 Dec 2021 04:21

Instrument :

BNA_N

ClientSampleId :

DUP120121RE






Tgt Ion:152 Resp: 1898
 Ion Ratio Lower Upper
 152 100
 150 151.1 123.0 184.4
 115 64.2 45.6 68.4


Manual Integrations

APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
 Supervised By :Sohil Jodhani 12/10/2021




#4
 2-Fluorophenol
 Concen: 0.817 ng
 RT: 5.410 min Scan# 233
 Delta R.T. 0.055 min
 Lab File: BN017750.D
 Acq: 07 Dec 2021 04:21




Tgt Ion:112 Resp: 33264
 Ion Ratio Lower Upper
 112 100
 64 0.0 47.6 71.4#
 63 0.0 24.6 37.0#





#5
Phenol-d6
Concen: 0.167 ng
RT: 6.959 min Scan# 401
Delta R.T. 0.028 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21




Instrument :
BNA_N
ClientSampleId :
DUP120121RE




Tgt Ion: 99 Resp: 7300
Ion Ratio Lower Upper
99 100
42 0.0 17.0 25.6
71 0.0 24.8 37.2

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

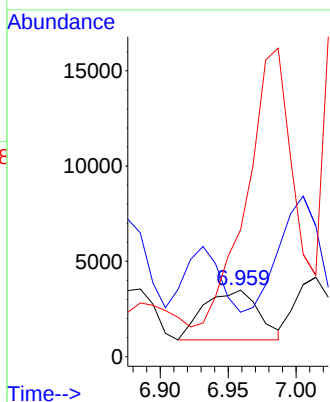


#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.545 min Scan# 724
Delta R.T. 0.013 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21




Tgt Ion:136 Resp: 76866
Ion Ratio Lower Upper
136 100
137 12.6 8.8 13.2
54 22.5 4.0 6.0#
68 17.0 3.0 4.6#





#8
Nitrobenzene-d5
Concen: 1.437 ng m
RT: 8.910 min Scan# 594
Delta R.T. 0.013 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21




Instrument :
BNA_N
ClientSampleId :
DUP120121RE



Tgt Ion: 82 Resp: 7468
Ion Ratio Lower Upper
82 100
128 39.7 27.7 41.5
54 50.2 49.2 73.8




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021



#9
Naphthalene
Concen: 128.912 ng
RT: 10.608 min Scan# 729
Delta R.T. 0.025 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21


Tgt Ion:128 Resp:24570632
Ion Ratio Lower Upper
128 100
129 14.6 8.8 13.2#
127 16.4 10.6 15.8#





#10
Hexachlorobutadiene
Concen: 0.000 ng
RT: 10.925 min Scan# 71
Delta R.T. 0.038 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21




Instrument :
BNA_N
ClientSampleId :
DUP120121RE



Tgt Ion:225 Resp:
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 0.0 51.1 76.7




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021



#11
2-Methylnaphthalene-d10
Concen: 0.350 ng
RT: 12.130 min Scan# 938
Delta R.T. 0.004 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21

Tgt Ion:152 Resp: 49303
Ion Ratio Lower Upper
152 100
151 30.5 16.2 24.4






#12
2-Methylnaphthalene
Concen: 79.765 ng
RT: 12.219 min Scan# 91
Delta R.T. 0.018 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21

Instrument :

BNA_N

ClientSampleId :

DUP120121RE






Tgt Ion:142 Resp:1042968
Ion Ratio Lower Upper
142 100
141 86.1 70.6 106.0
115 40.8 25.8 38.6


Manual Integrations

APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

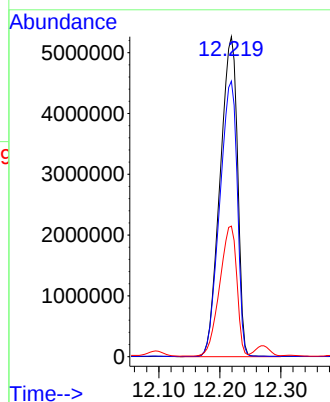


#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.373 min Scan# 1170
Delta R.T. 0.000 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21



Tgt Ion:164 Resp: 134238
Ion Ratio Lower Upper
164 100
162 108.5 81.4 122.2
160 129.1 36.8 55.2#






#14
2,4,6-Tribromophenol
Concen: 0.368 ng
RT: 15.870 min Scan# 1288
Delta R.T. 0.000 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21

Instrument :

BNA_N

ClientSampleId :

DUP120121RE






Tgt Ion:330 Resp: 19415
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 104.8 28.9 43.3


Manual Integrations

APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

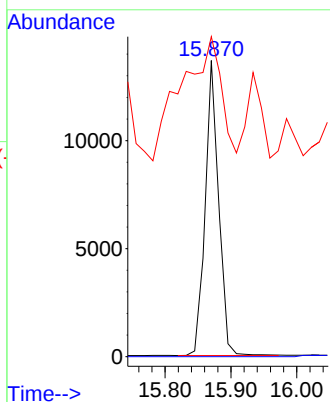


#15
2-Fluorobiphenyl
Concen: 0.185 ng
RT: 13.003 min Scan# 1062
Delta R.T. 0.000 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21




Tgt Ion:172 Resp: 92131
Ion Ratio Lower Upper
172 100
171 35.4 28.7 43.1
170 24.0 19.4 29.2





#17
Acenaphthene
Concen: 1.027 ng
RT: 14.436 min Scan# 1175
Delta R.T. 0.000 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21




Instrument :
BNA_N
ClientSampleId :
DUP120121RE




Tgt Ion:154 Resp: 358302
Ion Ratio Lower Upper
154 100
153 129.9 91.2 136.8
152 84.1 44.3 66.5

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

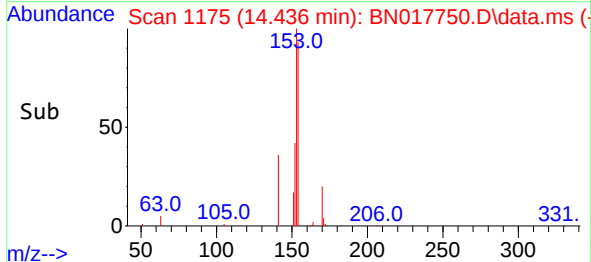


#18
Fluorene
Concen: 1.793 ng
RT: 15.426 min Scan# 1253
Delta R.T. 0.000 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21

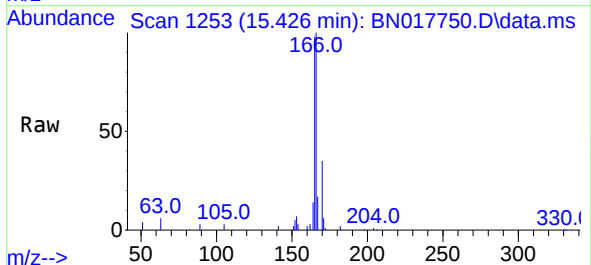


Tgt Ion:166 Resp: 802264
Ion Ratio Lower Upper
166 100
165 101.0 77.9 116.9
167 24.1 10.9 16.3

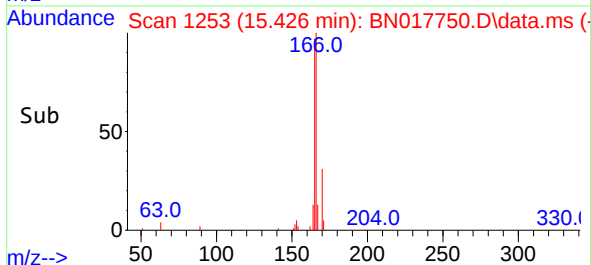



#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.117 min Scan# 114078
Delta R.T. 0.000 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21




Instrument :
BNA_N
ClientSampleId :
DUP120121RE




Tgt Ion:188 Resp: 114078
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 14.4 6.1 9.1

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

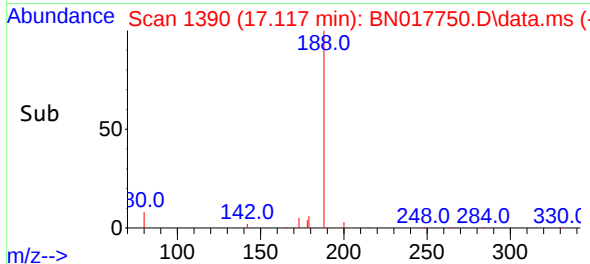


#21
4-Bromophenyl-phenylether
Concen: 0.015 ng
RT: 16.290 min Scan# 1322
Delta R.T. -0.024 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21

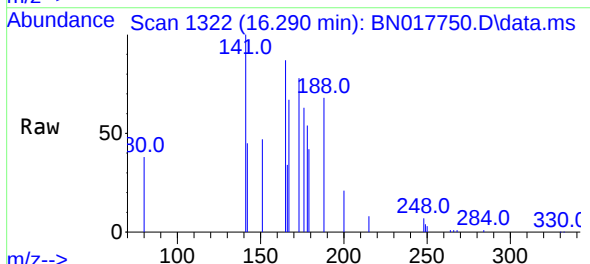


Tgt Ion:248 Resp: 995
Ion Ratio Lower Upper
248 100
250 37.9 71.8 107.8#
141 1443.5 70.9 106.3#

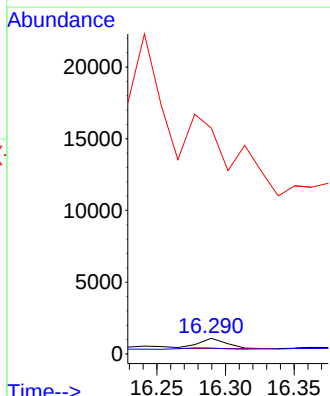



#22
Hexachlorobenzene
Concen: 0.001 ng
RT: 16.460 min Scan# 1336
Delta R.T. 0.024 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21




Instrument :
BNA_N
ClientSampleId :
DUP120121RE




Tgt Ion:284 Resp: 120
Ion Ratio Lower Upper
284 100
142 0.0 28.2 42.2
249 0.0 24.4 36.6

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021




#24
Pentachlorophenol
Concen: 0.191 ng
RT: 16.789 min Scan# 1363
Delta R.T. -0.000 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21

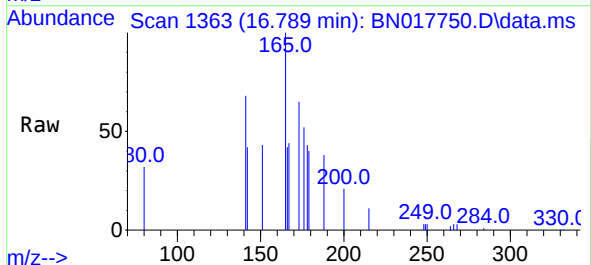


Tgt Ion:266 Resp: 525
Ion Ratio Lower Upper
266 100
264 50.3 49.8 74.8
268 81.1 51.3 76.9

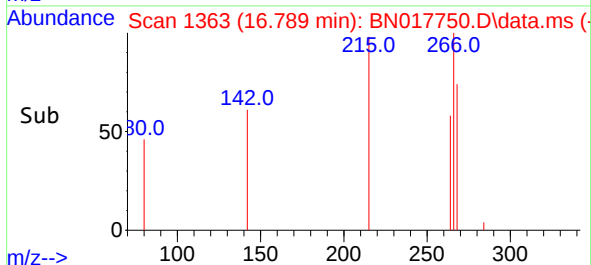



#25
Phenanthrene
Concen: 3.855 ng
RT: 17.166 min Scan# 11
Delta R.T. 0.012 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21




Instrument :
BNA_N
ClientSampleId :
DUP120121RE



Tgt Ion:178 Resp: 1158790
Ion Ratio Lower Upper
178 100
176 18.6 15.0 22.6
179 17.2 12.3 18.5




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

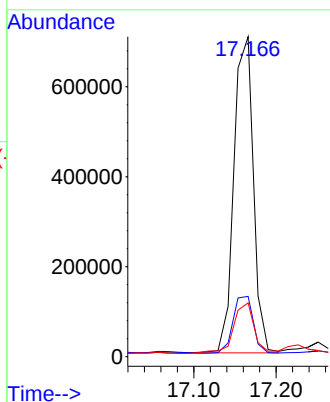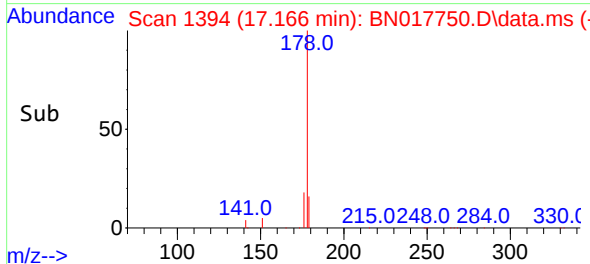

#26
Anthracene
Concen: 0.136 ng
RT: 17.251 min Scan# 1401
Delta R.T. 0.000 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21


Tgt Ion:178 Resp: 35736
Ion Ratio Lower Upper
178 100
176 24.1 14.6 22.0#
179 0.0 12.2 18.4#

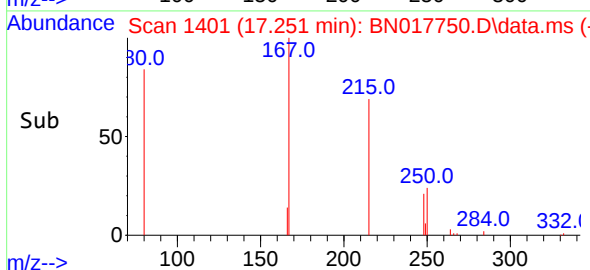



#27
Fluoranthene-d10
Concen: 0.414 ng
RT: 19.160 min Scan# 10
Delta R.T. 0.005 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21




Instrument :
BNA_N
ClientSampleId :
DUP120121RE




Tgt Ion:212 Resp: 159097
Ion Ratio Lower Upper
212 100
106 9.7 10.5 15.7
104 7.6 5.8 8.6

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

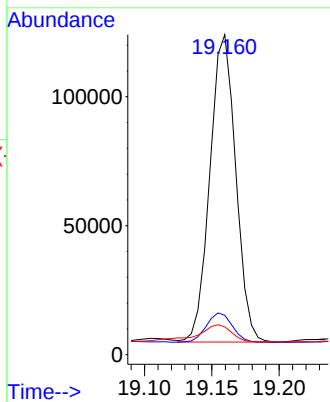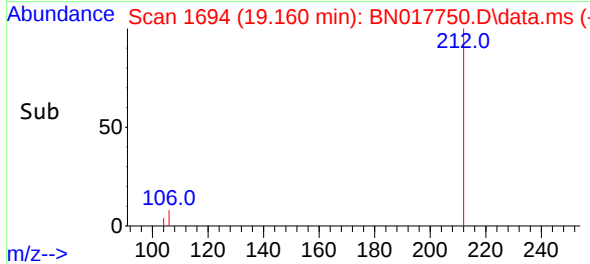


#28
Fluoranthene
Concen: 0.092 ng
RT: 19.189 min Scan# 1700
Delta R.T. 0.010 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21

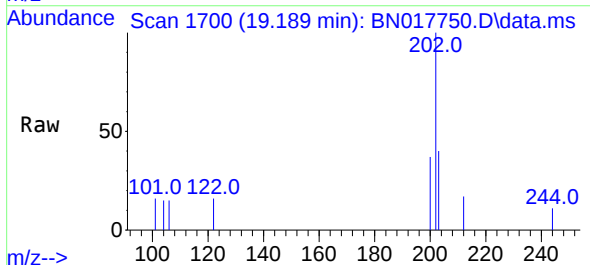


Tgt Ion:202 Resp: 33396
Ion Ratio Lower Upper
202 100
101 8.6 8.9 13.3
203 20.1 13.8 20.6

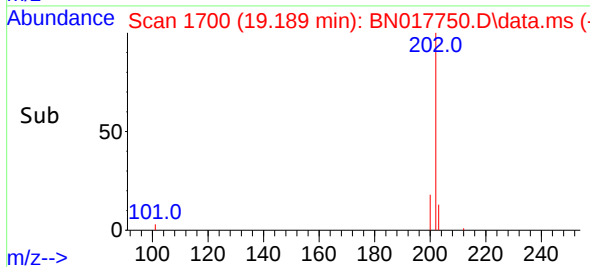



#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.304 min Scan# 1987
Delta R.T. 0.000 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21




Instrument :
BNA_N
ClientSampleId :
DUP120121RE




Tgt Ion:240 Resp: 11864
Ion Ratio Lower Upper
240 100
120 12.9 4.2 6.2
236 28.9 20.0 30.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

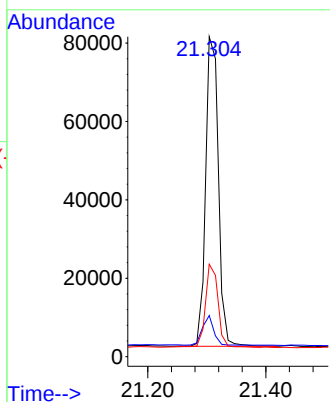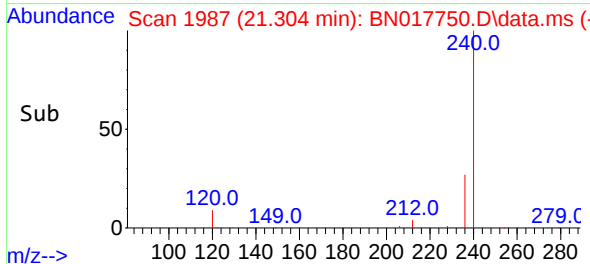


#30
Pyrene
Concen: 0.089 ng
RT: 19.547 min Scan# 1772
Delta R.T. 0.005 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21

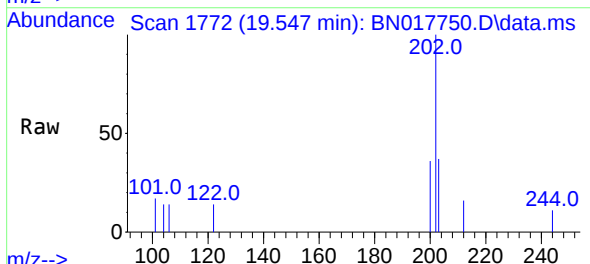

Tgt Ion:202 Resp: 39687
Ion Ratio Lower Upper
202 100
200 21.1 16.5 24.7
203 25.3 14.0 21.0






#31
 Terphenyl-d14
 Concen: 0.509 ng
 RT: 19.755 min Scan# 1814
 Delta R.T. 0.000 min
 Lab File: BN017750.D
 Acq: 07 Dec 2021 04:21

Instrument :

BNA_N

ClientSampleId :

DUP120121RE






Tgt Ion:244 Resp: 15490
 Ion Ratio Lower Upper
 244 100
 212 10.9 5.7 8.5#
 122 11.7 8.6 13.0#


Manual Integrations

APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
 Supervised By :Sohil Jodhani 12/10/2021

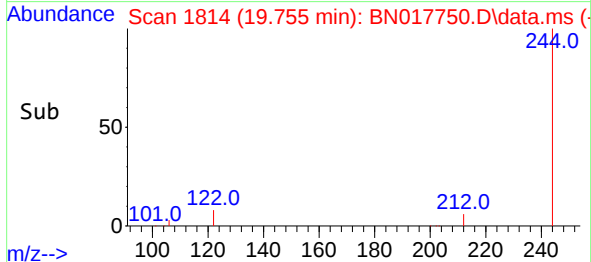


#32
 Benzo(a)anthracene
 Concen: 0.008 ng
 RT: 21.293 min Scan# 1986
 Delta R.T. 0.000 min
 Lab File: BN017750.D
 Acq: 07 Dec 2021 04:21




Tgt Ion:228 Resp: 3019
 Ion Ratio Lower Upper
 228 100
 226 76.4 21.3 31.9#
 229 88.4 15.7 23.5#





#33
Chrysene
Concen: 0.009 ng
RT: 21.347 min Scan# 1991
Delta R.T. 0.000 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21




Instrument :
BNA_N
ClientSampleId :
DUP120121RE




Tgt Ion:228 Resp: 3309
Ion Ratio Lower Upper
228 100
226 76.0 23.3 34.9
229 89.2 15.6 23.4

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

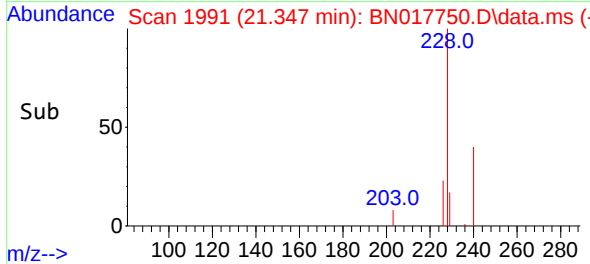


#34
Bis(2-ethylhexyl)phthalate
Concen: 0.244 ng
RT: 21.230 min Scan# 1980
Delta R.T. 0.000 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21

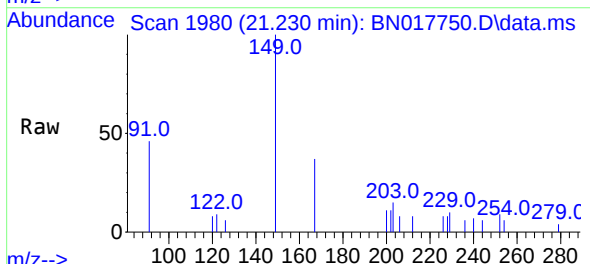


Tgt Ion:149 Resp: 45672
Ion Ratio Lower Upper
149 100
167 31.9 21.8 32.6
279 5.2 3.4 5.0





#35
Perylene-d12
Concen: 0.400 ng
RT: 23.617 min Scan# 2443
Delta R.T. 0.003 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21




Instrument :
BNA_N
ClientSampleId :
DUP120121RE




Tgt Ion:264 Resp: 110285
Ion Ratio Lower Upper
264 100
260 25.6 19.4 29.2
265 28.9 18.6 28.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

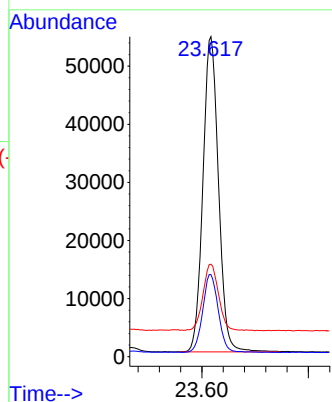


#36
Indeno(1,2,3-cd)pyrene
Concen: 0.004 ng
RT: 25.982 min Scan# 3135
Delta R.T. -0.010 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21




Tgt Ion:276 Resp: 1010
Ion Ratio Lower Upper
276 100
138 57.2 19.7 29.5#
277 10.7 20.0 30.0#

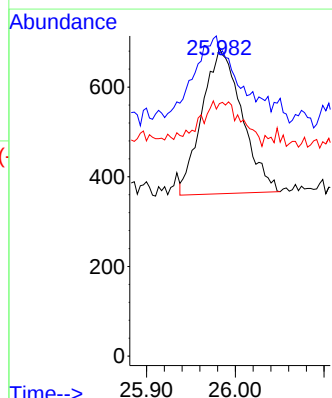



#37
Benzo(b)fluoranthene
Concen: 0.005 ng
RT: 22.919 min Scan# 2118
Delta R.T. 0.000 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21




Instrument :
BNA_N
ClientSampleId :
DUP120121RE




Tgt Ion:252 Resp: 1918
Ion Ratio Lower Upper
252 100
253 101.8 17.7 26.5#
125 90.0 7.8 11.8#

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

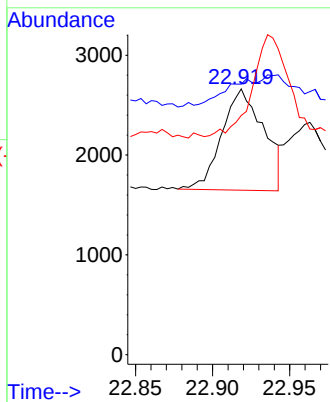


#38
Benzo(k)fluoranthene
Concen: 0.003 ng
RT: 22.963 min Scan# 2253
Delta R.T. 0.000 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21

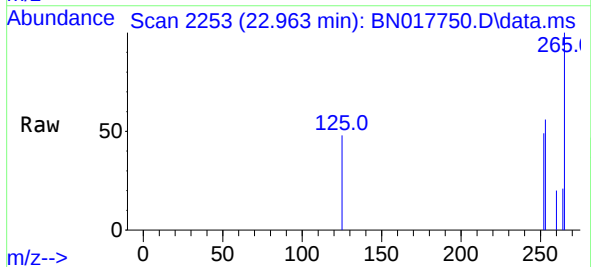


Tgt Ion:252 Resp: 1031
Ion Ratio Lower Upper
252 100
253 113.3 17.7 26.5#
125 97.1 8.2 12.2#

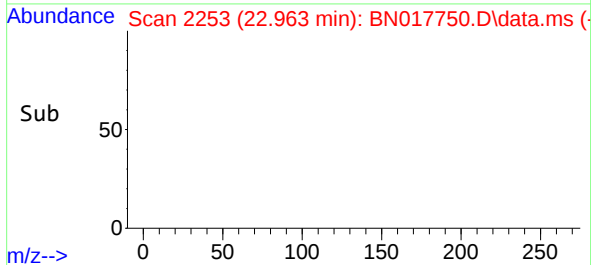



#39
Benzo(a)pyrene
Concen: 0.005 ng
RT: 23.518 min Scan# 2414
Delta R.T. 0.003 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21




Instrument :
BNA_N
ClientSampleId :
DUP120121RE



Tgt Ion:252 Resp: 155
Ion Ratio Lower Upper
252 100
253 119.0 17.9 26.9#
125 107.6 9.2 13.8#




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

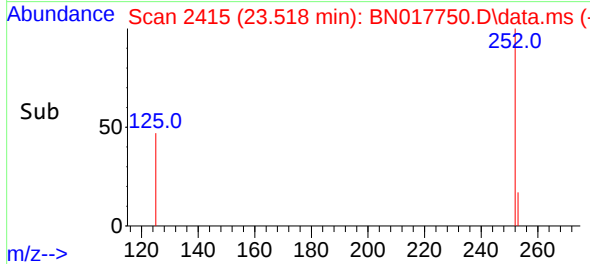

#40
Dibenzo(a,h)anthracene
Concen: 0.004 ng
RT: 26.003 min Scan# 3141
Delta R.T. -0.010 min
Lab File: BN017750.D
Acq: 07 Dec 2021 04:21

Tgt Ion:278 Resp: 590
Ion Ratio Lower Upper
278 100
139 210.2 13.0 19.6#
279 125.9 19.2 28.8#

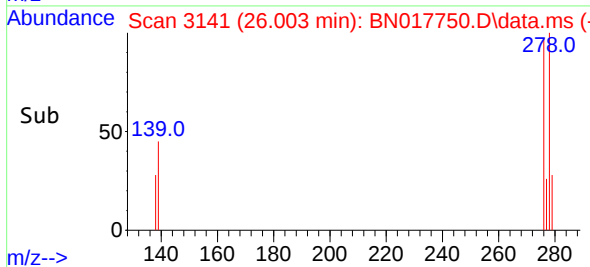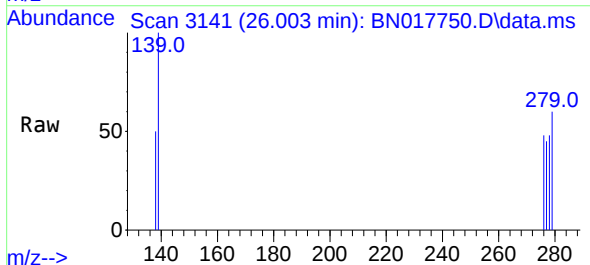

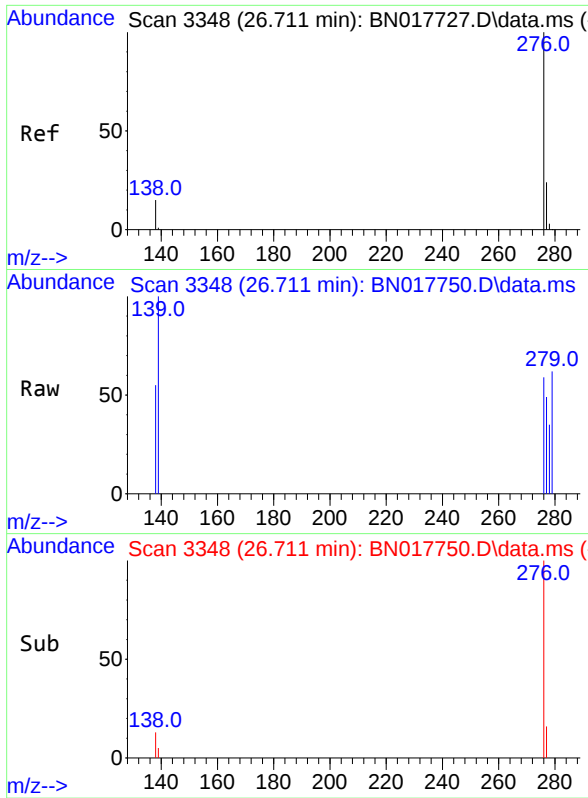

#41

Benzo(g,h,i)perylene

Concen: 0.004 ng

RT: 26.711 min Scan# 31

Delta R.T. 0.000 min

Lab File: BN017750.D

Acq: 07 Dec 2021 04:21

Instrument :

BNA_N

ClientSampleId :

DUP120121RE

Tgt Ion:276 Resp: 86

Ion Ratio Lower Upper

276 100

277 83.0 19.0 28.4

138 93.9 17.1 25.7

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 12/07/2021

Supervised By :Sohil Jodhani 12/10/2021

