

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120621\
 Data File : BN017753.D
 Acq On : 07 Dec 2021 06:09
 Operator : CG/JU
 Sample : M4918-06
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MW-40

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/07/2021
 Supervised By :Sohil Jodhani 12/10/2021

Quant Time: Dec 07 07:31:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN120621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 06 15:58:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.761	152	22924	0.400	ng	0.00
7) Naphthalene-d8	10.532	136	94274	0.400	ng	# 0.00
13) Acenaphthene-d10	14.373	164	96248	0.400	ng	0.00
19) Phenanthrene-d10	17.117	188	132114	0.400	ng	# 0.00
29) Chrysene-d12	21.304	240	132578	0.400	ng	# 0.00
35) Perylene-d12	23.617	264	124900	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.382	112	10975	0.223	ng	0.03
5) Phenol-d6	6.950	99	5191	0.098	ng	0.02
8) Nitrobenzene-d5	8.897	82	69604m	1.092	ng	0.00
11) 2-Methylnaphthalene-d10	12.125	152	53709	0.311	ng	0.00
14) 2,4,6-Tribromophenol	15.870	330	18483	0.444	ng	0.00
15) 2-Fluorobiphenyl	13.003	172	100404	0.282	ng	0.00
27) Fluoranthene-d10	19.154	212	156408	0.352	ng	0.00
31) Terphenyl-d14	19.755	244	148234	0.436	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.326	88	814	0.054	ng	# 47
9) Naphthalene	10.583	128	12238	0.052	ng	# 55
10) Hexachlorobutadiene	10.874	225	29	0.000	ng	# 49
12) 2-Methylnaphthalene	12.197	142	7878	0.049	ng	# 57
16) Acenaphthylene	14.094	152	2066	0.006	ng	# 1
17) Acenaphthene	14.436	154	3046	0.012	ng	# 89
18) Fluorene	15.426	166	2081	0.006	ng	# 91
21) 4-Bromophenyl-phenylether	16.289	248	324	0.004	ng	# 1
22) Hexachlorobenzene	16.436	284	110	0.001	ng	# 1
24) Pentachlorophenol	16.776	266	602	0.190	ng	# 80
25) Phenanthrene	17.154	178	4829	0.014	ng	# 1
26) Anthracene	17.251	178	4395	0.014	ng	# 1
28) Fluoranthene	19.184	202	3417	0.008	ng	# 70
30) Pyrene	19.547	202	3111	0.006	ng	# 49
32) Benzo(a)anthracene	21.293	228	1702	0.004	ng	# 1
33) Chrysene	21.346	228	1445	0.003	ng	# 1
34) Bis(2-ethylhexyl)phtha...	21.240	149	140989	0.674	ng	97
36) Indeno(1,2,3-cd)pyrene	25.982	276	772	0.003	ng	# 59
37) Benzo(b)fluoranthene	22.918	252	1296	0.003	ng	# 1
38) Benzo(k)fluoranthene	22.959	252	830	0.002	ng	# 1
39) Benzo(a)pyrene	23.511	252	911	0.003	ng	# 1
40) Dibenzo(a,h)anthracene	25.999	278	530	0.003	ng	# 1
41) Benzo(g,h,i)perylene	26.704	276	780	0.003	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120621\
Data File : BN017753.D
Acq On : 07 Dec 2021 06:09
Operator : CG/JU
Sample : M4918-06
Misc :
ALS Vial : 30 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
MW-40

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021


Quant Time: Dec 07 07:31:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN120621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 06 15:58:05 2021
Response via : Initial Calibration

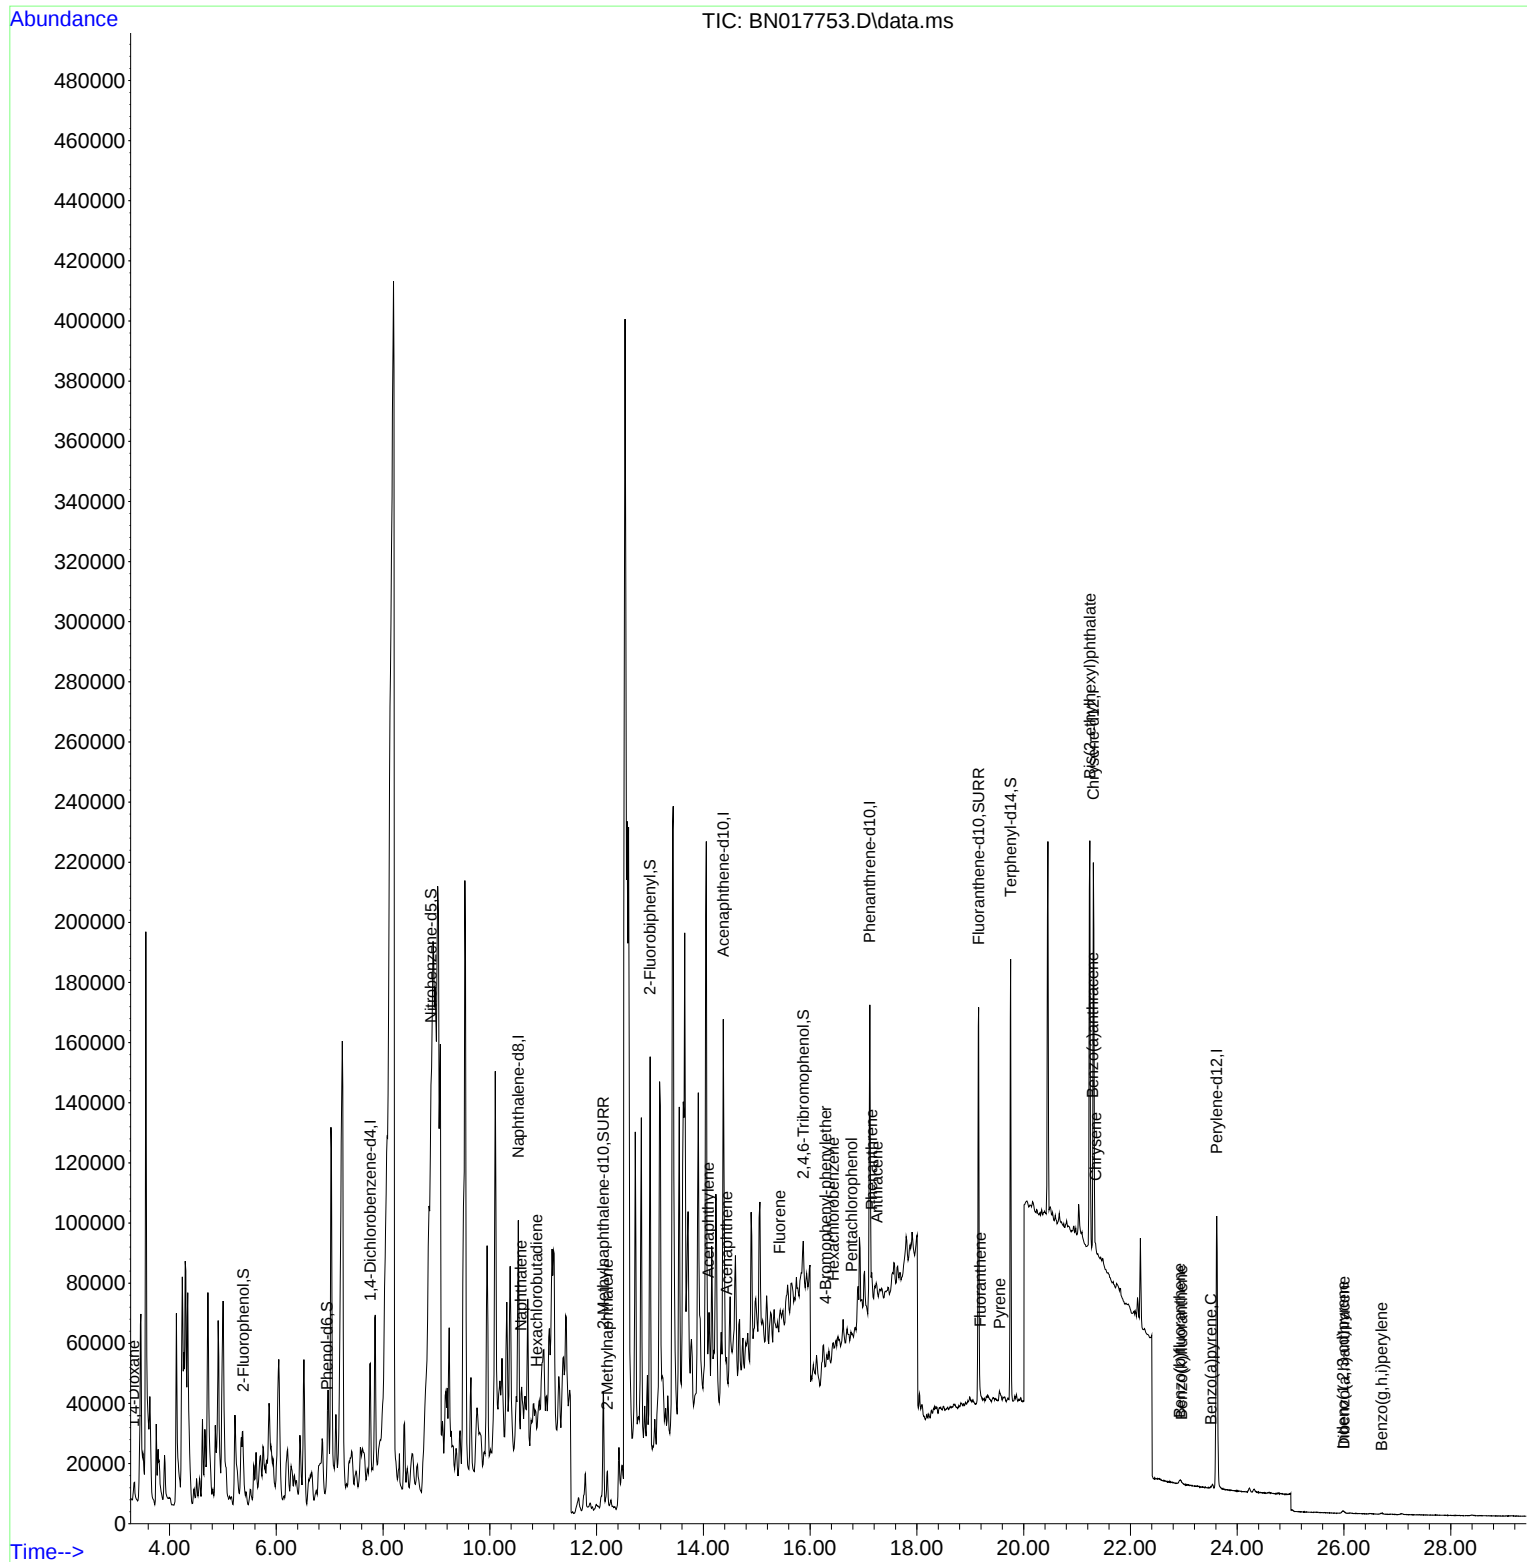

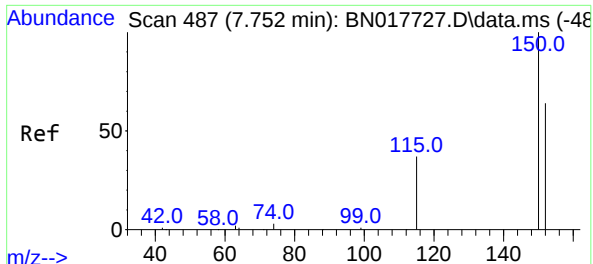

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.761 min Scan# 41
Delta R.T. 0.009 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09




Instrument :
BNA_N
ClientSampleId :
MW-40

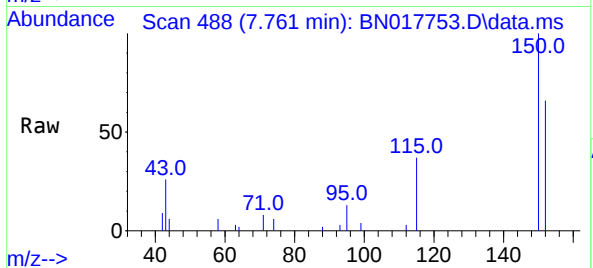


Tgt Ion:152 Resp: 22924
Ion Ratio Lower Upper
152 100
150 151.0 123.0 184.4
115 56.4 45.6 68.4

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

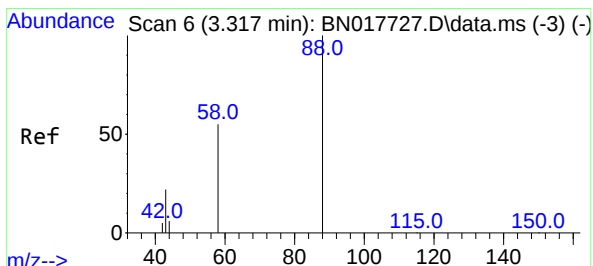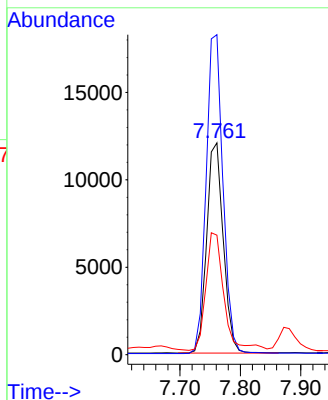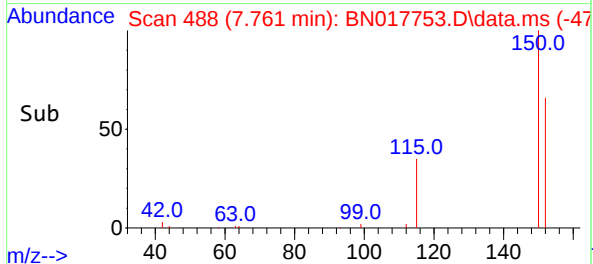


#2
1,4-Dioxane
Concen: 0.054 ng
RT: 3.326 min Scan# 7
Delta R.T. 0.009 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09

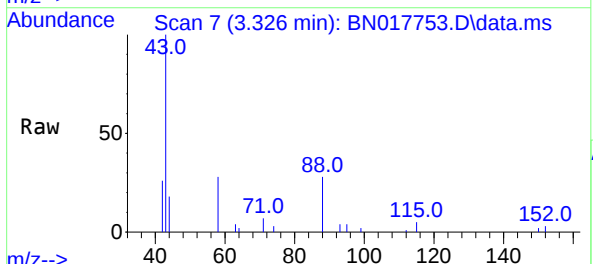

Tgt Ion: 88 Resp: 814
Ion Ratio Lower Upper
88 100
43 0.0 24.7 37.1#
58 124.4 63.0 94.6#

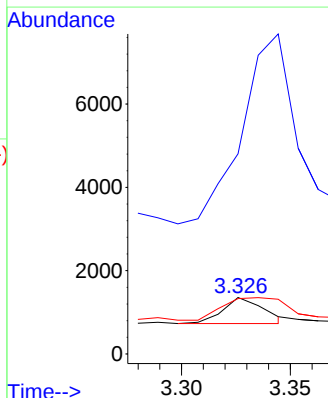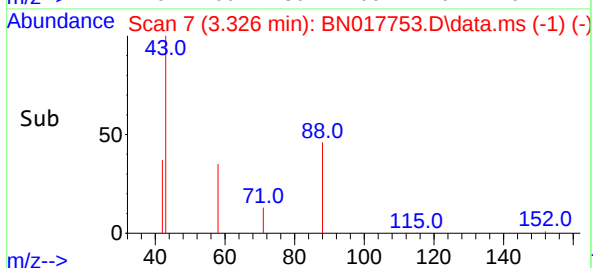



#4
2-Fluorophenol
Concen: 0.223 ng
RT: 5.382 min Scan# 21
Delta R.T. 0.027 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09

Instrument :

BNA_N

ClientSampleId :





MW-40

Tgt Ion:112 Resp: 1097
Ion Ratio Lower Upper
112 100
64 46.4 47.6 71.4
63 21.0 24.6 37.0

Manual Integrations




APPROVED


Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

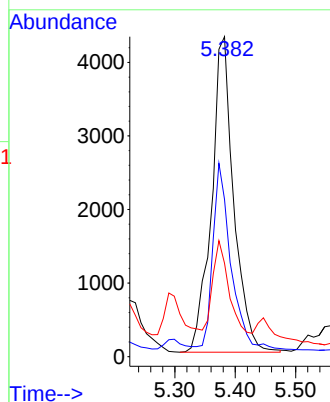

#5
Phenol-d6
Concen: 0.098 ng
RT: 6.950 min Scan# 400
Delta R.T. 0.018 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09


Tgt Ion: 99 Resp: 5191
Ion Ratio Lower Upper
99 100
42 66.2 17.0 25.6#
71 440.5 24.8 37.2#

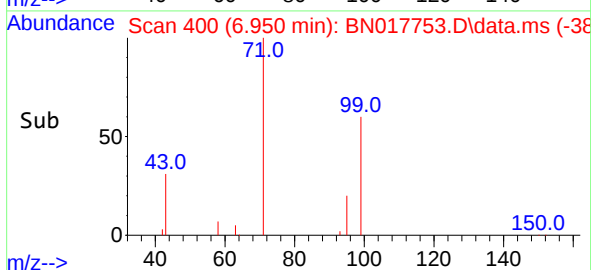



#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.532 min Scan# 723
Delta R.T. -0.000 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09




Instrument :
BNA_N
ClientSampleId :
MW-40



Tgt Ion:136 Resp: 94274
Ion Ratio Lower Upper
136 100
137 11.6 8.8 13.2
54 11.2 4.0 6.0
68 10.2 3.0 4.6




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

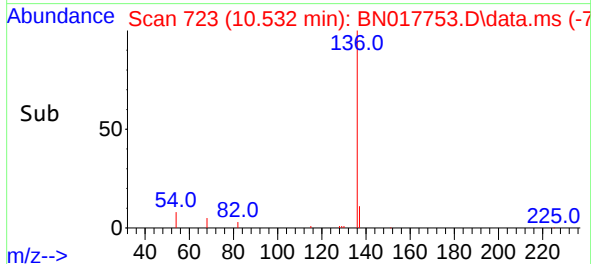

#8
Nitrobenzene-d5
Concen: 1.092 ng m
RT: 8.897 min Scan# 594
Delta R.T. -0.000 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09


Tgt Ion: 82 Resp: 69604
Ion Ratio Lower Upper
82 100
128 25.6 27.7 41.5
54 62.2 49.2 73.8

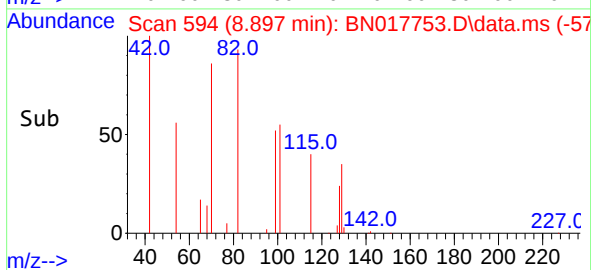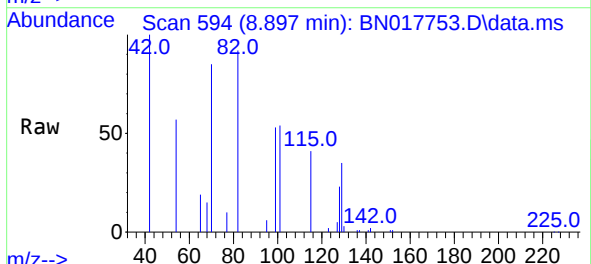

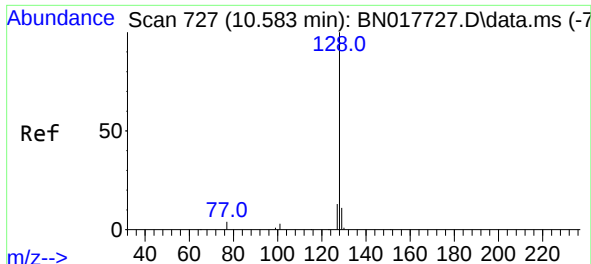

#9
Naphthalene
Concen: 0.052 ng
RT: 10.583 min Scan# 71
Delta R.T. -0.000 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09




Instrument :
BNA_N
ClientSampleId :
MW-40




Tgt Ion:128 Resp: 12238
Ion Ratio Lower Upper
128 100
129 26.5 8.8 13.2
127 32.3 10.6 15.8

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

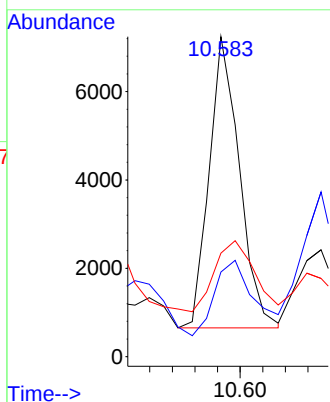


#10
Hexachlorobutadiene
Concen: 0.000 ng
RT: 10.874 min Scan# 750
Delta R.T. -0.013 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09

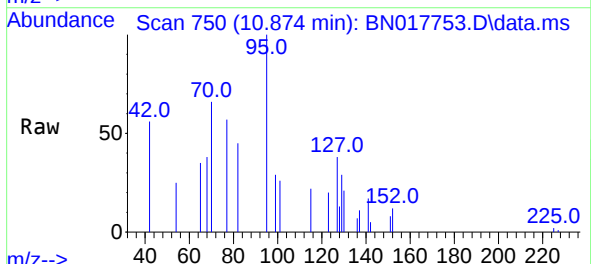

Tgt Ion:225 Resp: 29
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 103.4 51.1 76.7



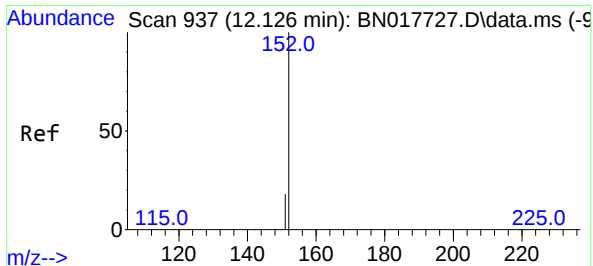

#11

2-Methylnaphthalene-d10

Concen: 0.311 ng

RT: 12.125 min Scan# 911

Delta R.T. -0.000 min

Lab File: BN017753.D

Acq: 07 Dec 2021 06:09

Instrument :

BNA_N

ClientSampleId :

MW-40

Tgt Ion:152 Resp: 53709

Ion Ratio Lower Upper

152 100





151 22.2 16.2 24.4

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 12/07/2021

Supervised By :Sohil Jodhani 12/10/2021

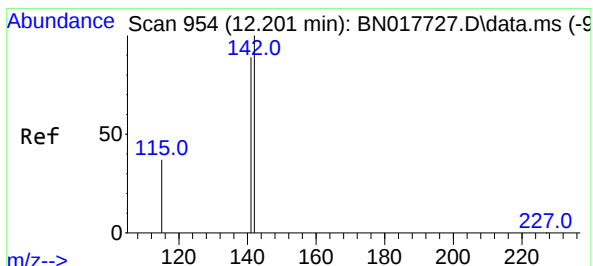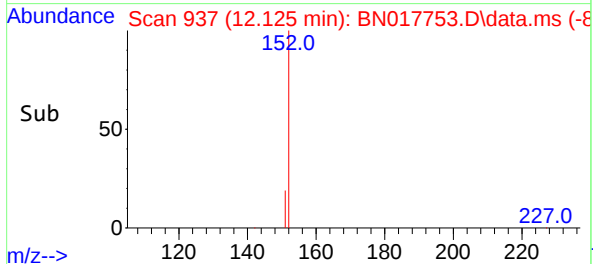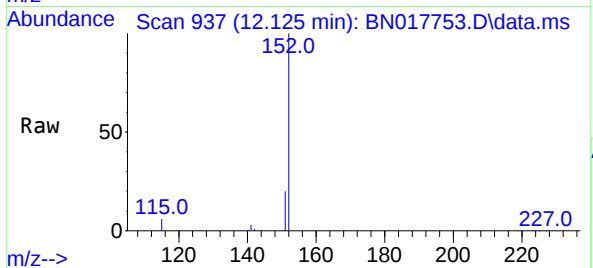

#12

2-Methylnaphthalene

Concen: 0.049 ng

RT: 12.197 min Scan# 953

Delta R.T. -0.005 min

Lab File: BN017753.D

Acq: 07 Dec 2021 06:09




Tgt Ion:142 Resp: 7878


Ion Ratio Lower Upper

142 100

141 102.8 70.6 106.0


115 97.4 25.8 38.6#

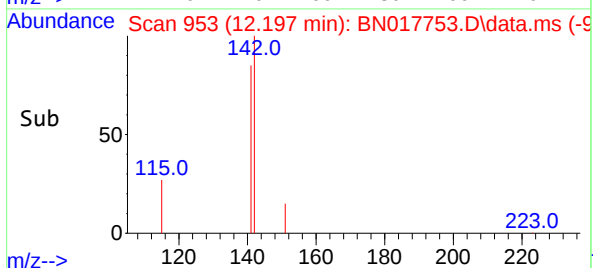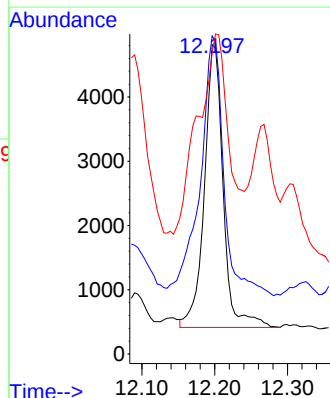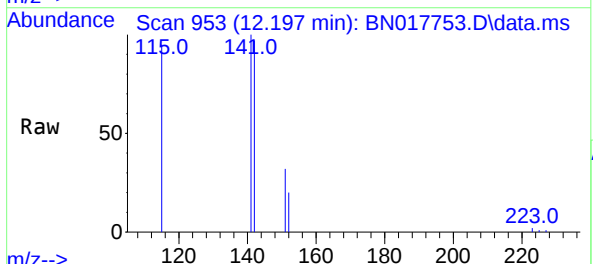



#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.373 min Scan# 1170
Delta R.T. -0.000 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09




Instrument :
BNA_N
ClientSampleId :
MW-40

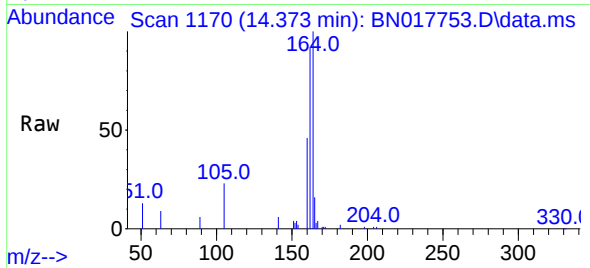


Tgt Ion:164 Resp: 96248
Ion Ratio Lower Upper
164 100
162 92.1 81.4 122.2
160 45.7 36.8 55.2

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

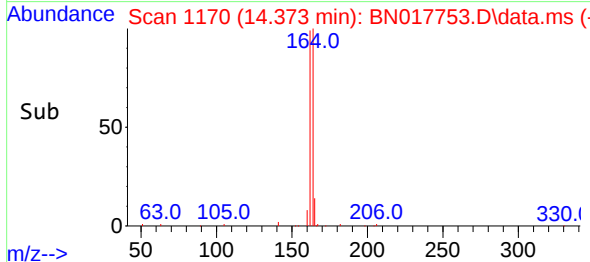


#14
2,4,6-Tribromophenol
Concen: 0.444 ng
RT: 15.870 min Scan# 1288
Delta R.T. -0.000 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09




Tgt Ion:330 Resp: 18483
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 31.2 28.9 43.3

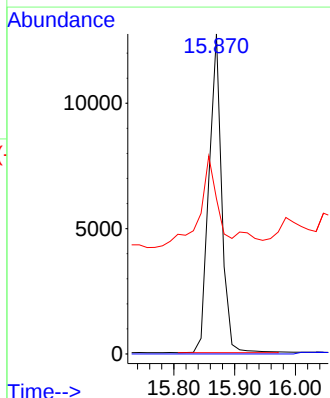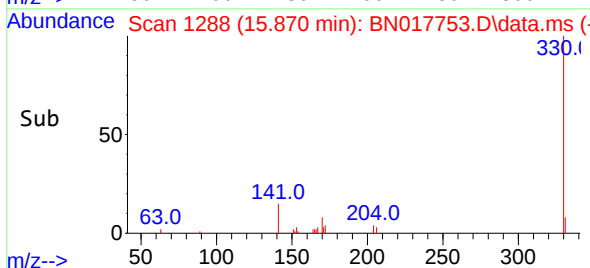



#15
2-Fluorobiphenyl
Concen: 0.282 ng
RT: 13.003 min Scan# 1062
Delta R.T. -0.000 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09




Instrument :
BNA_N
ClientSampleId :
MW-40




Tgt Ion:172 Resp: 100404
Ion Ratio Lower Upper
172 100
171 34.9 28.7 43.1
170 23.2 19.4 29.2

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

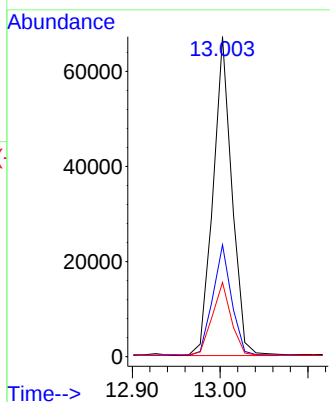


#16
Acenaphthylene
Concen: 0.006 ng
RT: 14.094 min Scan# 1148
Delta R.T. -0.000 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09




Tgt Ion:152 Resp: 2066
Ion Ratio Lower Upper
152 100
151 174.2 15.5 23.3#
153 85.7 10.4 15.6#

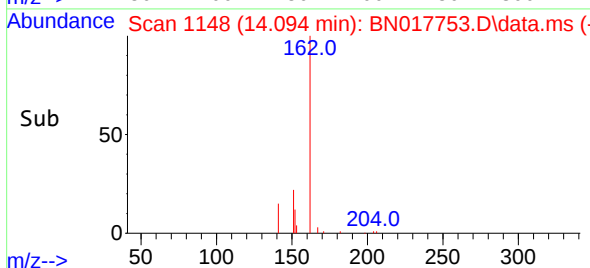



#17
Acenaphthene
Concen: 0.012 ng
RT: 14.436 min Scan# 1175
Delta R.T. -0.000 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09




Instrument :
BNA_N
ClientSampleId :
MW-40




Tgt Ion:154 Resp: 3040
Ion Ratio Lower Upper
154 100
153 123.1 91.2 136.8
152 68.3 44.3 66.5

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

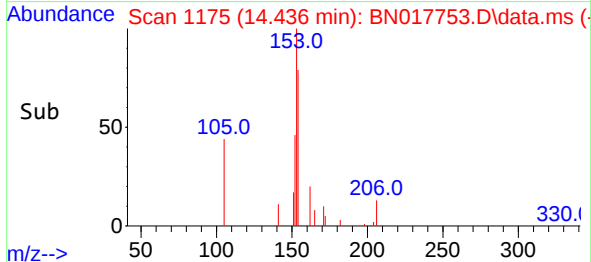


#18
Fluorene
Concen: 0.006 ng
RT: 15.426 min Scan# 1253
Delta R.T. -0.000 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09

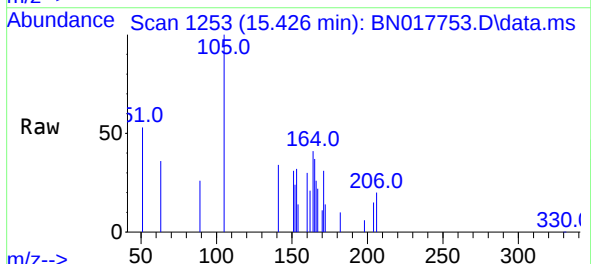


Tgt Ion:166 Resp: 2081
Ion Ratio Lower Upper
166 100
165 89.1 77.9 116.9
167 18.5 10.9 16.3

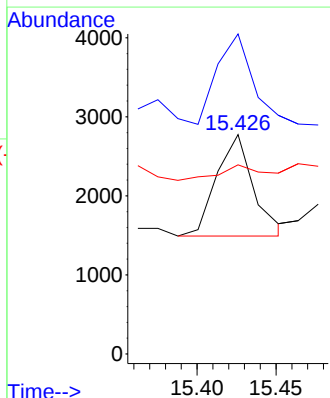



#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.117 min Scan# 1390
Delta R.T. 0.000 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09




Instrument :
BNA_N
ClientSampleId :
MW-40




Tgt Ion:188 Resp: 132114
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.9 6.1 9.1

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021




#21
4-Bromophenyl-phenylether
Concen: 0.004 ng
RT: 16.289 min Scan# 1322
Delta R.T. -0.024 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09




Tgt Ion:248 Resp: 324
Ion Ratio Lower Upper
248 100
250 62.0 71.8 107.8#
141 1249.4 70.9 106.3#

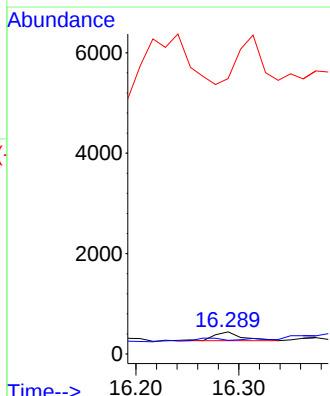



#22
Hexachlorobenzene
Concen: 0.001 ng
RT: 16.436 min Scan# 110
Delta R.T. -0.000 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09




Instrument :
BNA_N
ClientSampleId :
MW-40




Tgt Ion:284 Resp: 110
Ion Ratio Lower Upper
284 100
142 3088.2 28.2 42.2
249 81.8 24.4 36.6

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

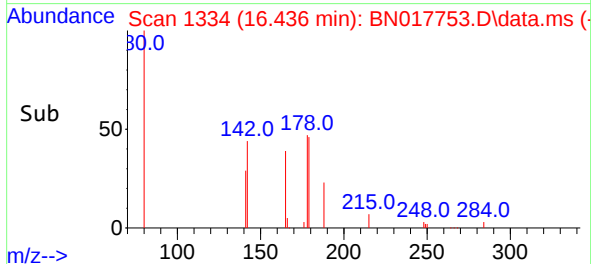


#24
Pentachlorophenol
Concen: 0.190 ng
RT: 16.776 min Scan# 1362
Delta R.T. -0.013 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09

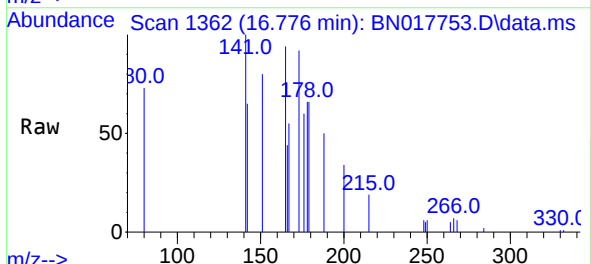


Tgt Ion:266 Resp: 602
Ion Ratio Lower Upper
266 100
264 41.5 49.8 74.8#
268 54.2 51.3 76.9

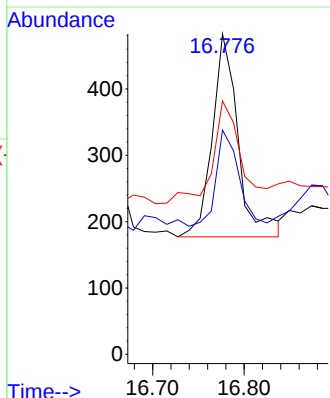



#25
Phenanthrene
Concen: 0.014 ng
RT: 17.154 min Scan# 1393
Delta R.T. -0.000 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09




Instrument :
BNA_N
ClientSampleId :
MW-40




Tgt Ion:178 Resp: 4829
Ion Ratio Lower Upper
178 100
176 86.9 15.0 22.6
179 0.0 12.3 18.5

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

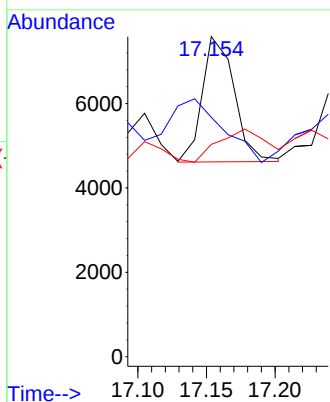


#26
Anthracene
Concen: 0.014 ng
RT: 17.251 min Scan# 1401
Delta R.T. -0.000 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09




Tgt Ion:178 Resp: 4395
Ion Ratio Lower Upper
178 100
176 166.5 14.6 22.0#
179 0.0 12.2 18.4#

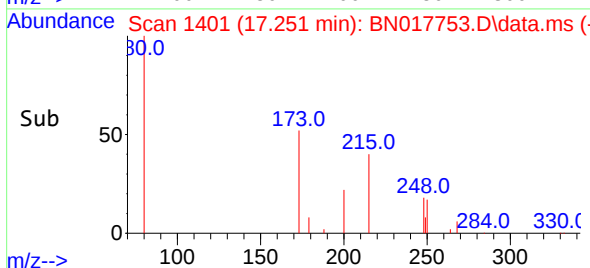



#27
Fluoranthene-d10
Concen: 0.352 ng
RT: 19.154 min Scan# 1693
Delta R.T. -0.000 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09




Instrument :
BNA_N
ClientSampleId :
MW-40




Tgt Ion:212 Resp: 156408
Ion Ratio Lower Upper
212 100
106 9.8 10.5 15.7#
104 5.6 5.8 8.6#

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

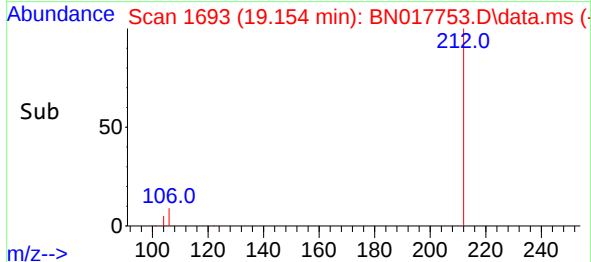


#28
Fluoranthene
Concen: 0.008 ng
RT: 19.184 min Scan# 1699
Delta R.T. 0.005 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09

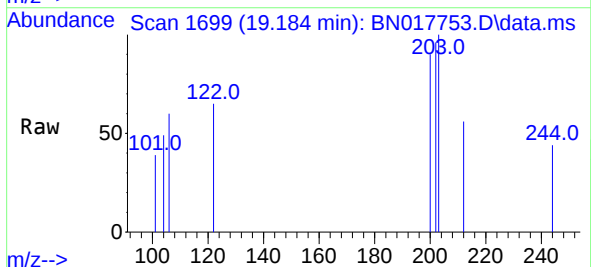


Tgt Ion:202 Resp: 3417
Ion Ratio Lower Upper
202 100
101 4.2 8.9 13.3#
203 33.7 13.8 20.6#

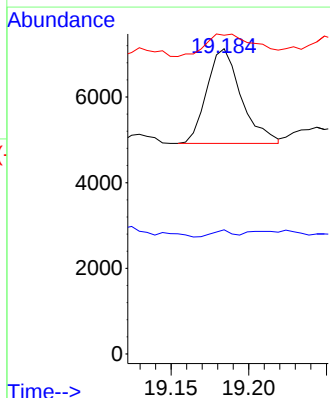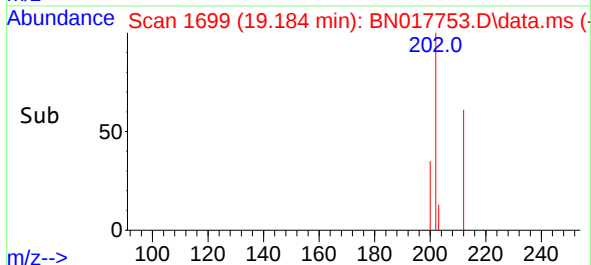



#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.304 min Scan# 1987
Delta R.T. -0.000 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09




Instrument :
BNA_N
ClientSampleId :
MW-40




Tgt Ion:240 Resp: 132578
Ion Ratio Lower Upper
240 100
120 12.6 4.2 6.2#
236 28.1 20.0 30.0#

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

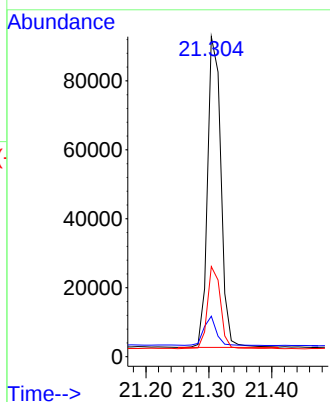


#30
Pyrene
Concen: 0.006 ng
RT: 19.547 min Scan# 1772
Delta R.T. 0.005 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09



Tgt Ion:202 Resp: 3111
Ion Ratio Lower Upper
202 100
200 25.2 16.5 24.7#
203 60.8 14.0 21.0#

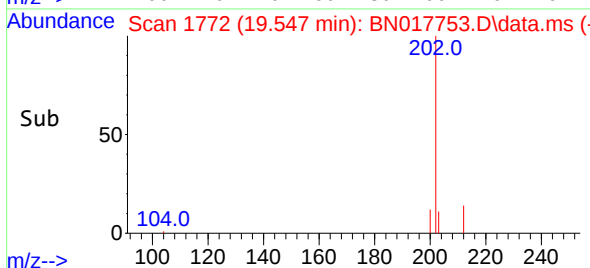




#31
 Terphenyl-d14
 Concen: 0.436 ng
 RT: 19.755 min Scan# 1814
 Delta R.T. -0.000 min
 Lab File: BN017753.D
 Acq: 07 Dec 2021 06:09

Instrument :

BNA_N

ClientSampleId :

MW-40





Tgt Ion:244 Resp: 148234
 Ion Ratio Lower Upper
 244 100
 212 10.1 5.7 8.5#
 122 11.9 8.6 13.0#


Manual Integrations

APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
 Supervised By :Sohil Jodhani 12/10/2021

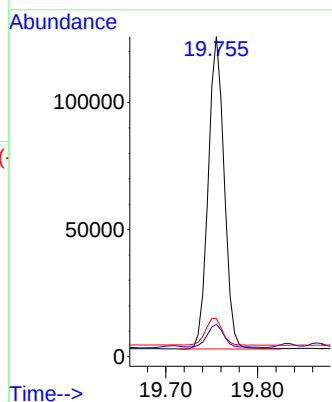


#32
 Benzo(a)anthracene
 Concen: 0.004 ng
 RT: 21.293 min Scan# 1986
 Delta R.T. -0.000 min
 Lab File: BN017753.D
 Acq: 07 Dec 2021 06:09

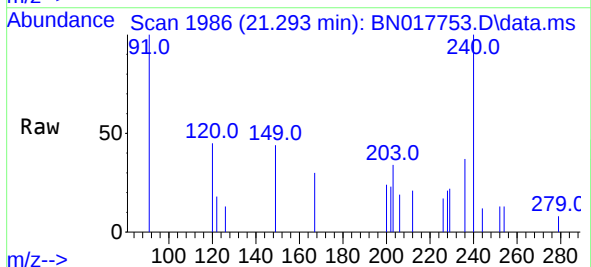


Tgt Ion:228 Resp: 1702
 Ion Ratio Lower Upper
 228 100
 226 84.4 21.3 31.9#
 229 104.7 15.7 23.5#

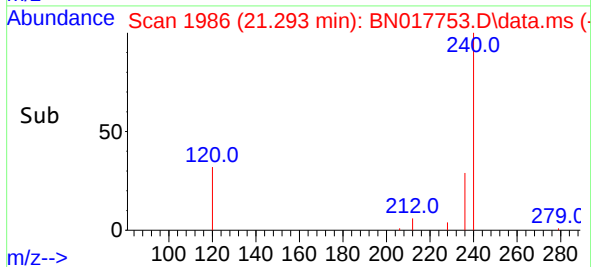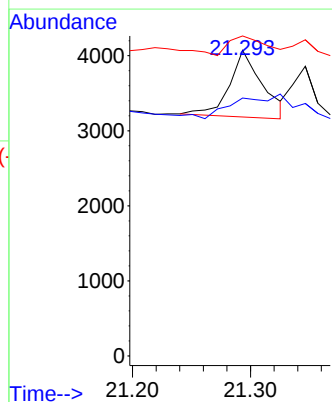



#33
Chrysene
Concen: 0.003 ng
RT: 21.346 min Scan# 1991
Delta R.T. -0.000 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09




Instrument :
BNA_N
ClientSampleId :
MW-40




Tgt Ion:228 Resp: 1445
Ion Ratio Lower Upper
228 100
226 87.2 23.3 34.9
229 109.1 15.6 23.4

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021




#34
Bis(2-ethylhexyl)phthalate
Concen: 0.674 ng
RT: 21.240 min Scan# 1981
Delta R.T. 0.010 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09




Tgt Ion:149 Resp: 140989
Ion Ratio Lower Upper
149 100
167 28.8 21.8 32.6
279 4.9 3.4 5.0

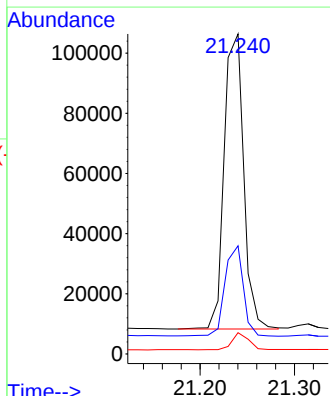



#35
Perylene-d12
Concen: 0.400 ng
RT: 23.617 min Scan# 2443
Delta R.T. 0.003 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09




Instrument :
BNA_N
ClientSampleId :
MW-40



Tgt Ion:264 Resp: 124900
Ion Ratio Lower Upper
264 100
260 25.5 19.4 29.2
265 28.0 18.6 28.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

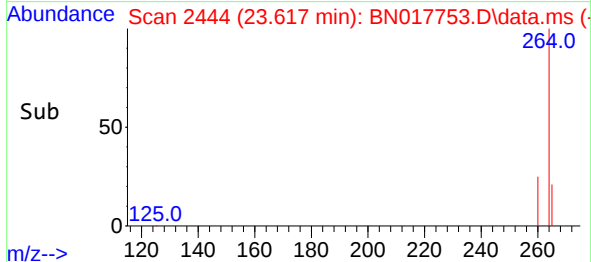

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.003 ng
RT: 25.982 min Scan# 3135
Delta R.T. -0.010 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09


Tgt Ion:276 Resp: 772
Ion Ratio Lower Upper
276 100
138 50.0 19.7 29.5#
277 9.7 20.0 30.0#

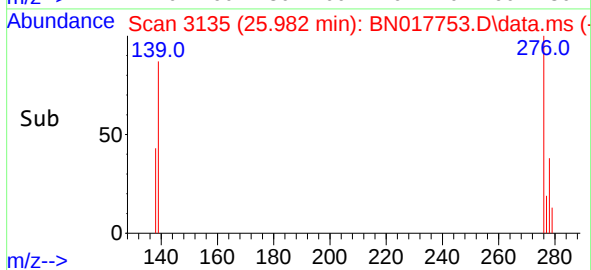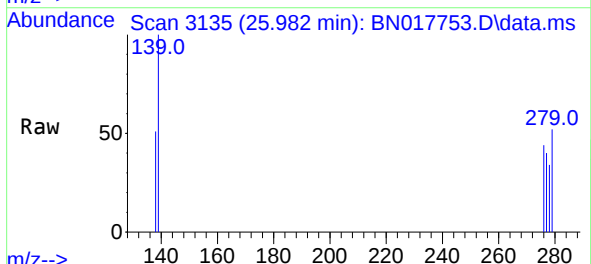



#37
Benzo(b)fluoranthene
Concen: 0.003 ng
RT: 22.918 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09




Instrument :
BNA_N
ClientSampleId :
MW-40




Tgt Ion:252 Resp: 1290
Ion Ratio Lower Upper
252 100
253 116.2 17.7 26.5#
125 116.4 7.8 11.8#

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

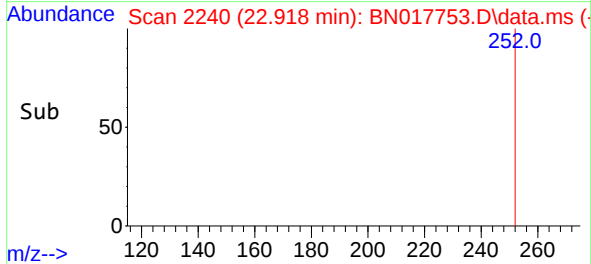


#38
Benzo(k)fluoranthene
Concen: 0.002 ng
RT: 22.959 min Scan# 2252
Delta R.T. -0.004 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09

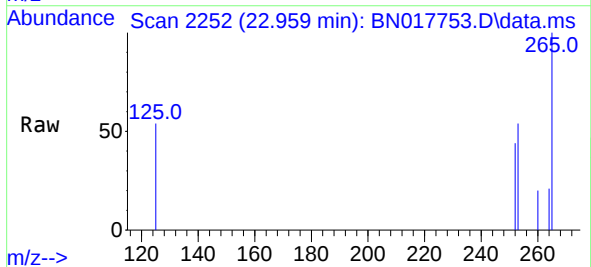


Tgt Ion:252 Resp: 830
Ion Ratio Lower Upper
252 100
253 123.2 17.7 26.5#
125 123.3 8.2 12.2#

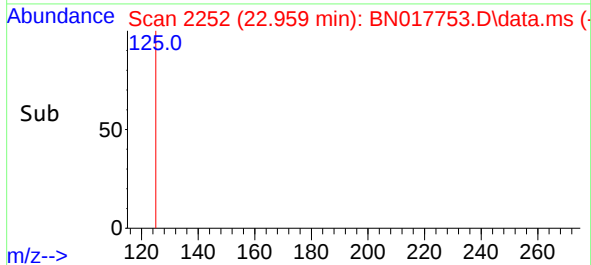



#39
Benzo(a)pyrene
Concen: 0.003 ng
RT: 23.511 min Scan# 2414
Delta R.T. -0.004 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09



Instrument :
BNA_N
ClientSampleId :
MW-40




Tgt Ion:252 Resp: 911
Ion Ratio Lower Upper
252 100
253 126.3 17.9 26.9#
125 122.5 9.2 13.8#

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021




#40
Dibenzo(a,h)anthracene
Concen: 0.003 ng
RT: 25.999 min Scan# 3140
Delta R.T. -0.014 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09

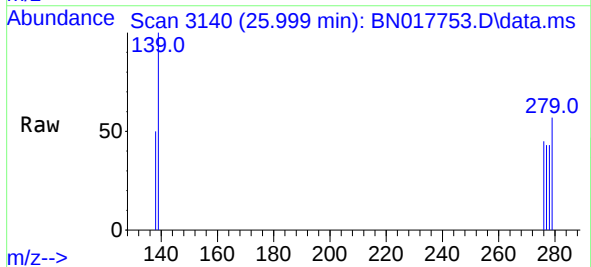


Tgt Ion:278 Resp: 530
Ion Ratio Lower Upper
278 100
139 230.8 13.0 19.6#
279 130.6 19.2 28.8#

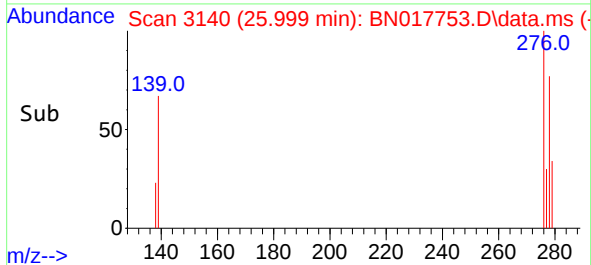

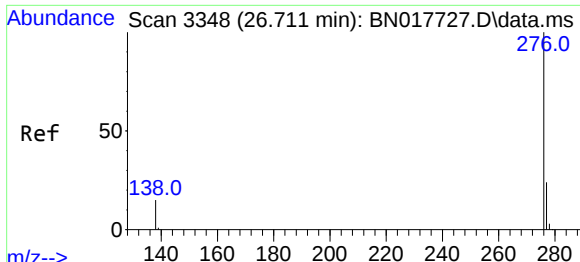

#41
Benzo(g,h,i)perylene
Concen: 0.003 ng
RT: 26.704 min Scan# 31
Delta R.T. -0.007 min
Lab File: BN017753.D
Acq: 07 Dec 2021 06:09

Instrument :
BNA_N
ClientSampleId :
MW-40

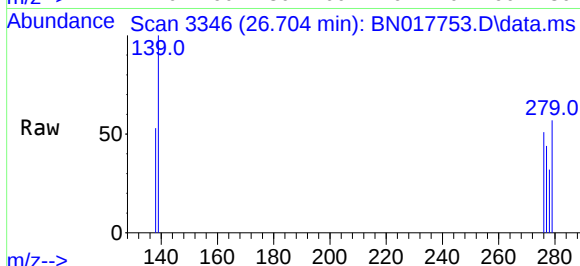

Tgt Ion:276 Resp: 780
Ion Ratio Lower Upper
276 100
277 86.7 19.0 28.4
138 104.7 17.1 25.7

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/07/2021
Supervised By :Sohil Jodhani 12/10/2021

