


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120621\
 Data File : BN017723.D
 Acq On : 06 Dec 2021 10:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN120621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 06 15:58:05 2021

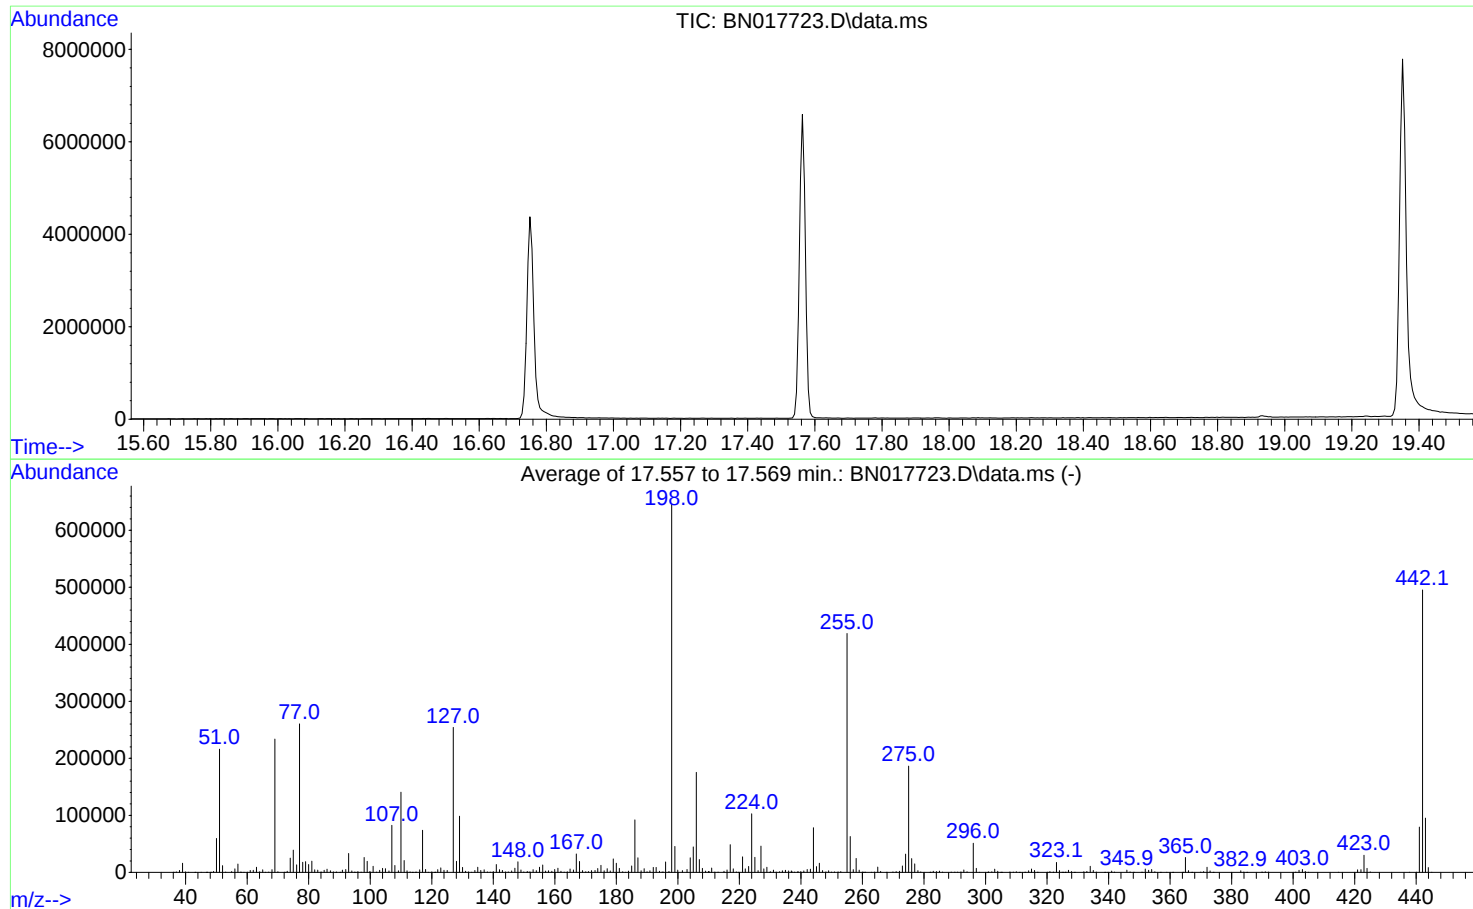




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	216085	PASS
68	69	0.00	2	2.0	4656	PASS
69	198	0.00	100	36.2	233792	PASS
70	69	0.00	2	0.5	1258	PASS
127	198	10	80	39.4	254208	PASS
197	198	0.00	2	0.3	1675	PASS
198	198	100	100	100.0	645163	PASS
199	198	5	9	7.1	45488	PASS
275	198	10	60	28.9	186475	PASS
365	198	1	100	4.1	26259	PASS
441	198	0.01	100	12.3	79411	PASS
442	442	50	100	100.0	495275	PASS
443	442	15	24	19.2	95283	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120621\
Data File : BN017723.D
Acq On : 06 Dec 2021 10:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 06 15:11:44 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 06 15:11:38 2021
Response via : Initial Calibration

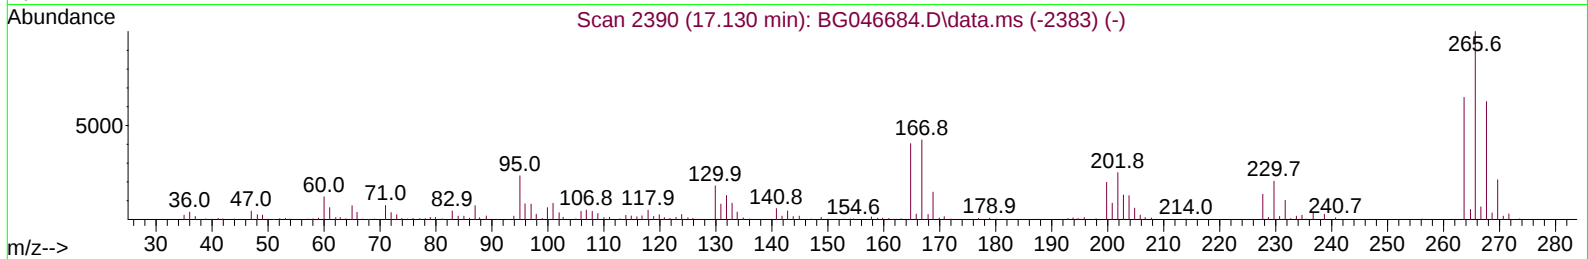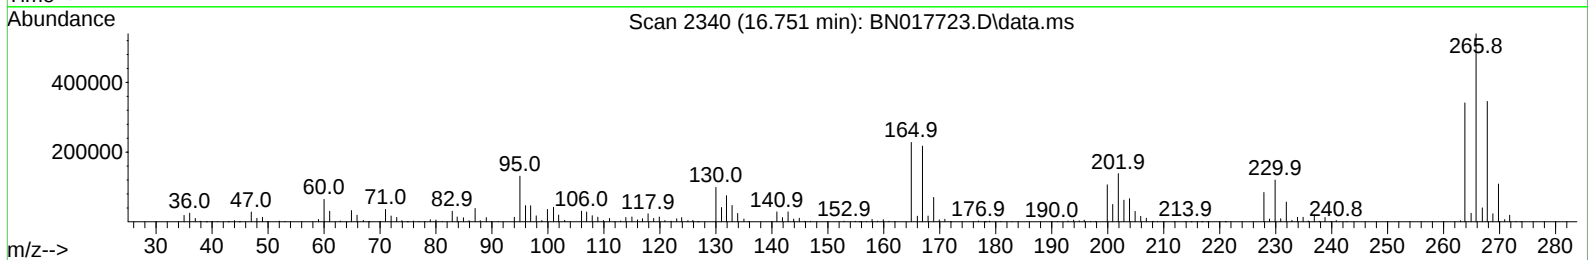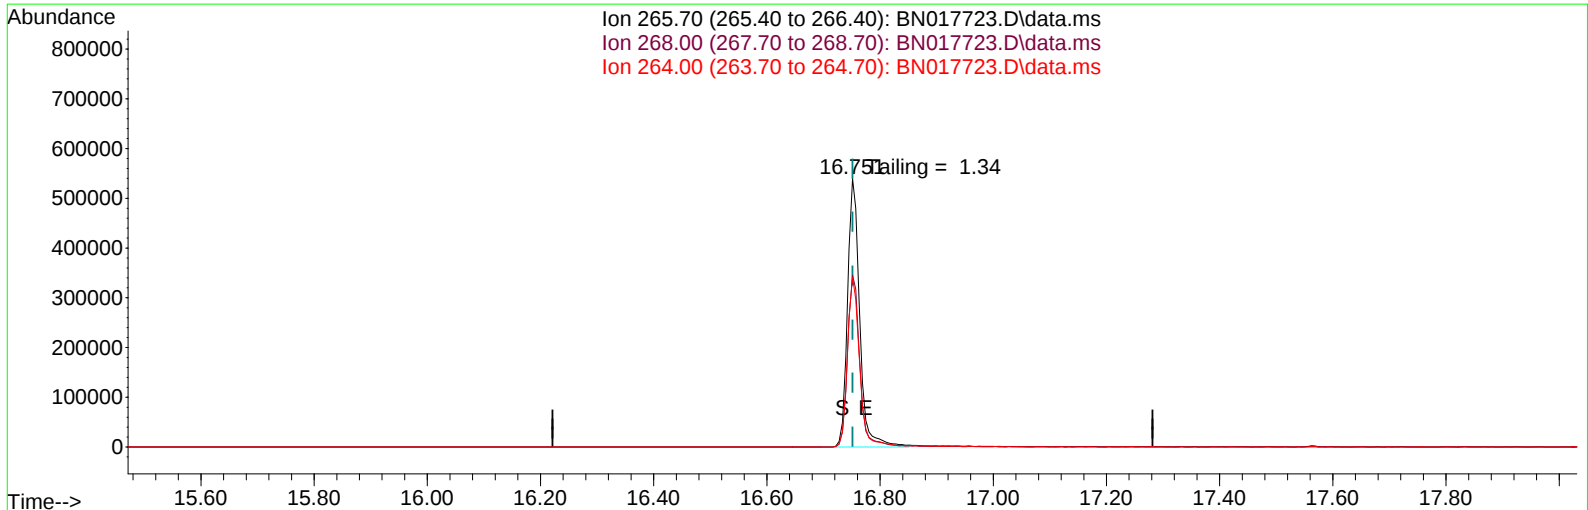

TIC: BN017723.D\data.ms

(70) Pentachlorophenol (C)

16.751min (0.000) 24899.13 ng




response 811114

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.05
264.00	61.60	63.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120621\
Data File : BN017723.D
Acq On : 06 Dec 2021 10:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 06 15:11:44 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 06 15:11:38 2021
Response via : Initial Calibration

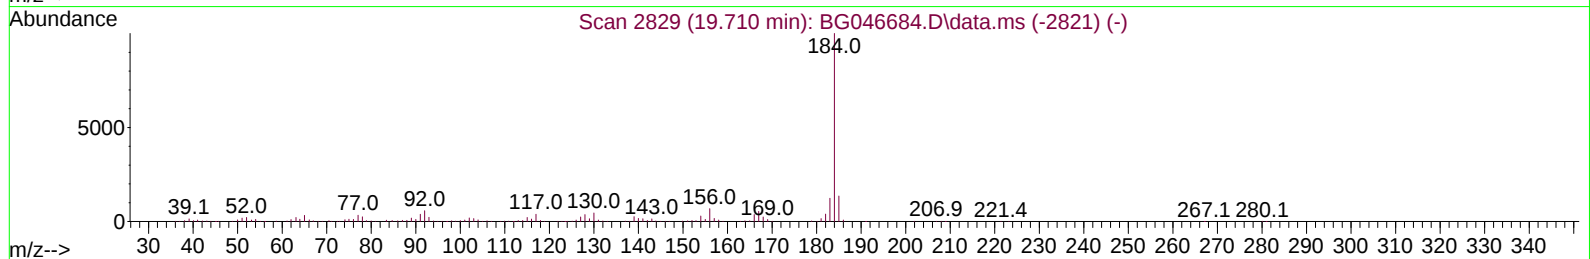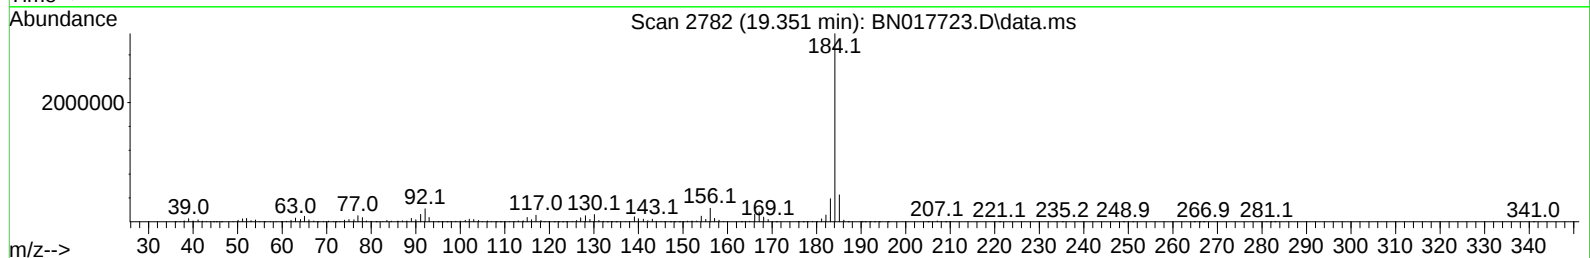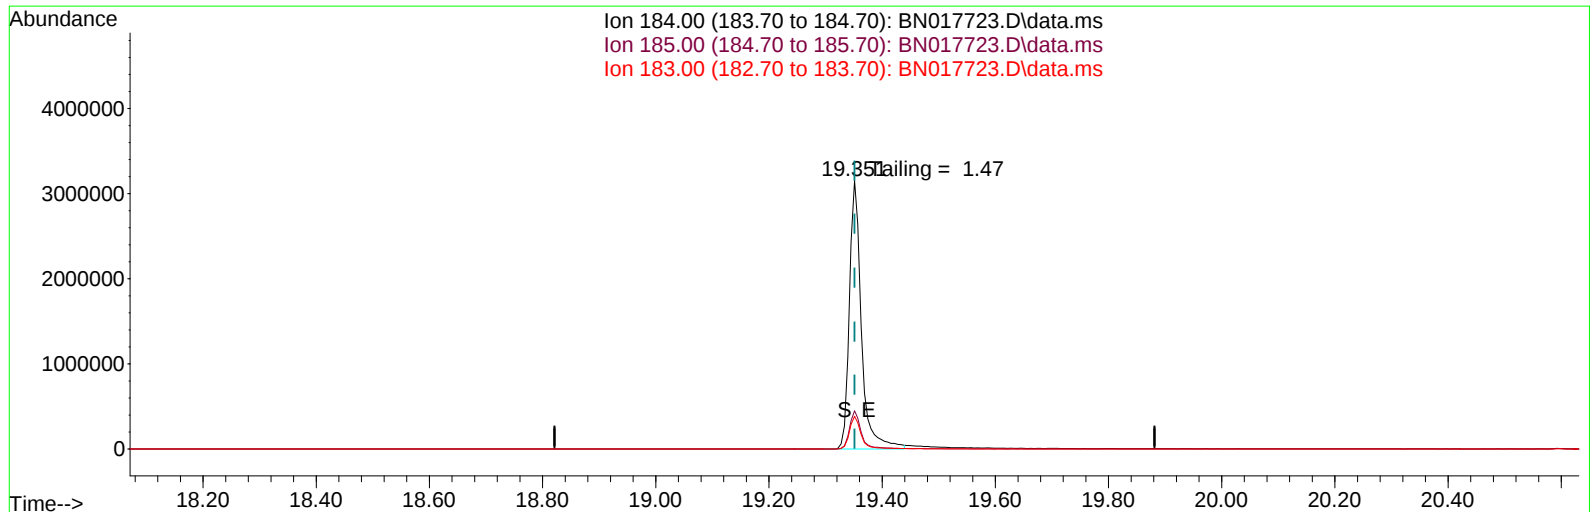

TIC: BN017723.D\data.ms

(77) Benzidine

19.351min (0.000) 693772.14 ng

response 4854573

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.29
183.00	13.20	12.26
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/6/2021	BNA_N	<u>BN017723.D</u>
Compound Name	Response	Retention Time
DDT	1836491	20.59
DDD	58266	20.15
DDE	9925	19.64
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
68191	1904682	3.58

Instrument :
BNA_N
ClientSampleId :
DFTPP