

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120622\
 Data File : BN023077.D
 Acq On : 06 Dec 2022 16:32
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Dec 07 01:31:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 07 01:27:45 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.035	152	6772	0.400	ng	0.00
7) Naphthalene-d8	10.861	136	19002	0.400	ng	0.00
13) Acenaphthene-d10	14.677	164	11247	0.400	ng	0.00
19) Phenanthrene-d10	17.427	188	23471	0.400	ng	0.00
29) Chrysene-d12	21.607	240	21902	0.400	ng	0.00
35) Perylene-d12	24.082	264	16410	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.572	112	76884	5.078	ng	0.00
5) Phenol-d6	7.183	99	103903	5.164	ng	0.00
8) Nitrobenzene-d5	9.196	82	79219	5.532	ng	0.00
11) 2-Methylnaphthalene-d10	12.442	152	214284	5.970	ng	0.00
14) 2,4,6-Tribromophenol	16.173	330	29220	6.263	ng	0.01
15) 2-Fluorobiphenyl	13.308	172	252694	5.013	ng	0.00
27) Fluoranthene-d10	19.452	212	368309	5.501	ng	0.00
31) Terphenyl-d14	20.049	244	233388	5.212	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.413	88	39206	4.637	ng	98
3) n-Nitrosodimethylamine	3.738	42	43775	4.661	ng	# 98
6) bis(2-Chloroethyl)ether	7.450	93	103316	4.722	ng	99
9) Naphthalene	10.904	128	291333	5.039	ng	99
10) Hexachlorobutadiene	11.192	225	52644	4.848	ng	# 99
12) 2-Methylnaphthalene	12.132	142	65459	6.658	ng	# 93
16) Acenaphthylene	14.399	152	315986	5.755	ng	100
17) Acenaphthene	14.741	154	206621	5.293	ng	97
18) Fluorene	15.726	166	250700	5.199	ng	100
20) 4,6-Dinitro-2-methylph...	15.788	198	25792	6.969	ng	90
21) 4-Bromophenyl-phenylether	16.620	248	79472	5.251	ng	# 64
22) Hexachlorobenzene	16.732	284	97027	5.187	ng	100
23) Atrazine	16.881	200	63178	6.319	ng	98
24) Pentachlorophenol	17.067	266	41681	9.121	ng	97
25) Phenanthrene	17.464	178	430071	5.286	ng	100
26) Anthracene	17.551	178	383193	5.734	ng	100
28) Fluoranthene	19.481	202	484995	5.339	ng	99
30) Pyrene	19.844	202	490259	5.299	ng	100
32) Benzo(a)anthracene	21.589	228	460480	5.687	ng	99
33) Chrysene	21.643	228	468023	5.211	ng	98
34) Bis(2-ethylhexyl)phtha...	21.518	149	210208	6.630	ng	99
36) Indeno(1,2,3-cd)pyrene	26.670	276	500741	5.657	ng	99
37) Benzo(b)fluoranthene	23.325	252	422364	5.628	ng	# 95
38) Benzo(k)fluoranthene	23.375	252	438555	5.687	ng	96
39) Benzo(a)pyrene	23.971	252	353329	6.001	ng	# 91
40) Dibenzo(a,h)anthracene	26.690	278	396372	5.614	ng	97
41) Benzo(g,h,i)perylene	27.468	276	411063	5.561	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120622\
 Data File : BN023077.D
 Acq On : 06 Dec 2022 16:32
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Dec 07 01:31:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 07 01:27:45 2022
 Response via : Initial Calibration




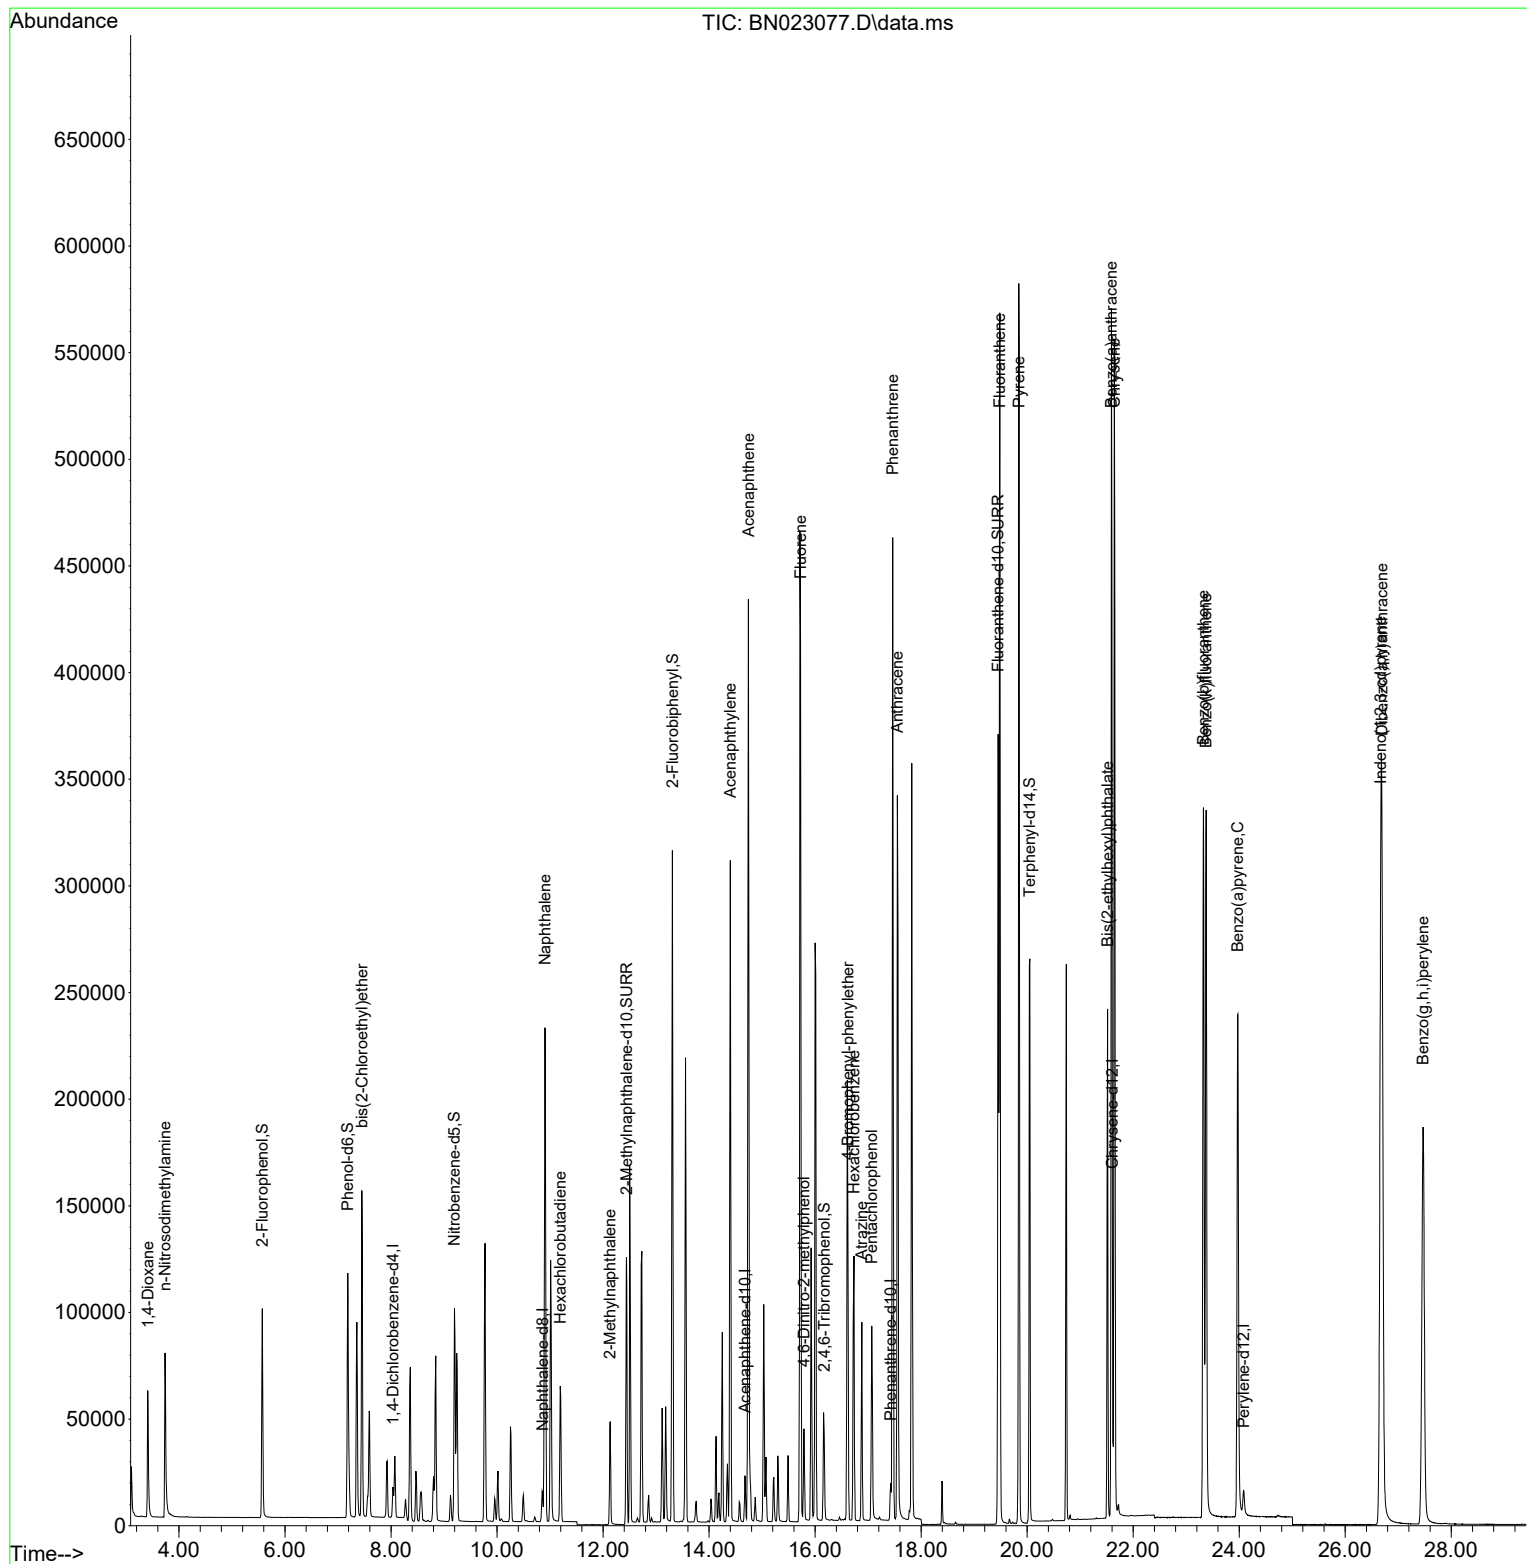




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 8.035 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN023077.D
 Acq: 06 Dec 2022 16:32




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:152 Resp: 6772
 Ion Ratio Lower Upper
 152 100
 150 157.4 125.7 188.5
 115 62.0 49.4 74.0

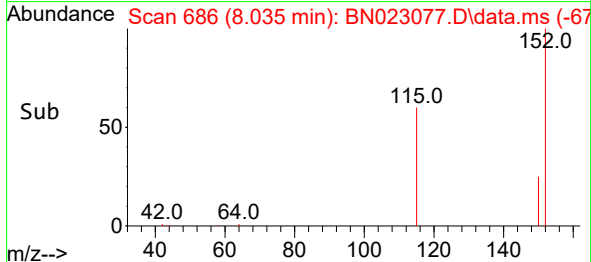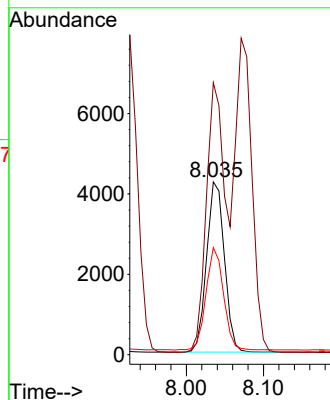

#2
 1,4-Dioxane
 Concen: 4.637 ng
 RT: 3.413 min Scan# 46
 Delta R.T. -0.007 min
 Lab File: BN023077.D
 Acq: 06 Dec 2022 16:32

Tgt Ion: 88 Resp: 39206
 Ion Ratio Lower Upper
 88 100
 43 28.3 22.0 33.0
 58 70.4 54.6 81.8


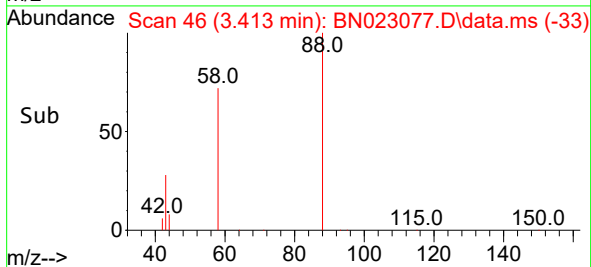
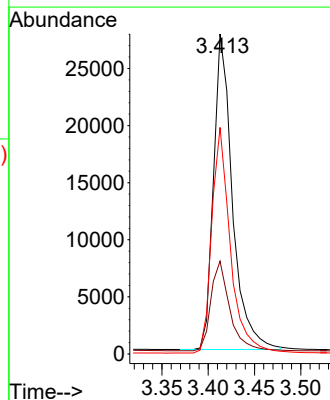
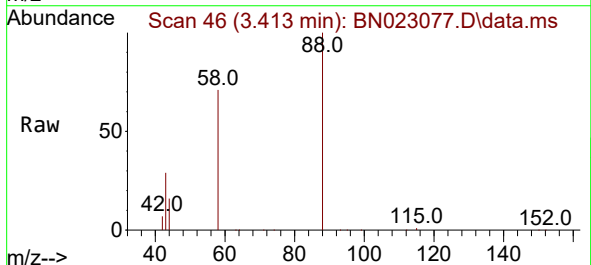




#3
 n-Nitrosodimethylamine
 Concen: 4.661 ng
 RT: 3.738 min Scan# 91
 Delta R.T. -0.015 min
 Lab File: BN023077.D
 Acq: 06 Dec 2022 16:32




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion: 42 Resp: 43775
 Ion Ratio Lower Upper
 42 100
 74 126.0 99.9 149.9
 44 6.6 9.0 13.6#

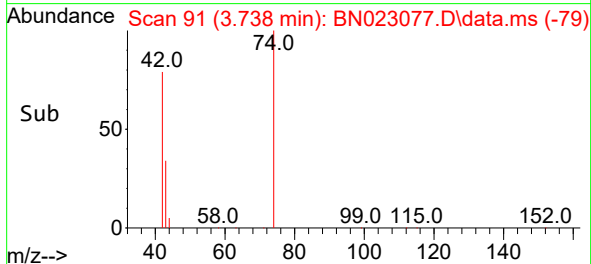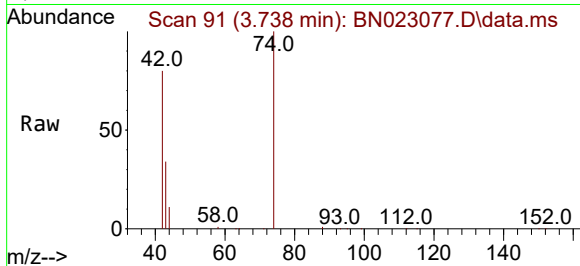

#4
 2-Fluorophenol
 Concen: 5.078 ng
 RT: 5.572 min Scan# 345
 Delta R.T. -0.000 min
 Lab File: BN023077.D
 Acq: 06 Dec 2022 16:32

Tgt Ion: 112 Resp: 76884
 Ion Ratio Lower Upper
 112 100
 64 55.9 45.0 67.6
 63 29.4 24.2 36.4


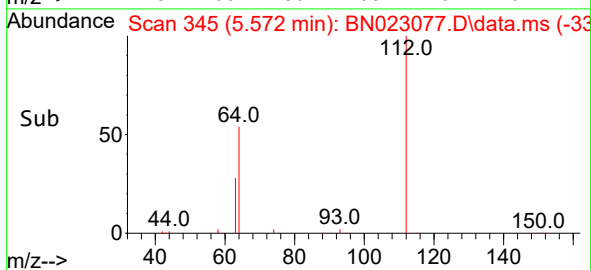

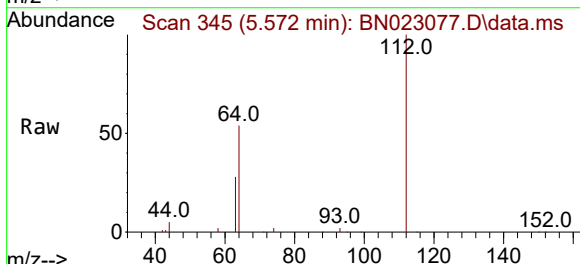




#5
Phenol-d6
Concen: 5.164 ng
RT: 7.183 min Scan# 568
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 103903
Ion Ratio Lower Upper
99 100
42 20.0 16.1 24.1
71 32.5 26.4 39.6

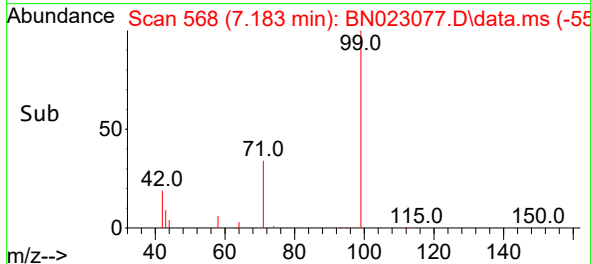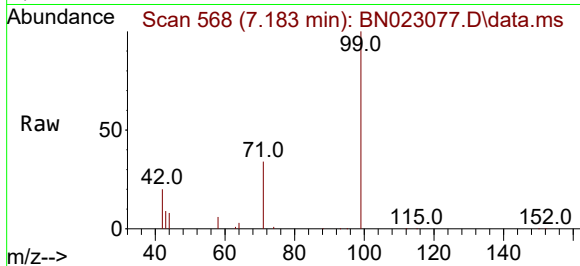

#6
bis(2-Chloroethyl)ether
Concen: 4.722 ng
RT: 7.450 min Scan# 605
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32

Tgt Ion: 93 Resp: 103316
Ion Ratio Lower Upper
93 100
63 75.0 59.3 88.9
95 32.4 25.8 38.6


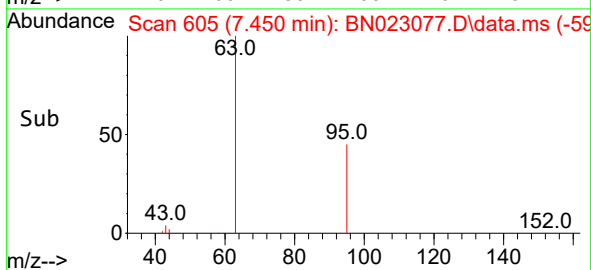

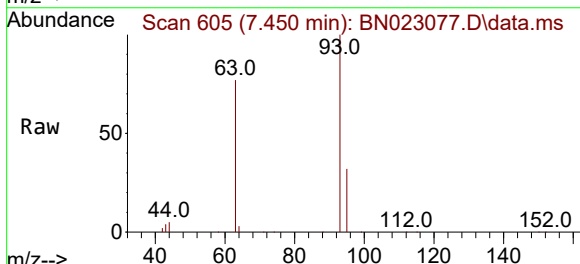




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.861 min Scan# 963
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	19002
Ion Ratio	Lower	Upper	
136	100		
137	11.4	8.8	13.2
54	6.2	4.6	7.0
68	5.2	4.2	6.4

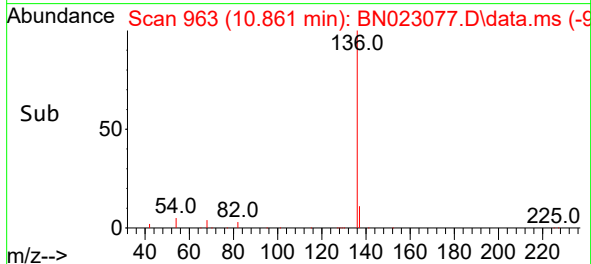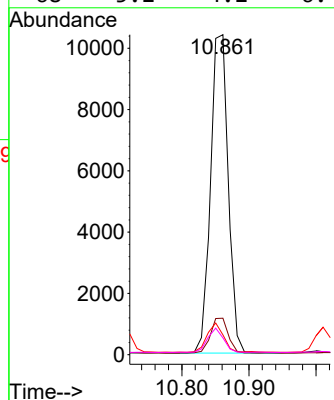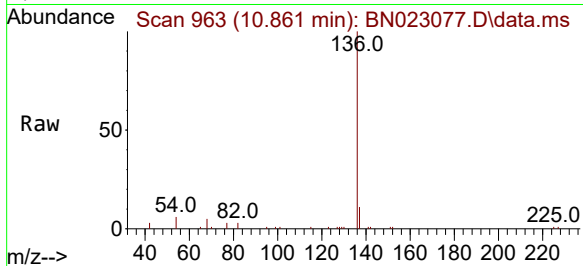

#8
Nitrobenzene-d5
Concen: 5.532 ng
RT: 9.196 min Scan# 807
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32

Tgt Ion:	82	Resp:	79219
Ion Ratio	Lower	Upper	
82	100		
128	34.9	28.9	43.3
54	52.6	43.4	65.2


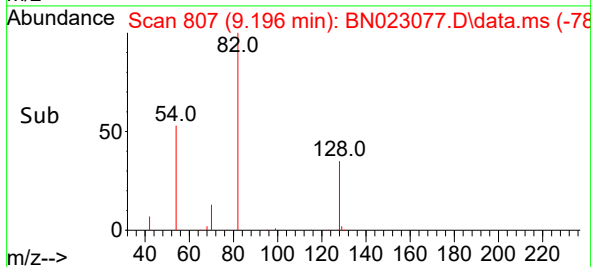
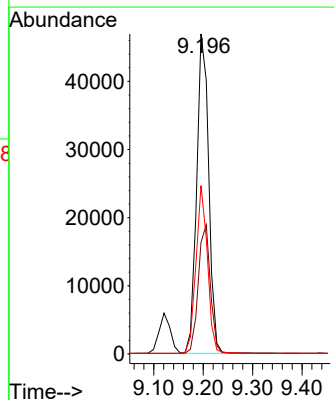
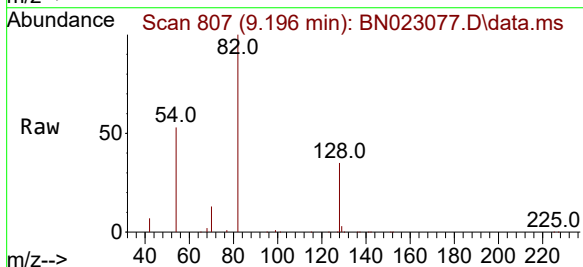




#9
Naphthalene
Concen: 5.039 ng
RT: 10.904 min Scan# 967
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:128 Resp: 291333
Ion Ratio Lower Upper
128 100
129 10.9 9.0 13.4
127 13.0 10.7 16.1

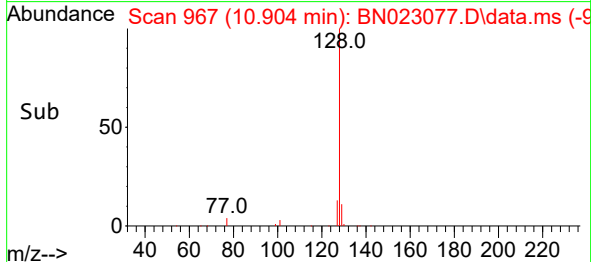

#10
Hexachlorobutadiene
Concen: 4.848 ng
RT: 11.192 min Scan# 994
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32

Tgt Ion:225 Resp: 52644
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.6 51.3 76.9

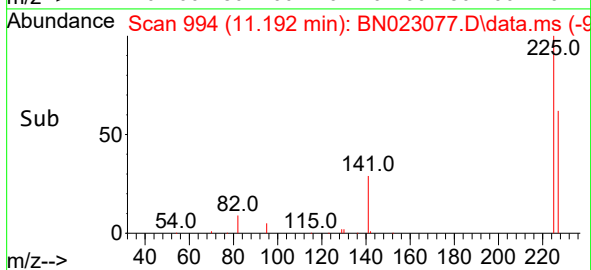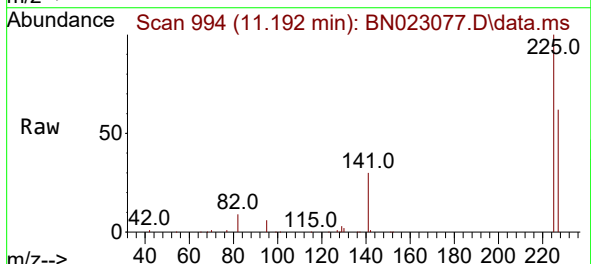



#11

2-Methylnaphthalene-d10

Concen: 5.970 ng

RT: 12.442 min Scan# 1187

Delta R.T. 0.004 min

Lab File: BN023077.D

Acq: 06 Dec 2022 16:32

Instrument :

BNA_N

ClientSampleId :





SSTDICC5.0

Tgt Ion:152 Resp: 214284

Ion Ratio Lower Upper

152 100

151 21.3 12.4 18.6#

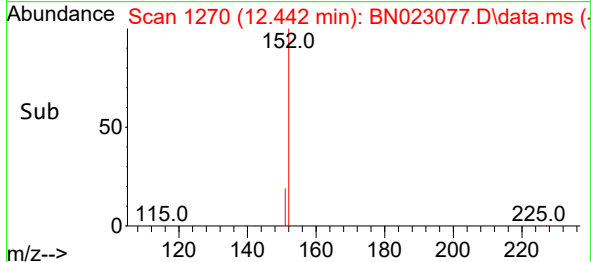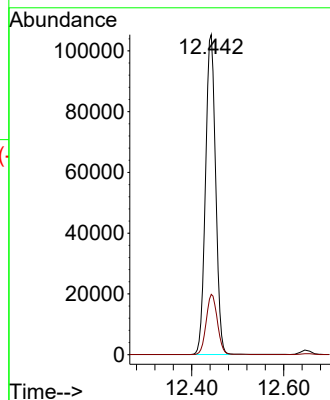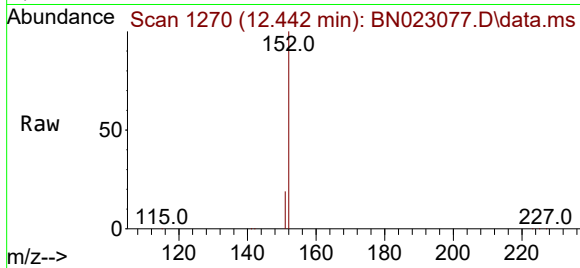

#12

2-Methylnaphthalene

Concen: 6.658 ng

RT: 12.132 min Scan# 1188

Delta R.T. 0.004 min

Lab File: BN023077.D

Acq: 06 Dec 2022 16:32




Tgt Ion:142 Resp: 65459


Ion Ratio Lower Upper

142 100

141 10.5 10.2 15.4

115 2.0 4.5 6.7#


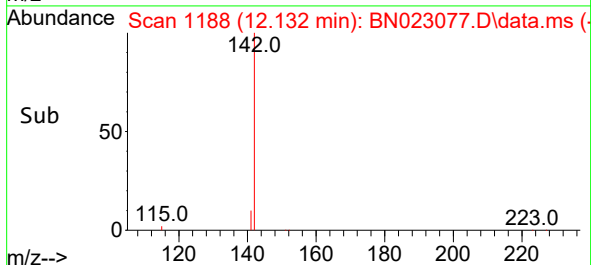
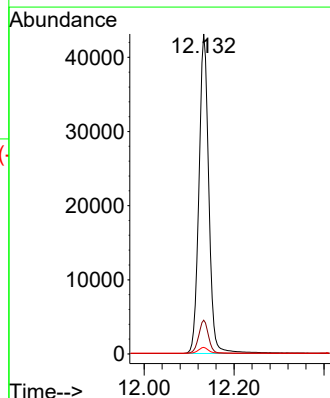
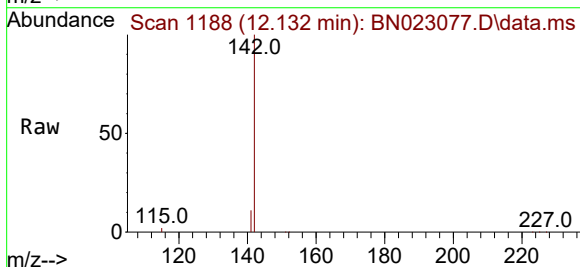


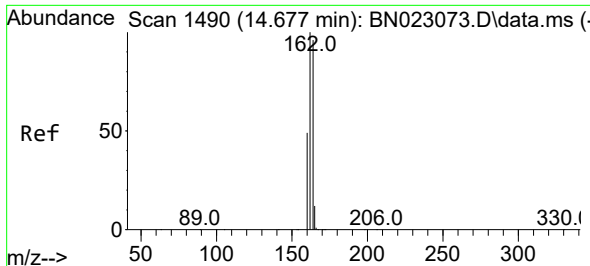

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.677 min Scan# 14
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:164 Resp: 11247
Ion Ratio Lower Upper
164 100
162 105.8 83.5 125.3
160 51.2 41.4 62.2

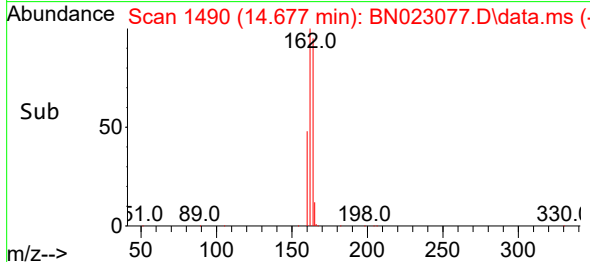

#14
2,4,6-Tribromophenol
Concen: 6.263 ng
RT: 16.173 min Scan# 1624
Delta R.T. 0.012 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32

Tgt Ion:330 Resp: 29220
Ion Ratio Lower Upper
330 100
332 96.8 77.4 116.0
141 40.9 33.4 50.2


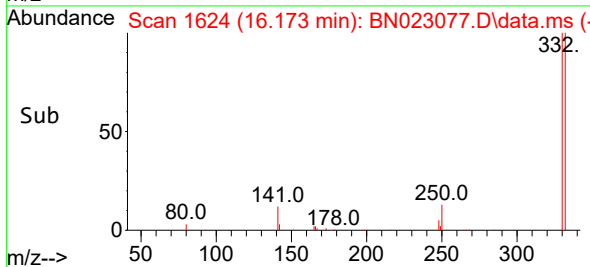

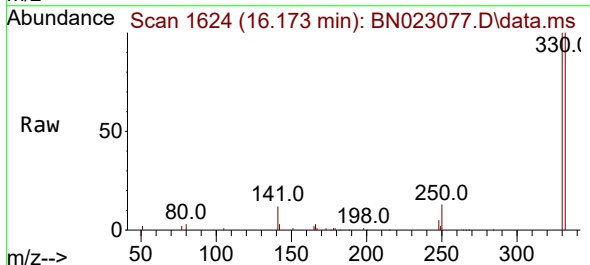




#15
2-Fluorobiphenyl
Concen: 5.013 ng
RT: 13.308 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:172 Resp: 252694
Ion Ratio Lower Upper
172 100
171 34.4 27.1 40.7
170 23.0 18.3 27.5

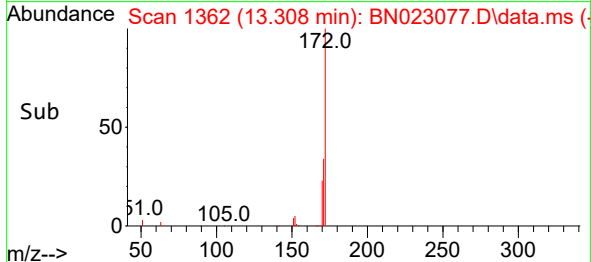

#16
Acenaphthylene
Concen: 5.755 ng
RT: 14.399 min Scan# 1464
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32

Tgt Ion:152 Resp: 315986
Ion Ratio Lower Upper
152 100
151 19.4 15.4 23.2
153 13.0 10.2 15.4


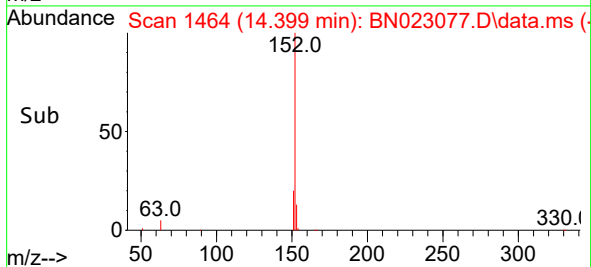

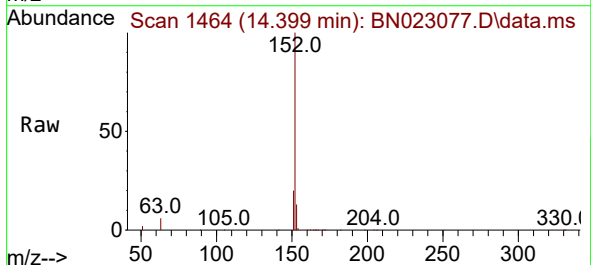




#17
Acenaphthene
Concen: 5.293 ng
RT: 14.741 min Scan# 1496
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:154 Resp: 206621
Ion Ratio Lower Upper
154 100
153 107.7 88.5 132.7
152 54.8 46.6 70.0

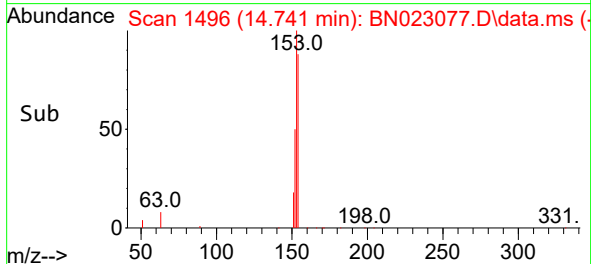

#18
Fluorene
Concen: 5.199 ng
RT: 15.726 min Scan# 1588
Delta R.T. 0.012 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32

Tgt Ion:166 Resp: 250700
Ion Ratio Lower Upper
166 100
165 95.0 76.3 114.5
167 13.2 10.6 16.0


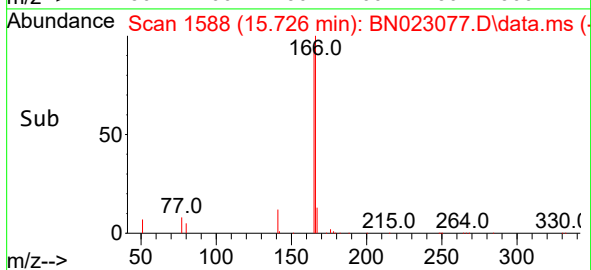

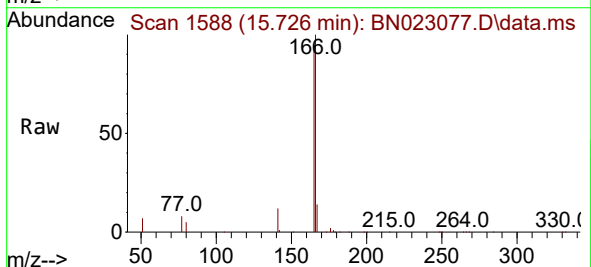




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.427 min Scan# 1725
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:188 Resp: 23471
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.0 6.5 9.7

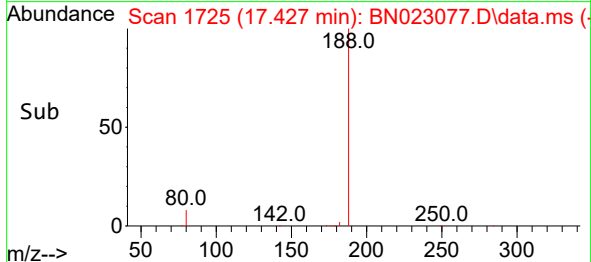

#20
4,6-Dinitro-2-methylphenol
Concen: 6.969 ng
RT: 15.788 min Scan# 1593
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32

Tgt Ion:198 Resp: 25792
Ion Ratio Lower Upper
198 100
51 57.2 56.6 85.0
105 58.1 45.7 68.5


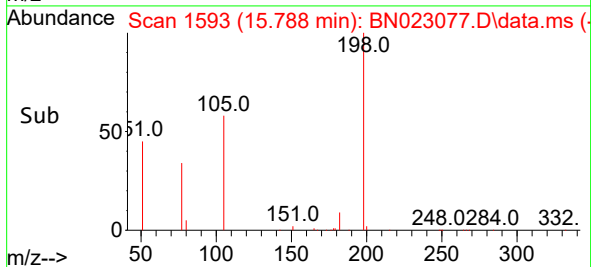

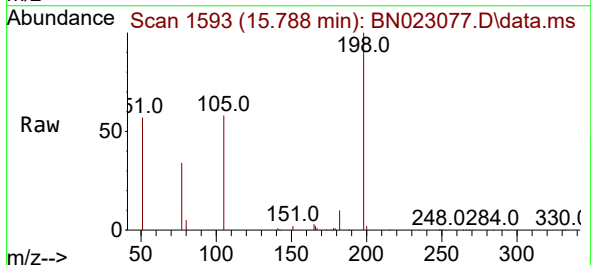


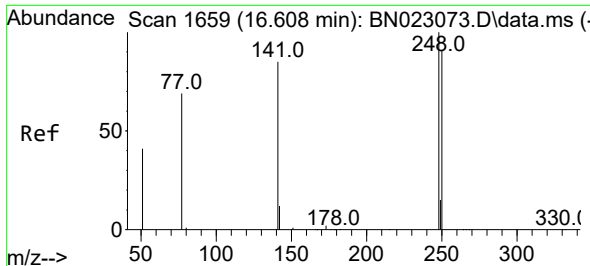

#21
4-Bromophenyl-phenylether
Concen: 5.251 ng
RT: 16.620 min Scan# 1660
Delta R.T. 0.012 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:248 Resp: 79472
Ion Ratio Lower Upper
248 100
250 103.5 72.7 109.1
141 31.1 68.3 102.5#

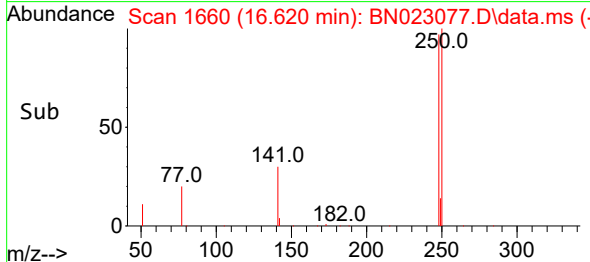

#22
Hexachlorobenzene
Concen: 5.187 ng
RT: 16.732 min Scan# 1669
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32

Tgt Ion:284 Resp: 97027
Ion Ratio Lower Upper
284 100
142 38.9 31.2 46.8
249 30.5 24.5 36.7

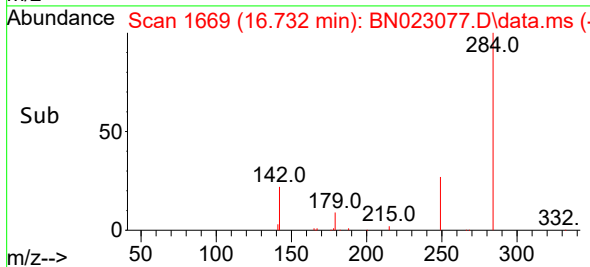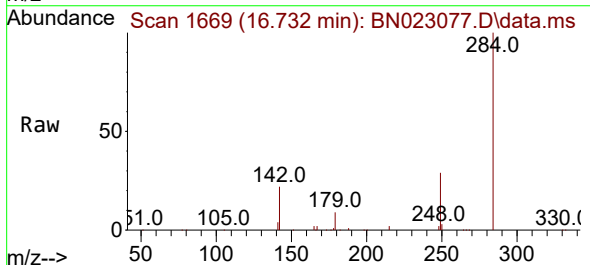



#23

Atrazine

Concen: 6.319 ng

RT: 16.881 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN023077.D

Acq: 06 Dec 2022 16:32

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:200 Resp: 63178

Ion Ratio Lower Upper

200 100

173 24.2 18.0 27.0

215 46.2 37.9 56.9

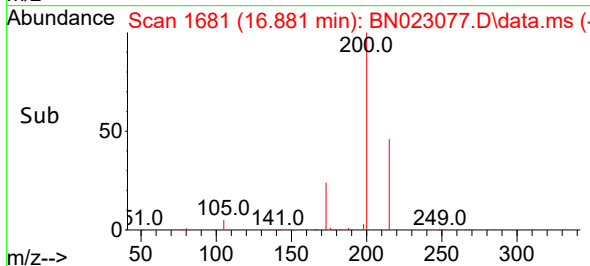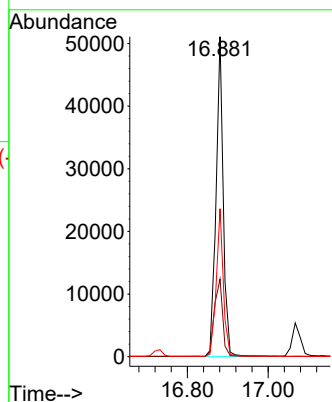

#24

Pentachlorophenol

Concen: 9.121 ng

RT: 17.067 min Scan# 1696

Delta R.T. -0.000 min

Lab File: BN023077.D

Acq: 06 Dec 2022 16:32




Tgt Ion:266 Resp: 41681


Ion Ratio Lower Upper

266 100

264 62.5 49.1 73.7

268 63.5 53.8 80.8


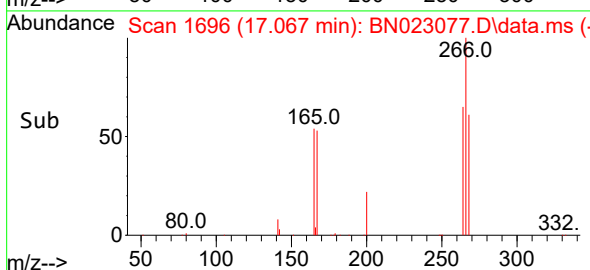

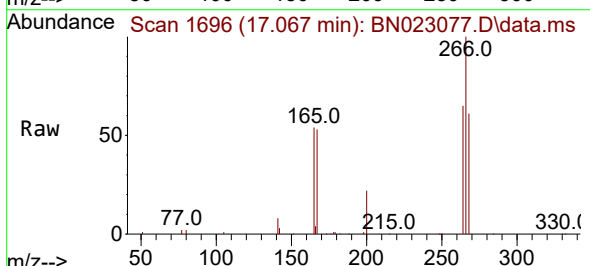




#25
Phenanthrene
Concen: 5.286 ng
RT: 17.464 min Scan# 1728
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:178 Resp: 430071
Ion Ratio Lower Upper
178 100
176 19.2 15.6 23.4
179 15.2 12.2 18.2

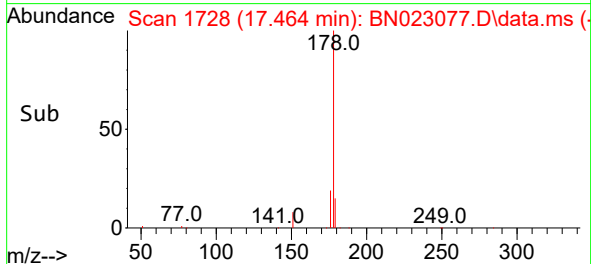

#26
Anthracene
Concen: 5.734 ng
RT: 17.551 min Scan# 1735
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32

Tgt Ion:178 Resp: 383193
Ion Ratio Lower Upper
178 100
176 18.7 15.0 22.6
179 15.3 12.4 18.6


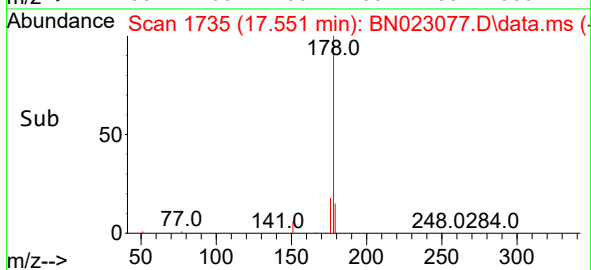

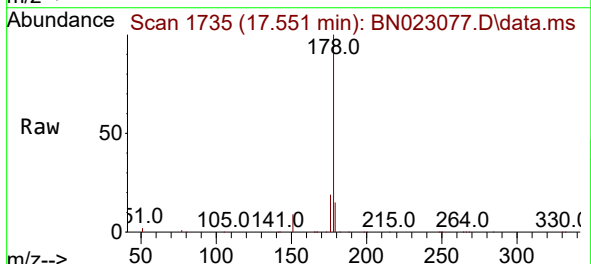




#27
Fluoranthene-d10
Concen: 5.501 ng
RT: 19.452 min Scan# 2114
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:212 Resp: 368309
Ion Ratio Lower Upper
212 100
106 16.2 13.0 19.6
104 9.0 7.4 11.0

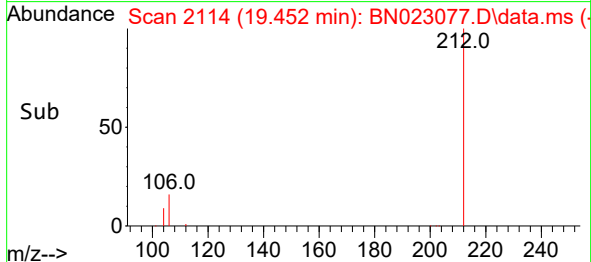

#28
Fluoranthene
Concen: 5.339 ng
RT: 19.481 min Scan# 2121
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32

Tgt Ion:202 Resp: 484995
Ion Ratio Lower Upper
202 100
101 12.3 10.2 15.2
203 17.3 13.7 20.5


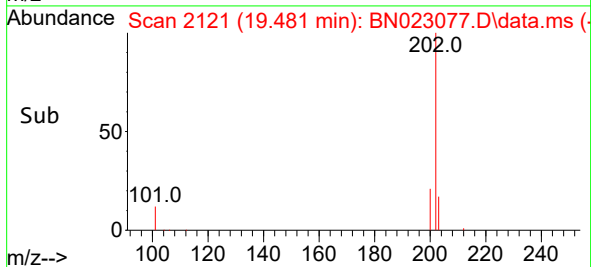

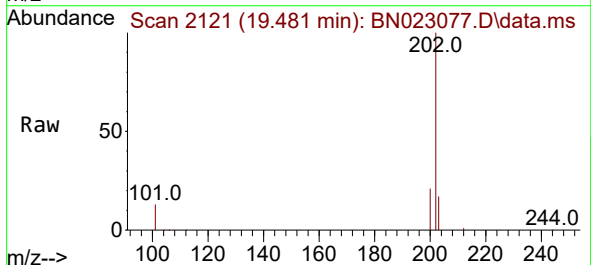




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.607 min Scan# 2424
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:240 Resp: 21902
Ion Ratio Lower Upper
240 100
120 15.9 14.8 22.2
236 28.4 22.8 34.2

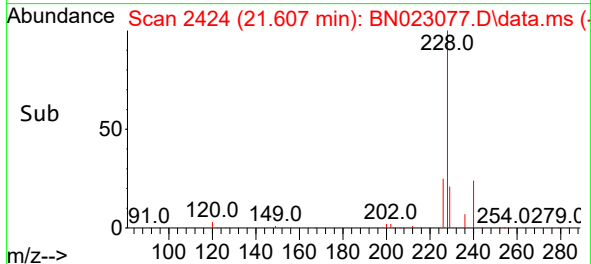

#30
Pyrene
Concen: 5.299 ng
RT: 19.844 min Scan# 2207
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32

Tgt Ion:202 Resp: 490259
Ion Ratio Lower Upper
202 100
200 21.1 16.7 25.1
203 17.8 14.2 21.2

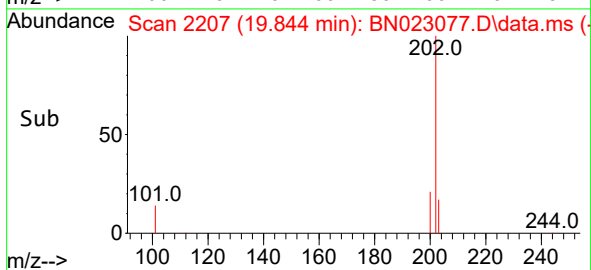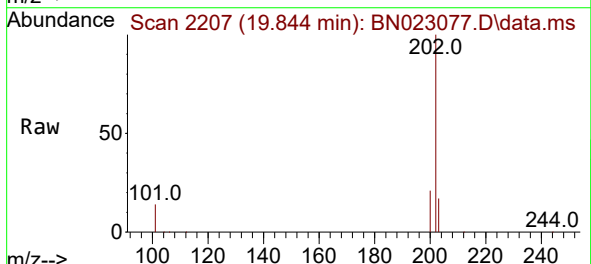

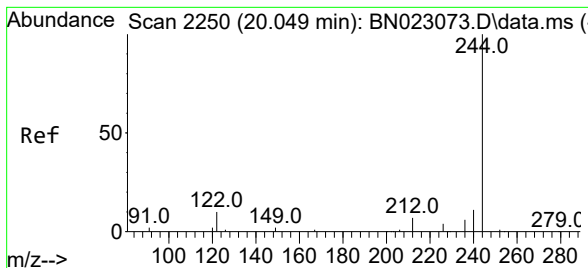

#31

Terphenyl-d14

Concen: 5.212 ng

RT: 20.049 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN023077.D

Acq: 06 Dec 2022 16:32

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:244 Resp: 233388

Ion Ratio Lower Upper

244 100

212 7.3 6.2 9.2

122 9.0 8.1 12.1

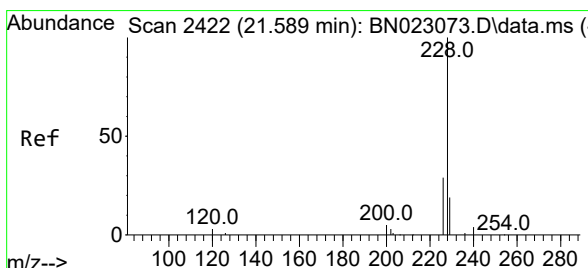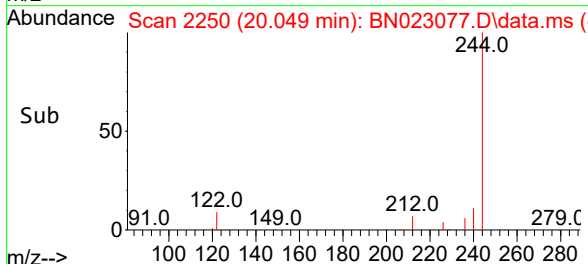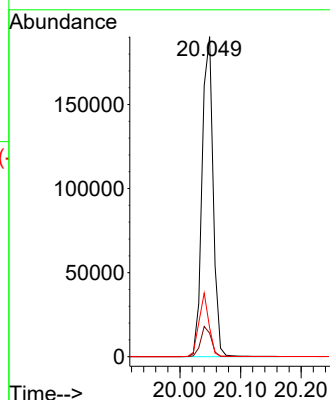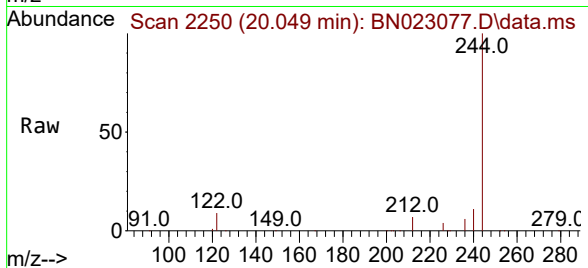

#32

Benzo(a)anthracene

Concen: 5.687 ng

RT: 21.589 min Scan# 2422

Delta R.T. -0.000 min

Lab File: BN023077.D

Acq: 06 Dec 2022 16:32




Tgt Ion:228 Resp: 460480


Ion Ratio Lower Upper

228 100

226 27.9 23.0 34.4

229 19.3 15.4 23.0

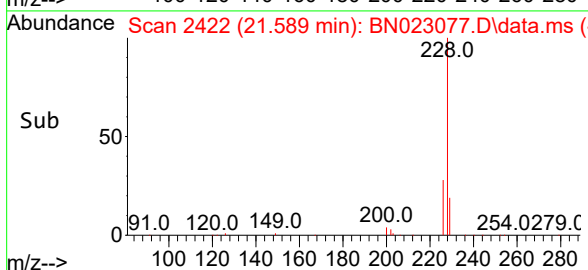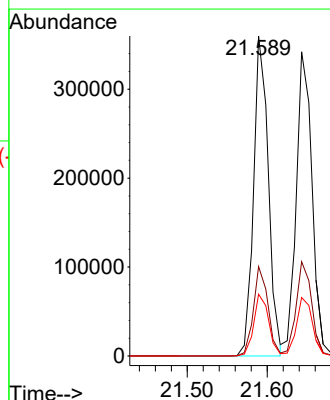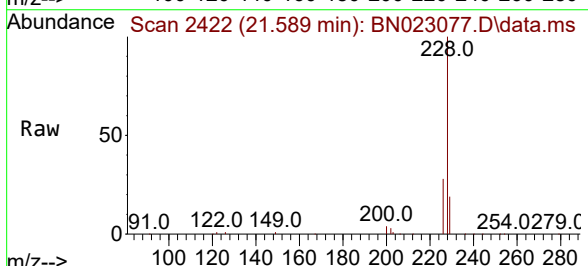



#33

Chrysene

Concen: 5.211 ng

RT: 21.643 min Scan# 2428

Delta R.T. -0.009 min

Lab File: BN023077.D

Acq: 06 Dec 2022 16:32

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:228 Resp: 468023

Ion Ratio Lower Upper

228 100

226 31.0 23.7 35.5

229 19.2 15.7 23.5

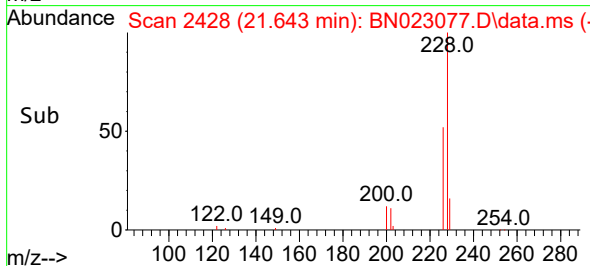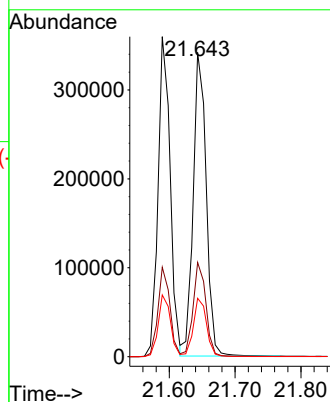

#34

Bis(2-ethylhexyl)phthalate

Concen: 6.630 ng

RT: 21.518 min Scan# 2414

Delta R.T. -0.000 min

Lab File: BN023077.D

Acq: 06 Dec 2022 16:32




Tgt Ion:149 Resp: 210208


Ion Ratio Lower Upper

149 100

167 26.2 20.6 31.0

279 2.5 2.2 3.2


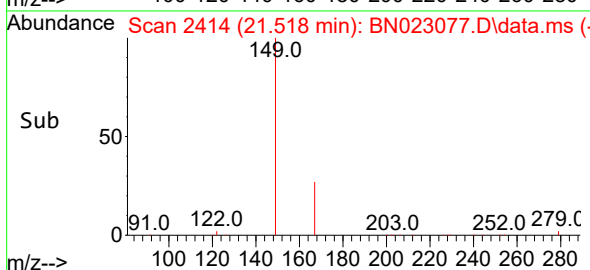
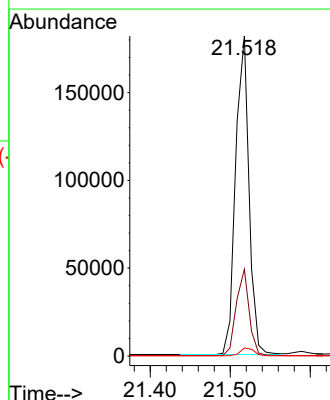
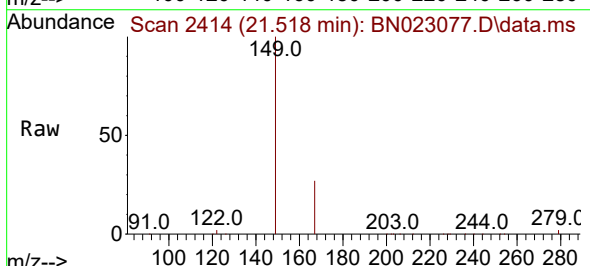




#35
Perylene-d12
Concen: 0.400 ng
RT: 24.082 min Scan# 3088
Delta R.T. -0.003 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:264 Resp: 16410
Ion Ratio Lower Upper
264 100
260 26.2 21.4 32.2
265 52.9 34.6 52.0#

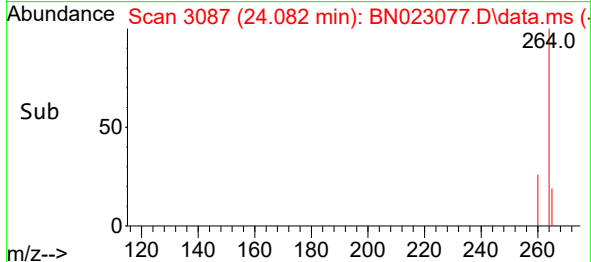

#36
Indeno(1,2,3-cd)pyrene
Concen: 5.657 ng
RT: 26.670 min Scan# 3972
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32

Tgt Ion:276 Resp: 500741
Ion Ratio Lower Upper
276 100
138 30.4 24.8 37.2
277 24.8 19.6 29.4

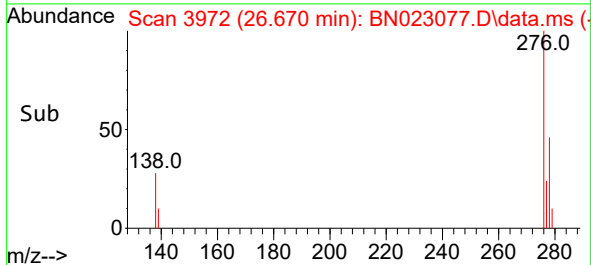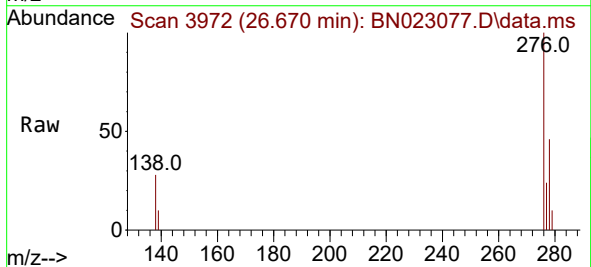



#37

Benzo(b)fluoranthene

Concen: 5.628 ng

RT: 23.325 min Scan# 2828

Delta R.T. -0.000 min

Lab File: BN023077.D

Acq: 06 Dec 2022 16:32

Instrument :

BN023077.D

ClientSampleId :

SSTDICC5.0





Tgt Ion:252 Resp: 422364

Ion Ratio Lower Upper

252 100

253 21.7 18.4 27.6

125 12.0 12.1 18.1#

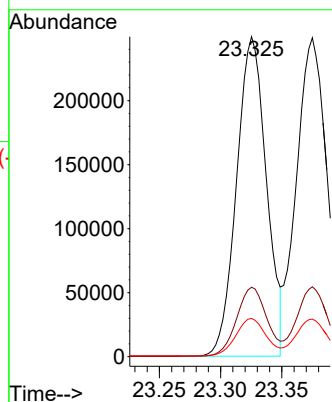

#38

Benzo(k)fluoranthene

Concen: 5.687 ng

RT: 23.375 min Scan# 2845

Delta R.T. -0.000 min

Lab File: BN023077.D

Acq: 06 Dec 2022 16:32




Tgt Ion:252 Resp: 438555


Ion Ratio Lower Upper

252 100

253 21.9 18.5 27.7

125 11.8 11.6 17.4


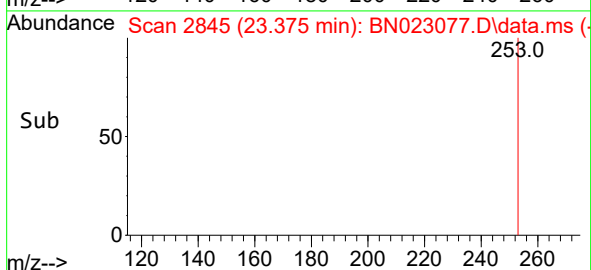






#39
Benzo(a)pyrene
Concen: 6.001 ng
RT: 23.971 min Scan# 3049
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 353329
Ion Ratio Lower Upper
252 100
253 21.5 19.6 29.4
125 13.4 15.3 22.9#

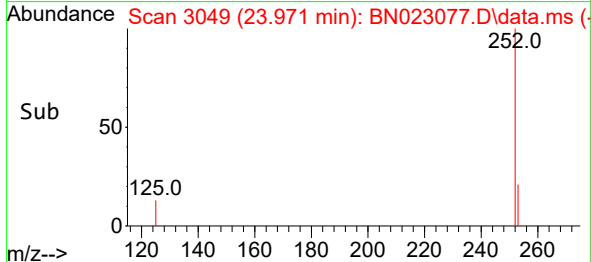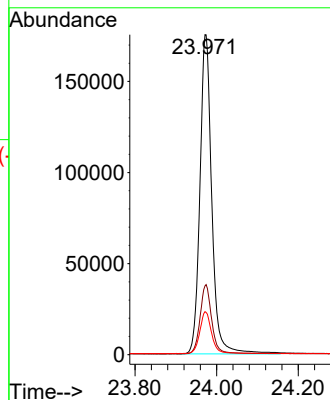

#40
Dibenzo(a,h)anthracene
Concen: 5.614 ng
RT: 26.690 min Scan# 3979
Delta R.T. -0.000 min
Lab File: BN023077.D
Acq: 06 Dec 2022 16:32


Tgt Ion:278 Resp: 396372
Ion Ratio Lower Upper
278 100
139 20.4 17.4 26.2
279 23.3 20.1 30.1

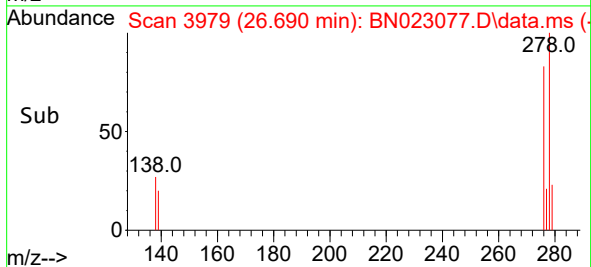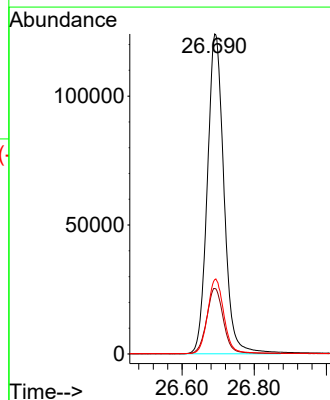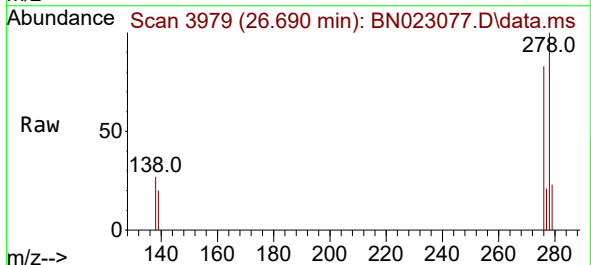

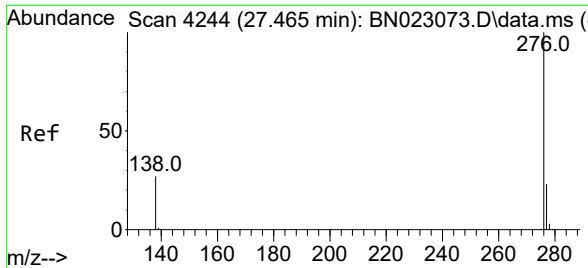

#41
 Benzo(g,h,i)perylene
 Concen: 5.561 ng
 RT: 27.468 min Scan# 41
 Delta R.T. 0.003 min
 Lab File: BN023077.D
 Acq: 06 Dec 2022 16:32

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

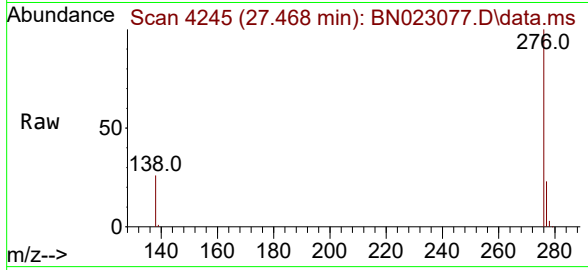

Tgt Ion:276 Resp: 411063
 Ion Ratio Lower Upper
 276 100
 277 23.3 19.0 28.6
 138 26.2 21.8 32.8

