
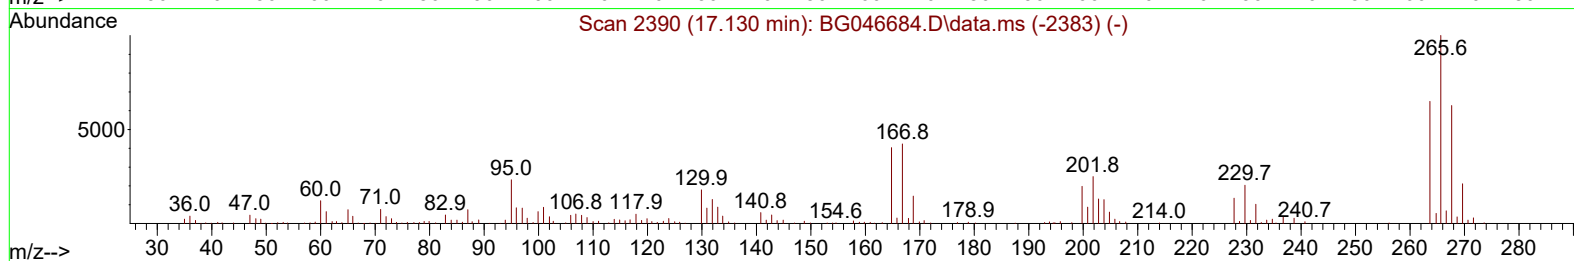
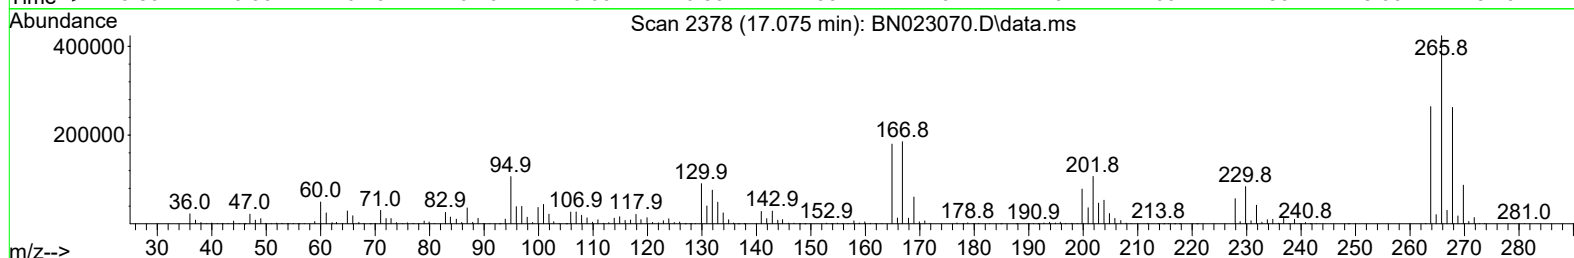


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120622\
Data File : BN023070.D
Acq On : 06 Dec 2022 12:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 06:27:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 07 06:27:50 2022
Response via : Initial Calibration

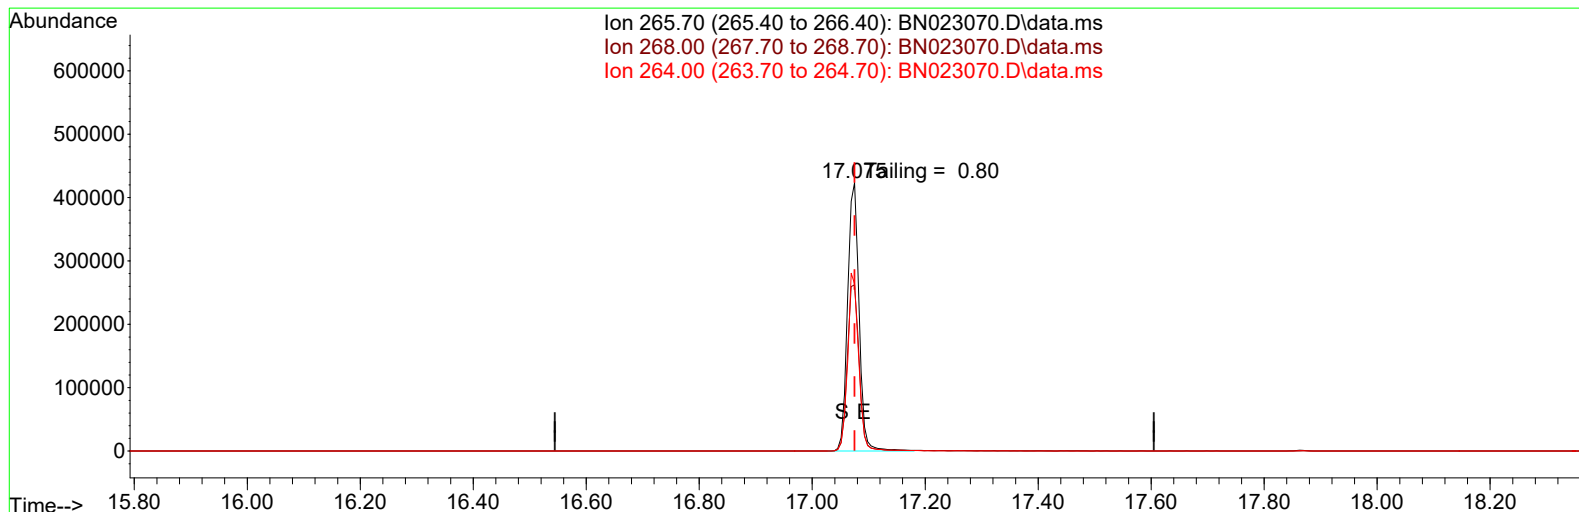

TIC: BN023070.D\data.ms

(70) Pentachlorophenol (C)




17.075min (0.000) 21498.56 ng

response 600289

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.91
264.00	61.60	62.34
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120622\  
Data File : BN023070.D  
Acq On    : 06 Dec 2022  12:12  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Dec 07 06:27:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 07 06:27:50 2022
Response via : Initial Calibration

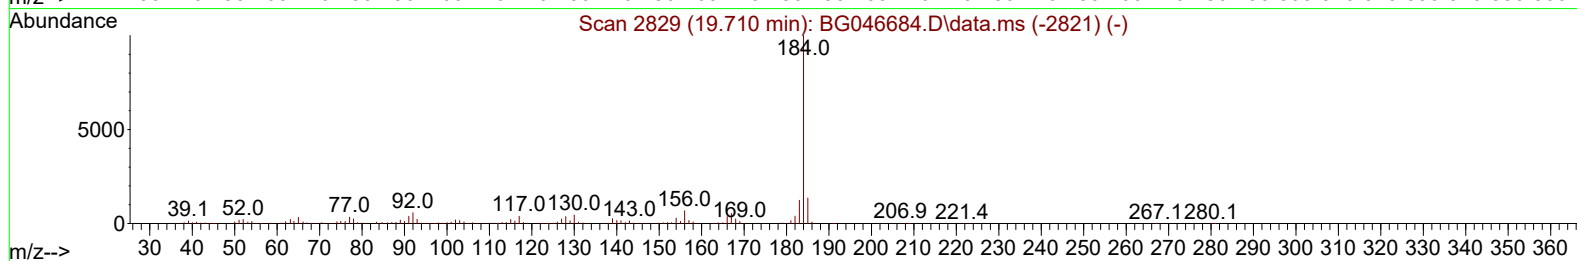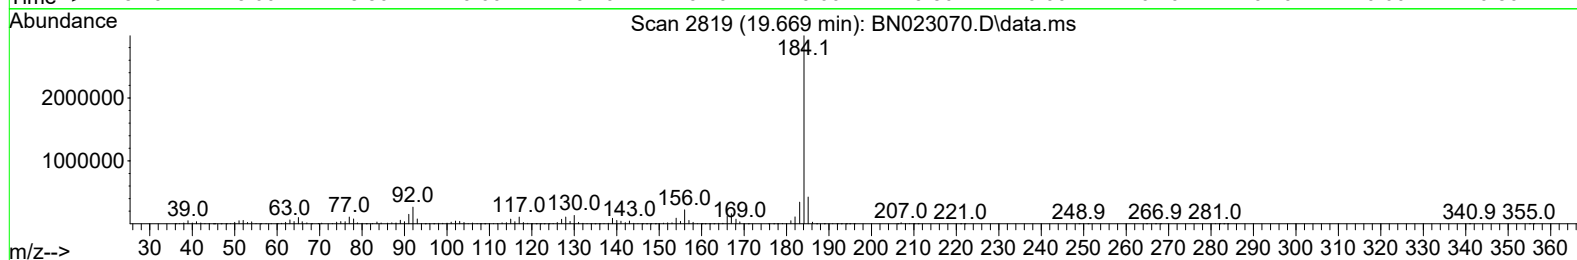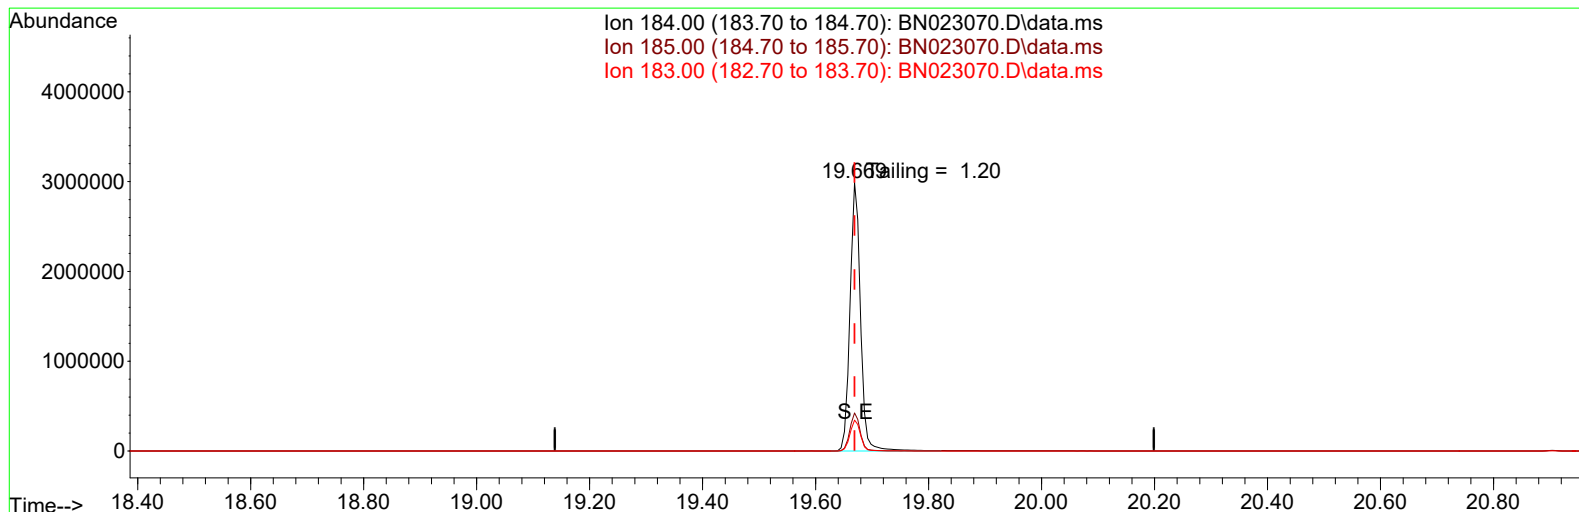

TIC: BN023070.D\data.ms

(77) Benzidine

19.669min (0.000) 0.00 ng

response **3898917**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.20
183.00	13.20	11.53
0.00	0.00	0.00