


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120622\
 Data File : BN023070.D
 Acq On : 06 Dec 2022 12:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 07 02:02:07 2022

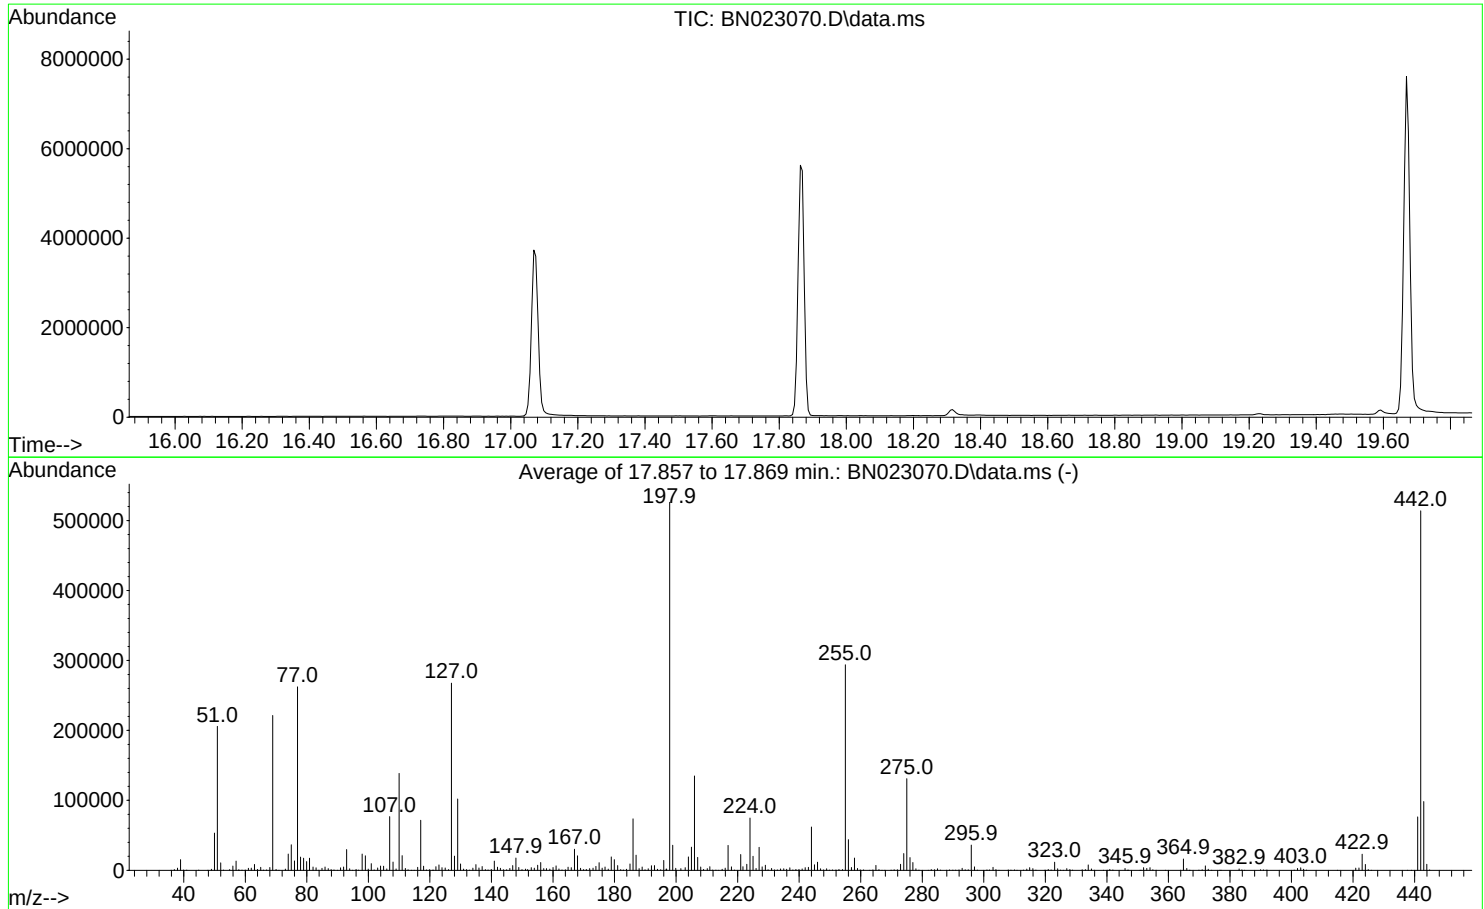




AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	205665	PASS
68	69	0.00	2	1.8	3967	PASS
69	198	0.00	100	42.1	221434	PASS
70	69	0.00	2	0.5	1161	PASS
127	198	10	80	50.9	267477	PASS
197	198	0.00	2	0.3	1720	PASS
198	198	100	100	100.0	525952	PASS
199	198	5	9	6.8	35808	PASS
275	198	10	60	24.9	131096	PASS
365	198	1	100	3.1	16196	PASS
441	198	0.01	100	14.5	76291	PASS
442	442	50	100	100.0	513941	PASS
443	442	15	24	19.1	98325	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120622\
Data File : BN023070.D
Acq On : 06 Dec 2022 12:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 07 06:27:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 07 06:27:50 2022
Response via : Initial Calibration

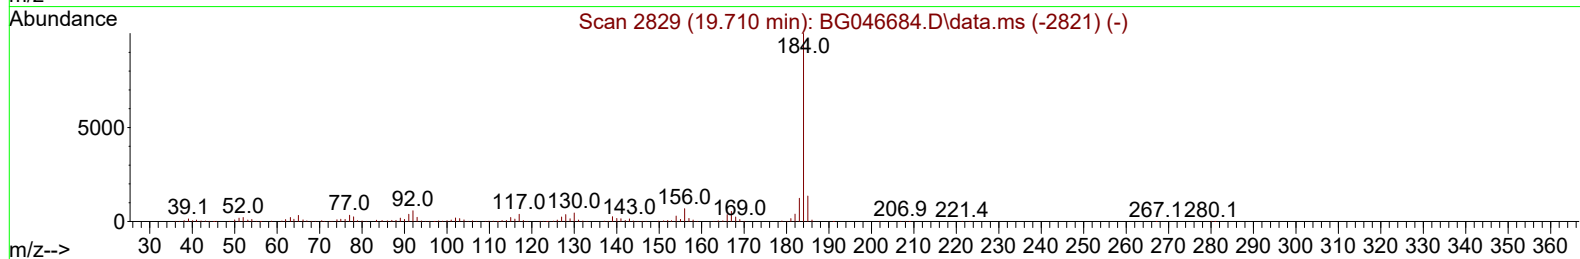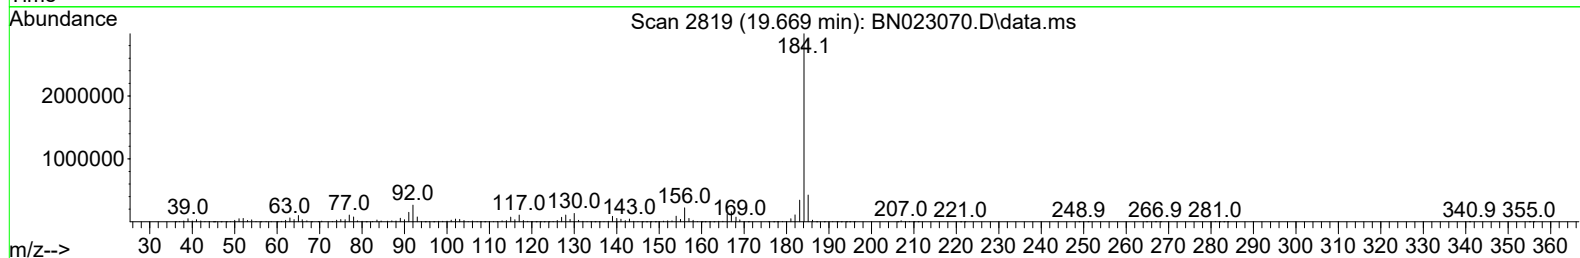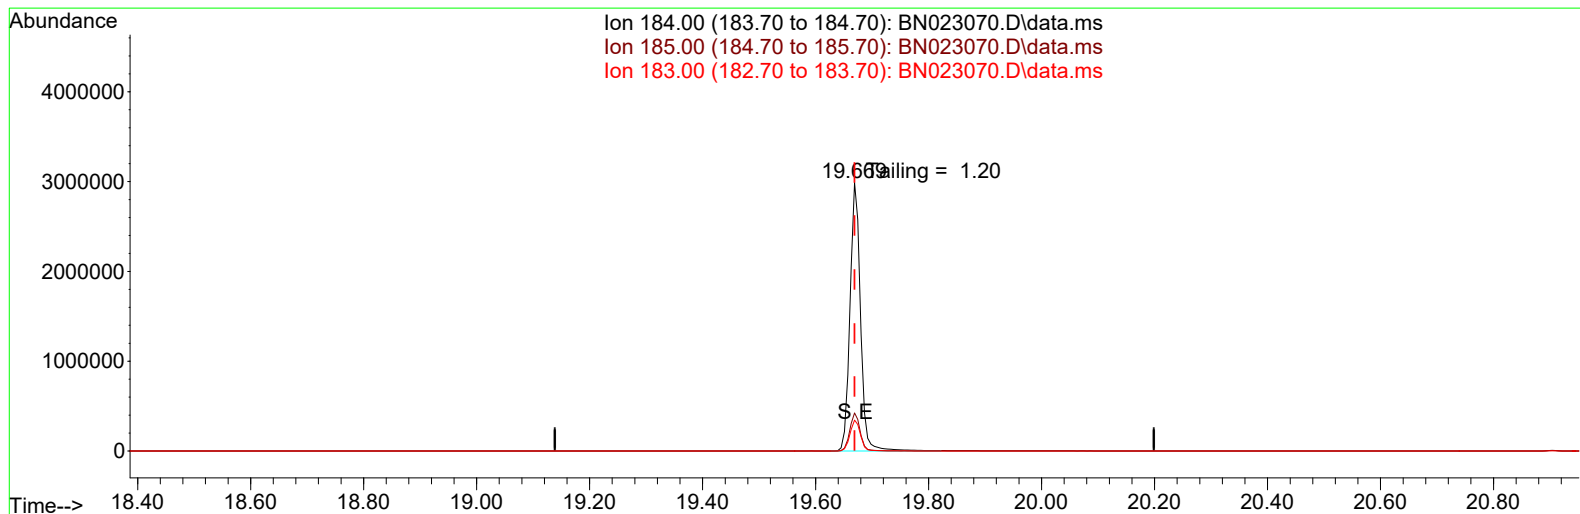

TIC: BN023070.D\data.ms

(77) Benzidine

19.669min (0.000) 0.00 ng

response 3898917

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.20
183.00	13.20	11.53
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/6/2022	BNA_N	<u>BN023070.D</u>
Compound Name	Response	Retention Time
DDT	1675602	20.904
DDD	13884	20.516
DDE	0	19.963
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13884	1689486	0.82

Instrument :
BNA_N
ClientSampleId :
DFTPP