




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035447.D
Acq On : 06 Dec 2024 04:47
Operator : RC/JU
Sample : P5104-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ71

Manual IntegrationsAPPROVED

Quant Time: Dec 06 05:15:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 02 18:25:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/13/2024

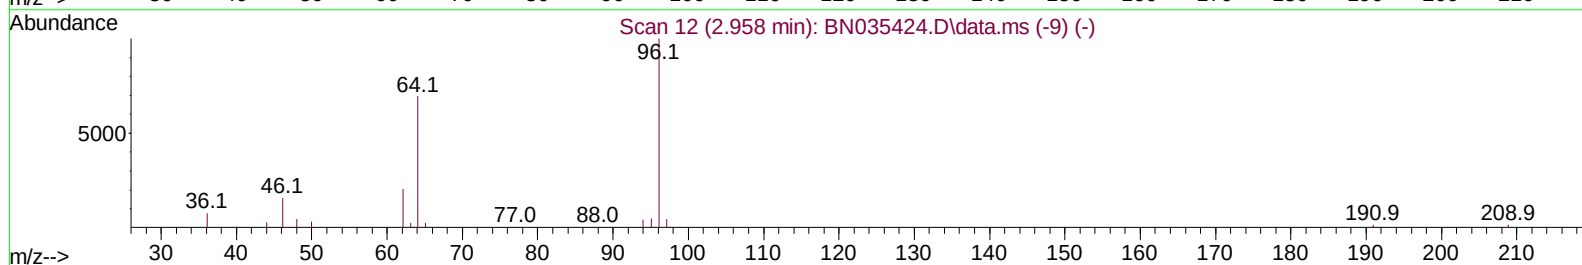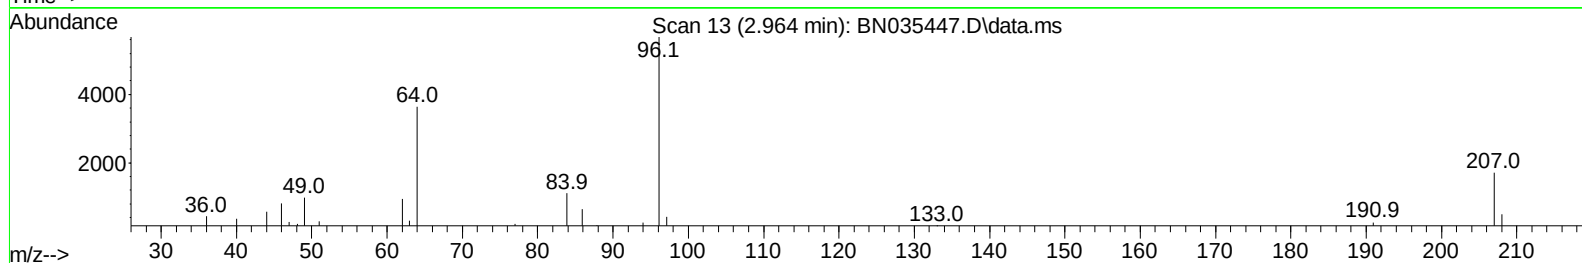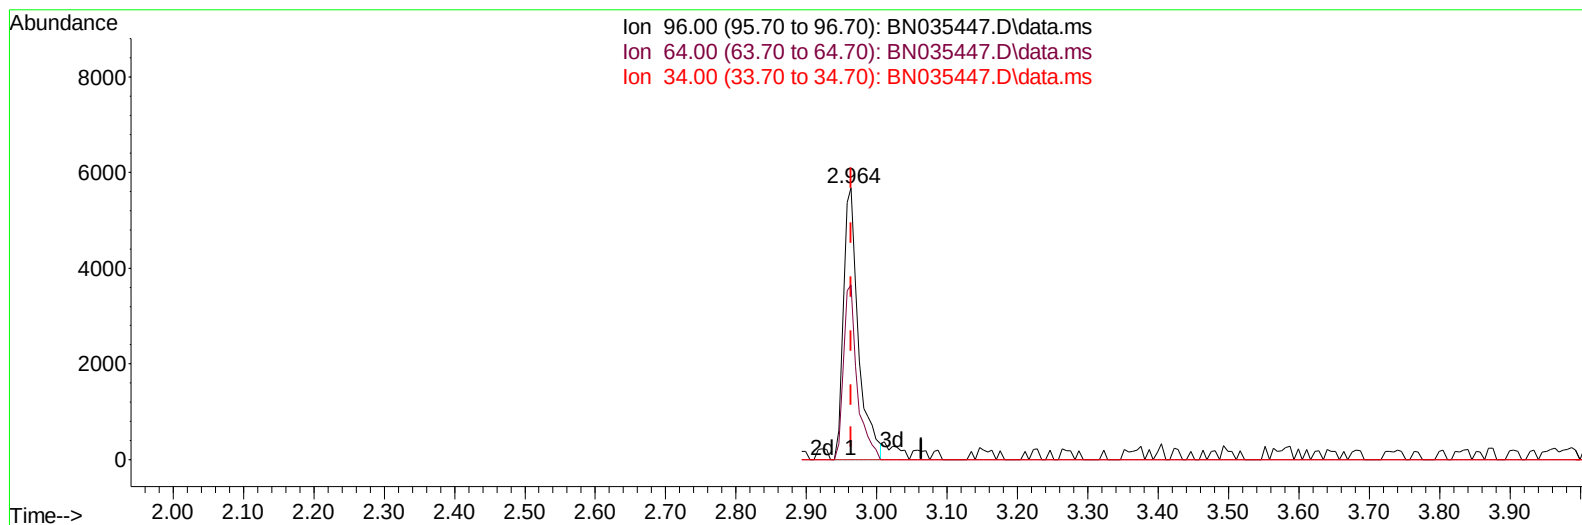

TIC: BN035447.D\data.ms

(3) 1,4-Dioxane-d8 (S)

2.964min (-0.000) 4.06 ng/uL

response 8350

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	62.30	64.22
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035447.D
Acq On : 06 Dec 2024 04:47
Operator : RC/JU
Sample : P5104-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ71

Manual IntegrationsAPPROVED

Quant Time: Dec 06 05:15:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 02 18:25:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/13/2024

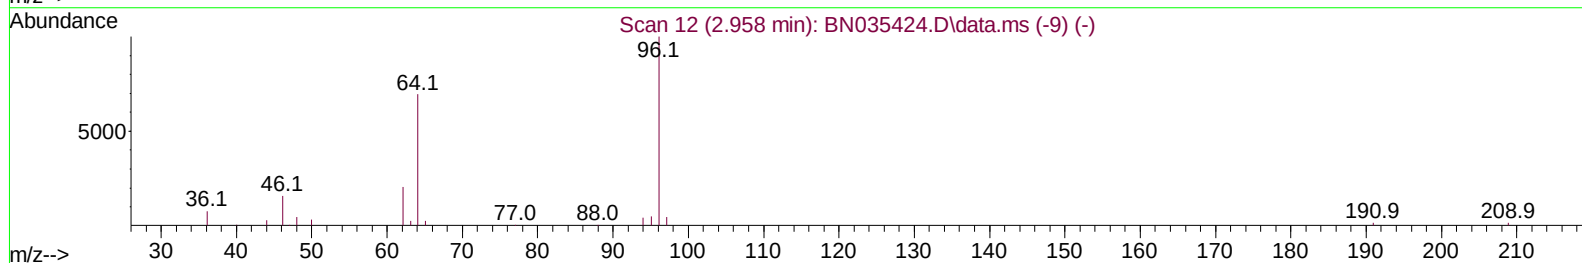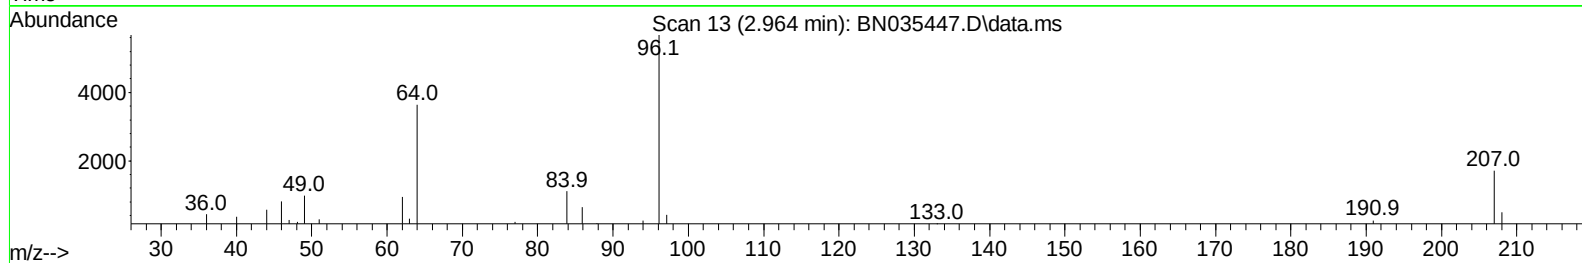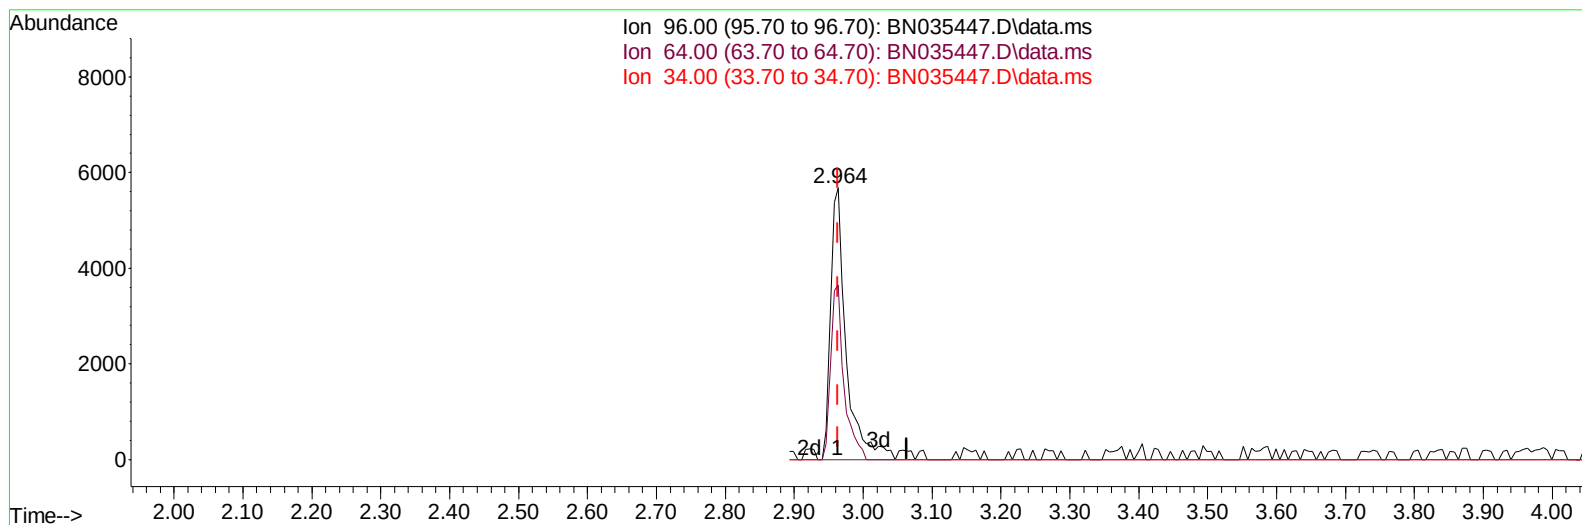

TIC: BN035447.D\data.ms

(3) 1,4-Dioxane-d8 (S)

2.964min (-0.000) 4.31 ng/uL m

response 8868

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	62.30	64.22
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035447.D
 Acq On : 06 Dec 2024 04:47
 Operator : RC/JU
 Sample : P5104-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHJ71

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/07/2024
 Supervised By :mohammad ahmed 12/13/2024

Quant Time: Dec 06 05:16:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 02 18:25:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.299	152	97282	20.000	ng/ul	0.00
20) Naphthalene-d8	10.046	136	410514	20.000	ng/ul	0.00
38) Acenaphthene-d10	13.957	164	321036	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.722	188	712093	20.000	ng/ul	0.00
79) Chrysene-d12	20.980	240	721779	20.000	ng/ul	0.00
88) Perylene-d12	23.645	264	810261	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.964	96	8868m	4.307	ng/uL	0.00
4) Pyridine-d5	3.346	84	25153	4.635	ng/ul	0.00
7) Phenol-d5	6.499	99	48929	7.060	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.658	67	110357	28.554	ng/ul	0.00
11) 2-Chlorophenol-d4	6.840	132	143758	24.479	ng/ul	0.00
15) 4-Methylphenol-d8	8.011	113	107116	17.736	ng/ul	0.00
21) Nitrobenzene-d5	8.434	128	80839	30.310	ng/ul	0.00
24) 2-Nitrophenol-d4	9.146	143	97323	31.526	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.681	165	189659	28.110	ng/ul	0.00
31) 4-Chloroaniline-d4	10.193	131	171318	20.564	ng/ul	0.00
46) Dimethylphthalate-d6	13.387	166	773033	33.535	ng/ul	0.00
49) Acenaphthylene-d8	13.646	160	768990	30.292	ng/ul	0.00
54) 4-Nitrophenol-d4	14.193	143	24560	6.470	ng/ul	0.00
60) Fluorene-d10	14.969	176	627930	31.543	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.098	200	117574	31.307	ng/ul	0.00
73) Anthracene-d10	16.828	188	1075788	34.252	ng/ul	0.00
81) Pyrene-d10	19.145	212	1315665	34.512	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.474	264	1438265	36.657	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035447.D
Acq On : 06 Dec 2024 04:47
Operator : RC/JU
Sample : P5104-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ71

Manual IntegrationsAPPROVED

Quant Time: Dec 06 05:16:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 02 18:25:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/07/2024
Supervised By :mohammad ahmed 12/13/2024

