

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035425.D
 Acq On : 05 Dec 2024 13:51
 Operator : RC/JU
 Sample : PB165386BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK386

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.963	9	13	19	rVB	15961	19057	0.78%	0.080%
2	3.340	73	77	101	rBV	184959	301214	12.29%	1.270%
3	3.640	125	128	131	rBV	5233	6325	0.26%	0.027%
4	6.498	608	614	626	rBV	272925	406088	16.57%	1.712%
5	6.657	635	641	651	rBV	224947	331487	13.52%	1.398%
6	6.840	665	672	684	rBV	290406	433070	17.67%	1.826%
7	7.298	743	750	760	rVB	328759	486204	19.84%	2.050%
8	8.010	864	871	884	rBV	370513	558739	22.80%	2.356%
9	8.434	935	943	953	rBV	253842	398630	16.26%	1.681%
10	9.145	1058	1064	1075	rBV	225788	346418	14.13%	1.461%
11	9.681	1148	1155	1167	rBV	380397	614903	25.09%	2.593%
12	10.045	1210	1217	1225	rBV	462442	737516	30.09%	3.110%
13	10.198	1236	1243	1254	rBV	366998	614878	25.09%	2.593%
14	11.645	1483	1489	1498	rVB3	4606	8834	0.36%	0.037%
15	13.386	1778	1785	1798	rBV	819102	1113605	45.44%	4.696%
16	13.645	1822	1829	1838	rBV	885659	1290459	52.65%	5.441%
17	13.957	1876	1882	1891	rBV	835970	1222516	49.88%	5.155%
18	14.192	1916	1922	1943	rBV	274380	451536	18.42%	1.904%
19	14.969	2047	2054	2061	rBV	1223010	1673162	68.27%	7.055%
20	15.098	2070	2076	2085	rBV	332219	420614	17.16%	1.774%
21	15.210	2091	2095	2100	rVB3	4253	5353	0.22%	0.023%
22	16.510	2313	2316	2323	rVB3	1887	2680	0.11%	0.011%
23	16.727	2346	2353	2362	rBV	1149188	1581183	64.51%	6.667%
24	16.821	2363	2369	2384	rVB2	1361112	1944130	79.32%	8.198%
25	18.704	2685	2689	2694	rBV2	14986	19371	0.79%	0.082%
26	18.774	2697	2701	2706	rBV	13069	18705	0.76%	0.079%
27	19.145	2758	2764	2774	rBV	1686166	2346344	95.73%	9.894%
28	20.980	3070	3076	3084	rBV	1380998	1908865	77.88%	8.049%
29	23.468	3491	3499	3514	rBV	1146536	2450964	100.00%	10.335%
30	23.651	3522	3530	3539	rBV	917479	2002892	81.72%	8.445%




Sum of corrected areas: 23715742

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035425.D
Acq On : 05 Dec 2024 13:51
Operator : RC/JU
Sample : PB165386BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK386

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

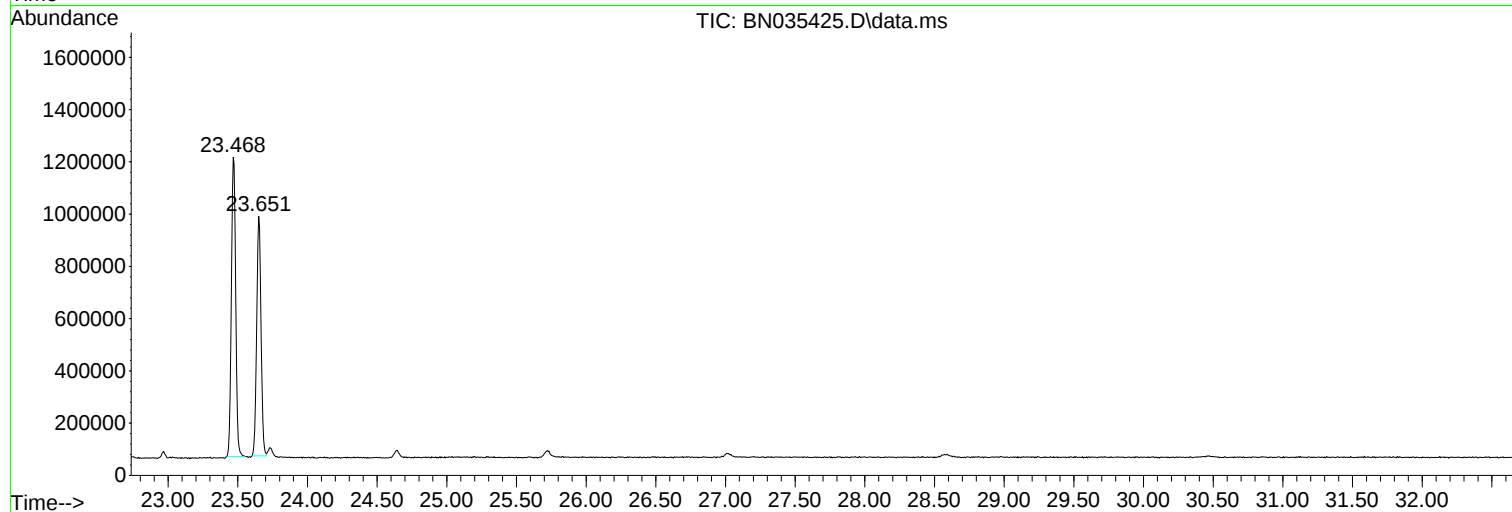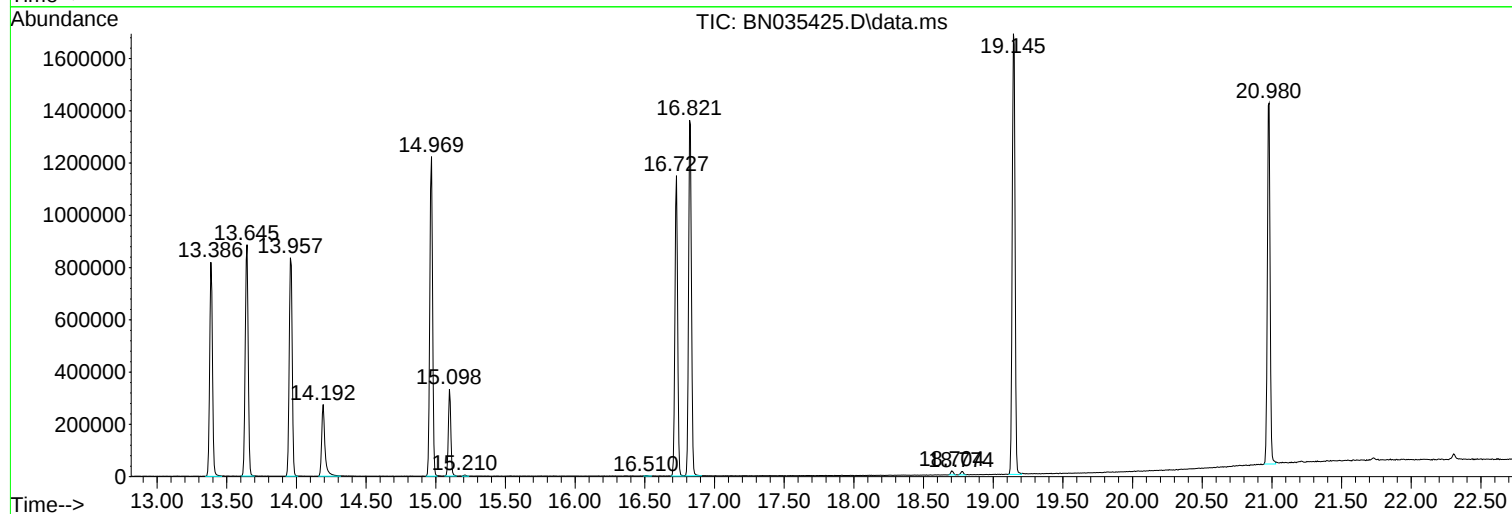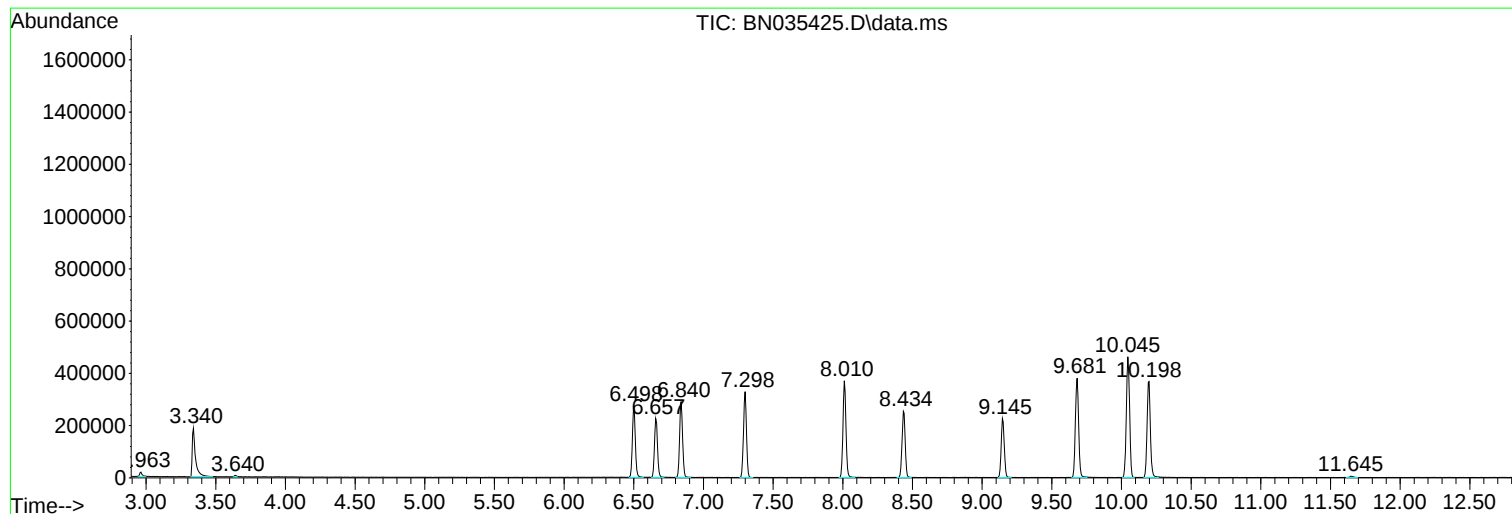

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035425.D
Acq On : 05 Dec 2024 13:51
Operator : RC/JU
Sample : PB165386BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK386

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035425.D
Acq On : 05 Dec 2024 13:51
Operator : RC/JU
Sample : PB165386BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK386

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc