

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035426.D
 Acq On : 05 Dec 2024 14:30
 Operator : RC/JU
 Sample : PB165388BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK388

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035426.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.964	9	13	19	rVB	14806	18486	0.78%	0.083%
2	3.340	73	77	101	rBV	179582	299743	12.64%	1.350%
3	3.640	124	128	132	rBV	3132	3948	0.17%	0.018%
4	6.499	608	614	624	rBV	257452	388949	16.40%	1.751%
5	6.658	635	641	652	rVB	215380	319643	13.47%	1.439%
6	6.840	666	672	684	rVB	283306	417558	17.60%	1.880%
7	7.299	744	750	760	rVB	293319	430951	18.17%	1.940%
8	8.010	865	871	883	rBV	348526	539463	22.74%	2.429%
9	8.434	937	943	956	rVB	243907	383166	16.15%	1.725%
10	9.146	1057	1064	1074	rBV	215824	335408	14.14%	1.510%
11	9.681	1148	1155	1169	rBV	368497	589638	24.86%	2.655%
12	10.046	1210	1217	1226	rVB	406459	651732	27.47%	2.934%
13	10.193	1235	1242	1258	rBV	350979	586757	24.73%	2.642%
14	11.645	1485	1489	1496	rBV2	3750	7343	0.31%	0.033%
15	13.387	1779	1785	1797	rBV	751825	1047181	44.14%	4.715%
16	13.645	1822	1829	1841	rBV	852407	1239323	52.24%	5.580%
17	13.957	1876	1882	1892	rBV	750445	1079975	45.53%	4.862%
18	14.192	1916	1922	1937	rBV	261158	419498	17.68%	1.889%
19	14.969	2047	2054	2065	rBV	1092153	1562182	65.85%	7.034%
20	15.098	2071	2076	2086	rBV	291780	377646	15.92%	1.700%
21	15.210	2089	2095	2099	rVB4	3805	5076	0.21%	0.023%
22	16.516	2312	2317	2321	rBV3	2009	3007	0.13%	0.014%
23	16.728	2347	2353	2363	rBV	1035982	1397685	58.92%	6.293%
24	16.822	2363	2369	2385	rVB	1267038	1837485	77.46%	8.273%
25	18.704	2685	2689	2695	rVB3	14205	19472	0.82%	0.088%
26	18.780	2697	2702	2707	rVB	11979	16881	0.71%	0.076%
27	19.145	2758	2764	2777	rBV	1632987	2232182	94.10%	10.050%
28	20.980	3070	3076	3086	rBV	1275159	1695217	71.46%	7.632%
29	22.304	3299	3301	3309	rVB4	21646	29346	1.24%	0.132%
30	22.968	3410	3414	3420	rVB3	25468	41730	1.76%	0.188%
31	23.474	3491	3500	3515	rBV	1096417	2372184	100.00%	10.680%
32	23.651	3522	3530	3539	rBV	811821	1798207	75.80%	8.096%
33	24.639	3694	3698	3705	rVB2	32191	63506	2.68%	0.286%




Sum of corrected areas: 22210568

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035426.D
Acq On : 05 Dec 2024 14:30
Operator : RC/JU
Sample : PB165388BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK388

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

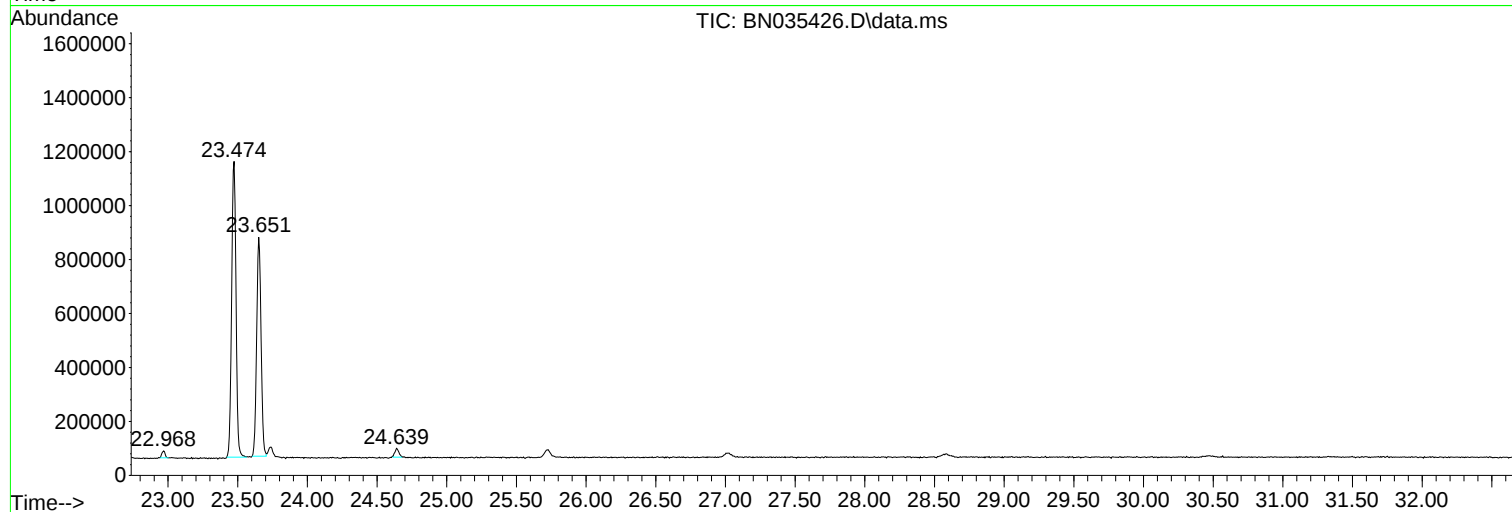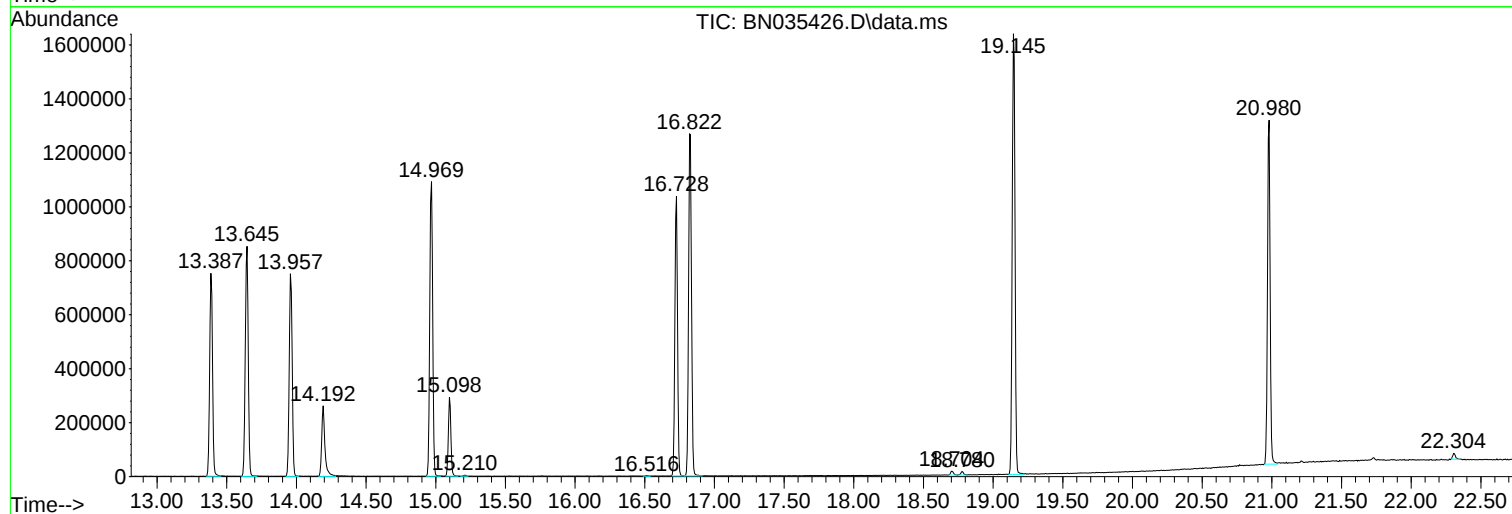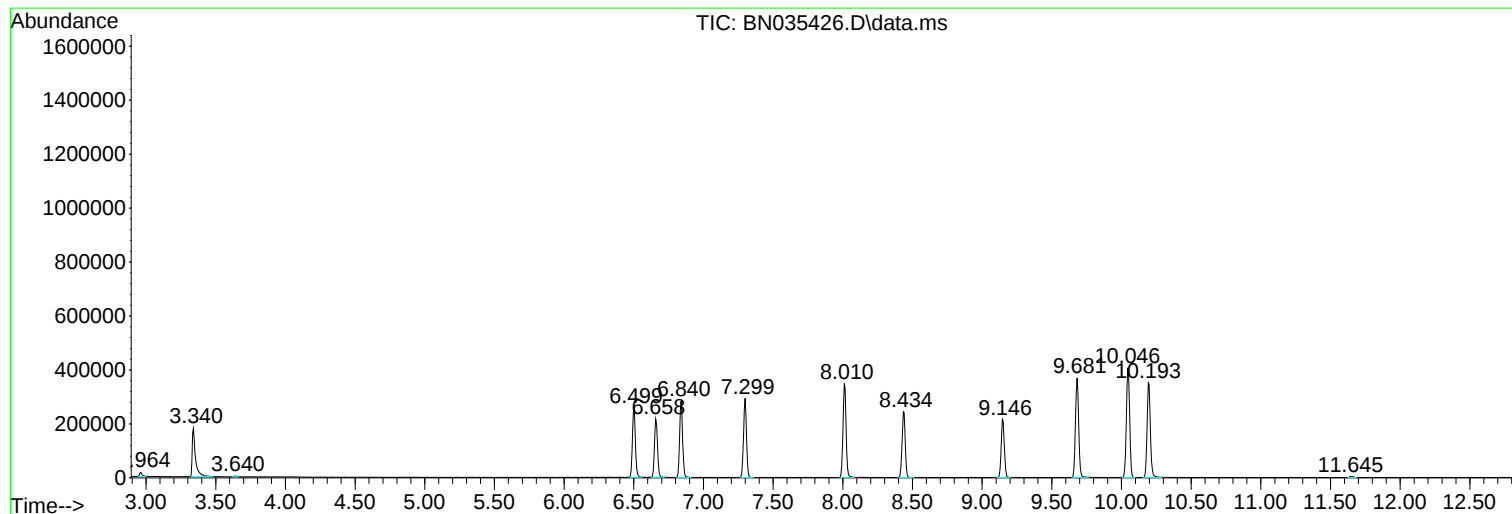

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035426.D
Acq On : 05 Dec 2024 14:30
Operator : RC/JU
Sample : PB165388BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK388

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035426.D
Acq On : 05 Dec 2024 14:30
Operator : RC/JU
Sample : PB165388BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK388

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc