

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035427.D
 Acq On : 05 Dec 2024 15:09
 Operator : RC/JU
 Sample : P5104-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH437

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.964	9	13	23	rVB	16546	21897	0.68%	0.084%
2	3.346	74	78	93	rBV	46518	73021	2.28%	0.281%
3	3.640	125	128	134	rBV3	3470	4504	0.14%	0.017%
4	4.069	198	201	206	rVB	8728	11946	0.37%	0.046%
5	6.499	609	614	623	rVB	87668	128429	4.01%	0.494%
6	6.658	635	641	651	rVB	250559	377681	11.79%	1.452%
7	6.840	665	672	681	rBV	297343	441329	13.77%	1.697%
8	7.299	743	750	759	rVB	333341	502008	15.67%	1.930%
9	8.010	865	871	881	rBV	267898	407862	12.73%	1.568%
10	8.434	935	943	953	rBV	295166	464676	14.50%	1.787%
11	8.904	1020	1023	1030	rVB3	3815	5405	0.17%	0.021%
12	9.146	1058	1064	1074	rBV	262252	411517	12.84%	1.582%
13	9.681	1148	1155	1164	rBV	466009	722690	22.56%	2.779%
14	10.046	1210	1217	1224	rBV	463095	748025	23.35%	2.876%
15	10.193	1236	1242	1256	rBV	319942	541114	16.89%	2.081%
16	11.387	1440	1445	1450	rVB3	1862	3210	0.10%	0.012%
17	11.651	1483	1490	1497	rBV3	6182	10303	0.32%	0.040%
18	13.387	1779	1785	1797	rBV	951273	1325737	41.38%	5.098%
19	13.645	1822	1829	1842	rBV	1036057	1500835	46.84%	5.771%
20	13.957	1875	1882	1894	rBV	841731	1234938	38.55%	4.749%
21	14.192	1916	1922	1935	rBV	66565	120954	3.78%	0.465%
22	14.828	2028	2030	2034	rVB	4720	4252	0.13%	0.016%
23	14.969	2047	2054	2062	rBV	1411010	1959884	61.17%	7.537%
24	15.098	2071	2076	2091	rVB	417874	542435	16.93%	2.086%
25	15.210	2091	2095	2100	rVB3	5581	6923	0.22%	0.027%
26	15.375	2119	2123	2126	rVB4	2815	3237	0.10%	0.012%
27	15.692	2173	2177	2182	rVB2	2387	3709	0.12%	0.014%
28	16.510	2312	2316	2320	rBV2	2817	3544	0.11%	0.014%
29	16.728	2346	2353	2363	rBV	1187350	1615456	50.42%	6.212%
30	16.828	2363	2370	2378	rBV	1711989	2428914	75.81%	9.340%
31	17.669	2510	2513	2520	rBV	8739	12324	0.38%	0.047%
32	17.739	2520	2525	2529	rVB	8830	10826	0.34%	0.042%
33	18.704	2682	2689	2695	rBV2	20836	28434	0.89%	0.109%
34	18.775	2696	2701	2705	rBV	18103	23082	0.72%	0.089%
35	18.851	2710	2714	2720	rBV2	13018	18384	0.57%	0.071%
36	18.980	2732	2736	2740	rBV3	9876	11925	0.37%	0.046%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035427.D
Acq On : 05 Dec 2024 15:09
Operator : RC/JU
Sample : P5104-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH437

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION

37	19.151	2758	2765	2774	rBV	2112681	2960705	92.41%	11.385%
38	20.574	3005	3007	3009	rBV	8632	5480	0.17%	0.021%
39	20.980	3070	3076	3086	rBV	1490884	1979241	61.78%	7.611%
40	23.474	3491	3500	3514	rBV	1454427	3203866	100.00%	12.320%
41	23.657	3522	3531	3540	rBV	967804	2124382	66.31%	8.169%




Sum of corrected areas: 26005084

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035427.D
Acq On : 05 Dec 2024 15:09
Operator : RC/JU
Sample : P5104-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH437

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

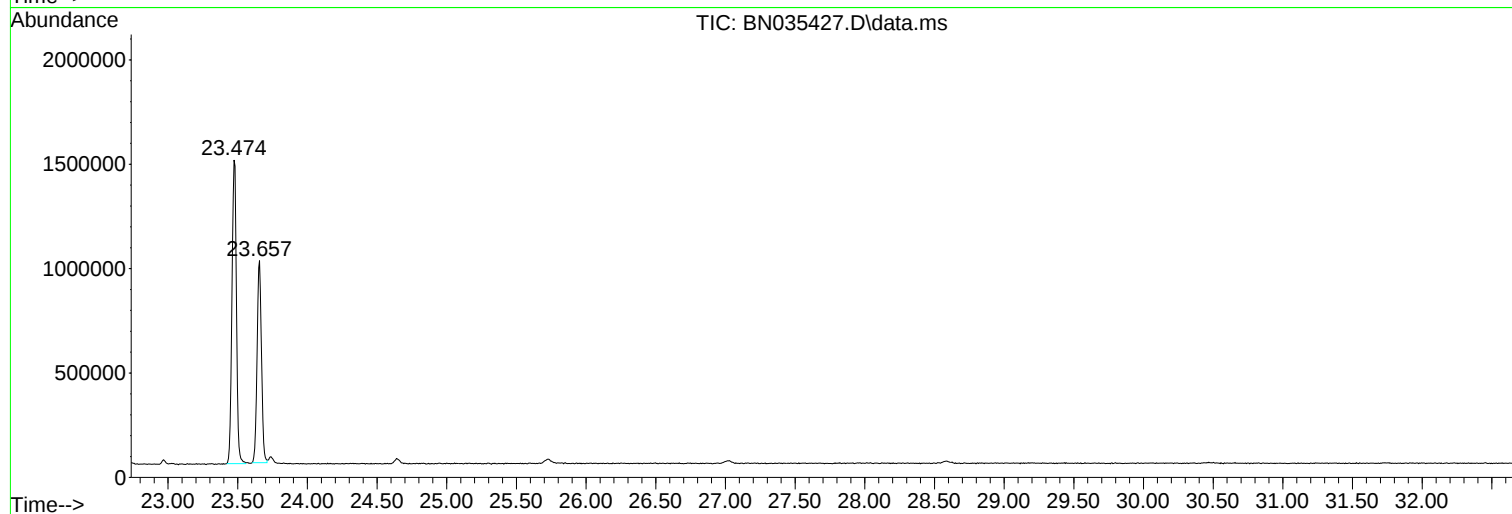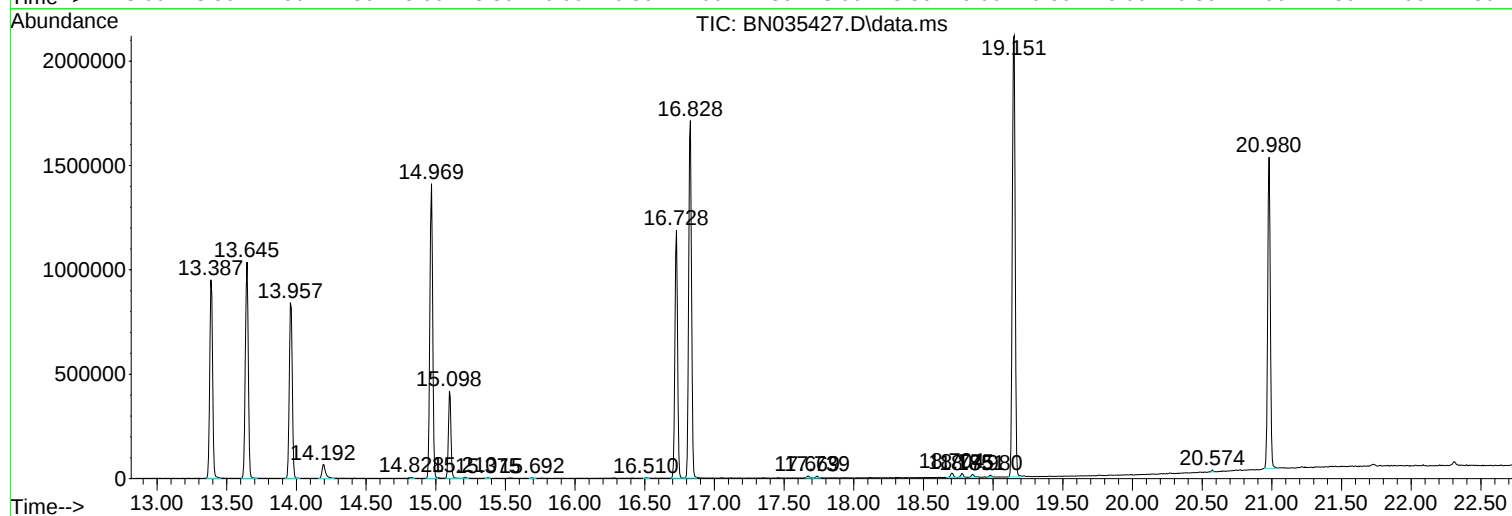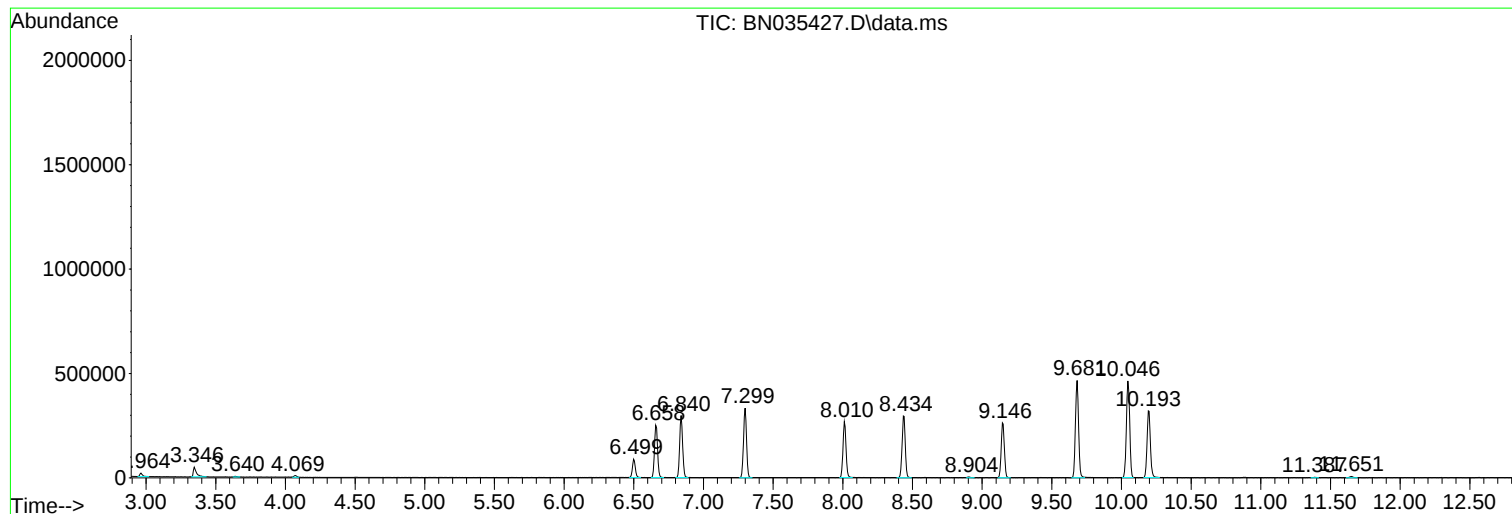

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035427.D
Acq On : 05 Dec 2024 15:09
Operator : RC/JU
Sample : P5104-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH437

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035427.D
Acq On : 05 Dec 2024 15:09
Operator : RC/JU
Sample : P5104-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH437

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc