

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035428.D
 Acq On : 05 Dec 2024 15:48
 Operator : RC/JU
 Sample : P5104-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHJ60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035428.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.964	9	13	22	rVB	18781	27083	0.74%	0.088%
2	3.346	75	78	94	rBV	39331	64226	1.76%	0.209%
3	3.640	125	128	132	rBV2	4353	5316	0.15%	0.017%
4	4.070	198	201	206	rVB	11229	15384	0.42%	0.050%
5	6.499	608	614	626	rBV	133401	199875	5.47%	0.649%
6	6.658	634	641	653	rBV	309627	466771	12.76%	1.515%
7	6.840	666	672	681	rBV	378967	551644	15.08%	1.791%
8	7.299	743	750	761	rVB	411944	612733	16.75%	1.989%
9	8.011	865	871	884	rBV	398574	597965	16.35%	1.941%
10	8.434	936	943	952	rBV	376793	584722	15.99%	1.898%
11	8.905	1017	1023	1028	rVB	6605	9437	0.26%	0.031%
12	9.146	1058	1064	1073	rBV	334947	519005	14.19%	1.685%
13	9.681	1148	1155	1166	rBV	568065	896867	24.52%	2.912%
14	10.046	1210	1217	1226	rBV	571266	912174	24.94%	2.961%
15	10.193	1234	1242	1261	rBV	305380	515397	14.09%	1.673%
16	11.387	1440	1445	1449	rVB2	3421	4765	0.13%	0.015%
17	11.646	1485	1489	1495	rBV2	6583	10802	0.30%	0.035%
18	13.387	1779	1785	1799	rBV	1092529	1552276	42.45%	5.040%
19	13.646	1822	1829	1841	rBV	1213750	1750993	47.88%	5.685%
20	13.957	1875	1882	1892	rBV	996867	1445981	39.54%	4.695%
21	14.193	1916	1922	1937	rBV	98142	160215	4.38%	0.520%
22	14.416	1952	1960	1963	rBV3	3715	5006	0.14%	0.016%
23	14.969	2047	2054	2062	rBV	1682923	2308614	63.13%	7.495%
24	15.098	2070	2076	2087	rVV	505966	667617	18.26%	2.168%
25	15.210	2089	2095	2099	rVB3	6547	8485	0.23%	0.028%
26	16.728	2347	2353	2362	rBV	1389249	1875774	51.29%	6.090%
27	16.828	2362	2370	2383	rBV	1982830	2738051	74.87%	8.889%
28	17.675	2508	2514	2520	rBV	25553	35935	0.98%	0.117%
29	17.739	2522	2525	2529	rVB2	2997	3784	0.10%	0.012%
30	18.122	2585	2590	2593	rBV3	2127	3827	0.10%	0.012%
31	18.704	2684	2689	2694	rVB	24908	30654	0.84%	0.100%
32	18.775	2696	2701	2706	rBV	22272	29675	0.81%	0.096%
33	18.857	2710	2715	2726	rVV	120419	159270	4.36%	0.517%
34	18.981	2732	2736	2743	rBV4	15096	18984	0.52%	0.062%
35	19.145	2758	2764	2776	rBV	2479708	3483436	95.25%	11.309%
36	19.869	2885	2887	2890	rBV4	4221	4762	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035428.D
Acq On : 05 Dec 2024 15:48
Operator : RC/JU
Sample : P5104-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ60

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION

37	20.980	3070	3076	3085	rBV	1767669	2356668	64.44%	7.651%
38	22.969	3411	3414	3419	rVB3	22129	34658	0.95%	0.113%
39	23.474	3491	3500	3514	rBV	1603405	3657105	100.00%	11.873%
40	23.657	3522	3531	3539	rBV	1108194	2475178	67.68%	8.036%




Sum of corrected areas: 30801114

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035428.D
Acq On : 05 Dec 2024 15:48
Operator : RC/JU
Sample : P5104-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

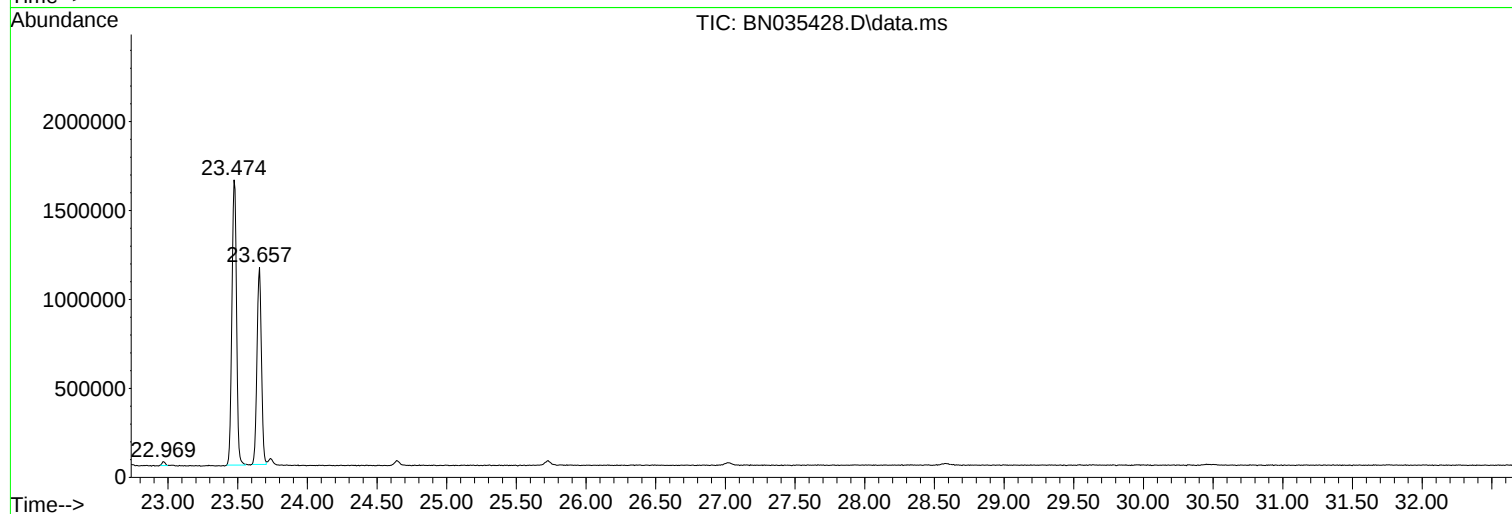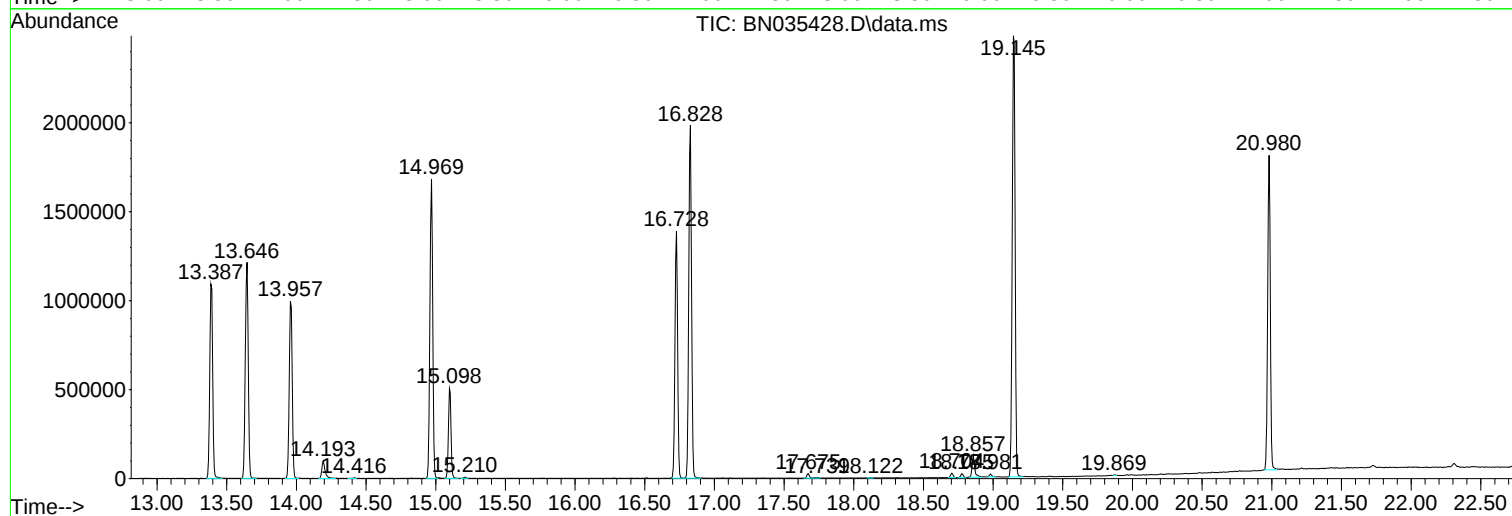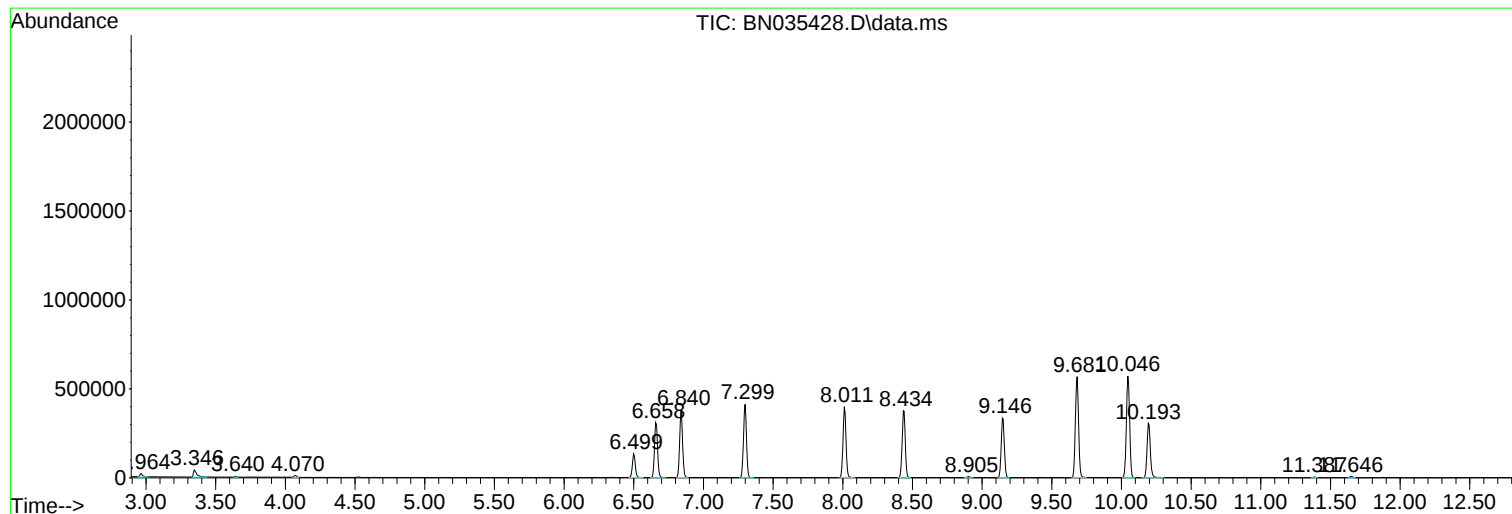

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035428.D
Acq On : 05 Dec 2024 15:48
Operator : RC/JU
Sample : P5104-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035428.D
Acq On : 05 Dec 2024 15:48
Operator : RC/JU
Sample : P5104-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------