

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035432.D
 Acq On : 05 Dec 2024 18:24
 Operator : RC/JU
 Sample : P5104-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHJ64

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035432.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	9	12	22	rVB	13275	18445	0.56%	0.069%
2	3.346	74	78	92	rBV	53654	92933	2.84%	0.350%
3	3.640	125	128	134	rVB2	3729	5491	0.17%	0.021%
4	4.069	197	201	209	rVB	8147	12248	0.37%	0.046%
5	4.528	270	279	284	rVB3	2345	4780	0.15%	0.018%
6	6.499	608	614	628	rVB	92564	137895	4.21%	0.519%
7	6.657	634	641	652	rBV	253658	371859	11.36%	1.399%
8	6.840	663	672	680	rBV	294112	431124	13.17%	1.622%
9	7.299	744	750	759	rVB	329981	492951	15.06%	1.855%
10	8.010	865	871	884	rBV	288069	443308	13.54%	1.668%
11	8.434	935	943	952	rBV	294861	467118	14.27%	1.758%
12	8.904	1018	1023	1028	rBV3	5128	7195	0.22%	0.027%
13	9.146	1058	1064	1076	rVB	264054	409660	12.52%	1.542%
14	9.681	1148	1155	1166	rBV	450365	712448	21.77%	2.681%
15	10.046	1210	1217	1224	rBV	482565	753549	23.02%	2.836%
16	10.193	1236	1242	1257	rBV	366329	614604	18.78%	2.313%
17	11.651	1485	1490	1496	rBV2	5701	8619	0.26%	0.032%
18	13.387	1779	1785	1804	rBV	987888	1344173	41.07%	5.058%
19	13.645	1822	1829	1839	rBV	1068563	1511979	46.19%	5.690%
20	13.957	1875	1882	1891	rBV	857470	1243622	38.00%	4.680%
21	14.192	1915	1922	1933	rBV	70974	122400	3.74%	0.461%
22	14.969	2047	2054	2062	rBV	1458049	2026490	61.91%	7.626%
23	15.098	2071	2076	2086	rVB	453620	579501	17.71%	2.181%
24	15.210	2091	2095	2100	rVB	5159	6340	0.19%	0.024%
25	16.510	2312	2316	2320	rBV3	2183	3326	0.10%	0.013%
26	16.728	2346	2353	2363	rBV	1132932	1616809	49.40%	6.084%
27	16.828	2363	2370	2382	rBV	1796681	2537055	77.51%	9.547%
28	17.116	2413	2419	2423	rBV5	1915	3628	0.11%	0.014%
29	17.669	2510	2513	2519	rBV2	17556	23656	0.72%	0.089%
30	18.704	2684	2689	2697	rBV2	22140	29749	0.91%	0.112%
31	18.774	2697	2701	2705	rVV	21525	26103	0.80%	0.098%
32	18.857	2710	2715	2725	rBV	90585	118287	3.61%	0.445%
33	18.980	2733	2736	2743	rVB3	11723	14733	0.45%	0.055%
34	19.145	2758	2764	2773	rBV	2217648	3072572	93.87%	11.563%
35	19.292	2785	2789	2793	rVB5	10937	12769	0.39%	0.048%
36	19.404	2806	2808	2812	rBV3	3470	3462	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035432.D
Acq On : 05 Dec 2024 18:24
Operator : RC/JU
Sample : P5104-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ64

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION

37	20.974	3070	3075	3086	rBV	1436547	1948513	59.53%	7.333%
38	23.474	3491	3500	3513	rBV	1492071	3273092	100.00%	12.317%
39	23.651	3521	3530	3539	rBV	930448	2070603	63.26%	7.792%




Sum of corrected areas: 26573089

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035432.D
Acq On : 05 Dec 2024 18:24
Operator : RC/JU
Sample : P5104-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ64

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

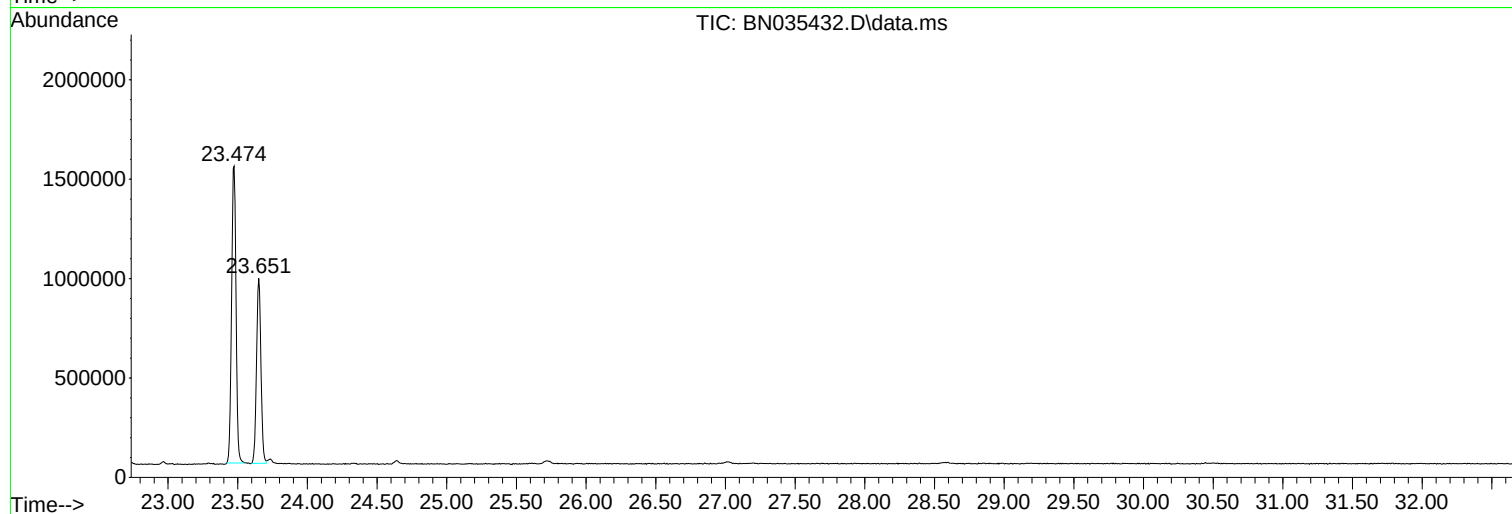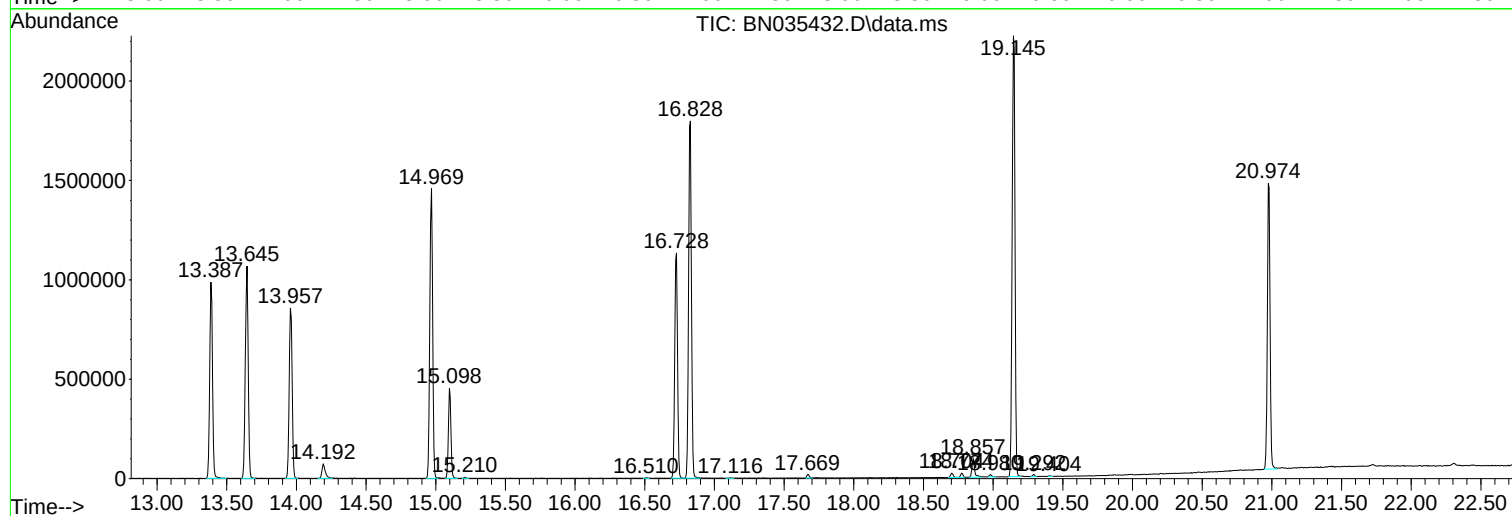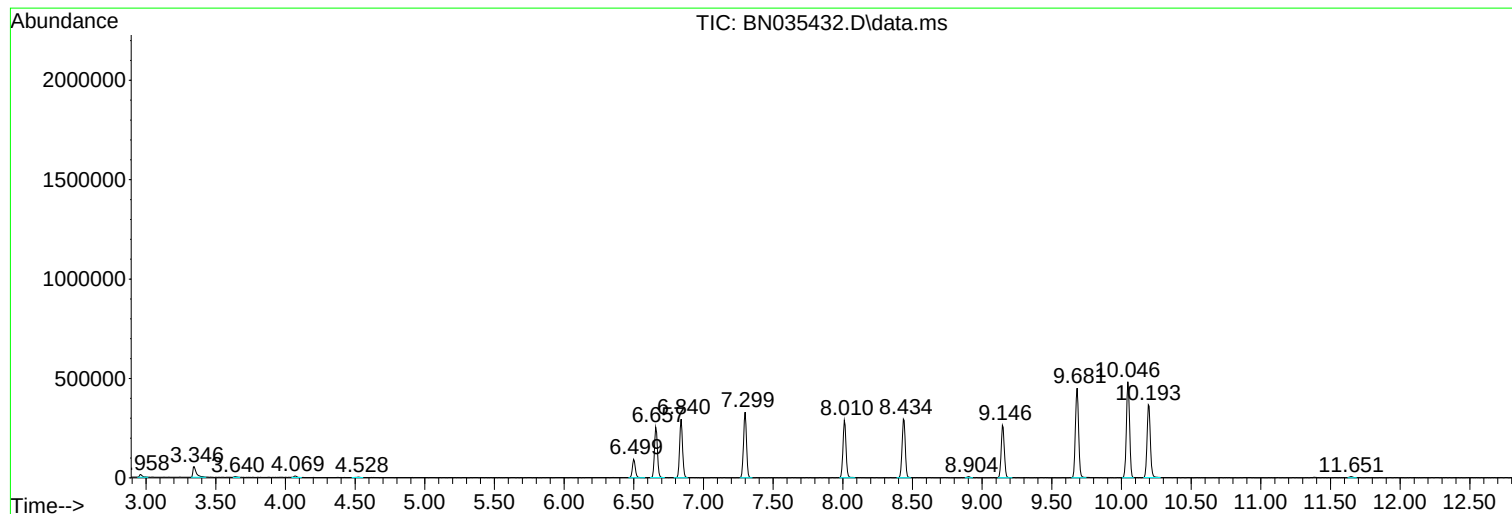

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035432.D
Acq On : 05 Dec 2024 18:24
Operator : RC/JU
Sample : P5104-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ64

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035432.D
Acq On : 05 Dec 2024 18:24
Operator : RC/JU
Sample : P5104-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ64

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc