

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035433.D
 Acq On : 05 Dec 2024 19:03
 Operator : RC/JU
 Sample : P5104-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHJ65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035433.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.964	9	13	22	rBV	14379	19052	0.60%	0.073%
2	3.346	74	78	92	rVB	54889	93517	2.95%	0.357%
3	3.640	123	128	132	rBV2	3792	5058	0.16%	0.019%
4	4.070	197	201	206	rVB	9080	11585	0.37%	0.044%
5	6.499	605	614	624	rBV	98505	145836	4.60%	0.557%
6	6.658	634	641	654	rBV	255587	380987	12.01%	1.455%
7	6.840	665	672	681	rVB	303362	454217	14.31%	1.734%
8	7.299	743	750	757	rBV	324875	488328	15.39%	1.864%
9	8.011	865	871	885	rBV	298190	450475	14.20%	1.720%
10	8.434	932	943	953	rVB	310195	473339	14.92%	1.807%
11	8.905	1019	1023	1028	rVB	6486	8493	0.27%	0.032%
12	9.146	1057	1064	1072	rBV	273549	417025	13.14%	1.592%
13	9.681	1148	1155	1168	rBV	452243	732296	23.08%	2.796%
14	10.046	1210	1217	1224	rBV	464389	741265	23.36%	2.830%
15	10.193	1235	1242	1257	rBV	383401	630031	19.86%	2.405%
16	11.646	1485	1489	1499	rVB2	5581	9578	0.30%	0.037%
17	13.387	1779	1785	1799	rBV	996323	1373322	43.28%	5.243%
18	13.646	1822	1829	1839	rBV	1047736	1528304	48.16%	5.835%
19	13.957	1876	1882	1894	rBV	857405	1192413	37.58%	4.552%
20	14.193	1916	1922	1934	rBV	78844	135782	4.28%	0.518%
21	14.416	1957	1960	1964	rVB3	3761	4809	0.15%	0.018%
22	14.969	2047	2054	2061	rBV	1475578	2079052	65.52%	7.937%
23	15.098	2071	2076	2084	rBV	444895	563004	17.74%	2.149%
24	15.210	2091	2095	2098	rVB2	5552	6846	0.22%	0.026%
25	16.510	2313	2316	2320	rBV	2593	3313	0.10%	0.013%
26	16.728	2346	2353	2361	rBV	1129931	1554297	48.98%	5.934%
27	16.828	2363	2370	2380	rVV	1751181	2471518	77.89%	9.436%
28	17.669	2509	2513	2518	rBV2	17834	22035	0.69%	0.084%
29	17.739	2521	2525	2531	rVB2	2903	4956	0.16%	0.019%
30	18.116	2587	2589	2595	rVB5	2653	3484	0.11%	0.013%
31	18.704	2685	2689	2693	rBV2	20737	27835	0.88%	0.106%
32	18.775	2693	2701	2706	rBV	19262	25848	0.81%	0.099%
33	18.857	2710	2715	2729	rVV	89534	125030	3.94%	0.477%
34	18.981	2732	2736	2743	rVB8	9156	14363	0.45%	0.055%
35	19.145	2758	2764	2776	rBV	2222226	2998270	94.49%	11.447%
36	19.404	2805	2808	2814	rVB	5246	7812	0.25%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035433.D
Acq On : 05 Dec 2024 19:03
Operator : RC/JU
Sample : P5104-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ65

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION

37	20.980	3070	3076	3086	rBV	1377019	1882318	59.32%	7.186%
38	23.474	3490	3500	3513	rBV	1417745	3173067	100.00%	12.114%
39	23.651	3522	3530	3540	rBV	885468	1934591	60.97%	7.386%




Sum of corrected areas: 26193351

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035433.D
Acq On : 05 Dec 2024 19:03
Operator : RC/JU
Sample : P5104-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ65

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

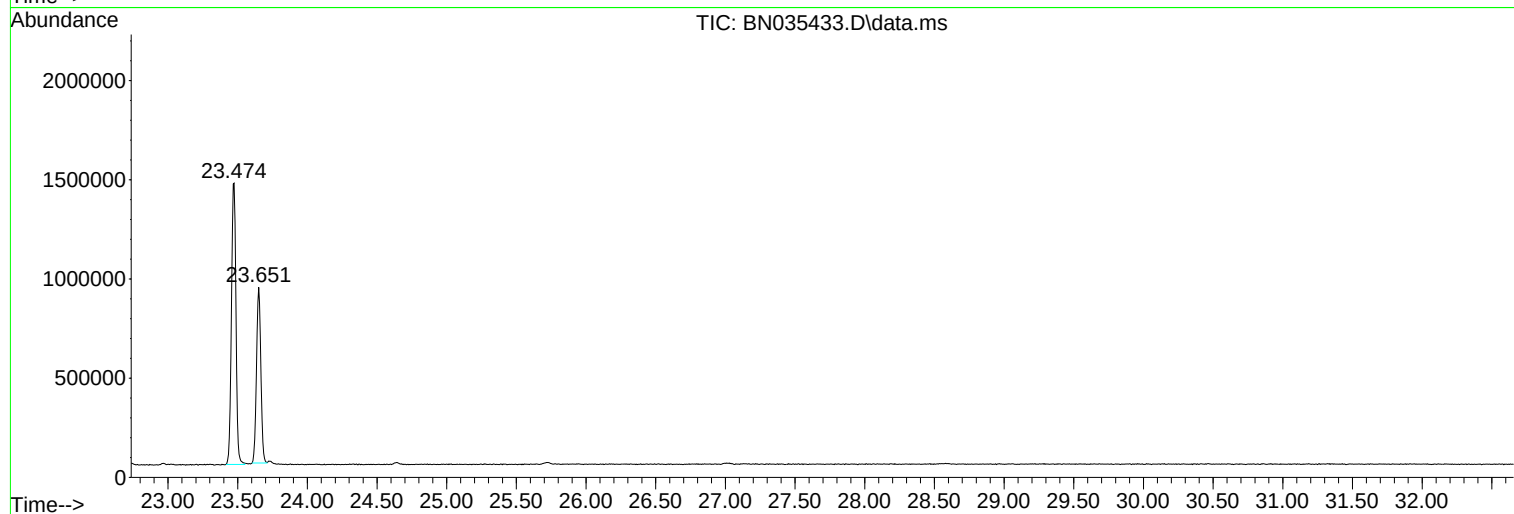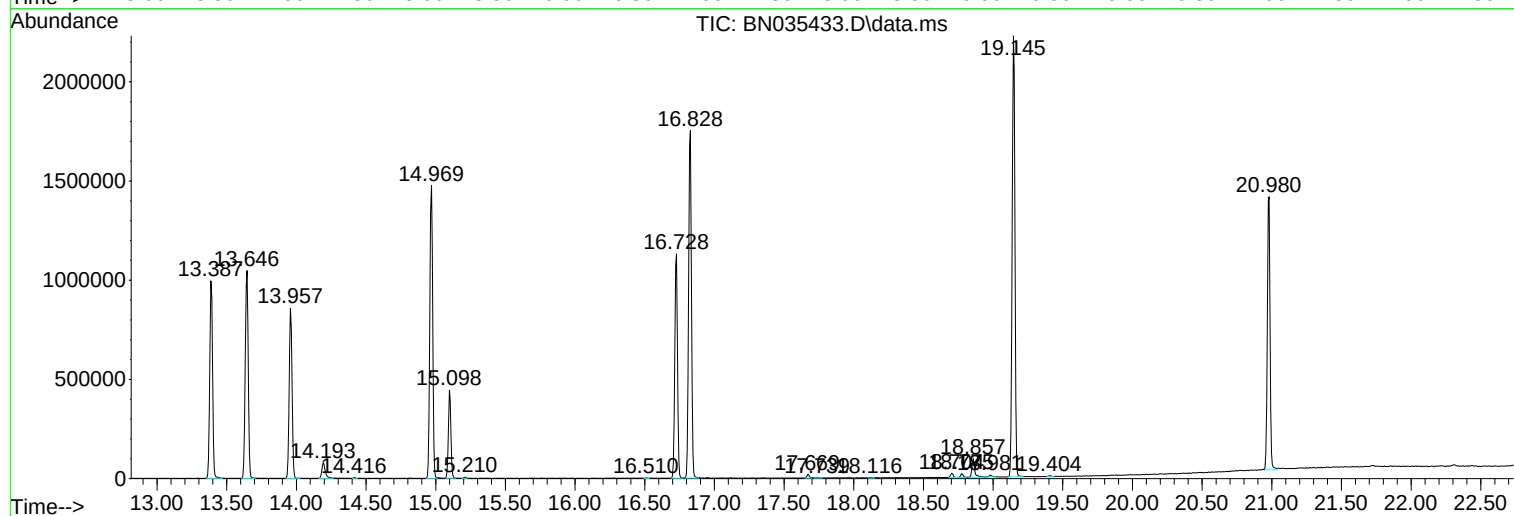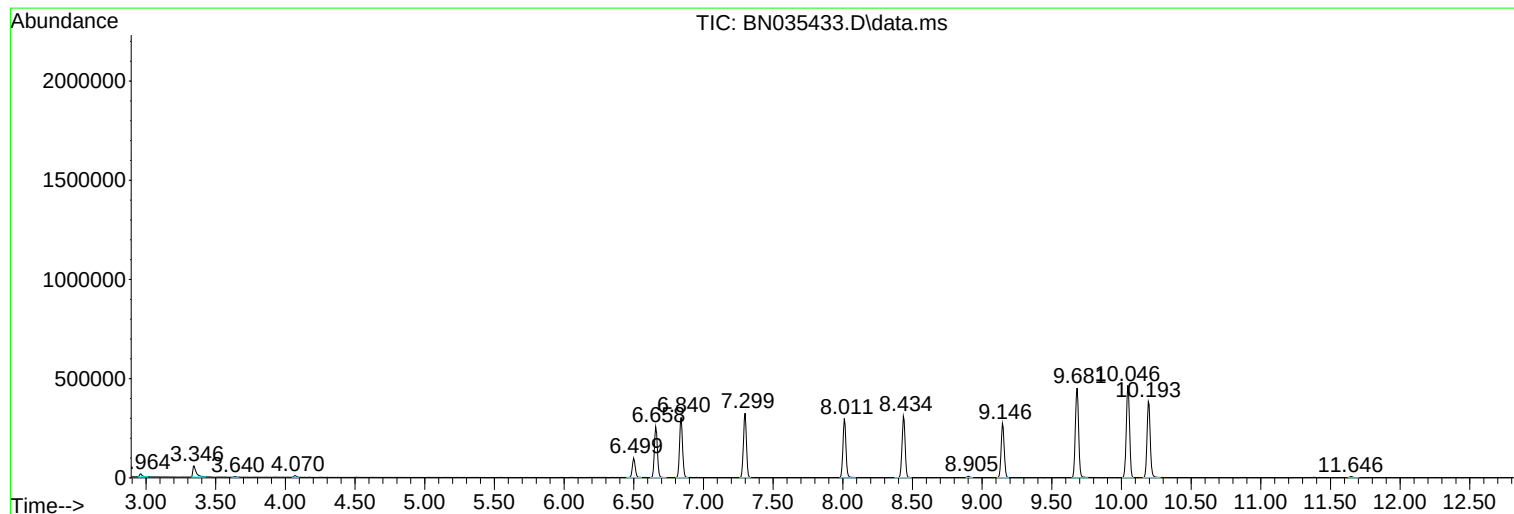

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035433.D
Acq On : 05 Dec 2024 19:03
Operator : RC/JU
Sample : P5104-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ65

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035433.D
Acq On : 05 Dec 2024 19:03
Operator : RC/JU
Sample : P5104-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ65

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc