

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035441.D
 Acq On : 06 Dec 2024 00:54
 Operator : RC/JU
 Sample : PB165400BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK400

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035441.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	9	12	22	rVB	16284	21865	0.81%	0.084%
2	3.340	73	77	93	rBV	192607	322039	12.00%	1.238%
3	3.646	124	129	132	rBV2	3707	4697	0.18%	0.018%
4	6.499	608	614	624	rBV	303311	449923	16.76%	1.729%
5	6.658	635	641	652	rBV	240148	357459	13.32%	1.374%
6	6.840	665	672	680	rBV	313875	471896	17.58%	1.814%
7	7.299	742	750	760	rBV	360882	547082	20.38%	2.103%
8	8.010	865	871	883	rBV	407477	617065	22.99%	2.372%
9	8.434	936	943	955	rVB	290432	446700	16.64%	1.717%
10	9.146	1058	1064	1076	rBV	262081	393732	14.67%	1.513%
11	9.681	1148	1155	1169	rBV	425000	681793	25.40%	2.621%
12	10.046	1210	1217	1224	rBV	513516	822780	30.66%	3.163%
13	10.193	1236	1242	1252	rBV	405303	665416	24.79%	2.558%
14	11.646	1484	1489	1496	rVB	5528	9411	0.35%	0.036%
15	13.387	1779	1785	1799	rBV	886993	1197438	44.61%	4.603%
16	13.645	1822	1829	1842	rVB	934658	1382126	51.50%	5.313%
17	13.957	1875	1882	1891	rBV	945872	1347637	50.21%	5.180%
18	14.192	1916	1922	1936	rBV	319205	508988	18.96%	1.956%
19	14.969	2047	2054	2061	rBV	1227435	1744569	65.00%	6.706%
20	15.098	2071	2076	2090	rBV	367568	470946	17.55%	1.810%
21	15.204	2090	2094	2099	rVB3	5031	6268	0.23%	0.024%
22	16.510	2312	2316	2320	rBV3	2074	3021	0.11%	0.012%
23	16.722	2346	2352	2360	rBV	1202017	1718360	64.02%	6.605%
24	16.822	2363	2369	2382	rVV2	1468185	2031509	75.69%	7.809%
25	18.704	2684	2689	2693	rBV2	16989	21279	0.79%	0.082%
26	18.780	2698	2702	2707	rVB	13013	18375	0.68%	0.071%
27	19.145	2758	2764	2777	rBV	1862764	2446838	91.17%	9.405%
28	19.586	2837	2839	2842	rBV4	2094	2727	0.10%	0.010%
29	20.974	3070	3075	3084	rBV	1520370	2066984	77.01%	7.945%
30	22.304	3298	3301	3308	rVB3	29275	45575	1.70%	0.175%
31	22.963	3409	3413	3419	rVB3	32619	58523	2.18%	0.225%
32	23.468	3491	3499	3515	rVB	1243090	2683945	100.00%	10.317%
33	23.651	3522	3530	3539	rBV	992964	2247046	83.72%	8.637%
34	23.733	3540	3544	3552	rVB2	52832	112350	4.19%	0.432%
35	24.639	3695	3698	3708	rVB4	42767	89280	3.33%	0.343%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035441.D
Acq On : 06 Dec 2024 00:54
Operator : RC/JU
Sample : PB165400BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK400

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 26015642

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035441.D
Acq On : 06 Dec 2024 00:54
Operator : RC/JU
Sample : PB165400BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK400

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

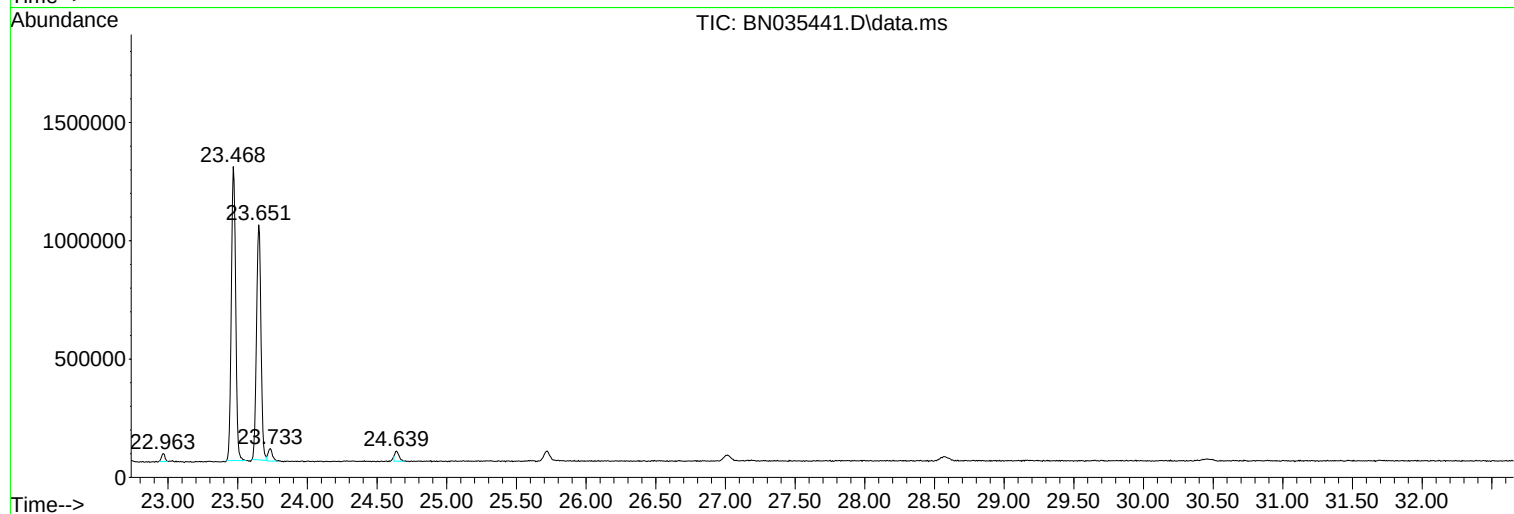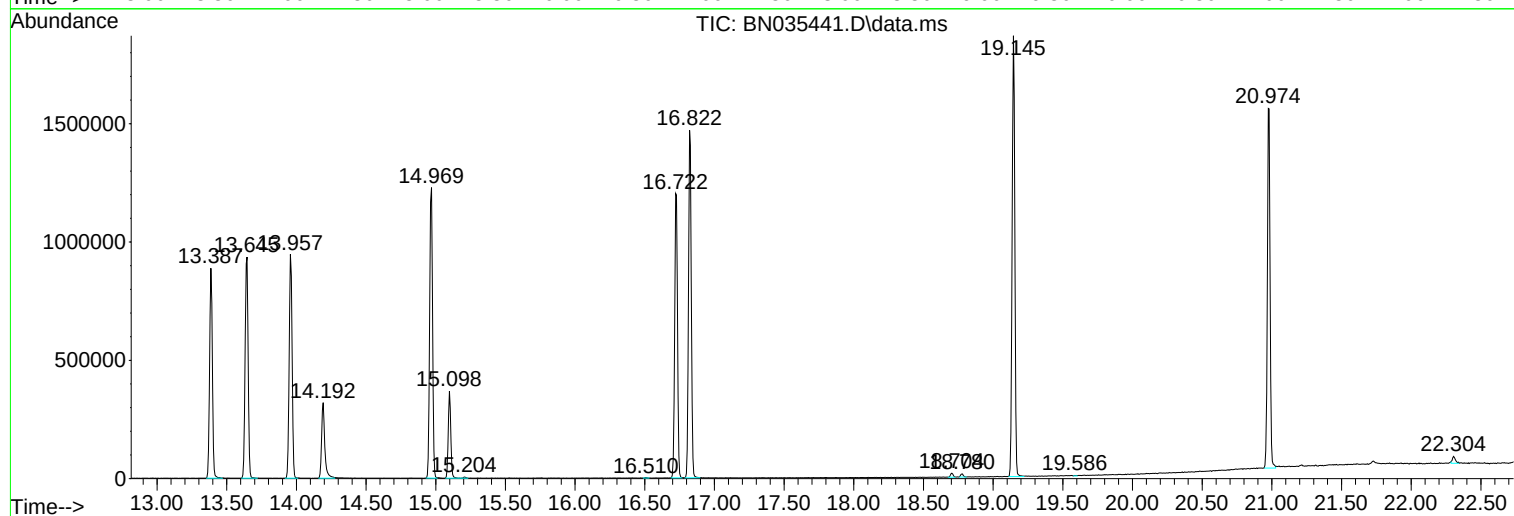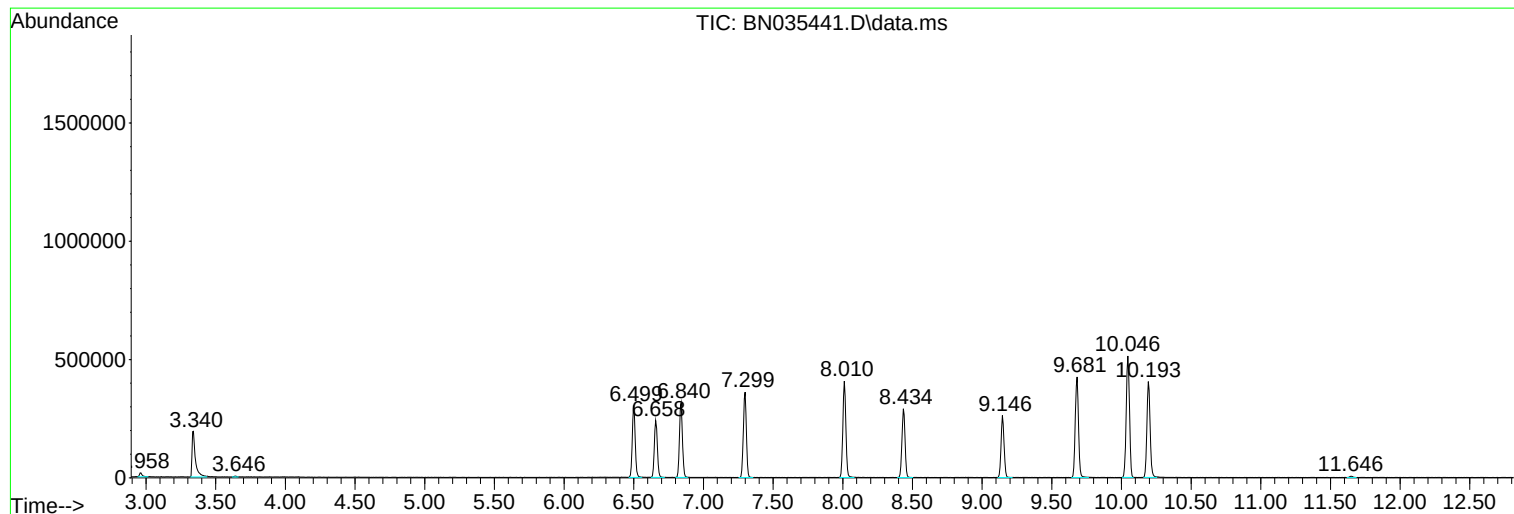

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035441.D
Acq On : 06 Dec 2024 00:54
Operator : RC/JU
Sample : PB165400BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK400

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035441.D
Acq On : 06 Dec 2024 00:54
Operator : RC/JU
Sample : PB165400BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK400

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------