

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035443.D
 Acq On : 06 Dec 2024 02:12
 Operator : RC/JU
 Sample : P5104-13
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHJ70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035443.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	9	12	17	rBV	12374	15556	0.52%	0.063%
2	3.340	74	77	91	rBV	58849	97943	3.29%	0.396%
3	3.640	125	128	134	rBV3	3875	5293	0.18%	0.021%
4	4.070	196	201	207	rVB2	7356	11834	0.40%	0.048%
5	6.499	608	614	622	rBV	79880	115814	3.89%	0.469%
6	6.658	635	641	649	rBV	221166	324849	10.91%	1.314%
7	6.840	666	672	683	rBV	260043	390706	13.13%	1.581%
8	7.299	743	750	758	rBV	329781	496771	16.69%	2.010%
9	8.011	864	871	880	rBV	244900	362415	12.18%	1.466%
10	8.434	936	943	953	rBV	268144	410773	13.80%	1.662%
11	8.581	965	968	972	rBV3	2815	3655	0.12%	0.015%
12	8.899	1018	1022	1028	rVB3	3529	5267	0.18%	0.021%
13	9.146	1058	1064	1073	rBV	241708	360566	12.11%	1.459%
14	9.681	1148	1155	1164	rBV	398682	637858	21.43%	2.581%
15	10.046	1210	1217	1228	rVB	478595	758248	25.48%	3.068%
16	10.193	1236	1242	1254	rBV	341786	565177	18.99%	2.287%
17	10.881	1354	1359	1364	rBV5	5492	8013	0.27%	0.032%
18	11.646	1484	1489	1496	rVB	4596	7856	0.26%	0.032%
19	13.387	1778	1785	1803	rBV	917784	1236178	41.53%	5.002%
20	13.646	1822	1829	1837	rBV	913094	1369370	46.01%	5.541%
21	13.957	1876	1882	1889	rBV	871862	1257429	42.25%	5.088%
22	14.193	1916	1922	1932	rBV	65636	116644	3.92%	0.472%
23	14.410	1954	1959	1966	rVB5	3314	6330	0.21%	0.026%
24	14.822	2021	2029	2036	rVB2	6882	14131	0.47%	0.057%
25	14.969	2047	2054	2061	rBV	1314895	1880339	63.18%	7.608%
26	15.098	2070	2076	2088	rBV	416000	518746	17.43%	2.099%
27	15.210	2092	2095	2098	rBV2	4868	5718	0.19%	0.023%
28	15.369	2117	2122	2129	rBV3	4467	6992	0.23%	0.028%
29	16.722	2346	2352	2360	rBV	1134889	1598073	53.69%	6.466%
30	16.822	2363	2369	2384	rVV	1573552	2178622	73.20%	8.815%
31	17.051	2405	2408	2412	rVB	2825	2992	0.10%	0.012%
32	17.116	2415	2419	2423	rBV4	1929	3524	0.12%	0.014%
33	17.669	2509	2513	2517	rBV4	12832	15070	0.51%	0.061%
34	17.734	2520	2524	2528	rBV	11008	12917	0.43%	0.052%
35	18.116	2584	2589	2593	rBV6	2378	3709	0.12%	0.015%
36	18.704	2684	2689	2693	rBV	19157	25382	0.85%	0.103%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035443.D
Acq On : 06 Dec 2024 02:12
Operator : RC/JU
Sample : P5104-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ70

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION

37	18.775	2696	2701	2706	rBV	16921	22296	0.75%	0.090%
38	18.851	2710	2714	2724	rBV2	53213	79244	2.66%	0.321%
39	18.981	2732	2736	2741	rBV4	7477	10177	0.34%	0.041%
40	19.145	2758	2764	2774	rBV	2007841	2696991	90.62%	10.913%
41	19.410	2804	2809	2810	rBV5	2731	3838	0.13%	0.016%
42	20.975	3070	3075	3086	rBV	1416530	1941842	65.24%	7.857%
43	23.469	3491	3499	3514	rVB	1386595	2976255	100.00%	12.043%
44	23.651	3521	3530	3539	rBV2	981926	2153127	72.34%	8.712%




Sum of corrected areas: 24714530

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035443.D
Acq On : 06 Dec 2024 02:12
Operator : RC/JU
Sample : P5104-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ70

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

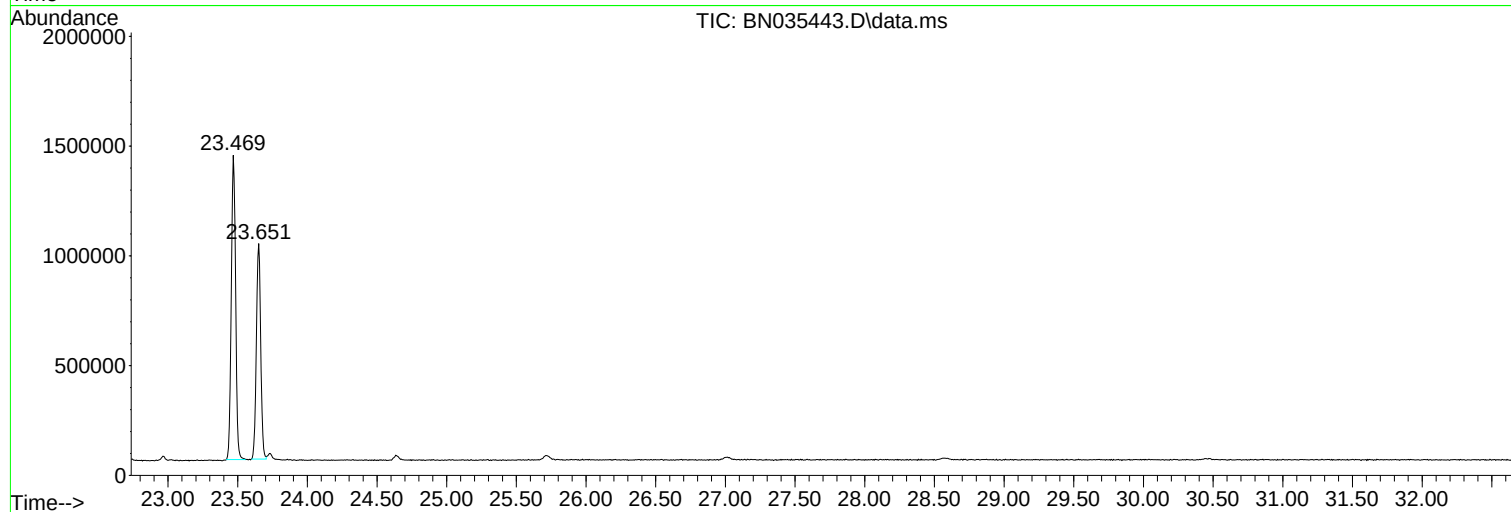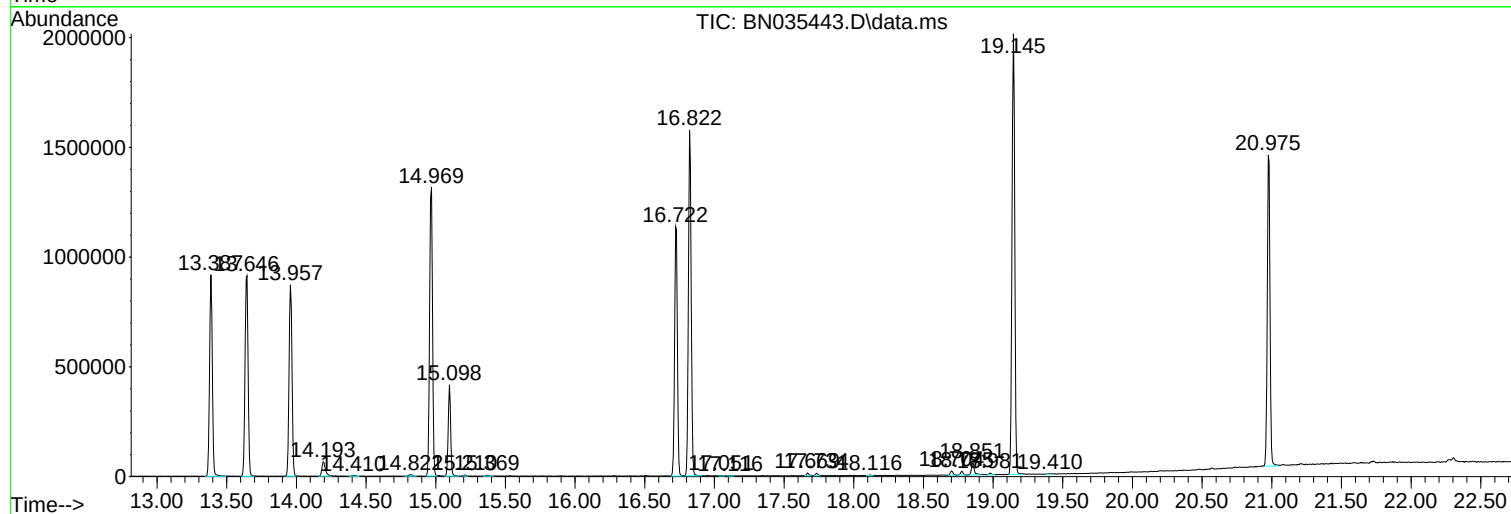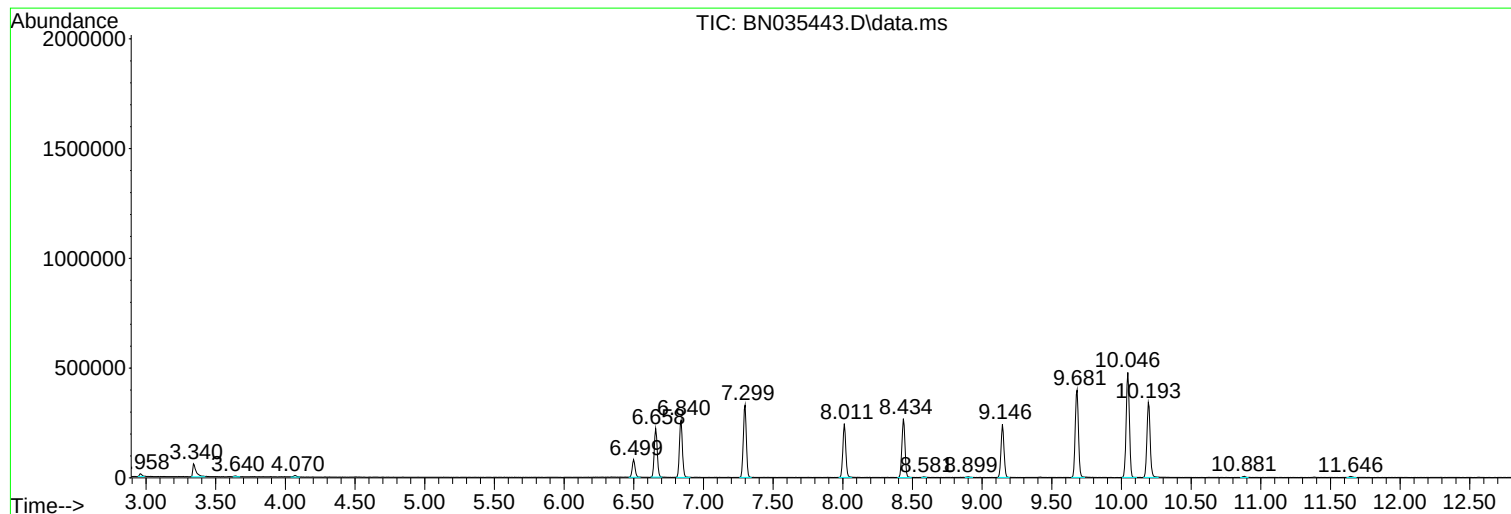

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035443.D
Acq On : 06 Dec 2024 02:12
Operator : RC/JU
Sample : P5104-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ70

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035443.D
Acq On : 06 Dec 2024 02:12
Operator : RC/JU
Sample : P5104-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ70

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc