

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035444.D
 Acq On : 06 Dec 2024 02:51
 Operator : RC/JU
 Sample : P5104-20
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHJ96

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035444.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	9	12	20	rVB	12955	16899	0.56%	0.068%
2	3.640	125	128	132	rVB	2897	3343	0.11%	0.014%
3	4.070	195	201	208	rVB2	7972	11867	0.39%	0.048%
4	6.499	608	614	624	rVB	126129	188246	6.19%	0.762%
5	6.658	634	641	651	rBV	236470	344312	11.32%	1.393%
6	6.840	665	672	681	rVB	298363	448614	14.75%	1.816%
7	7.299	742	750	757	rBV	325155	494248	16.25%	2.000%
8	8.011	865	871	882	rBV	329314	488510	16.06%	1.977%
9	8.434	937	943	953	rVB	282242	427689	14.06%	1.731%
10	8.899	1017	1022	1028	rVB3	4430	5636	0.19%	0.023%
11	9.146	1058	1064	1073	rBV	250744	386906	12.72%	1.566%
12	9.681	1148	1155	1166	rBV	423014	669641	22.01%	2.710%
13	10.046	1210	1217	1224	rVB	465371	739022	24.30%	2.991%
14	10.193	1236	1242	1252	rBV	83147	145749	4.79%	0.590%
15	11.387	1440	1445	1451	rVB3	1959	3604	0.12%	0.015%
16	11.646	1483	1489	1497	rBV	4677	8465	0.28%	0.034%
17	13.387	1779	1785	1801	rBV	919270	1281050	42.12%	5.185%
18	13.646	1822	1829	1840	rBV	868641	1313159	43.17%	5.315%
19	13.957	1876	1882	1893	rBV	872094	1228798	40.40%	4.973%
20	14.193	1915	1922	1932	rBV	129432	216629	7.12%	0.877%
21	14.416	1957	1960	1965	rVB6	2757	3498	0.11%	0.014%
22	14.969	2047	2054	2061	rBV	1324235	1883782	61.93%	7.624%
23	15.016	2061	2062	2068	rVV5	2972	3797	0.12%	0.015%
24	15.098	2071	2076	2085	rVB	446728	566255	18.62%	2.292%
25	15.210	2091	2095	2098	rBV	5750	6340	0.21%	0.026%
26	16.510	2312	2316	2323	rBV2	2434	4454	0.15%	0.018%
27	16.722	2346	2352	2362	rVB	1095649	1530955	50.33%	6.196%
28	16.822	2363	2369	2381	rBV2	1638989	2324799	76.43%	9.409%
29	17.669	2510	2513	2519	rBV4	9028	11709	0.38%	0.047%
30	18.704	2683	2689	2694	rBV2	20383	26847	0.88%	0.109%
31	18.775	2697	2701	2706	rVV	17843	22163	0.73%	0.090%
32	18.857	2710	2715	2728	rVV	86184	114229	3.76%	0.462%
33	18.981	2732	2736	2741	rVV3	11418	13409	0.44%	0.054%
34	19.145	2758	2764	2776	rBV	2112971	2901120	95.38%	11.741%
35	20.975	3070	3075	3085	rBV	1434987	1881620	61.86%	7.615%
36	23.469	3490	3499	3515	rBV	1385451	3041752	100.00%	12.311%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035444.D
Acq On : 06 Dec 2024 02:51
Operator : RC/JU
Sample : P5104-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ96

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION

37	23.651	3521	3530	3538	rBV2	857669	1949368	64.09%	7.889%
----	--------	------	------	------	------	--------	---------	--------	--------


Sum of corrected areas: 24708484

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035444.D
Acq On : 06 Dec 2024 02:51
Operator : RC/JU
Sample : P5104-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ96

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

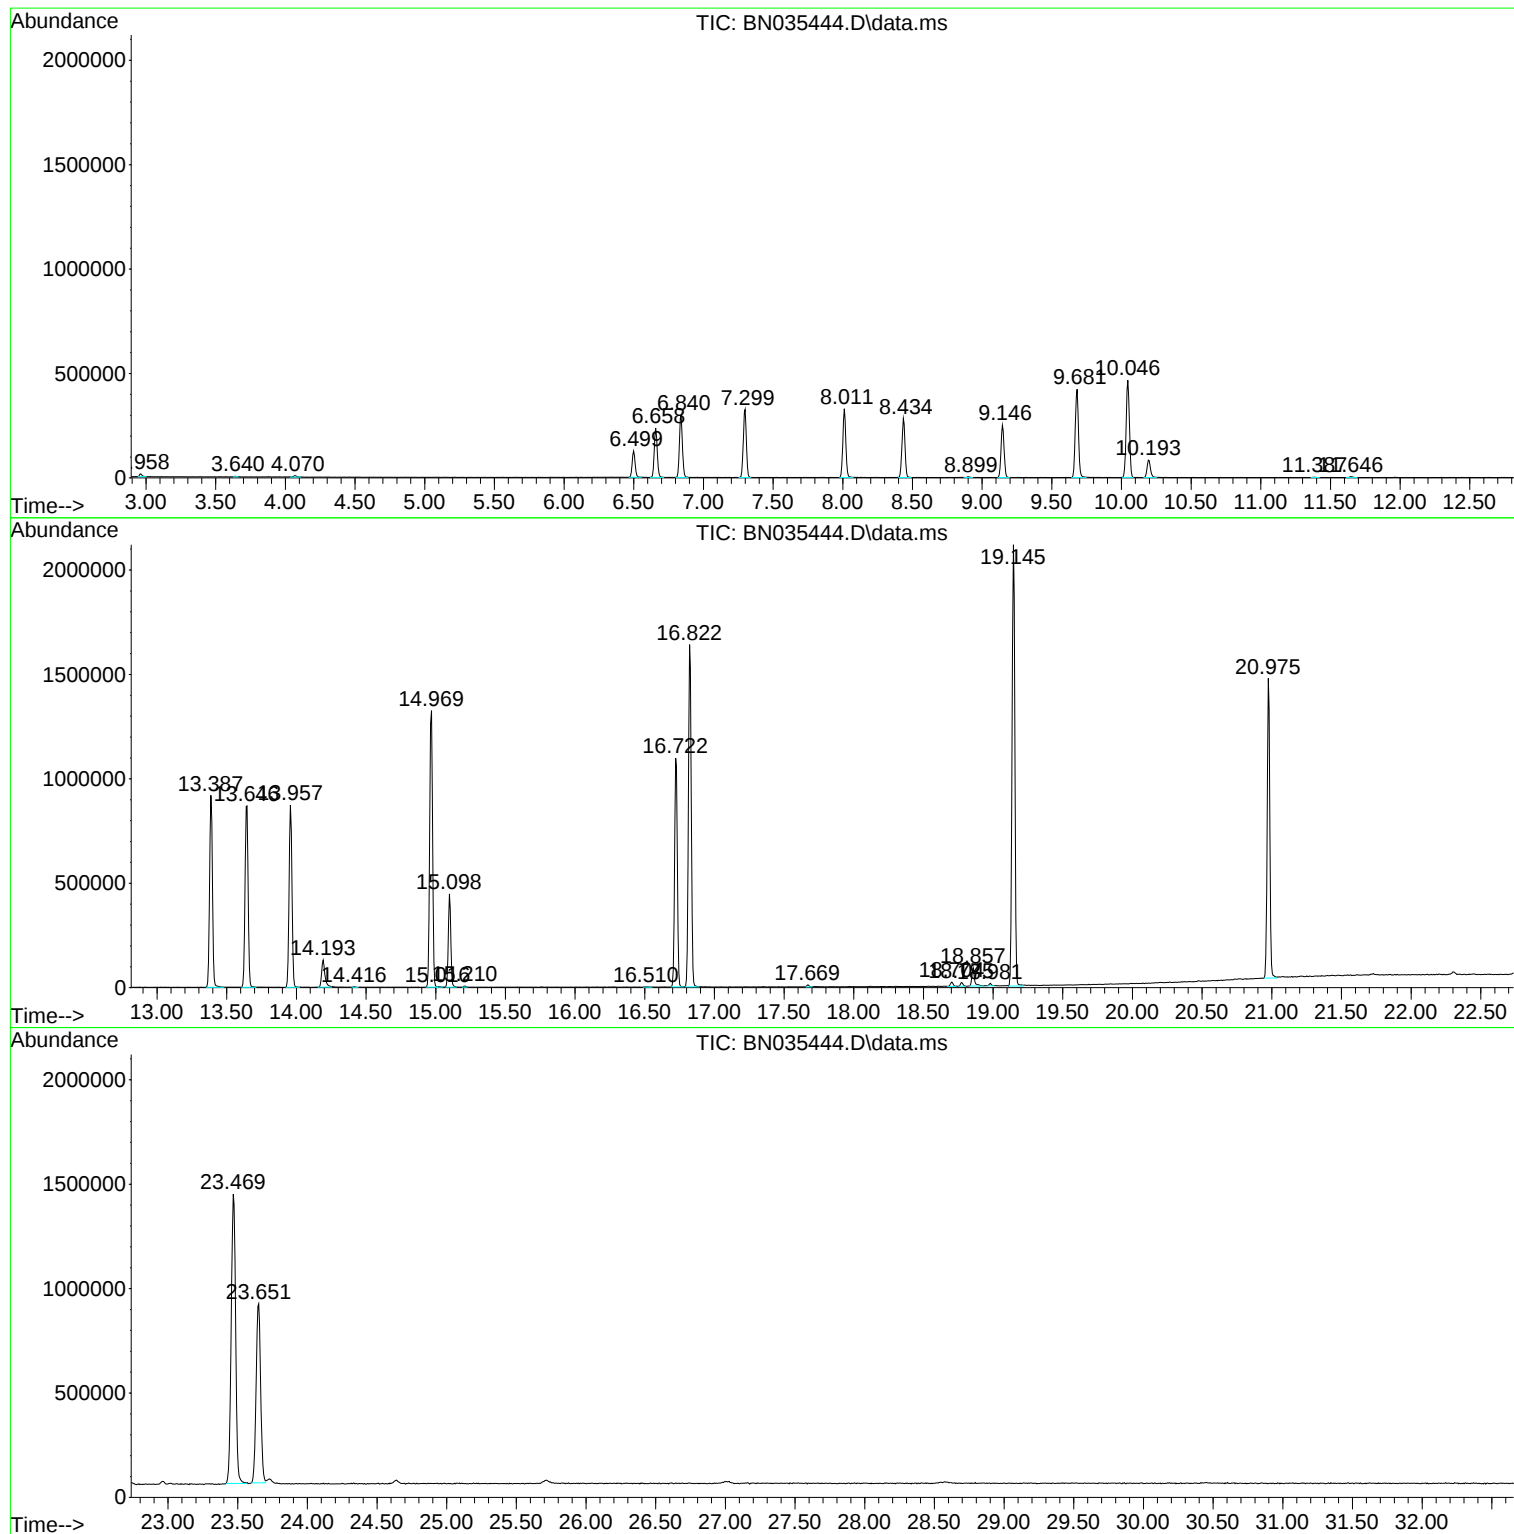

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035444.D
Acq On : 06 Dec 2024 02:51
Operator : RC/JU
Sample : P5104-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ96

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035444.D
Acq On : 06 Dec 2024 02:51
Operator : RC/JU
Sample : P5104-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ96

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------