

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035448.D
 Acq On : 06 Dec 2024 05:26
 Operator : RC/JU
 Sample : P5104-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHJ72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035448.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	9	12	23	rVB	14637	21679	0.65%	0.078%
2	3.346	75	78	94	rVB	30418	51913	1.56%	0.187%
3	3.640	125	128	135	rVB2	4633	6739	0.20%	0.024%
4	4.070	195	201	206	rVB	7194	9893	0.30%	0.036%
5	6.499	608	614	624	rVB	86846	128999	3.89%	0.464%
6	6.658	635	641	652	rBV	271654	396961	11.96%	1.426%
7	6.840	666	672	684	rVB	305926	461598	13.91%	1.659%
8	7.299	743	750	759	rVB	344041	531609	16.02%	1.910%
9	8.011	862	871	880	rBV	277892	413612	12.46%	1.486%
10	8.434	936	943	955	rVB	330300	503059	15.16%	1.808%
11	8.587	965	969	974	rVB2	2324	3369	0.10%	0.012%
12	8.905	1017	1023	1031	rBV3	3413	6280	0.19%	0.023%
13	9.146	1057	1064	1073	rBV	297078	450572	13.58%	1.619%
14	9.681	1148	1155	1165	rBV	475177	769272	23.18%	2.764%
15	10.046	1209	1217	1224	rBV	514261	811641	24.46%	2.916%
16	10.193	1236	1242	1255	rBV	364281	596867	17.99%	2.145%
17	10.881	1354	1359	1366	rBV4	3398	6265	0.19%	0.023%
18	11.381	1441	1444	1450	rVB4	2605	3862	0.12%	0.014%
19	11.646	1483	1489	1495	rBV2	6945	11126	0.34%	0.040%
20	13.387	1778	1785	1800	rBV	1103957	1461953	44.05%	5.253%
21	13.646	1821	1829	1838	rBV	1089998	1621687	48.87%	5.827%
22	13.957	1876	1882	1890	rBV	949348	1325994	39.96%	4.765%
23	14.193	1916	1922	1938	rBV	77241	135405	4.08%	0.487%
24	14.810	2023	2027	2034	rVB5	1998	3886	0.12%	0.014%
25	14.969	2047	2054	2060	rVV	1537438	2175852	65.56%	7.818%
26	15.016	2060	2062	2067	rVV4	4085	5644	0.17%	0.020%
27	15.098	2070	2076	2088	rVV	511646	640241	19.29%	2.300%
28	15.210	2090	2095	2098	rVB3	6061	7973	0.24%	0.029%
29	15.534	2145	2150	2154	rVB4	2141	3345	0.10%	0.012%
30	15.693	2170	2177	2181	rBV3	2985	4295	0.13%	0.015%
31	15.740	2181	2185	2193	rVV4	9764	13974	0.42%	0.050%
32	16.540	2317	2321	2325	rVV	22149	25599	0.77%	0.092%
33	16.592	2325	2330	2332	rVV3	4081	4291	0.13%	0.015%
34	16.722	2346	2352	2362	rBV	1163936	1674886	50.47%	6.018%
35	16.822	2363	2369	2378	rBV	1818430	2548900	76.81%	9.159%
36	16.963	2390	2393	2397	rVB5	2334	3805	0.11%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035448.D
Acq On : 06 Dec 2024 05:26
Operator : RC/JU
Sample : P5104-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION

37	17.016	2397	2402	2405	rBV6	3233	5834	0.18%	0.021%
38	17.281	2442	2447	2451	rBV	32748	39617	1.19%	0.142%
39	17.451	2472	2476	2480	rVB	43019	49002	1.48%	0.176%
40	17.557	2491	2494	2496	rBV3	2934	3833	0.12%	0.014%
41	17.669	2509	2513	2519	rBV2	22900	28941	0.87%	0.104%
42	17.734	2519	2524	2529	rVB	9101	15182	0.46%	0.055%
43	17.787	2529	2533	2535	rBV3	3495	5396	0.16%	0.019%
44	17.975	2560	2565	2569	rBV	36294	42849	1.29%	0.154%
45	18.110	2586	2588	2594	rVB6	4264	6604	0.20%	0.024%
46	18.445	2643	2645	2649	rVB5	3350	3955	0.12%	0.014%
47	18.557	2660	2664	2668	rVB6	2872	3804	0.11%	0.014%
48	18.622	2669	2675	2677	rBV4	32991	67748	2.04%	0.243%
49	18.698	2684	2688	2693	rVB2	24560	34921	1.05%	0.125%
50	18.775	2697	2701	2706	rBV2	31383	45992	1.39%	0.165%
51	18.822	2706	2709	2711	rBV3	12421	15063	0.45%	0.054%
52	18.851	2711	2714	2718	rVB3	26163	29985	0.90%	0.108%
53	18.975	2732	2735	2744	rBV4	14469	21704	0.65%	0.078%
54	19.145	2758	2764	2772	rBV	2282775	3133147	94.41%	11.258%
55	19.216	2773	2776	2780	rVB2	20837	24744	0.75%	0.089%
56	19.404	2802	2808	2814	rBV2	7461	14302	0.43%	0.051%
57	19.763	2866	2869	2873	rBV3	10707	11105	0.33%	0.040%
58	20.975	3070	3075	3086	rBV	1483607	1972203	59.43%	7.086%
59	23.469	3490	3499	3512	rBV	1515587	3318628	100.00%	11.924%
60	23.645	3521	3529	3539	rBV	935529	2092934	63.07%	7.520%




Sum of corrected areas: 27830539

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035448.D
Acq On : 06 Dec 2024 05:26
Operator : RC/JU
Sample : P5104-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

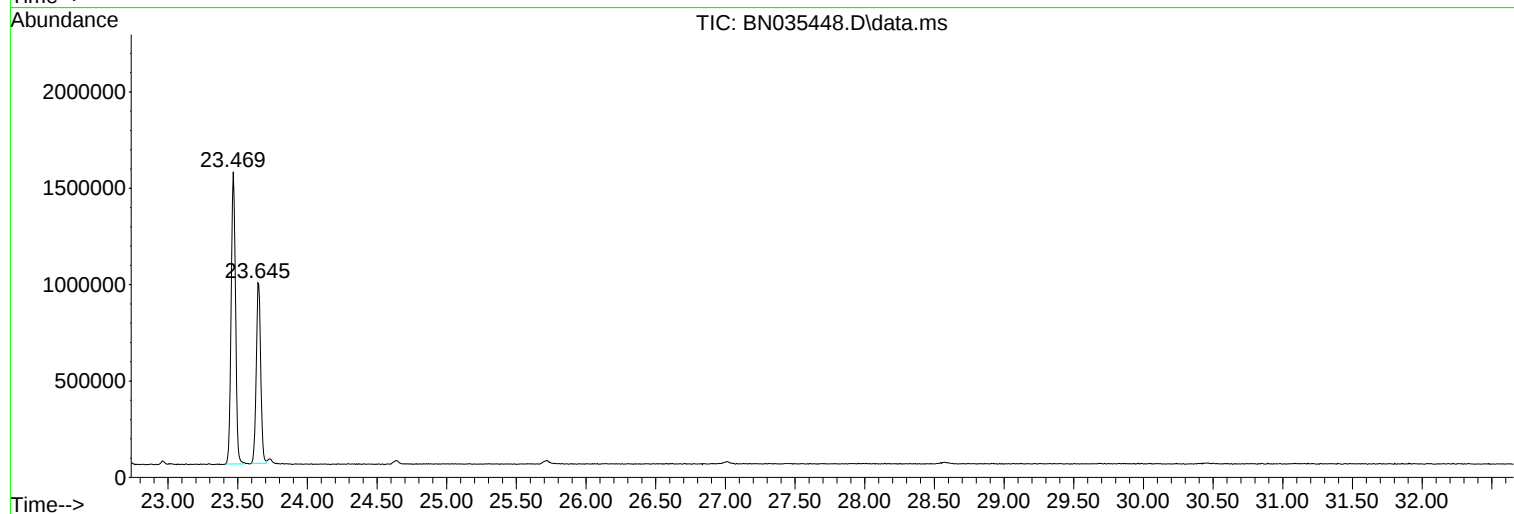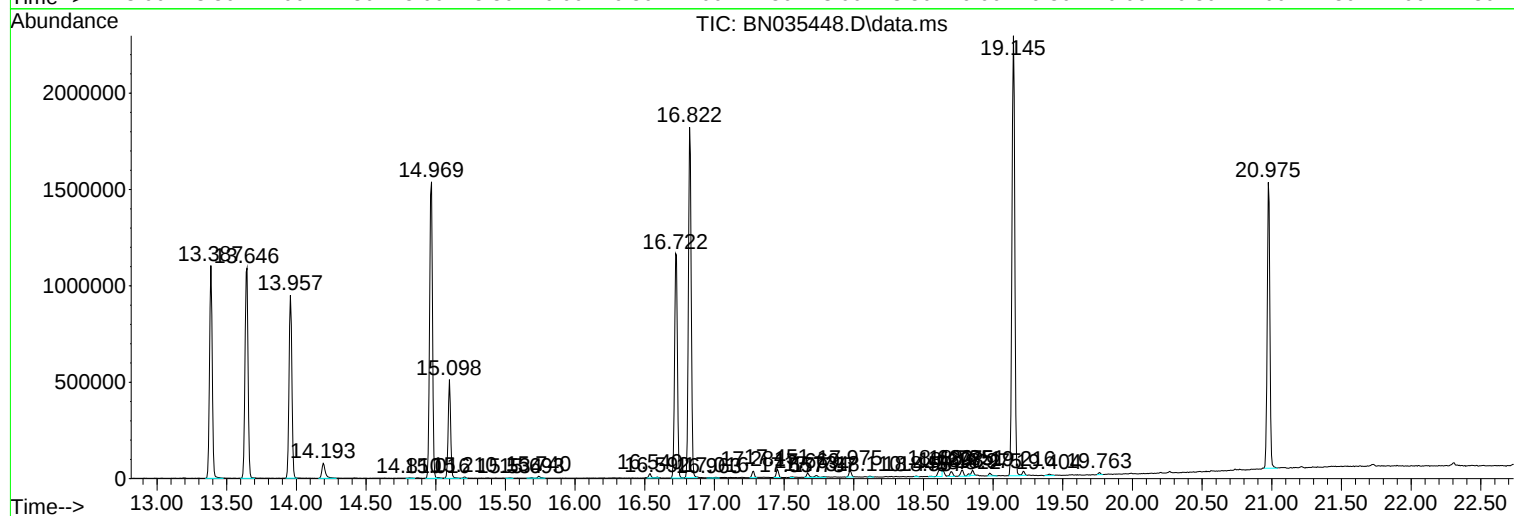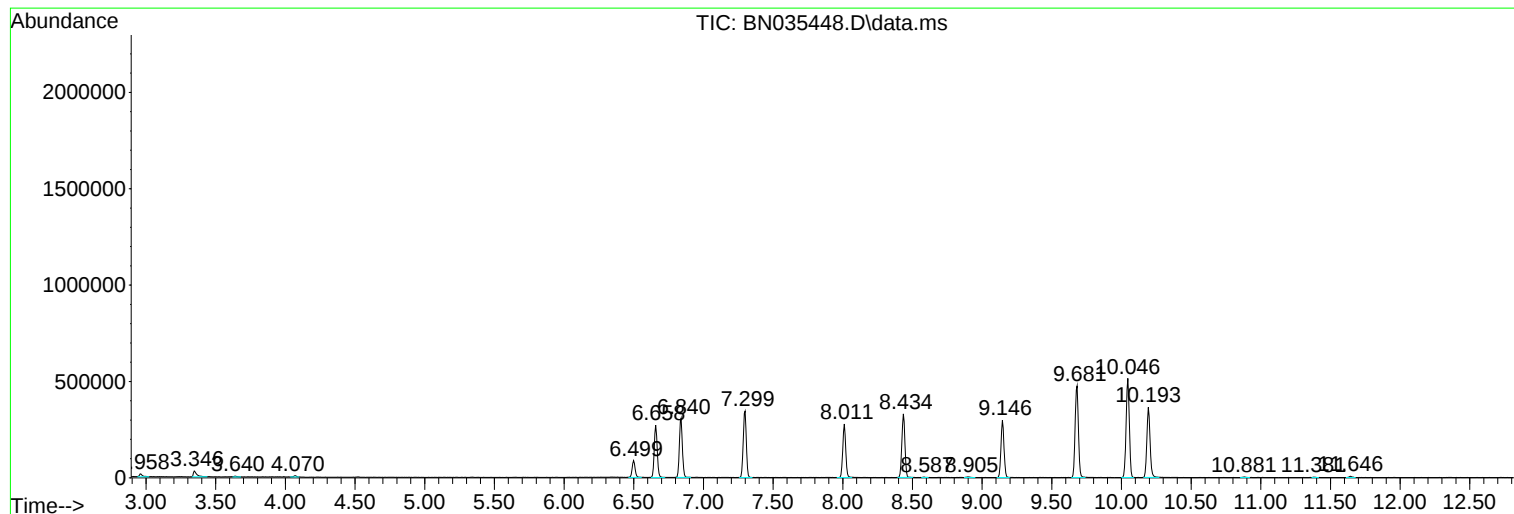

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035448.D
Acq On : 06 Dec 2024 05:26
Operator : RC/JU
Sample : P5104-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035448.D
Acq On : 06 Dec 2024 05:26
Operator : RC/JU
Sample : P5104-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------