

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035449.D
 Acq On : 06 Dec 2024 06:05
 Operator : RC/JU
 Sample : P5104-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHJ73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035449.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	9	12	19	rBV	12803	15885	0.48%	0.058%
2	3.346	74	78	90	rBV	39046	65993	1.98%	0.239%
3	3.640	125	128	133	rVB	4917	5289	0.16%	0.019%
4	4.069	196	201	206	rVB	8365	12226	0.37%	0.044%
5	6.499	609	614	623	rVB	87231	126538	3.79%	0.459%
6	6.658	635	641	652	rBV	259650	388559	11.65%	1.410%
7	6.840	665	672	682	rBV	306320	455149	13.64%	1.652%
8	7.299	743	750	758	rBV	344952	518007	15.53%	1.880%
9	8.010	865	871	882	rBV	280484	408457	12.24%	1.482%
10	8.434	935	943	956	rBV	321994	489618	14.67%	1.777%
11	8.593	965	970	974	rBV2	14691	21337	0.64%	0.077%
12	8.904	1017	1023	1027	rBV4	3873	5837	0.17%	0.021%
13	9.146	1057	1064	1072	rBV	288639	436397	13.08%	1.584%
14	9.681	1148	1155	1167	rBV	477189	773676	23.19%	2.808%
15	10.046	1210	1217	1225	rBV	481926	793033	23.77%	2.878%
16	10.193	1235	1242	1256	rBV	252301	418904	12.56%	1.520%
17	10.881	1354	1359	1363	rBV3	4466	8416	0.25%	0.031%
18	11.387	1440	1445	1449	rBV5	1998	3852	0.12%	0.014%
19	11.646	1480	1489	1496	rBV2	6557	12927	0.39%	0.047%
20	13.387	1778	1785	1799	rBV	1009721	1377839	41.30%	5.000%
21	13.640	1822	1828	1841	rBV	1059309	1582063	47.42%	5.741%
22	13.904	1869	1873	1876	rBV3	3188	4153	0.12%	0.015%
23	13.957	1876	1882	1889	rBV	914915	1301529	39.01%	4.723%
24	14.192	1917	1922	1933	rBV	72998	129386	3.88%	0.470%
25	14.275	1933	1936	1939	rVB3	2732	3688	0.11%	0.013%
26	14.698	2002	2008	2013	rBV3	5647	10383	0.31%	0.038%
27	14.822	2023	2029	2032	rBV3	1834	3482	0.10%	0.013%
28	14.869	2034	2037	2041	rVB3	6413	7253	0.22%	0.026%
29	14.963	2047	2053	2061	rBV	1449926	2098035	62.88%	7.614%
30	15.016	2061	2062	2067	rVV4	3926	3667	0.11%	0.013%
31	15.098	2070	2076	2087	rVB	495477	627971	18.82%	2.279%
32	15.210	2090	2095	2101	rVB3	6599	8279	0.25%	0.030%
33	15.369	2117	2122	2127	rBV5	5722	7360	0.22%	0.027%
34	15.739	2180	2185	2187	rBV2	7125	10155	0.30%	0.037%
35	15.763	2187	2189	2198	rVB3	4643	6891	0.21%	0.025%
36	16.533	2317	2320	2324	rVV3	5724	6770	0.20%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035449.D
 Acq On : 06 Dec 2024 06:05
 Operator : RC/JU
 Sample : P5104-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHJ73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

37	16.586	2326	2329	2335	rVB6	4737	6005	0.18%	0.022%
38	16.722	2346	2352	2361	rVB	1182107	1632665	48.93%	5.925%
39	16.822	2363	2369	2381	rVB2	1796904	2473142	74.12%	8.975%
40	17.063	2406	2410	2415	rBV6	3403	6666	0.20%	0.024%
41	17.281	2442	2447	2450	rBV2	7014	9653	0.29%	0.035%
42	17.451	2473	2476	2479	rVB4	4287	5448	0.16%	0.020%
43	17.669	2509	2513	2520	rBV2	48109	66046	1.98%	0.240%
44	17.975	2561	2565	2570	rVB4	7682	10131	0.30%	0.037%
45	18.122	2586	2590	2593	rVB6	2727	3763	0.11%	0.014%
46	18.310	2618	2622	2626	rBB5	2588	3978	0.12%	0.014%
47	18.627	2670	2676	2682	rBV8	6581	14581	0.44%	0.053%
48	18.704	2684	2689	2694	rVB	24358	33253	1.00%	0.121%
49	18.775	2697	2701	2706	rVB	23148	30061	0.90%	0.109%
50	18.857	2710	2715	2725	rBV	110724	166351	4.99%	0.604%
51	18.980	2731	2736	2747	rBV	35441	54303	1.63%	0.197%
52	19.145	2758	2764	2773	rBV	2307499	3028850	90.78%	10.992%
53	19.216	2773	2776	2780	rVB4	5576	7549	0.23%	0.027%
54	19.763	2866	2869	2873	rBV5	6770	8373	0.25%	0.030%
55	20.974	3069	3075	3087	rBV	1481414	2002898	60.03%	7.268%
56	22.463	3323	3328	3338	rVB	173294	282341	8.46%	1.025%
57	22.963	3408	3413	3418	rBV4	35650	65066	1.95%	0.236%
58	23.468	3490	3499	3514	rVB	1470900	3336547	100.00%	12.108%
59	23.645	3521	3529	3538	rBV	977314	2159195	64.71%	7.836%




Sum of corrected areas: 27555869

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035449.D
Acq On : 06 Dec 2024 06:05
Operator : RC/JU
Sample : P5104-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ73

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

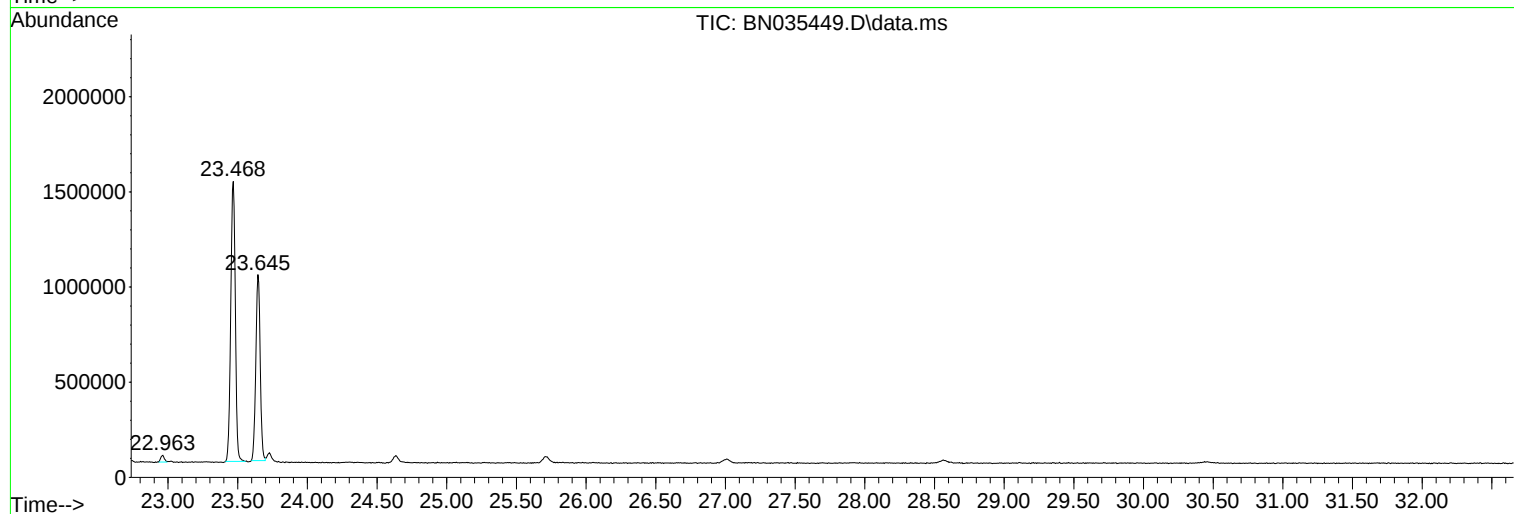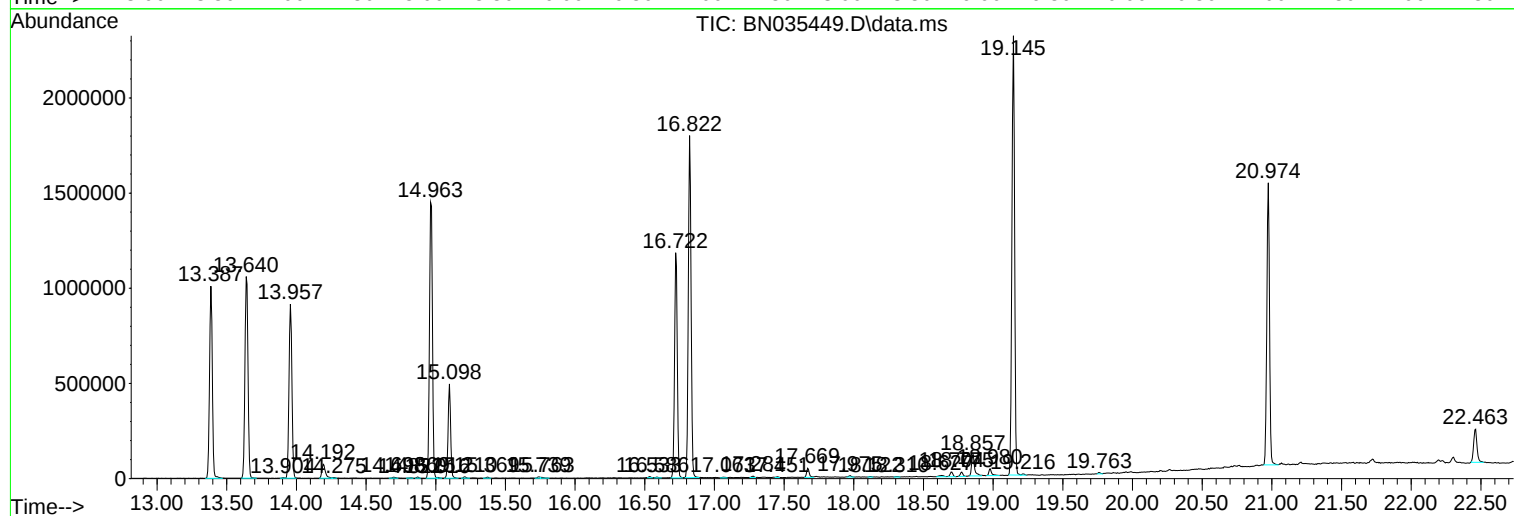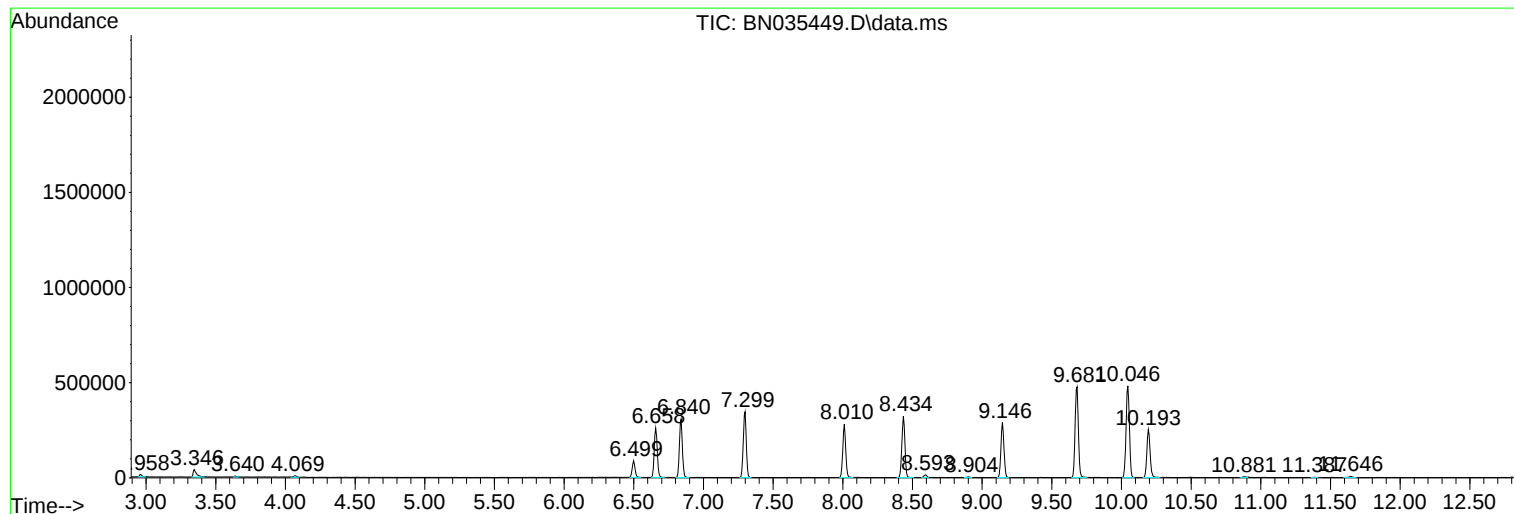

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035449.D
Acq On : 06 Dec 2024 06:05
Operator : RC/JU
Sample : P5104-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ73

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035449.D
Acq On : 06 Dec 2024 06:05
Operator : RC/JU
Sample : P5104-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ73

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------