

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035453.D
 Acq On : 06 Dec 2024 09:19
 Operator : RC/JU
 Sample : PB165400BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK400

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035453.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.963	9	13	19	rVB	22370	29240	0.87%	0.082%
2	3.340	73	77	95	rBV	280053	449656	13.39%	1.255%
3	3.640	125	128	134	rVB	5738	8360	0.25%	0.023%
4	6.498	608	614	625	rVB	427854	637876	19.00%	1.780%
5	6.657	634	641	649	rBV	335045	499042	14.86%	1.393%
6	6.840	664	672	681	rBV	452993	677602	20.18%	1.891%
7	7.298	743	750	760	rVB	505201	771264	22.97%	2.153%
8	8.010	864	871	886	rBV	573493	873340	26.01%	2.437%
9	8.434	936	943	954	rBV	422426	647365	19.28%	1.807%
10	9.145	1057	1064	1073	rBV	384104	580595	17.29%	1.620%
11	9.681	1148	1155	1166	rBV	601847	973317	28.99%	2.716%
12	10.045	1209	1217	1225	rBV	724914	1150586	34.27%	3.211%
13	10.192	1235	1242	1253	rBV	572385	951443	28.34%	2.655%
14	11.645	1483	1489	1495	rVB	8062	13493	0.40%	0.038%
15	13.386	1777	1785	1800	rBV	1199935	1641504	48.89%	4.581%
16	13.645	1819	1829	1837	rBV	1282218	1930300	57.49%	5.387%
17	13.957	1876	1882	1896	rVB	1312877	1868997	55.66%	5.216%
18	14.192	1915	1922	1937	rBV	517043	770946	22.96%	2.152%
19	14.969	2047	2054	2067	rBV	1696254	2435888	72.54%	6.798%
20	15.098	2070	2076	2086	rVV	572256	706609	21.04%	1.972%
21	15.210	2089	2095	2098	rBV	6013	8021	0.24%	0.022%
22	16.510	2311	2316	2320	rBV2	3321	4733	0.14%	0.013%
23	16.721	2346	2352	2363	rBV	1604469	2293531	68.30%	6.401%
24	16.821	2363	2369	2383	rVB	1924721	2727562	81.23%	7.612%
25	17.110	2415	2418	2425	rBV4	2046	3653	0.11%	0.010%
26	18.704	2684	2689	2694	rVB	22696	31264	0.93%	0.087%
27	18.774	2696	2701	2707	rVV	20579	27372	0.82%	0.076%
28	18.892	2717	2721	2725	rVB4	8340	9943	0.30%	0.028%
29	19.145	2758	2764	2774	rBV	2480300	3302277	98.35%	9.216%
30	20.198	2940	2943	2947	rBV4	18499	19429	0.58%	0.054%
31	20.974	3069	3075	3088	rBV	2018873	2747669	81.83%	7.669%
32	21.727	3200	3203	3208	rVB2	24704	30830	0.92%	0.086%
33	22.298	3296	3300	3314	rVB2	60071	107088	3.19%	0.299%
34	22.962	3408	3413	3419	rVB2	72273	123966	3.69%	0.346%
35	23.468	3490	3499	3514	rVB	1519277	3357795	100.00%	9.371%
36	23.651	3521	3530	3538	rBV	1238585	2808952	83.65%	7.840%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035453.D
Acq On : 06 Dec 2024 09:19
Operator : RC/JU
Sample : PB165400BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK400

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION

37	23.727	3539	3543	3553	rVB	100160	211442	6.30%	0.590%
38	24.639	3691	3698	3707	rVB3	78673	202325	6.03%	0.565%
39	25.709	3874	3880	3891	rVB3	68379	195124	5.81%	0.545%




Sum of corrected areas: 35830399

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035453.D
Acq On : 06 Dec 2024 09:19
Operator : RC/JU
Sample : PB165400BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK400

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

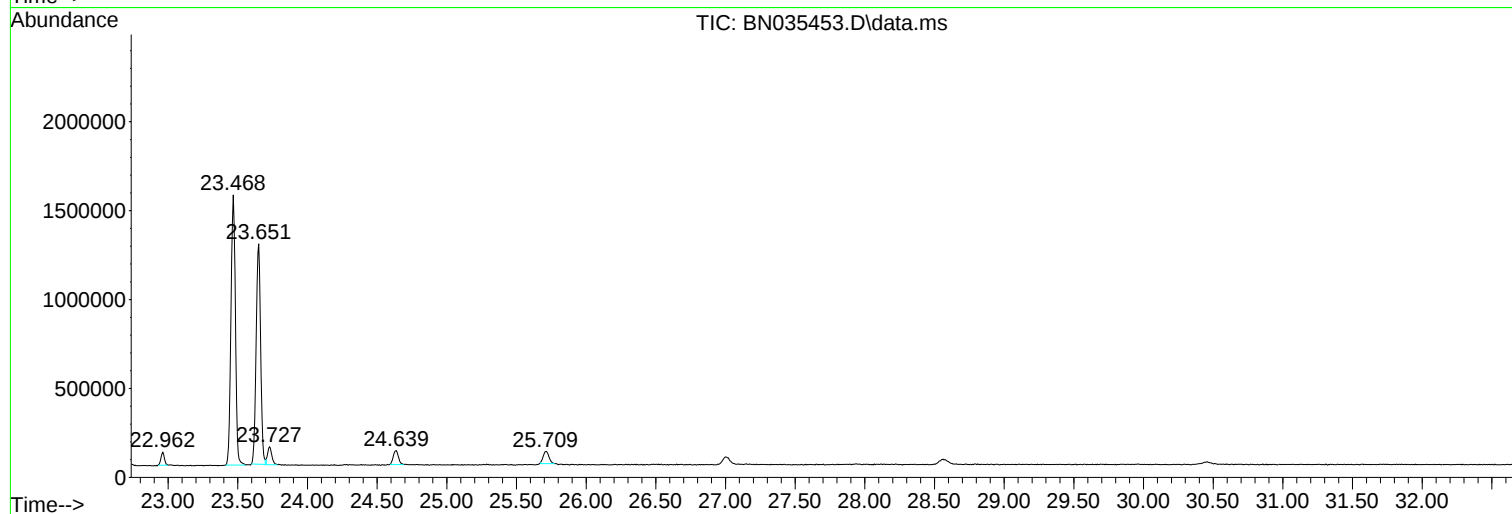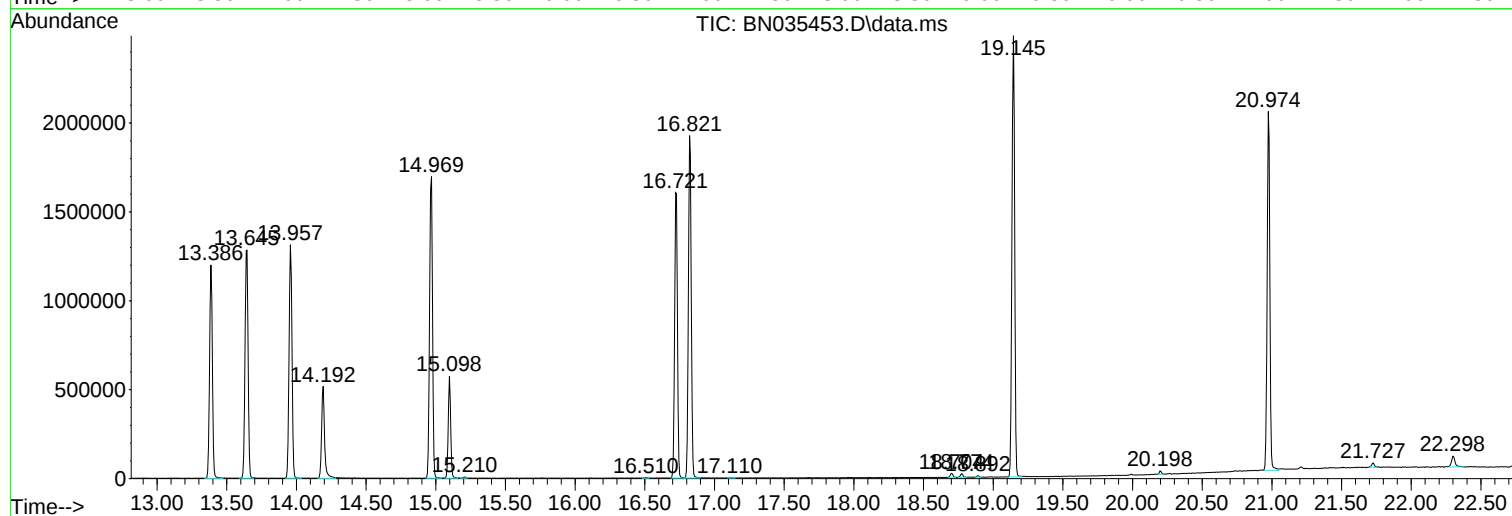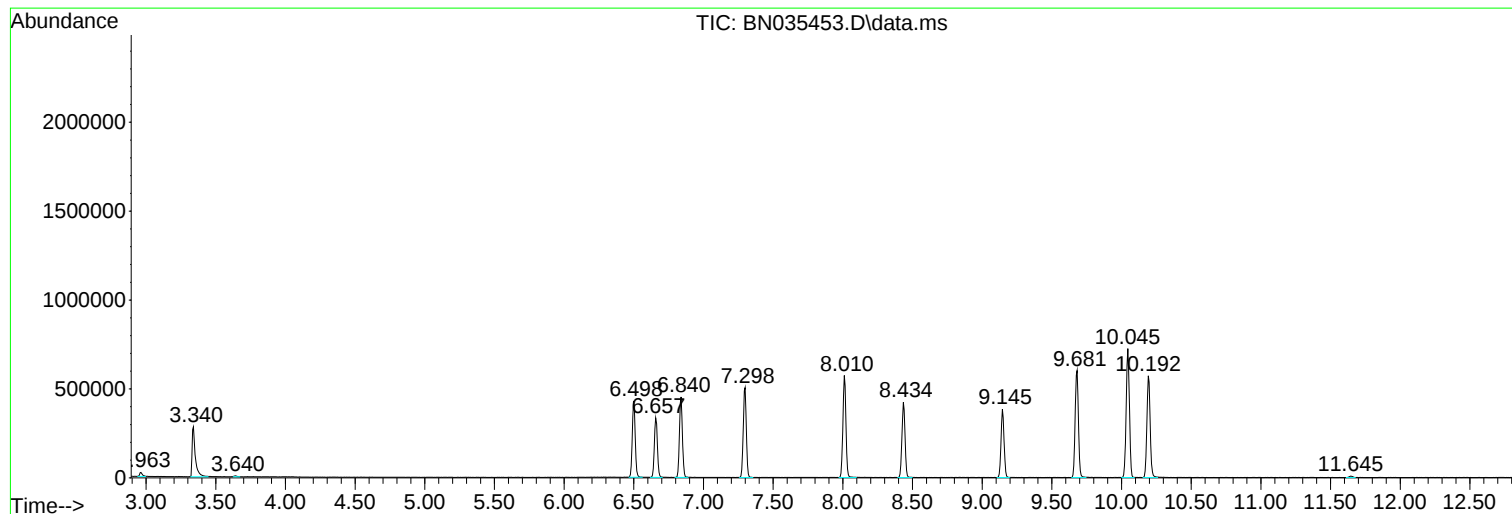

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035453.D
Acq On : 06 Dec 2024 09:19
Operator : RC/JU
Sample : PB165400BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK400

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035453.D
Acq On : 06 Dec 2024 09:19
Operator : RC/JU
Sample : PB165400BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK400

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------