

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035454.D
 Acq On : 06 Dec 2024 10:02
 Operator : RC/JU
 Sample : PB165409BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK409

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035454.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	9	12	20	rBV	19528	27561	0.96%	0.096%
2	3.334	73	76	94	rBV	265317	408340	14.17%	1.427%
3	3.640	124	128	131	rBV2	4066	4688	0.16%	0.016%
4	6.499	605	614	624	rBV	367856	556855	19.33%	1.945%
5	6.658	635	641	650	rVB	293816	432432	15.01%	1.511%
6	6.834	664	671	684	rBV	387084	588234	20.42%	2.055%
7	7.293	743	749	758	rVB	375298	569054	19.75%	1.988%
8	8.010	864	871	883	rBV	495340	752243	26.11%	2.628%
9	8.434	936	943	955	rVB	368646	556574	19.32%	1.944%
10	9.146	1058	1064	1075	rBV	323145	492938	17.11%	1.722%
11	9.675	1148	1154	1163	rBV	508856	828520	28.76%	2.894%
12	10.046	1209	1217	1226	rVB	528568	849061	29.47%	2.966%
13	10.193	1230	1242	1254	rBV	496383	819606	28.45%	2.863%
14	11.651	1484	1490	1495	rVB	6867	11061	0.38%	0.039%
15	13.387	1777	1785	1796	rBV	1040138	1397562	48.51%	4.882%
16	13.640	1822	1828	1839	rBV	1118120	1652364	57.36%	5.773%
17	13.957	1875	1882	1896	rBV	990171	1388001	48.18%	4.849%
18	14.192	1915	1922	1939	rBV	395643	636318	22.09%	2.223%
19	14.969	2047	2054	2067	rBV	1429374	2085884	72.41%	7.287%
20	15.098	2070	2076	2088	rVV	433445	565125	19.62%	1.974%
21	15.210	2091	2095	2100	rVB	5597	7103	0.25%	0.025%
22	16.504	2310	2315	2321	rBV6	2346	4062	0.14%	0.014%
23	16.722	2346	2352	2359	rBV	1207008	1718997	59.67%	6.005%
24	16.822	2363	2369	2382	rVB2	1661647	2339892	81.22%	8.174%
25	18.704	2684	2689	2694	rBV2	18306	25148	0.87%	0.088%
26	18.775	2697	2701	2706	rVB	16820	21319	0.74%	0.074%
27	19.145	2758	2764	2776	rBV	2167535	2818769	97.85%	9.847%
28	20.974	3070	3075	3086	rBV	1530435	2061400	71.56%	7.201%
29	23.468	3490	3499	3512	rBV	1338341	2880780	100.00%	10.064%
30	23.651	3521	3530	3540	rBV	964168	2124806	73.76%	7.423%




Sum of corrected areas: 28624697

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035454.D
Acq On : 06 Dec 2024 10:02
Operator : RC/JU
Sample : PB165409BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK409

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

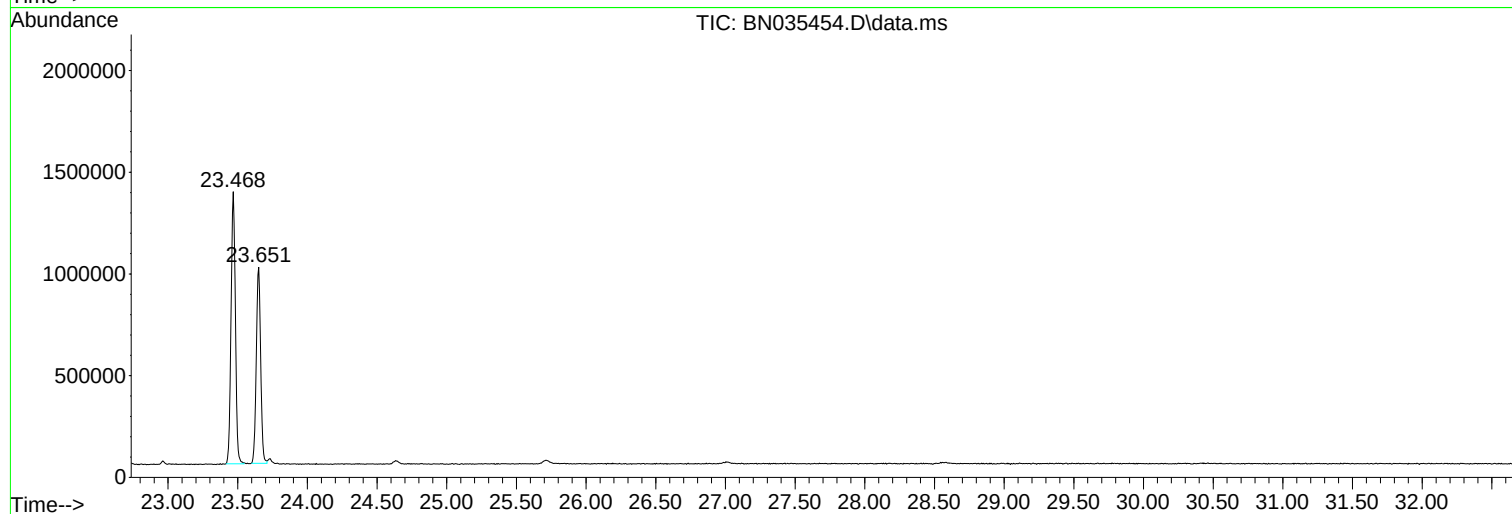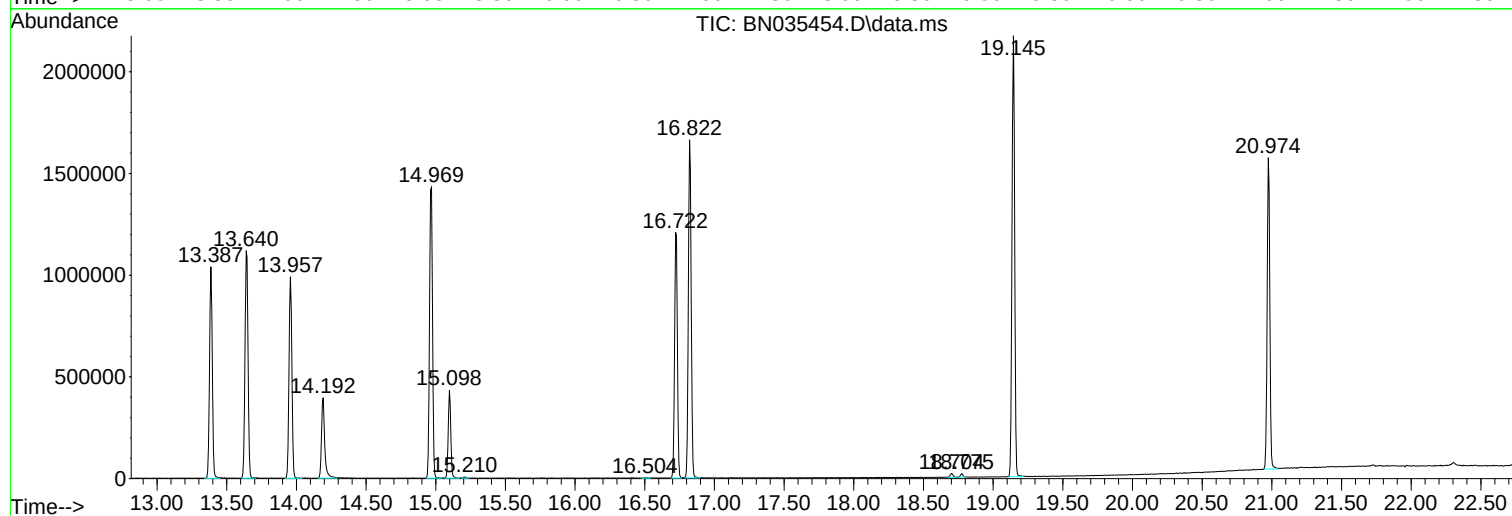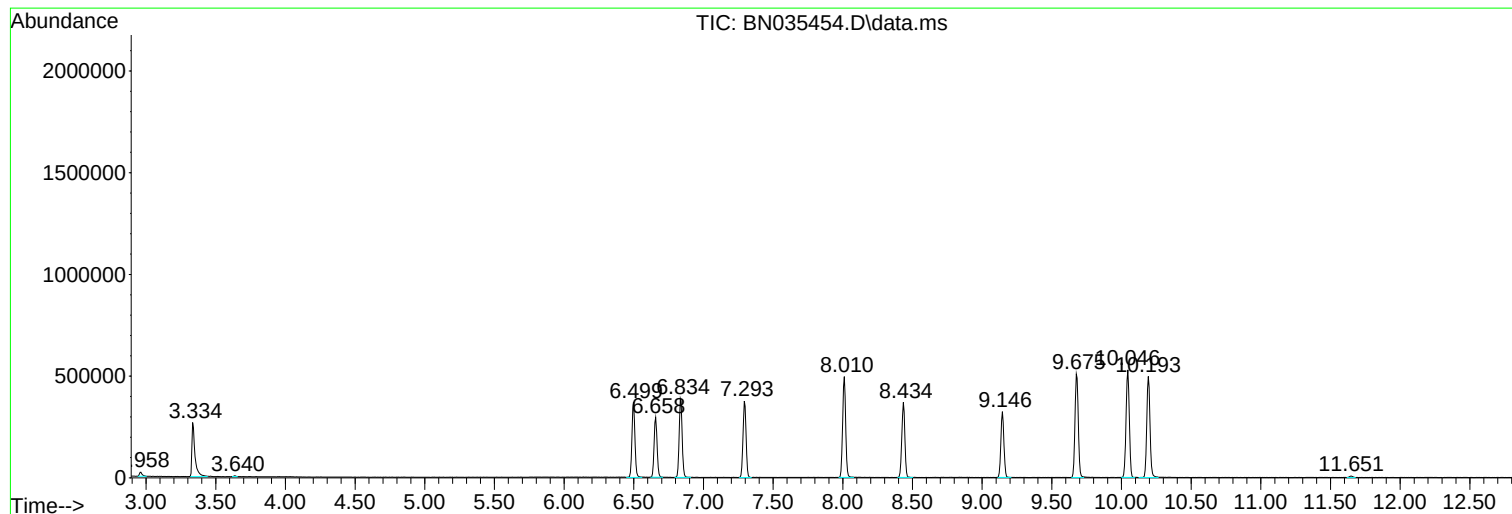

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035454.D
Acq On : 06 Dec 2024 10:02
Operator : RC/JU
Sample : PB165409BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK409

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035454.D
Acq On : 06 Dec 2024 10:02
Operator : RC/JU
Sample : PB165409BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK409

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------