

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035455.D
 Acq On : 06 Dec 2024 10:41
 Operator : RC/JU
 Sample : PB165411BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK411

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035455.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	8	12	21	rBV	21755	27135	1.02%	0.103%
2	3.358	76	80	97	rBV	99647	280377	10.49%	1.068%
3	3.634	125	127	132	rVB2	4833	6298	0.24%	0.024%
4	6.505	609	615	628	rVB	414840	603885	22.60%	2.300%
5	6.658	635	641	655	rVB	265590	397508	14.88%	1.514%
6	6.840	666	672	682	rBV	420961	619980	23.21%	2.361%
7	7.293	742	749	760	rBV	325997	500549	18.74%	1.906%
8	8.011	865	871	882	rBV	499873	784995	29.38%	2.989%
9	8.434	936	943	952	rBV	322320	490637	18.36%	1.868%
10	9.146	1057	1064	1071	rBV	283216	437757	16.38%	1.667%
11	9.681	1148	1155	1168	rBV	536745	858164	32.12%	3.268%
12	10.046	1210	1217	1225	rBV	436434	707451	26.48%	2.694%
13	10.199	1235	1243	1261	rBV	362285	667882	25.00%	2.543%
14	11.528	1463	1469	1476	rBV5	2591	5614	0.21%	0.021%
15	11.646	1484	1489	1495	rVB4	6142	10586	0.40%	0.040%
16	13.387	1779	1785	1797	rBV	962572	1306475	48.90%	4.975%
17	13.640	1821	1828	1838	rBV	1008835	1491864	55.84%	5.681%
18	13.957	1874	1882	1895	rBV	842214	1176812	44.05%	4.481%
19	14.193	1915	1922	1939	rBV	368105	612545	22.93%	2.333%
20	14.963	2047	2053	2066	rBV	1365681	1952895	73.10%	7.437%
21	15.098	2070	2076	2085	rBV	426493	548956	20.55%	2.090%
22	15.204	2090	2094	2099	rBV4	5745	7634	0.29%	0.029%
23	16.510	2313	2316	2322	rVB4	2047	3406	0.13%	0.013%
24	16.722	2346	2352	2363	rBV	1109962	1550336	58.03%	5.904%
25	16.822	2363	2369	2382	rVV2	1628592	2198012	82.27%	8.370%
26	18.704	2684	2689	2694	rVB	16981	23612	0.88%	0.090%
27	18.775	2696	2701	2705	rVV2	16770	21807	0.82%	0.083%
28	19.145	2758	2764	2775	rBV	2091749	2671696	100.00%	10.174%
29	20.975	3070	3075	3083	rBV	1446819	1827389	68.40%	6.959%
30	23.469	3490	3499	3513	rBV	1211541	2634365	98.60%	10.032%
31	23.645	3521	3529	3540	rBV2	837375	1833796	68.64%	6.983%




Sum of corrected areas: 26260418

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035455.D
Acq On : 06 Dec 2024 10:41
Operator : RC/JU
Sample : PB165411BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK411

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

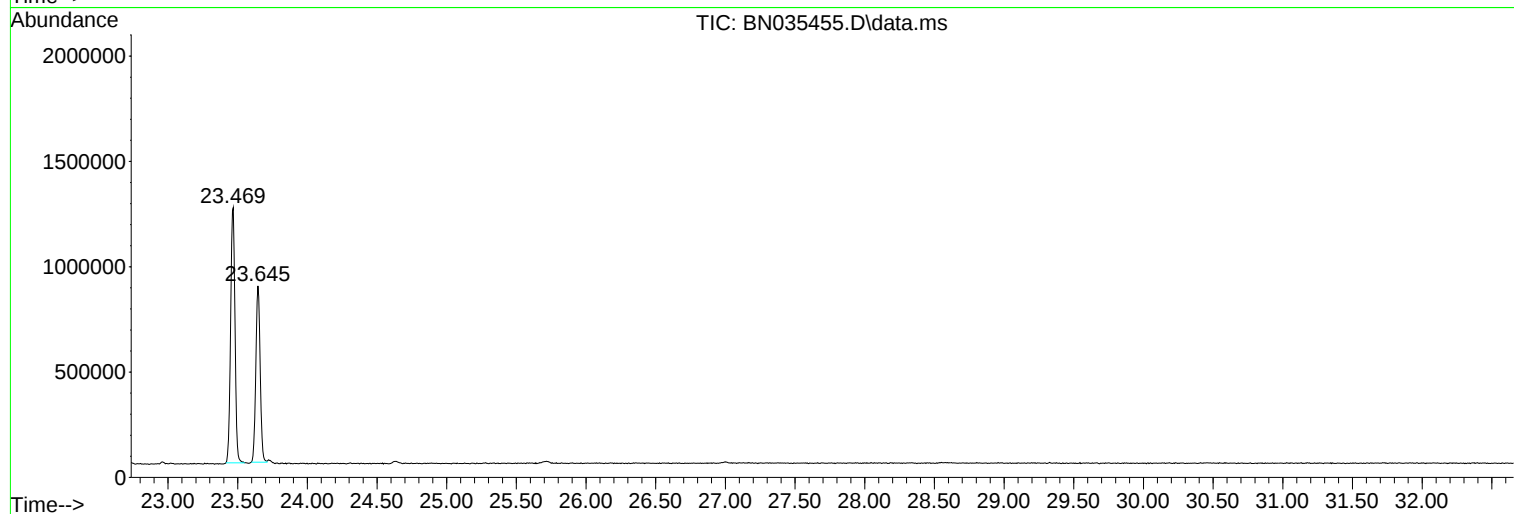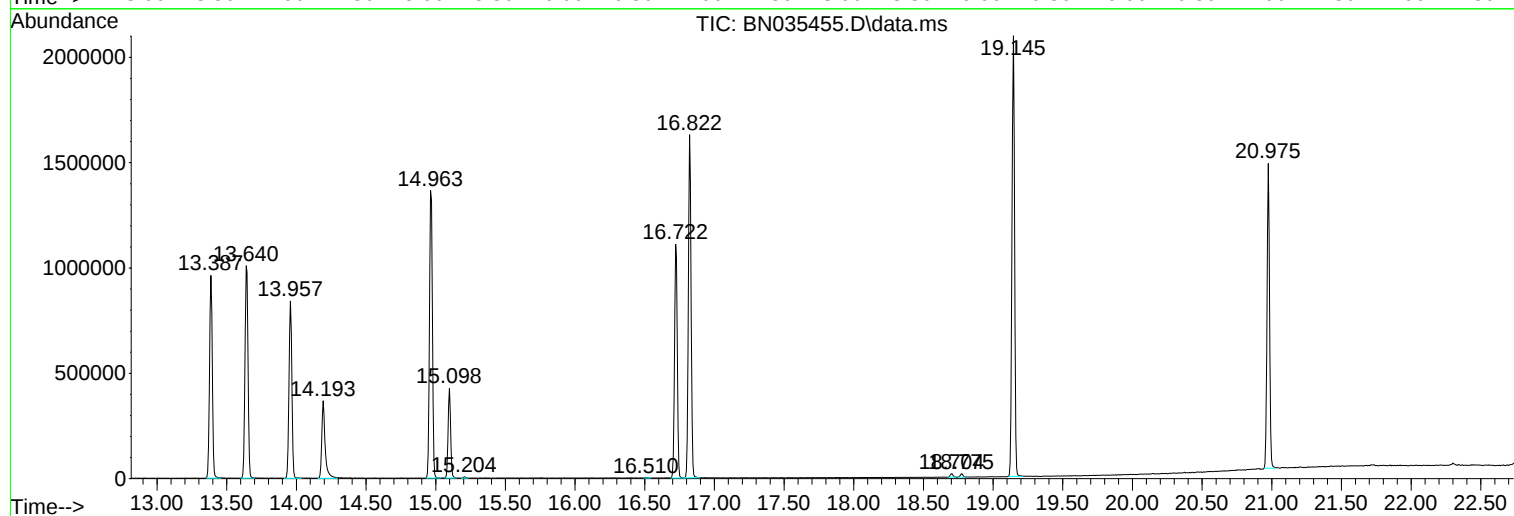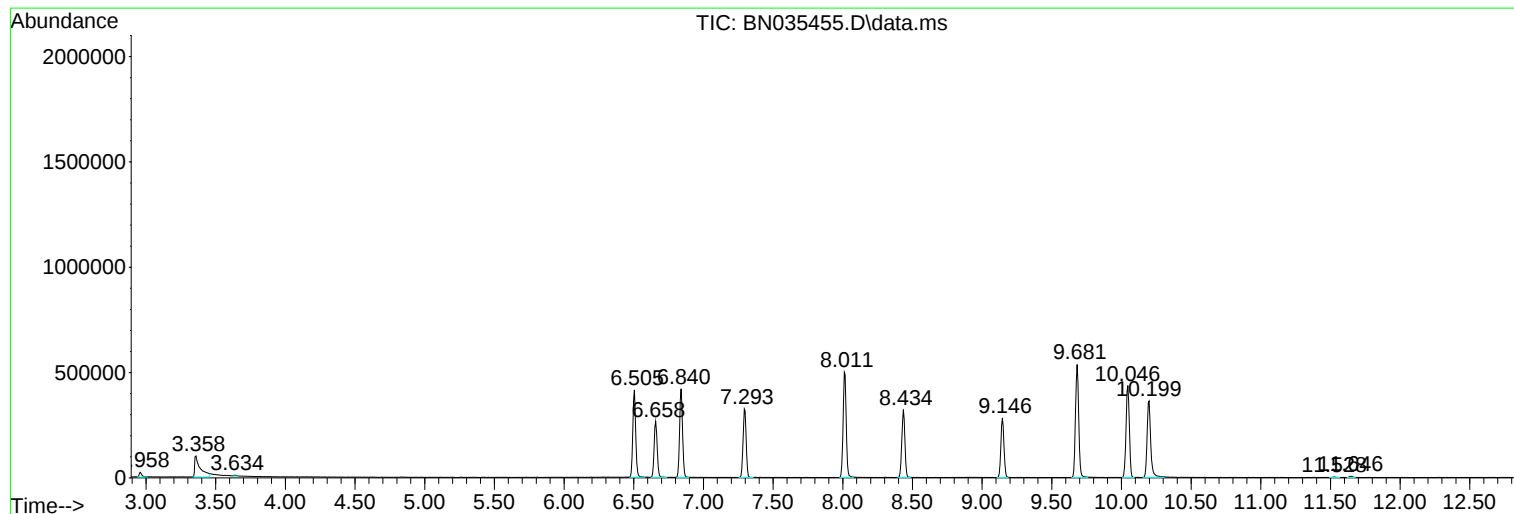

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035455.D
Acq On : 06 Dec 2024 10:41
Operator : RC/JU
Sample : PB165411BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK411

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035455.D
Acq On : 06 Dec 2024 10:41
Operator : RC/JU
Sample : PB165411BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK411

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc