

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035457.D
 Acq On : 06 Dec 2024 11:59
 Operator : RC/JU
 Sample : P5104-18
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHJ75

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035457.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	9	12	19	rVB	11622	15103	0.47%	0.059%
2	3.346	74	78	88	rBV	34309	55184	1.73%	0.215%
3	3.640	124	128	132	rBV2	3636	4268	0.13%	0.017%
4	4.069	196	201	210	rVB	8646	14318	0.45%	0.056%
5	6.499	608	614	623	rVB	136109	201295	6.30%	0.783%
6	6.657	633	641	651	rBV	246554	362622	11.35%	1.410%
7	6.840	666	672	684	rVB	312325	472958	14.80%	1.839%
8	7.299	742	750	758	rVB	294784	455830	14.26%	1.772%
9	8.010	864	871	881	rBV	355835	526262	16.47%	2.046%
10	8.434	935	943	952	rBV	301671	459830	14.39%	1.788%
11	8.898	1018	1022	1026	rVB3	4552	6184	0.19%	0.024%
12	9.146	1057	1064	1071	rBV	268883	410995	12.86%	1.598%
13	9.681	1148	1155	1169	rBV	453288	722373	22.60%	2.809%
14	10.045	1210	1217	1225	rBV	436421	699266	21.88%	2.719%
15	10.193	1235	1242	1253	rBV	315386	501168	15.68%	1.949%
16	11.381	1438	1444	1450	rBV2	2018	3738	0.12%	0.015%
17	11.645	1484	1489	1495	rBV2	5267	9008	0.28%	0.035%
18	13.386	1779	1785	1798	rBV	996103	1347695	42.17%	5.240%
19	13.639	1821	1828	1842	rBV	1022922	1484355	46.45%	5.772%
20	13.957	1875	1882	1892	rBV	820675	1168297	36.56%	4.543%
21	14.192	1916	1922	1938	rBV2	124232	219713	6.88%	0.854%
22	14.416	1956	1960	1963	rVB2	5529	6417	0.20%	0.025%
23	14.969	2047	2054	2061	rBV	1449144	2036834	63.74%	7.920%
24	15.016	2061	2062	2067	rVV2	3569	4082	0.13%	0.016%
25	15.098	2070	2076	2089	rVV	465800	605436	18.95%	2.354%
26	15.210	2090	2095	2101	rVB3	4701	6515	0.20%	0.025%
27	16.722	2346	2352	2363	rBV	1064312	1463998	45.81%	5.693%
28	16.822	2363	2369	2379	rBV2	1692780	2393440	74.90%	9.307%
29	17.669	2509	2513	2517	rBV2	13854	16102	0.50%	0.063%
30	18.704	2684	2689	2694	rVB	19692	26293	0.82%	0.102%
31	18.774	2697	2701	2707	rVB	18488	21702	0.68%	0.084%
32	18.851	2710	2714	2719	rBV2	58540	73966	2.31%	0.288%
33	18.974	2732	2735	2740	rVB4	7544	8980	0.28%	0.035%
34	19.145	2757	2764	2776	rBV	2104374	2912373	91.14%	11.325%
35	19.451	2811	2816	2820	rBV	39546	45474	1.42%	0.177%
36	20.974	3069	3075	3086	rBV	1370271	1782370	55.77%	6.931%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035457.D
Acq On : 06 Dec 2024 11:59
Operator : RC/JU
Sample : P5104-18
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ75

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION

37	22.962	3409	3413	3419	rVB4	26013	42625	1.33%	0.166%
38	23.468	3490	3499	3518	rVB	1453661	3195669	100.00%	12.426%
39	23.645	3521	3529	3538	rBV2	878917	1934558	60.54%	7.522%




Sum of corrected areas: 25717296

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035457.D
Acq On : 06 Dec 2024 11:59
Operator : RC/JU
Sample : P5104-18
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ75

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

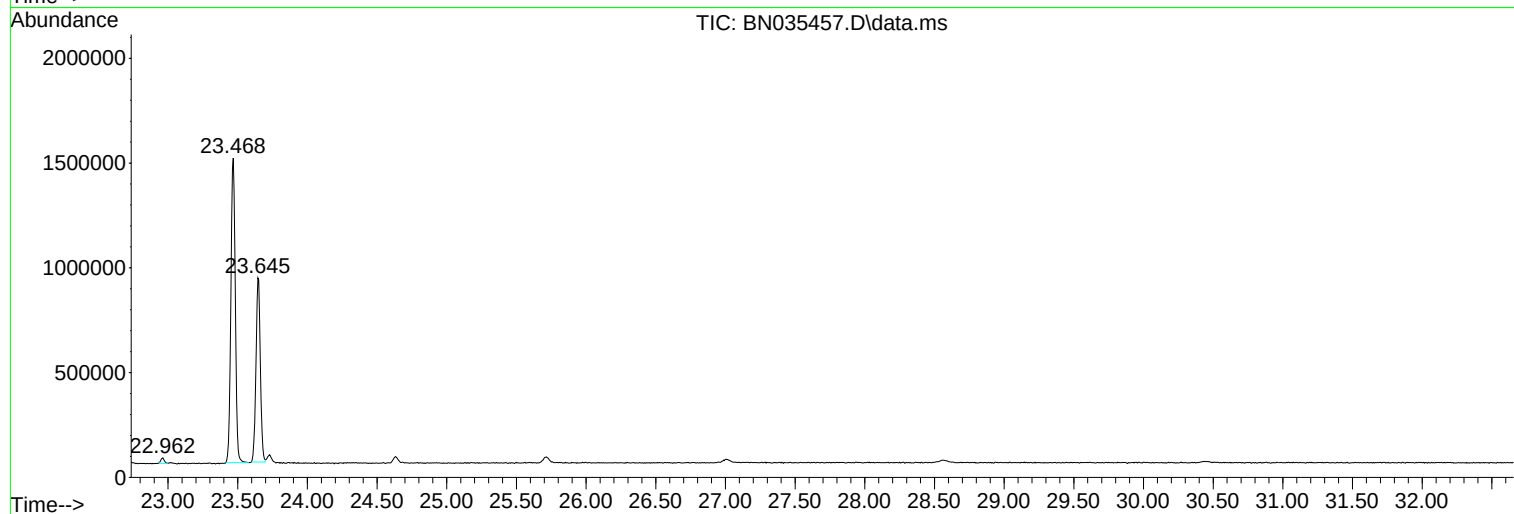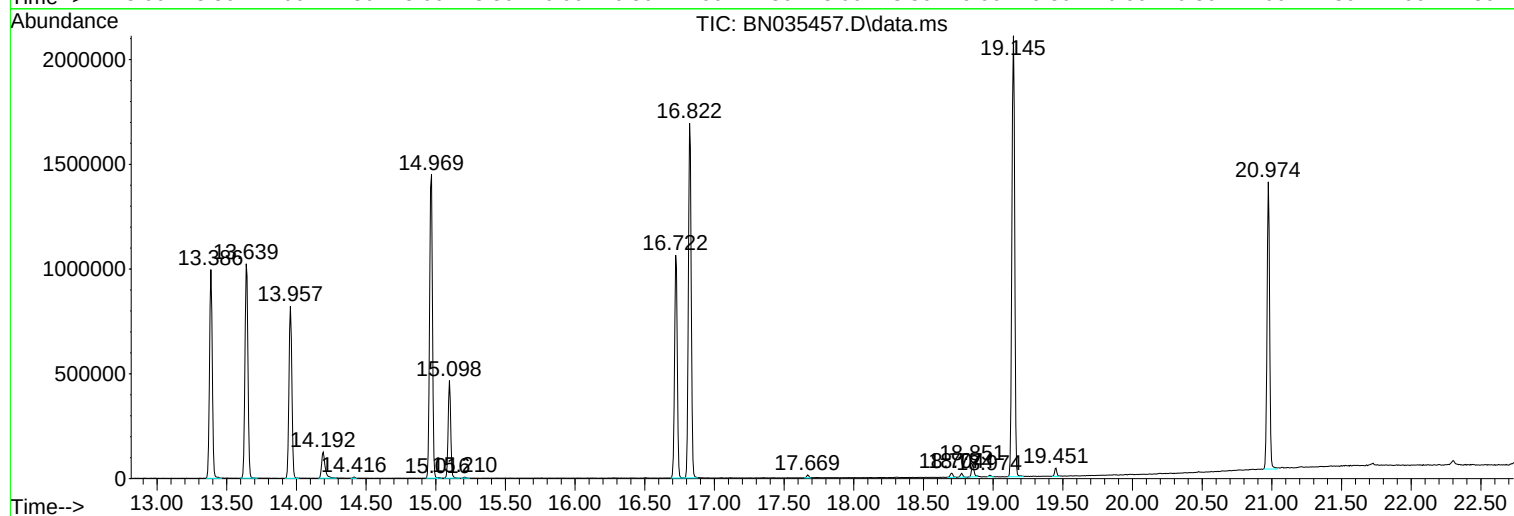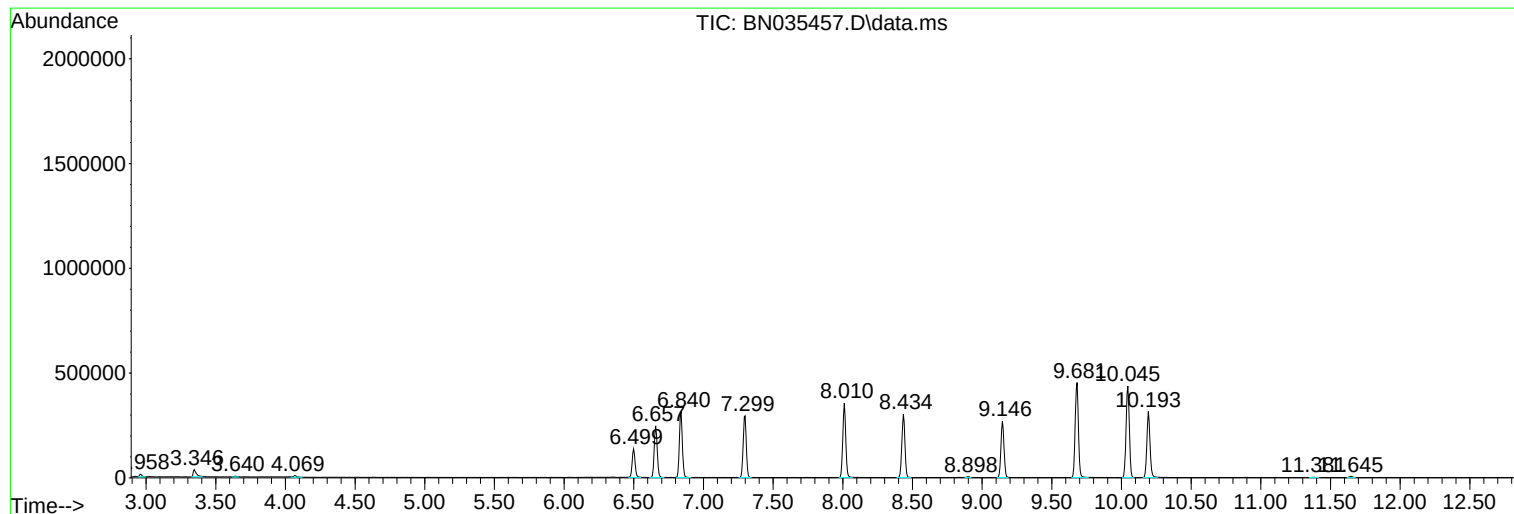

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035457.D
Acq On : 06 Dec 2024 11:59
Operator : RC/JU
Sample : P5104-18
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ75

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035457.D
Acq On : 06 Dec 2024 11:59
Operator : RC/JU
Sample : P5104-18
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ75

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc