

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035462.D
 Acq On : 06 Dec 2024 15:14
 Operator : RC/JU
 Sample : P5107-04
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHJ81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035462.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.928	4	7	9	rBV3	2782	3360	0.11%	0.013%
2	2.958	9	12	20	rVB	13468	18152	0.57%	0.070%
3	3.346	74	78	91	rBV	46170	78349	2.48%	0.303%
4	3.640	124	128	131	rBV	5372	7044	0.22%	0.027%
5	4.064	196	200	209	rVB	9133	16059	0.51%	0.062%
6	6.499	607	614	620	rBV	92865	134190	4.25%	0.518%
7	6.658	635	641	649	rBV	244878	358818	11.36%	1.386%
8	6.840	665	672	680	rBV	284320	433485	13.73%	1.674%
9	7.293	743	749	759	rVB	319329	491828	15.58%	1.900%
10	8.011	864	871	882	rBV	278389	413869	13.11%	1.598%
11	8.434	936	943	951	rBV	307858	453394	14.36%	1.751%
12	8.587	965	969	972	rBV2	3028	3591	0.11%	0.014%
13	8.905	1019	1023	1026	rVB3	3914	5034	0.16%	0.019%
14	9.146	1057	1064	1075	rBV	267221	408420	12.93%	1.577%
15	9.681	1148	1155	1174	rBV	442450	723207	22.90%	2.793%
16	10.046	1210	1217	1225	rVB	473047	752576	23.83%	2.907%
17	10.193	1235	1242	1254	rBV	302318	486800	15.42%	1.880%
18	11.387	1440	1445	1449	rVB3	2594	4386	0.14%	0.017%
19	11.646	1484	1489	1494	rBV2	5120	8858	0.28%	0.034%
20	13.387	1779	1785	1793	rBV	984349	1332828	42.21%	5.148%
21	13.640	1822	1828	1840	rBV	1047785	1484544	47.02%	5.734%
22	13.957	1875	1882	1895	rVB	886813	1253002	39.68%	4.839%
23	14.193	1917	1922	1938	rBV	85726	147257	4.66%	0.569%
24	14.963	2047	2053	2061	rVV	1402327	2018476	63.93%	7.796%
25	15.016	2061	2062	2067	rVV3	4029	4504	0.14%	0.017%
26	15.098	2070	2076	2087	rVV	480550	602461	19.08%	2.327%
27	15.210	2091	2095	2099	rVV	5476	6905	0.22%	0.027%
28	15.345	2113	2118	2126	rVB	21300	28627	0.91%	0.111%
29	16.722	2346	2352	2362	rBV	1155777	1570095	49.73%	6.064%
30	16.822	2362	2369	2380	rBV2	1699172	2401391	76.05%	9.275%
31	17.669	2509	2513	2522	rBV2	23574	30693	0.97%	0.119%
32	18.557	2661	2664	2667	rVB3	2773	3236	0.10%	0.012%
33	18.704	2684	2689	2694	rVB	22132	27854	0.88%	0.108%
34	18.775	2697	2701	2706	rBV	20228	24574	0.78%	0.095%
35	18.857	2710	2715	2728	rVV	66020	97996	3.10%	0.378%
36	18.975	2731	2735	2742	rBV4	15762	21855	0.69%	0.084%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035462.D
Acq On : 06 Dec 2024 15:14
Operator : RC/JU
Sample : P5107-04
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ81

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION

37	19.145	2758	2764	2772	rBV	2224812	2992869	94.79%	11.559%
38	20.728	3031	3033	3037	rBV5	8625	11486	0.36%	0.044%
39	20.975	3069	3075	3083	rBV	1406219	1872370	59.30%	7.231%
40	23.469	3490	3499	3510	rBV	1420427	3157491	100.00%	12.195%
41	23.645	3521	3529	3538	rBV	881238	1937744	61.37%	7.484%
42	24.633	3693	3697	3708	rVB7	25664	62498	1.98%	0.241%




Sum of corrected areas: 25892176

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035462.D
Acq On : 06 Dec 2024 15:14
Operator : RC/JU
Sample : P5107-04
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ81

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

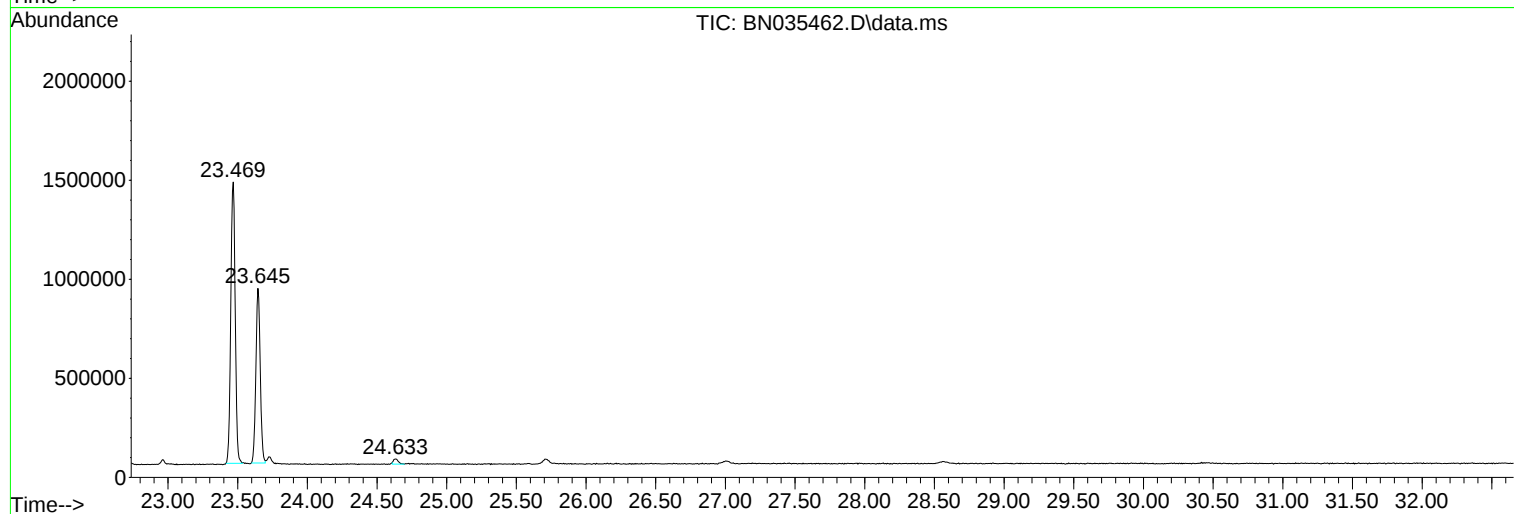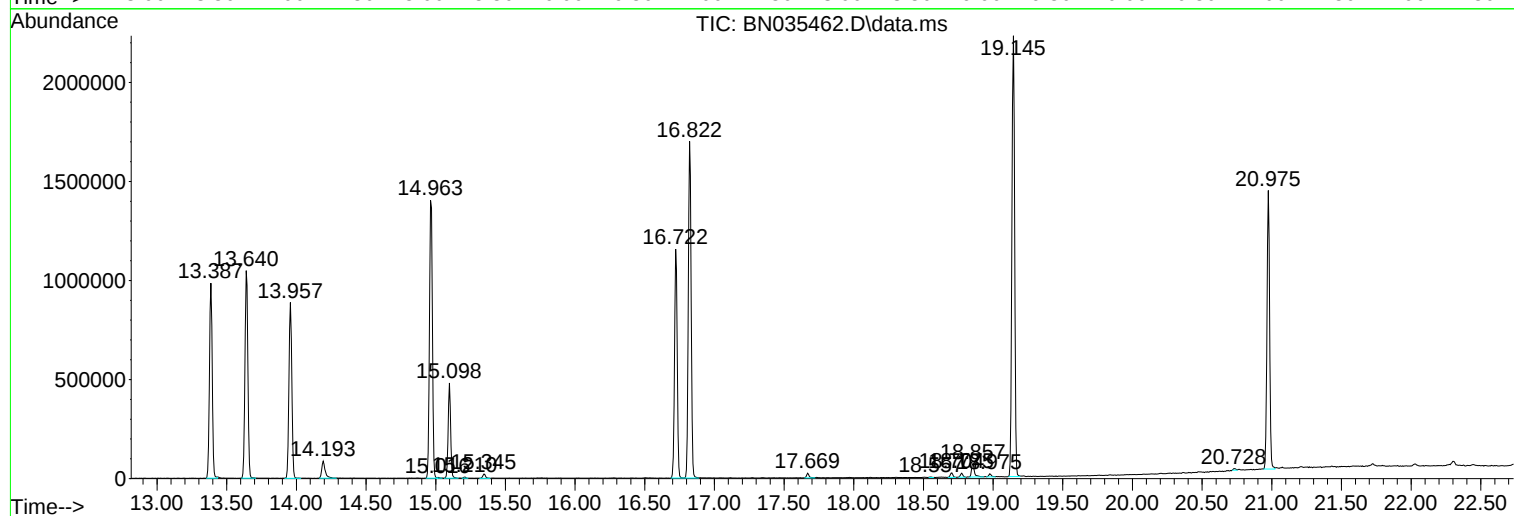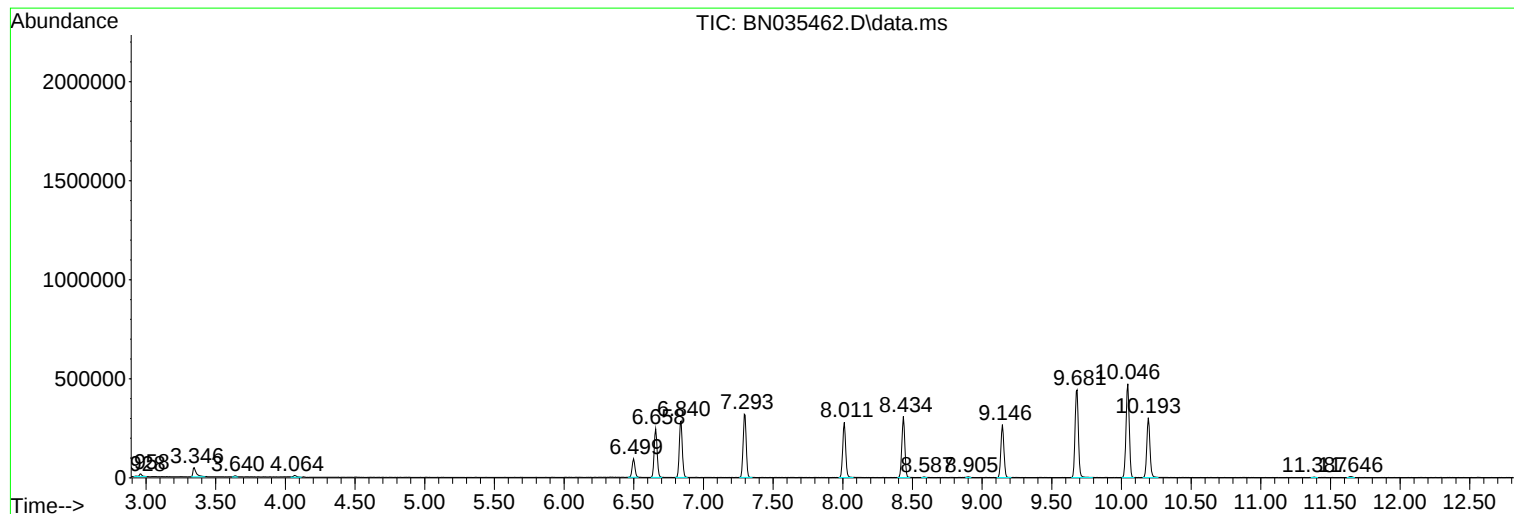

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035462.D
Acq On : 06 Dec 2024 15:14
Operator : RC/JU
Sample : P5107-04
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ81

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035462.D
Acq On : 06 Dec 2024 15:14
Operator : RC/JU
Sample : P5107-04
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ81

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc