

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035469.D
 Acq On : 06 Dec 2024 20:26
 Operator : RC/JU
 Sample : PB165417BL
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK417

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035469.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.957	9	12	18	rBV	20935	27084	0.96%	0.094%
2	3.352	76	79	104	rBV	114171	326846	11.53%	1.140%
3	3.640	124	128	132	rVB3	5172	7831	0.28%	0.027%
4	6.504	608	615	626	rBV	421398	632961	22.33%	2.207%
5	6.657	635	641	649	rVB	283536	418744	14.77%	1.460%
6	6.840	665	672	682	rBV	441383	648368	22.87%	2.261%
7	7.293	741	749	758	rBV	364190	556703	19.64%	1.941%
8	8.010	865	871	886	rBV	536310	835094	29.46%	2.912%
9	8.434	936	943	956	rVB	342256	520012	18.35%	1.813%
10	9.145	1057	1064	1072	rBV	307367	462081	16.30%	1.611%
11	9.681	1148	1155	1169	rBV	563647	907955	32.03%	3.166%
12	10.045	1209	1217	1224	rBV	501013	804702	28.39%	2.806%
13	10.192	1235	1242	1261	rBV	377025	721078	25.44%	2.515%
14	11.528	1460	1469	1473	rBV3	2975	7093	0.25%	0.025%
15	11.645	1483	1489	1496	rVB3	6880	11679	0.41%	0.041%
16	13.386	1779	1785	1797	rBV	1018033	1391315	49.08%	4.852%
17	13.639	1821	1828	1835	rBV	1089039	1604245	56.60%	5.594%
18	13.957	1875	1882	1892	rBV	975204	1352769	47.72%	4.717%
19	14.192	1916	1922	1939	rBV	383142	655289	23.12%	2.285%
20	14.963	2047	2053	2070	rBV	1427438	2050199	72.33%	7.149%
21	15.098	2070	2076	2084	rBV	441561	565104	19.94%	1.971%
22	15.204	2090	2094	2098	rBV3	4926	6260	0.22%	0.022%
23	16.510	2311	2316	2321	rVB2	2392	3450	0.12%	0.012%
24	16.721	2346	2352	2362	rVB	1263717	1763395	62.21%	6.149%
25	16.821	2363	2369	2381	rVB	1682371	2335949	82.41%	8.146%
26	18.704	2684	2689	2693	rBV	20269	27353	0.96%	0.095%
27	18.774	2696	2701	2706	rVV	19037	24441	0.86%	0.085%
28	19.145	2758	2764	2775	rBV	2132748	2834543	100.00%	9.885%
29	20.974	3069	3075	3085	rBV	1637479	2091801	73.80%	7.295%
30	22.298	3298	3300	3309	rVB2	32705	46810	1.65%	0.163%
31	22.956	3409	3412	3419	rVB3	29196	48904	1.73%	0.171%
32	23.462	3490	3498	3515	rVB	1300781	2783097	98.19%	9.705%
33	23.645	3521	3529	3538	rBV	932212	2046063	72.18%	7.135%
34	23.727	3539	3543	3549	rVB3	39915	78046	2.75%	0.272%
35	24.633	3692	3697	3707	rVB6	32802	78985	2.79%	0.275%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035469.D
Acq On : 06 Dec 2024 20:26
Operator : RC/JU
Sample : PB165417BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK417

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 28676249

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035469.D
Acq On : 06 Dec 2024 20:26
Operator : RC/JU
Sample : PB165417BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK417

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

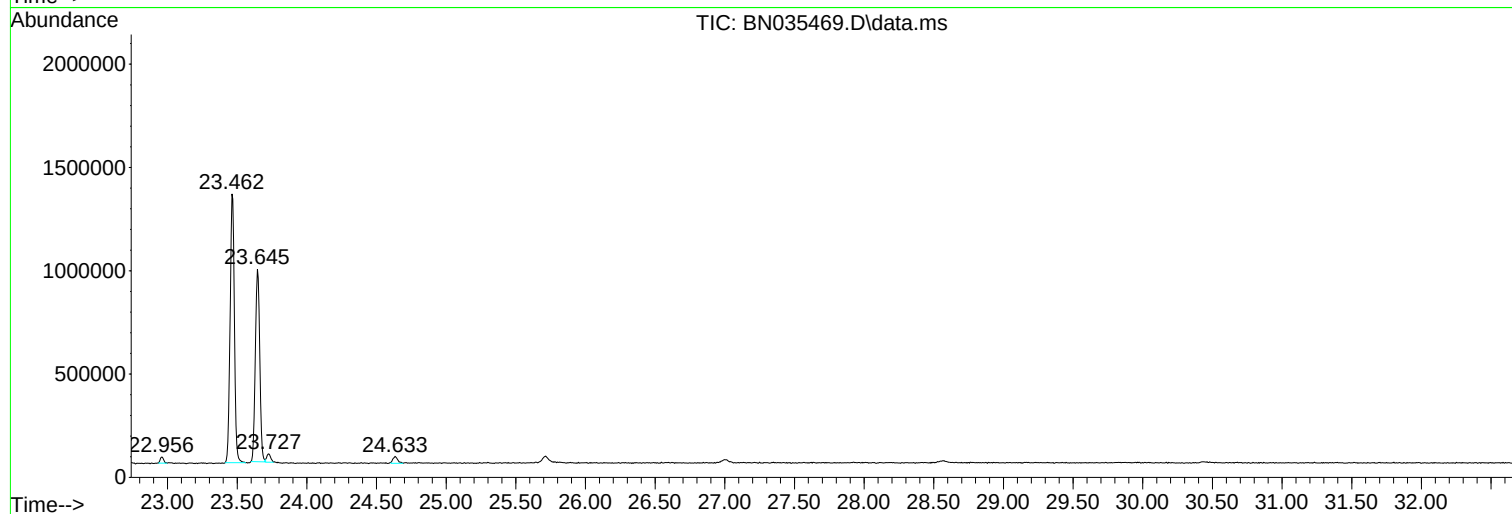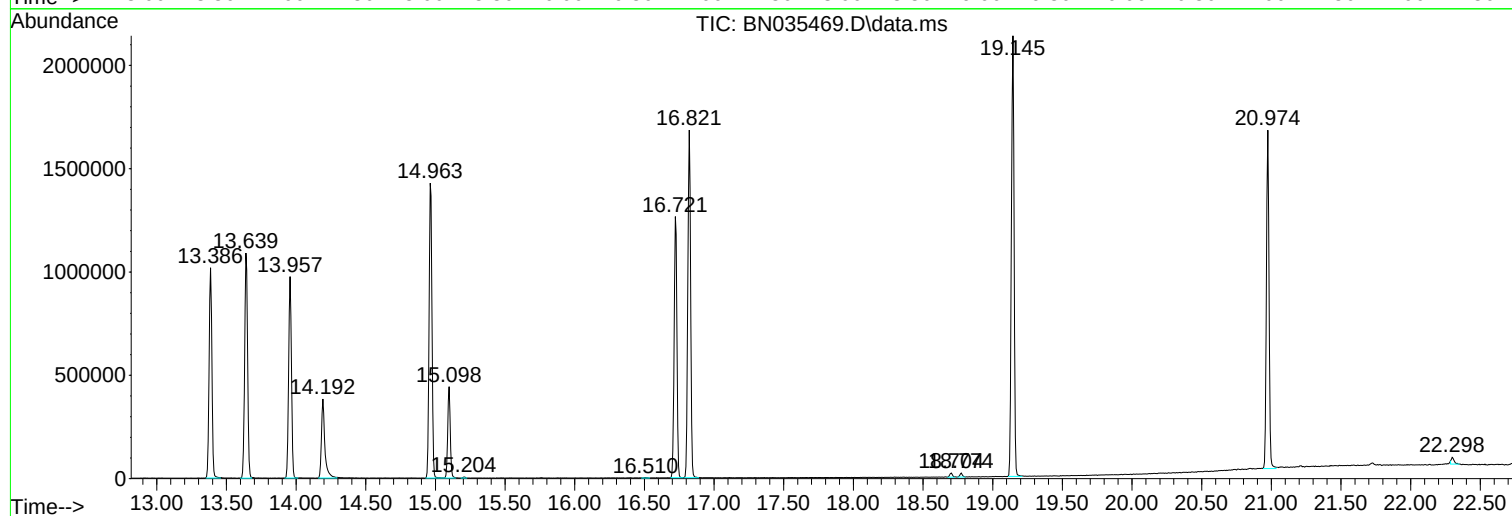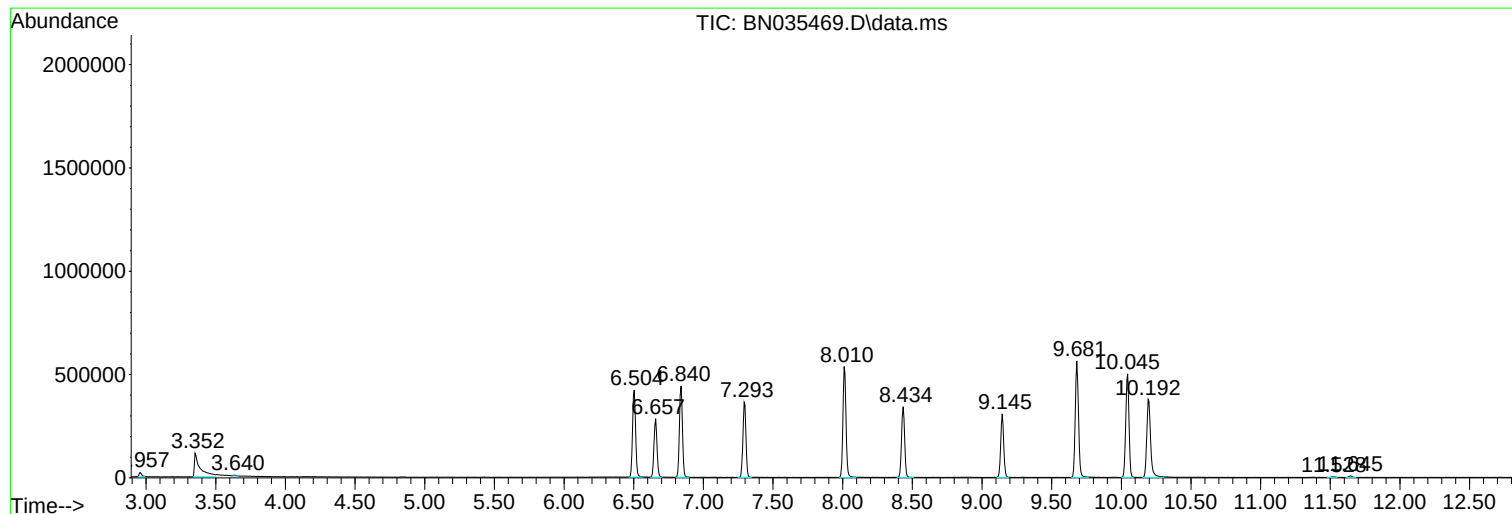

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035469.D
Acq On : 06 Dec 2024 20:26
Operator : RC/JU
Sample : PB165417BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK417

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035469.D
Acq On : 06 Dec 2024 20:26
Operator : RC/JU
Sample : PB165417BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK417

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc