

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035470.D
 Acq On : 06 Dec 2024 21:04
 Operator : RC/JU
 Sample : PB165443BL
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK443

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	8	12	21	rVB	21699	27376	1.03%	0.102%
2	3.352	76	79	101	rBV	109662	303488	11.45%	1.134%
3	3.634	124	127	130	rVB2	2948	3637	0.14%	0.014%
4	6.016	529	532	540	rBV4	1397	2784	0.11%	0.010%
5	6.505	608	615	626	rVB	396095	599881	22.63%	2.242%
6	6.657	634	641	650	rVB	259847	391022	14.75%	1.461%
7	6.840	666	672	685	rVB	416801	611989	23.09%	2.287%
8	7.293	741	749	757	rBV	343070	523199	19.74%	1.955%
9	8.010	865	871	880	rBV	514324	787384	29.70%	2.943%
10	8.434	936	943	954	rBV	320374	492272	18.57%	1.840%
11	9.146	1057	1064	1071	rBV	286635	434534	16.39%	1.624%
12	9.681	1148	1155	1167	rBV	527679	857309	32.34%	3.204%
13	10.046	1209	1217	1226	rBV	466943	758682	28.62%	2.836%
14	10.193	1234	1242	1258	rBV	365747	671706	25.34%	2.510%
15	11.522	1463	1468	1472	rBV4	3495	5917	0.22%	0.022%
16	11.645	1483	1489	1494	rVB2	5829	10523	0.40%	0.039%
17	13.387	1777	1785	1797	rBV	974073	1317809	49.71%	4.925%
18	13.639	1821	1828	1838	rBV2	1031845	1530462	57.73%	5.720%
19	13.957	1875	1882	1891	rBV	878057	1269758	47.90%	4.746%
20	14.192	1916	1922	1942	rBV	347788	613892	23.16%	2.294%
21	14.963	2047	2053	2070	rBV	1399863	1982941	74.80%	7.411%
22	15.098	2070	2076	2089	rVV	405675	530619	20.02%	1.983%
23	15.204	2091	2094	2099	rVB	5455	6610	0.25%	0.025%
24	16.510	2312	2316	2322	rVB2	2641	4182	0.16%	0.016%
25	16.722	2346	2352	2362	rBV	1201042	1657364	62.52%	6.194%
26	16.822	2363	2369	2383	rVB	1641271	2205352	83.19%	8.242%
27	18.698	2684	2688	2694	rVB3	17515	24214	0.91%	0.090%
28	18.774	2697	2701	2707	rVV	16299	21376	0.81%	0.080%
29	18.886	2716	2720	2724	rBV6	1487	2802	0.11%	0.010%
30	19.145	2758	2764	2776	rBV	1946723	2651008	100.00%	9.908%
31	20.974	3069	3075	3086	rBV	1487936	1957543	73.84%	7.316%
32	23.462	3490	3498	3514	rBV	1234398	2591918	97.77%	9.687%
33	23.645	3521	3529	3538	rBV	882764	1906493	71.92%	7.125%




Sum of corrected areas: 26756046

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035470.D
Acq On : 06 Dec 2024 21:04
Operator : RC/JU
Sample : PB165443BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK443

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

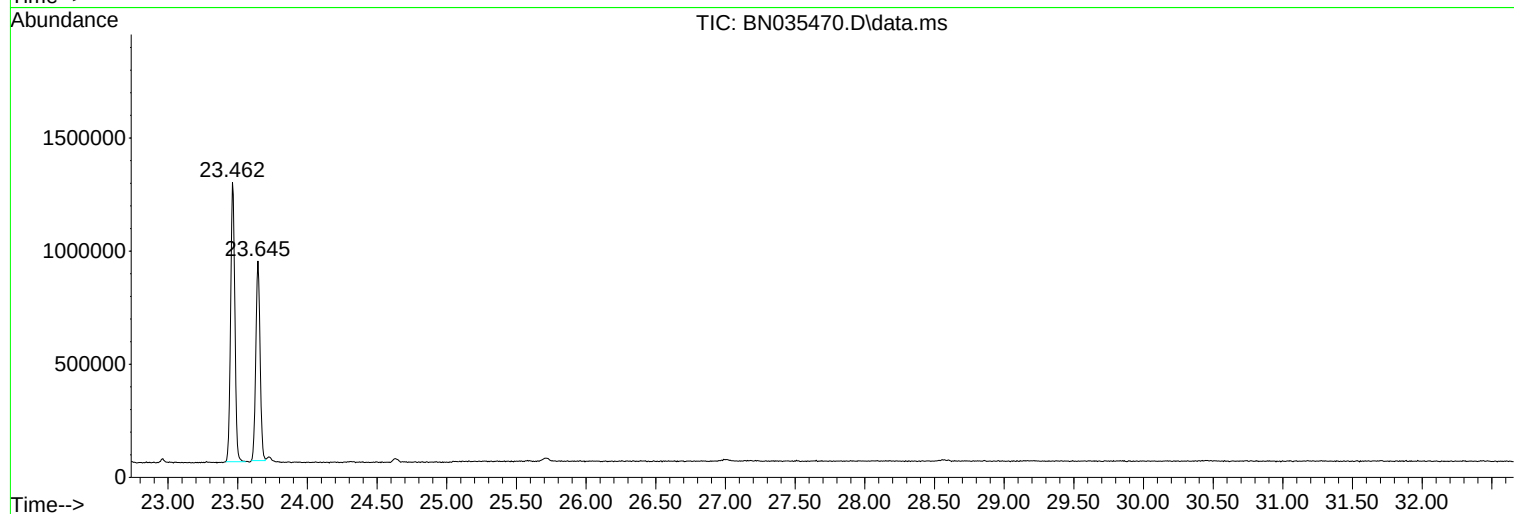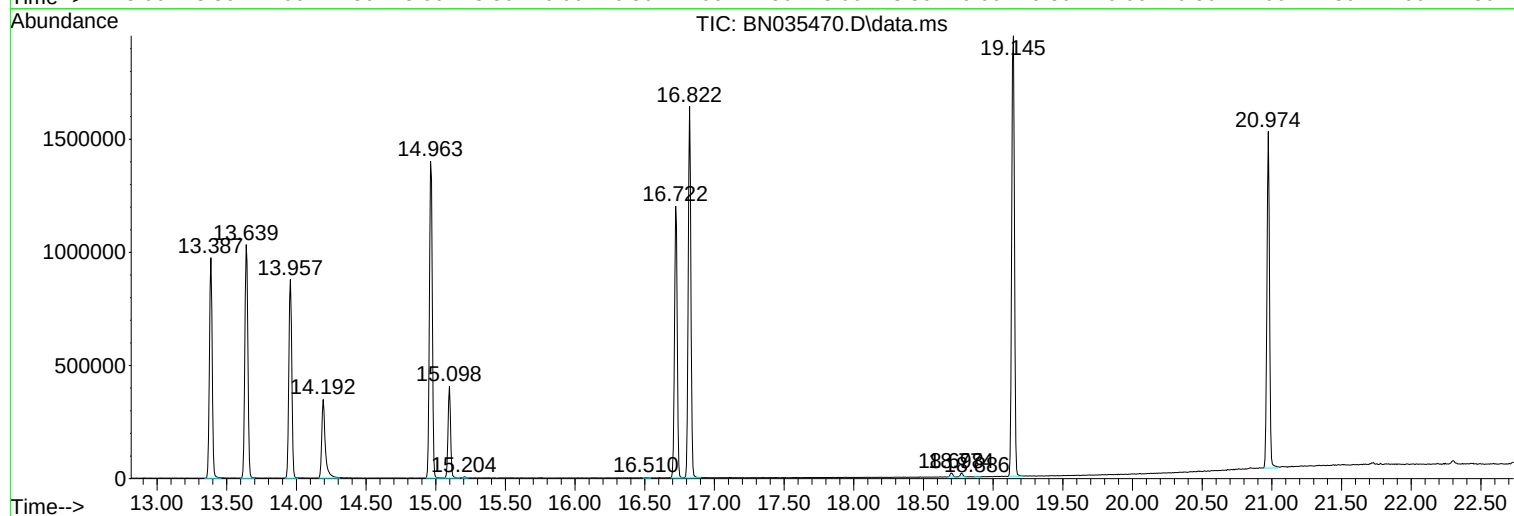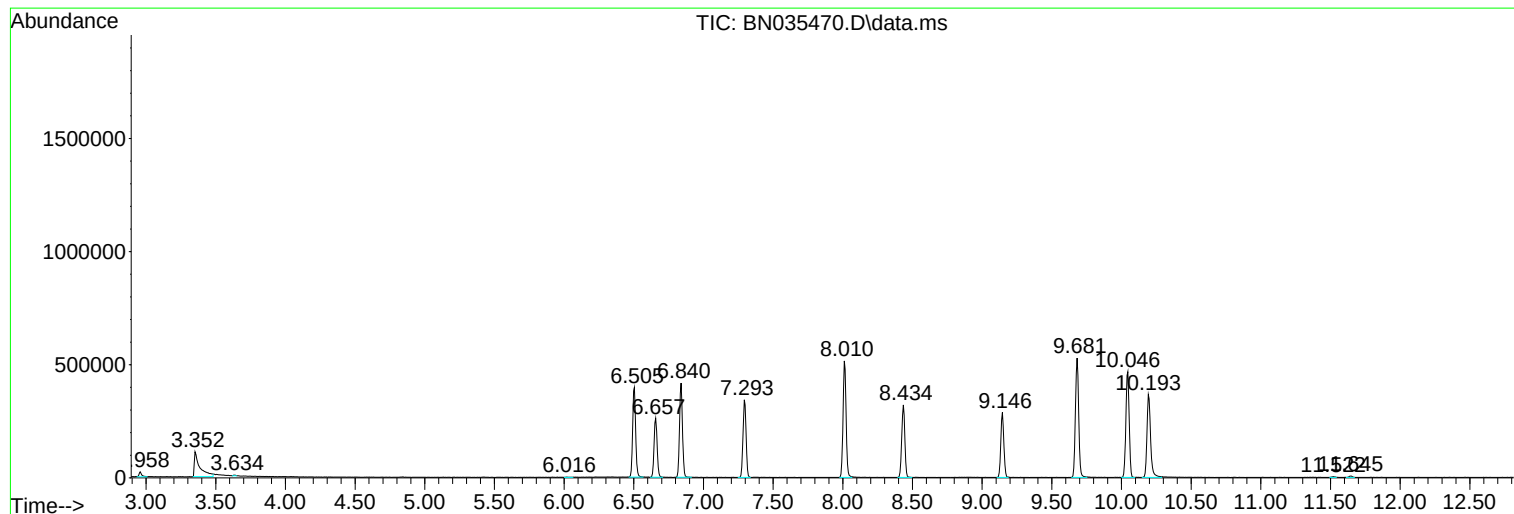

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035470.D
Acq On : 06 Dec 2024 21:04
Operator : RC/JU
Sample : PB165443BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK443

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035470.D
Acq On : 06 Dec 2024 21:04
Operator : RC/JU
Sample : PB165443BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK443

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------